
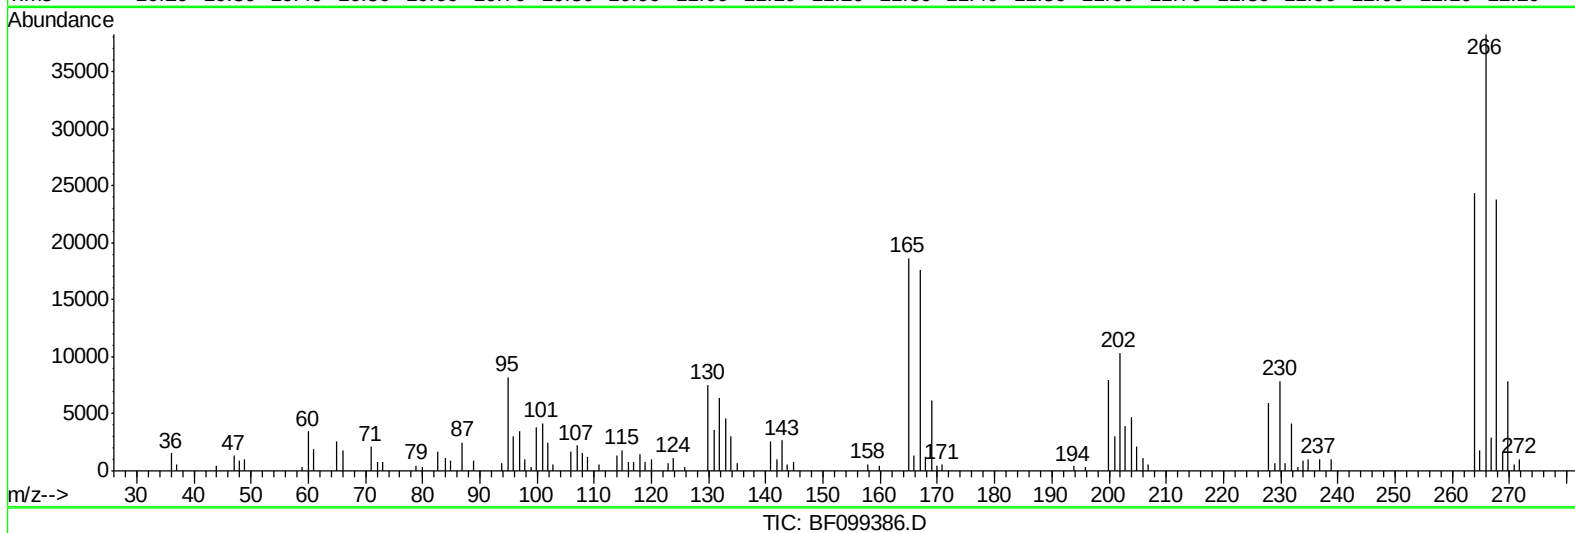


Data Path : Z:\HPCHEM1\BNA F\DATA\BF101217\
Data File : BF099386.D
Acq On : 12 Oct 2017 10:45
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 13 07:32:54 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 11 16:25:21 2017
Response via : Initial Calibration

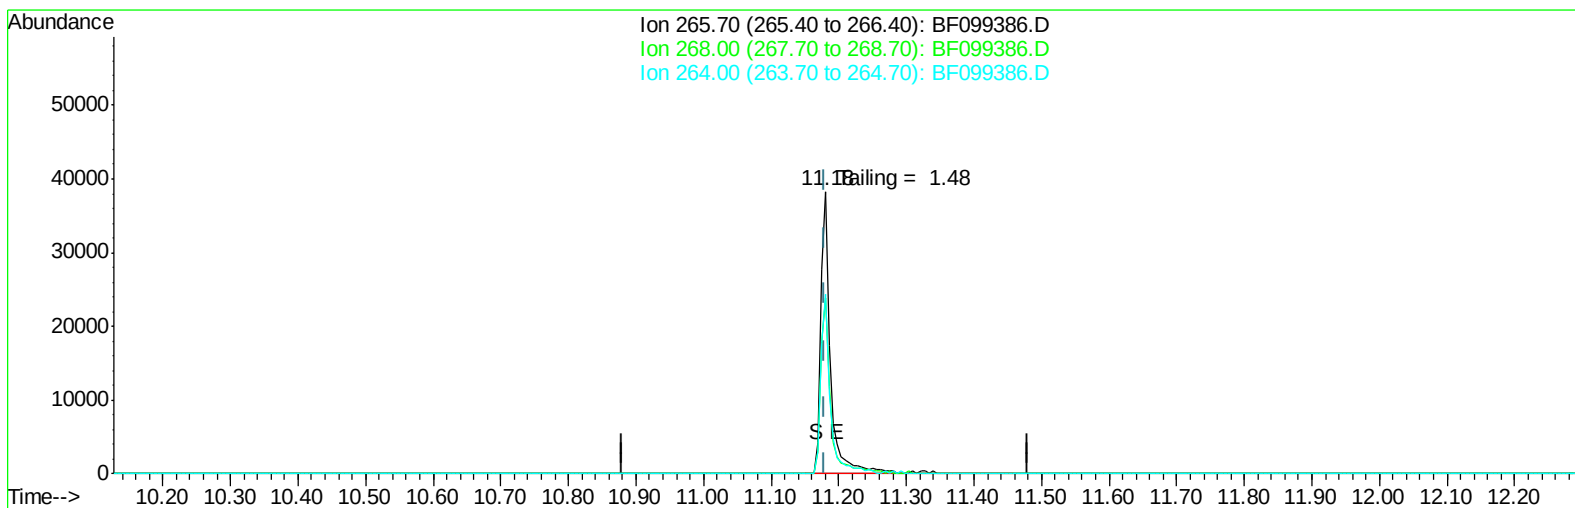

TIC: BF099386.D

(69) Pentachlorophenol (C)



11.180min (0.000) 19800.89ng

response 39165

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.28
264.00	61.90	63.76
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101217\
Data File : BF099386.D
Acq On : 12 Oct 2017 10:45
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 13 07:32:54 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 11 16:25:21 2017
Response via : Initial Calibration

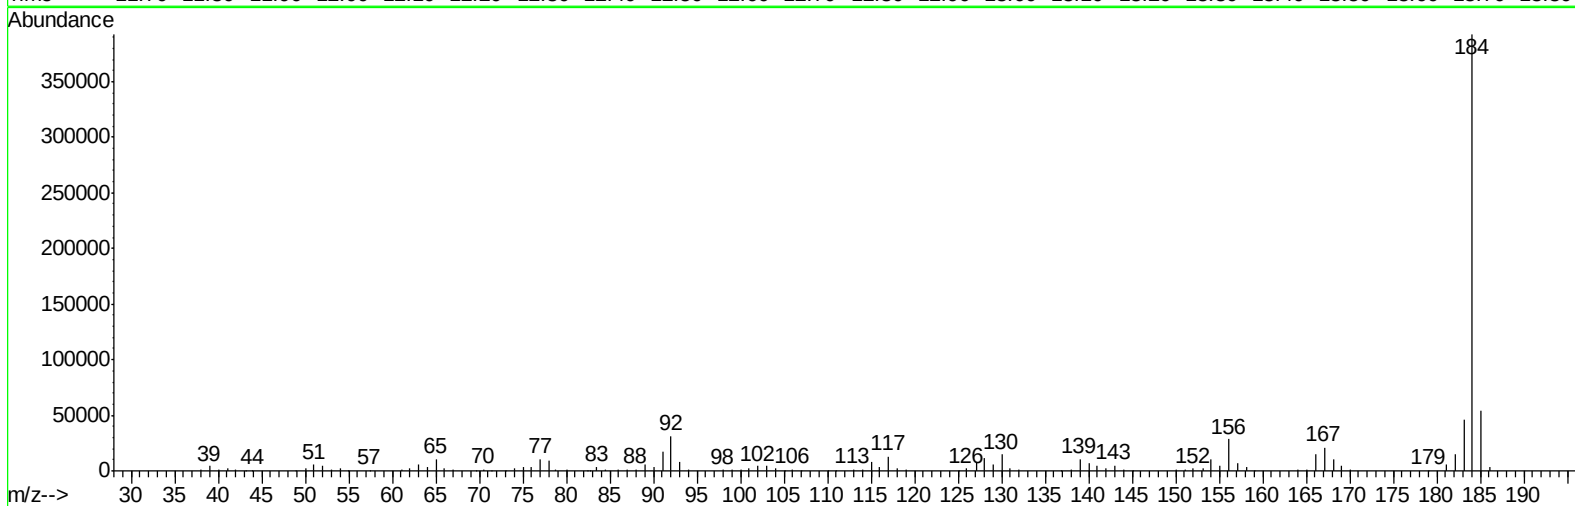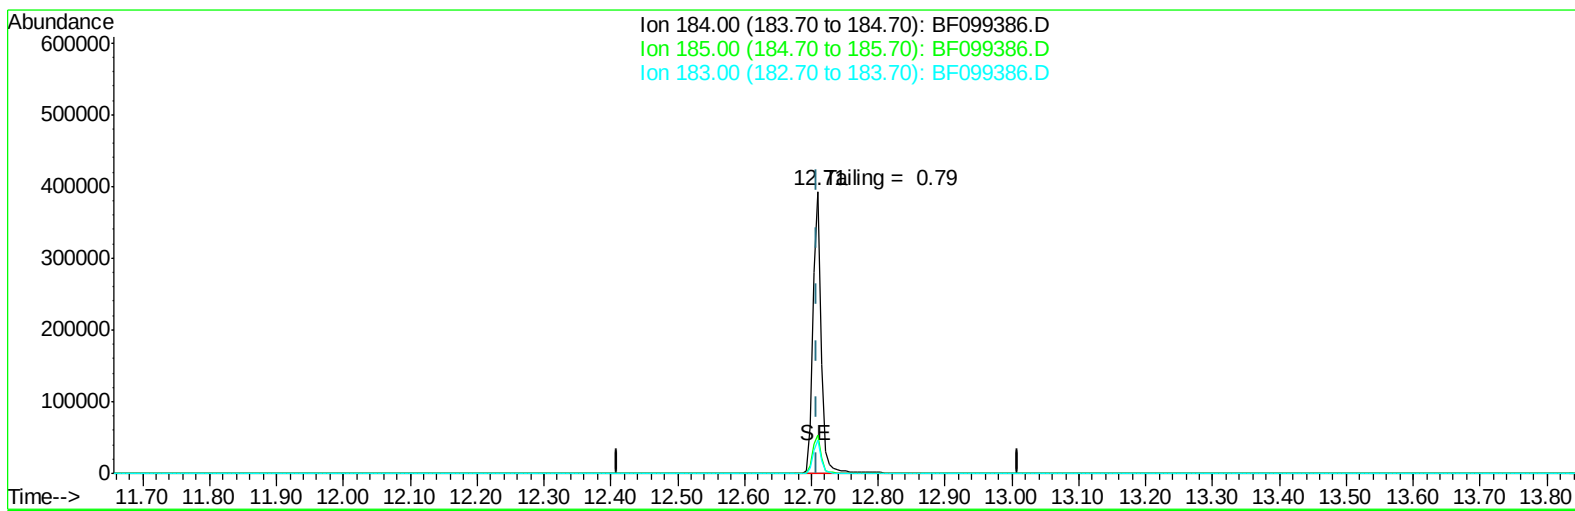

TIC: BF099386.D

(76) Benzidine

12.710min (0.000) 4424.71ng

response 343838

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.74
183.00	11.60	11.87
0.00	0.00	0.00