
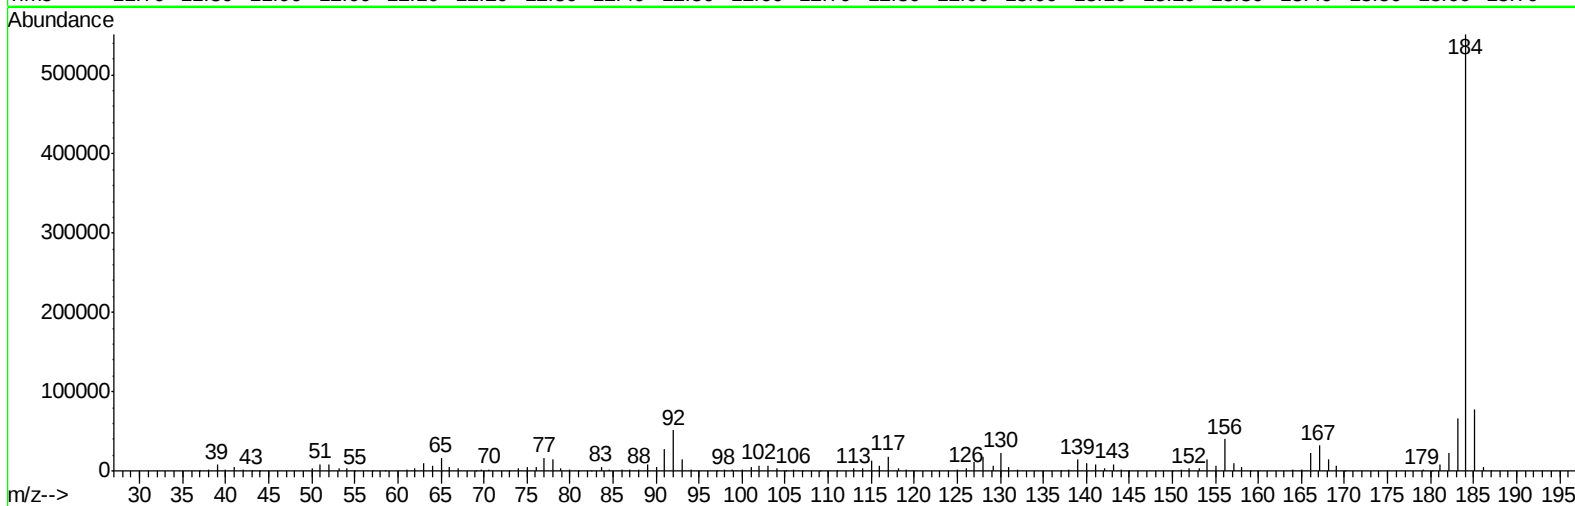


Data Path : Z:\HPCHEM1\BNA F\DATA\BF101217\
Data File : BF099396.D
Acq On : 12 Oct 2017 15:47
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 13 07:34:38 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 11 16:25:21 2017
Response via : Initial Calibration

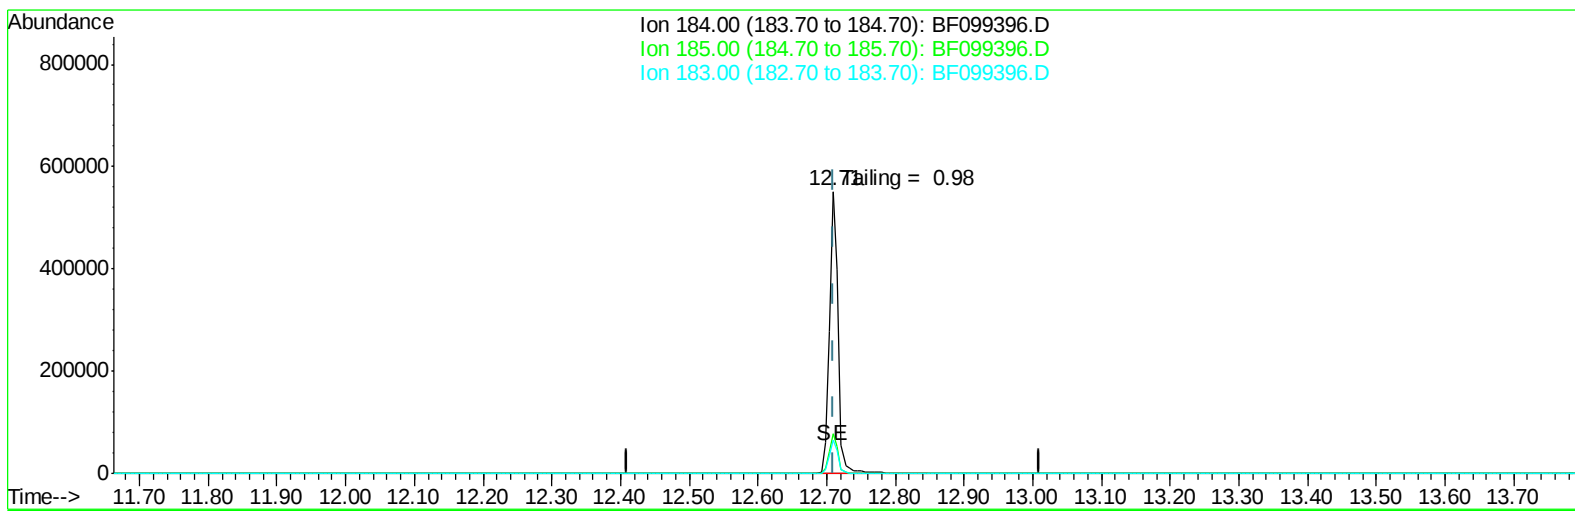

TIC: BF099396.D

(76) Benzidine



12.710min (-0.000) 0.00ng

response 493663

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.09
183.00	11.60	11.89
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101217\
Data File : BF099396.D
Acq On : 12 Oct 2017 15:47
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 13 07:48:36 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 11 16:25:21 2017
Response via : Initial Calibration

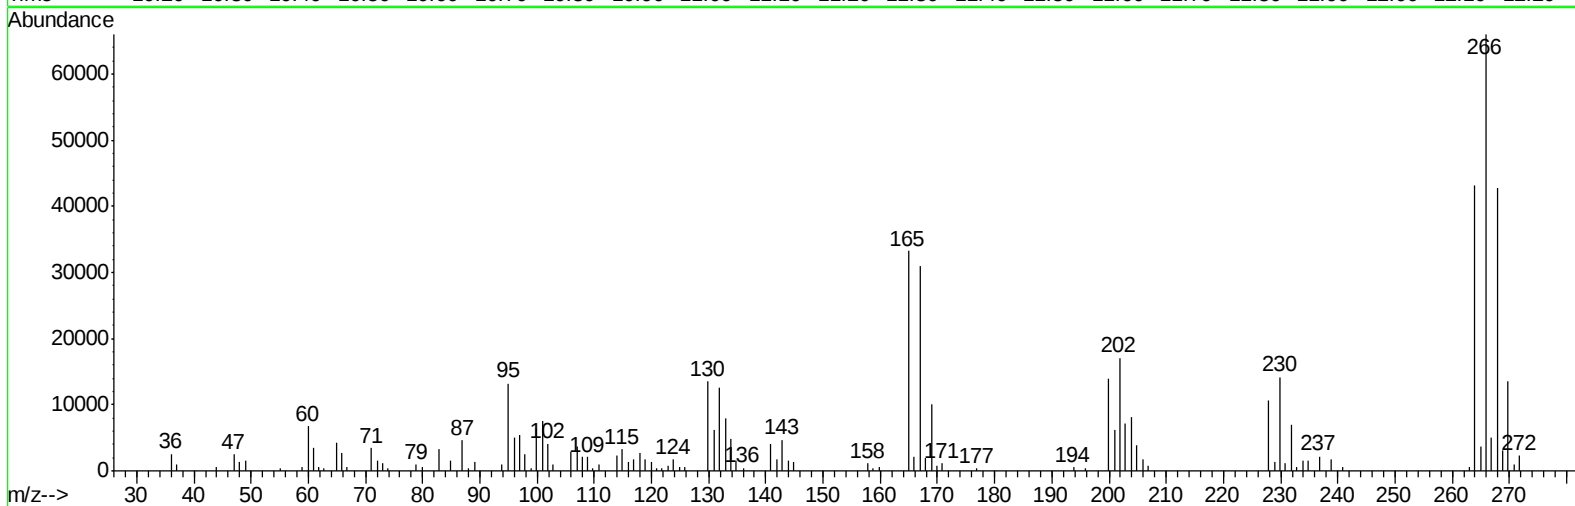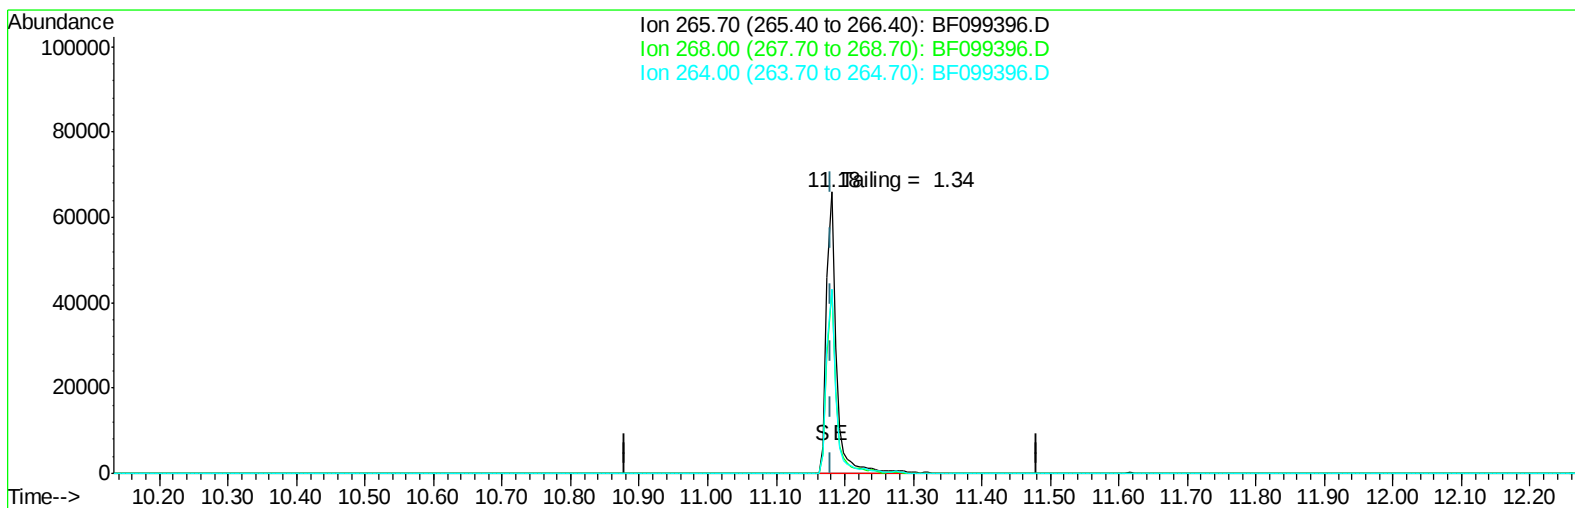

TIC: BF099396.D

(69) Pentachlorophenol (C)

11.180min (-0.000) 85660.80ng

response 63537

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.82
264.00	61.90	65.48
0.00	0.00	0.00