
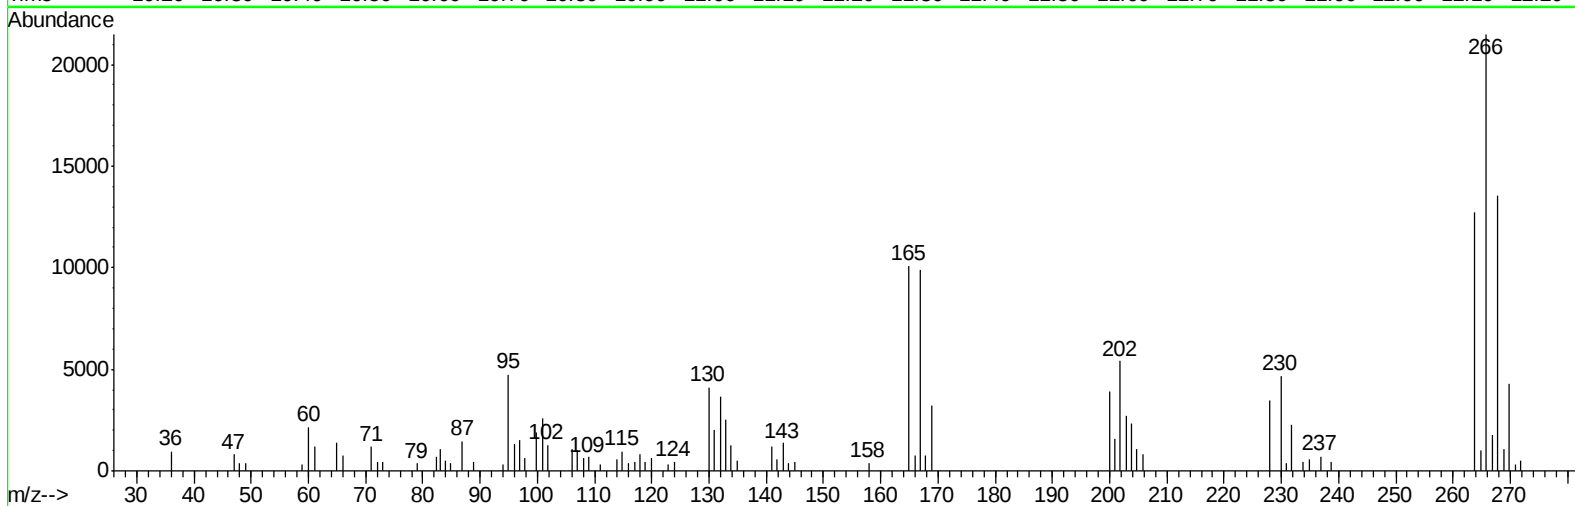


Data Path : Z:\HPCHEM1\BNA F\DATA\BF101217\
Data File : BF099422.D
Acq On : 13 Oct 2017 4:24
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 13 07:36:14 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 11 16:25:21 2017
Response via : Initial Calibration

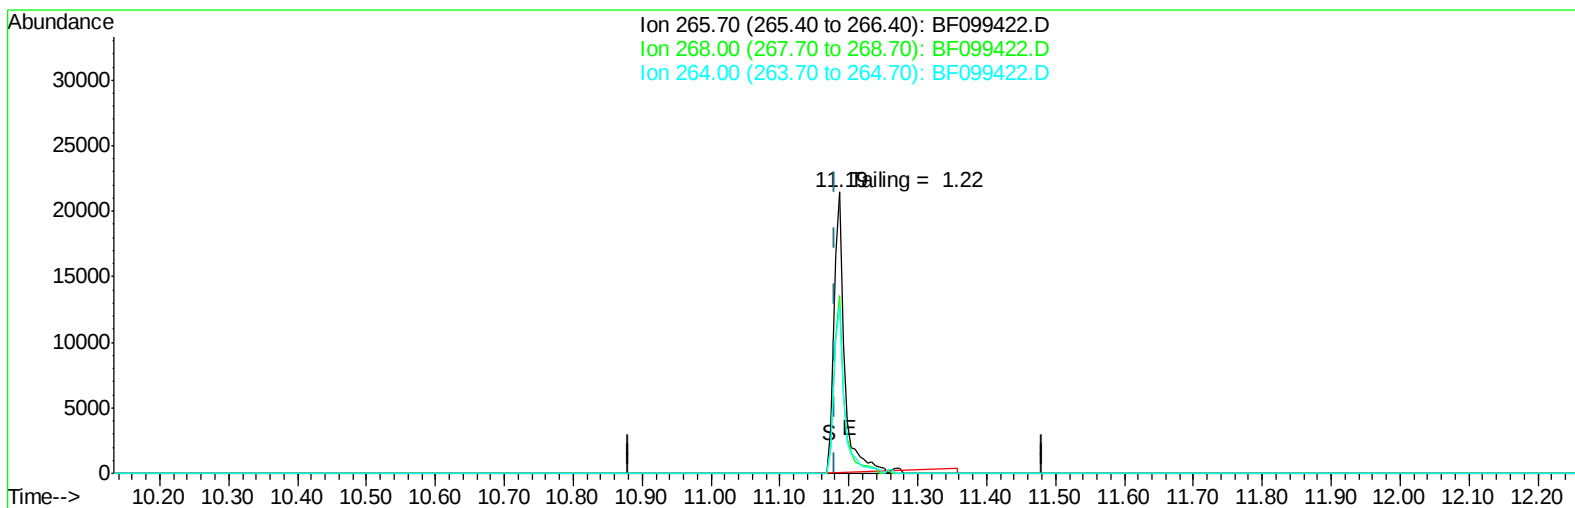

TIC: BF099422.D

(69) Pentachlorophenol (C)



11.186min (+0.006) 12240.46ng

response 22857

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.08
264.00	61.90	59.33
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101217\
Data File : BF099422.D
Acq On : 13 Oct 2017 4:24
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 13 07:36:14 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 11 16:25:21 2017
Response via : Initial Calibration

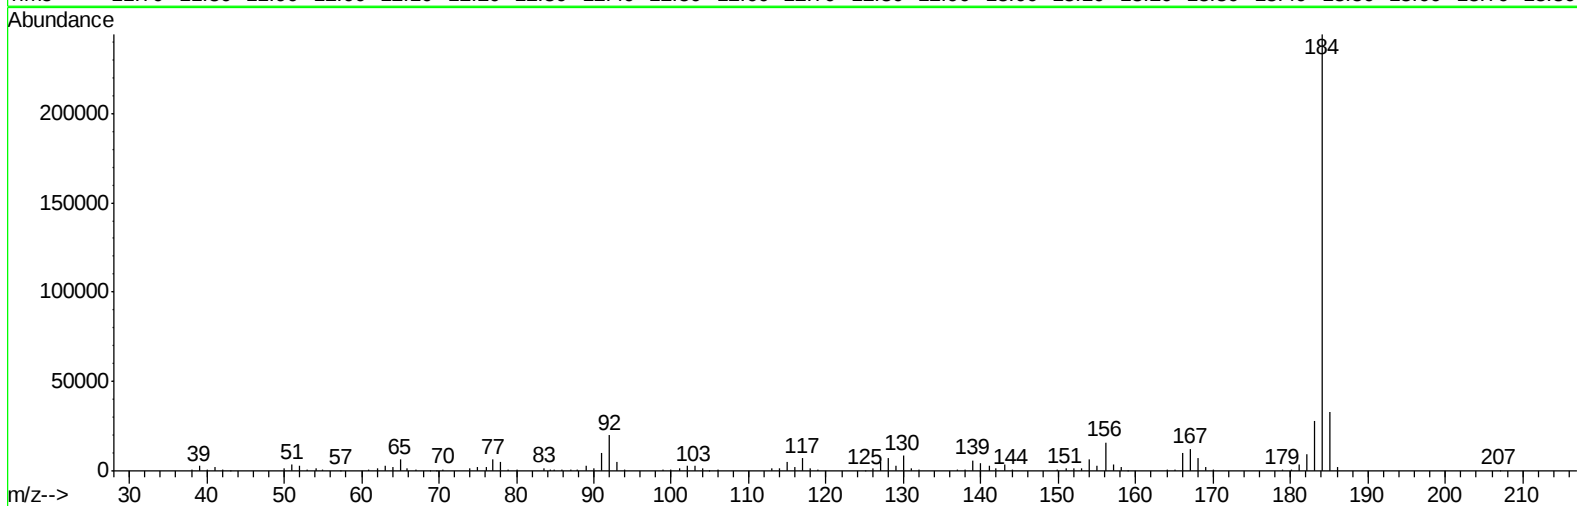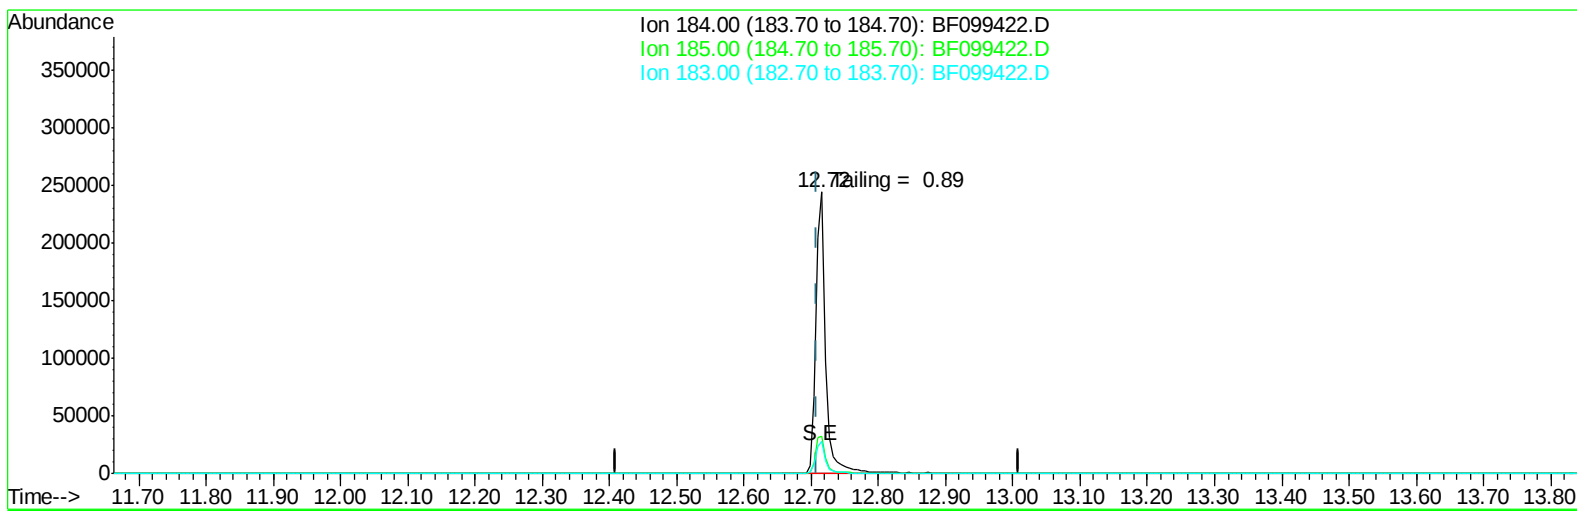

TIC: BF099422.D

(76) Benzidine

12.715min (+0.006) 17081.59ng

response 250820

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.38
183.00	11.60	11.40
0.00	0.00	0.00