


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF101217\
 Data File : BF099396.D
 Acq On : 12 Oct 2017 15:47
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 11 16:25:21 2017

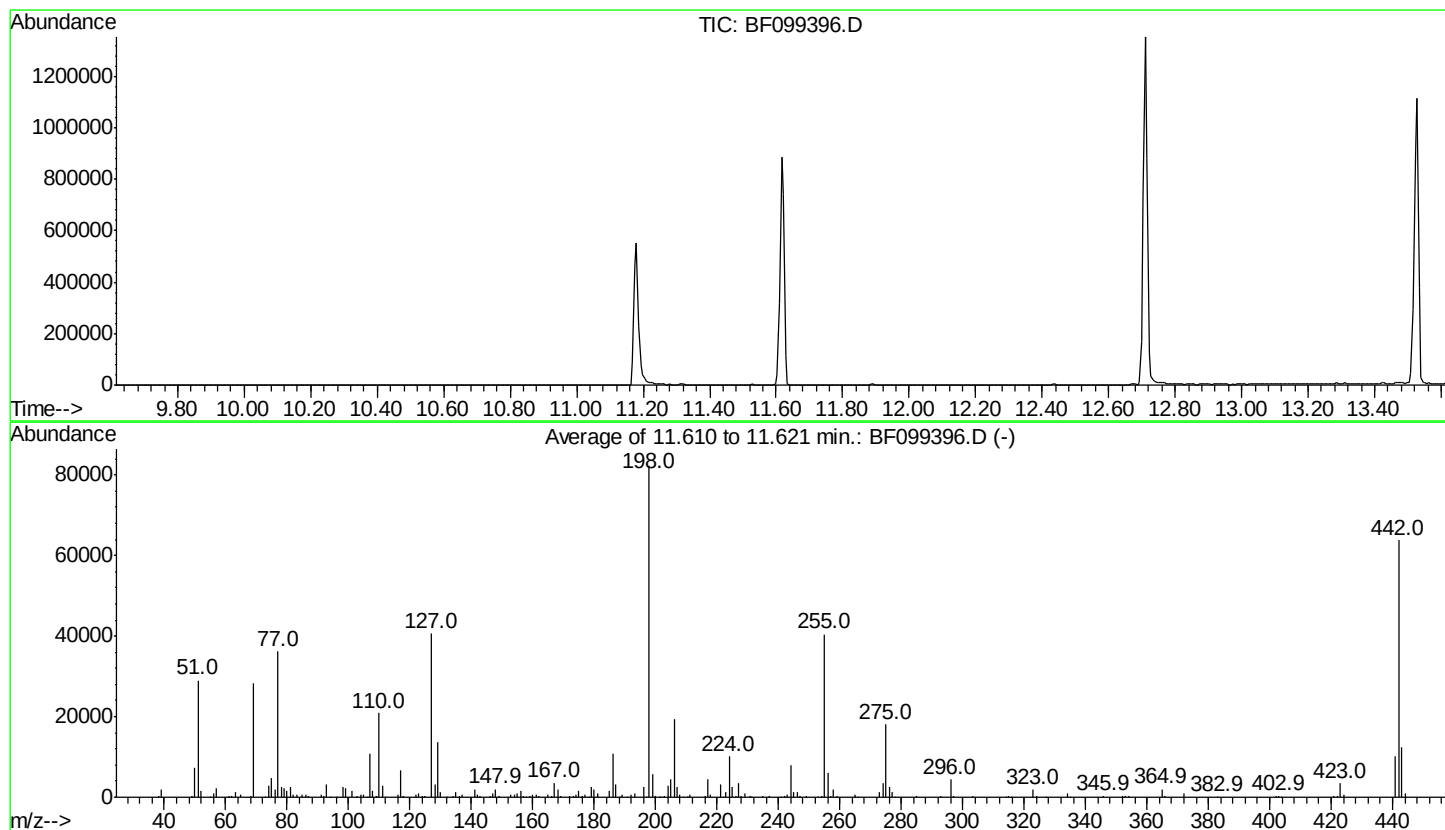

AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.2	28954	PASS
68	69	0.00	2	1.7	487	PASS
69	198	0.00	100	34.3	28240	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.3	40594	PASS
197	198	0.00	2	0.2	140	PASS
198	198	100	100	100.0	82282	PASS
199	198	5	9	7.1	5862	PASS
275	198	10	60	21.8	17962	PASS
365	198	1	100	2.4	1958	PASS
441	442	0.01	24	15.8	10060	PASS
442	198	50	100	77.6	63843	PASS
443	442	15	24	19.3	12346	PASS