

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF101218\
 Data File : BF109836.D
 Acq On : 12 Oct 2018 16:24
 Operator : JU/SJ
 Sample : J5371-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 100818-SIDI-E-D-B

Quant Time: Oct 12 17:50:47 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF100818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 08 16:02:11 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.69	152	101279	20.00	ng	0.00
21) Naphthalene-d8	7.97	136	429893	20.00	ng	0.00
38) Acenaphthene-d10	9.72	164	200694	20.00	ng	0.00
63) Phenanthrene-d10	11.20	188	383547	20.00	ng	0.00
75) Chrysene-d12	13.83	240	243298	20.00	ng	0.00
86) Perylene-d12	15.23	264	202678	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.31	112	221010	38.73	ng	-0.01
7) Phenol-d6	6.34	99	191215	25.09	ng	-0.02
23) Nitrobenzene-d5	7.26	82	790595	101.37	ng	0.00
41) 2,4,6-Tribromophenol	10.51	330	209914	95.99	ng	0.00
44) 2-Fluorobiphenyl	9.05	172	1397655	95.91	ng	0.00
78) Terphenyl-d14	12.79	244	1262187	100.43	ng	0.00
Target Compounds						Qvalue
49) Dimethylphthalate	9.45	163	33803	2.297	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF101218\
Data File : BF109836.D
Acq On : 12 Oct 2018 16:24
Operator : JU/SJ
Sample : J5371-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
100818-SIDI-E-D-B

Quant Time: Oct 12 17:50:47 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF100818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 08 16:02:11 2018
Response via : Initial Calibration

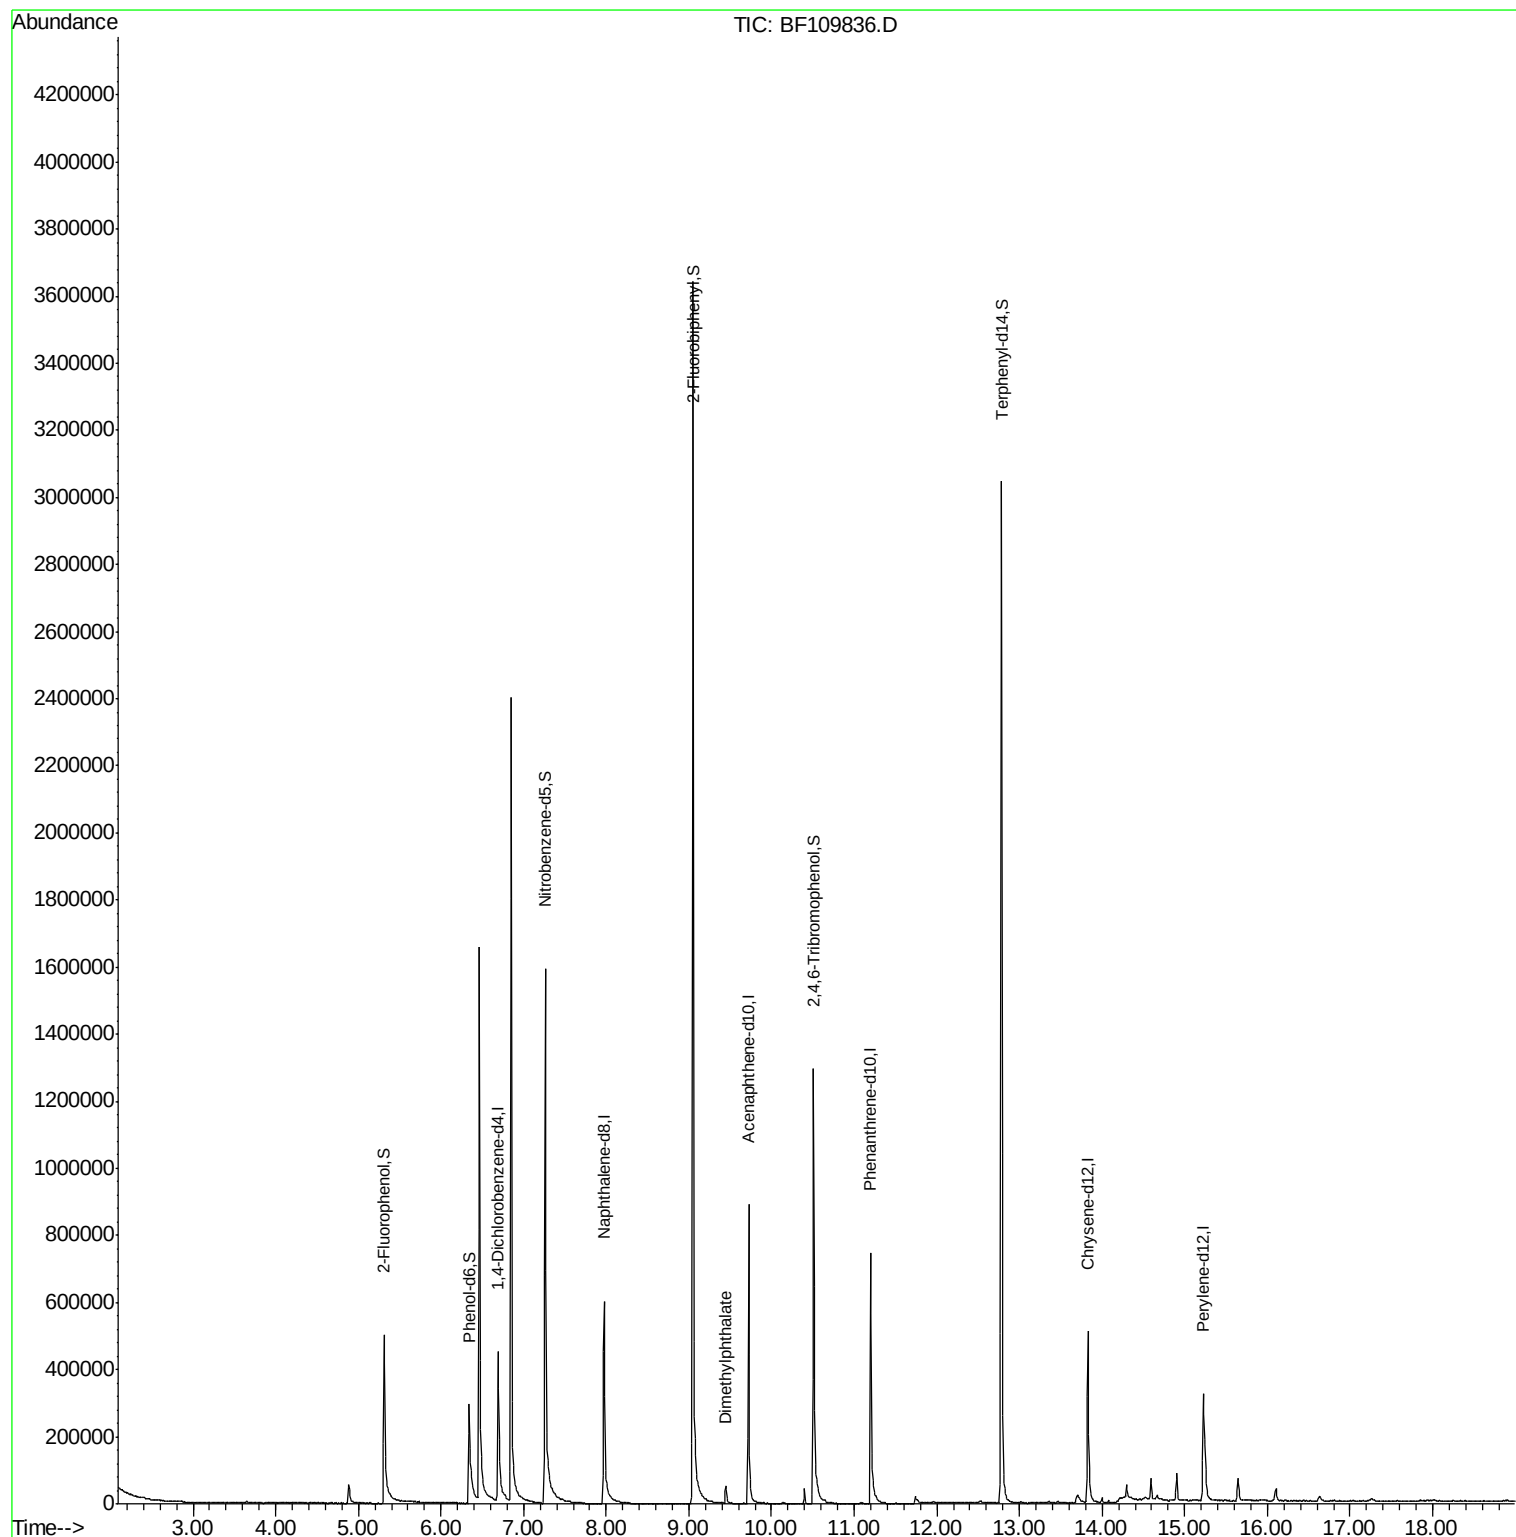

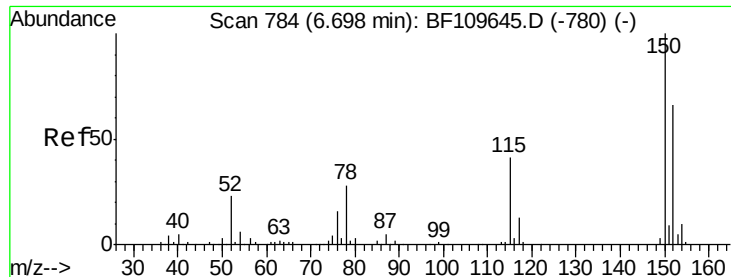


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.69 min Scan# 783
Delta R.T. -0.01 min
Lab File: BF109836.D
Acq: 12 Oct 2018 16:24

Instrument :
BNA_F
ClientSampleId :
100818-SIDI-E-D-B

Tot Ion:152 Resp: 101279
Ion Ratio Lower Upper
152 100
150 155.7 122.7 184.1
115 61.9 49.1 73.7

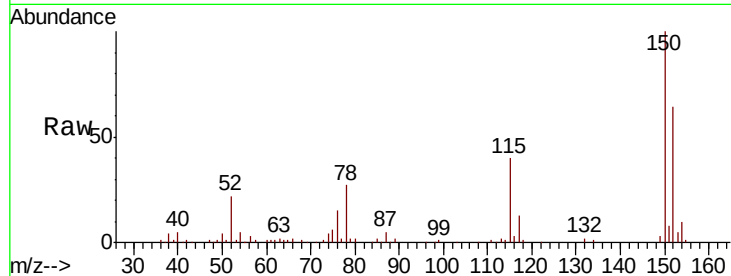


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

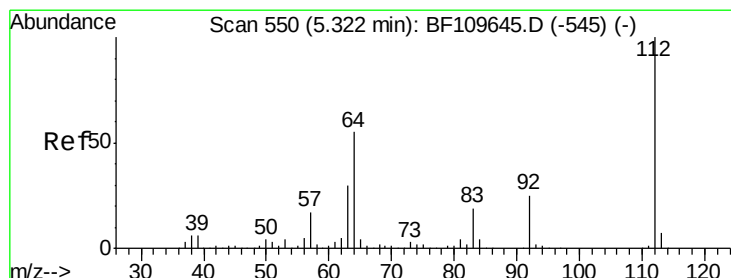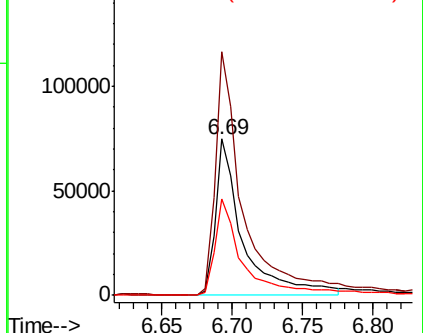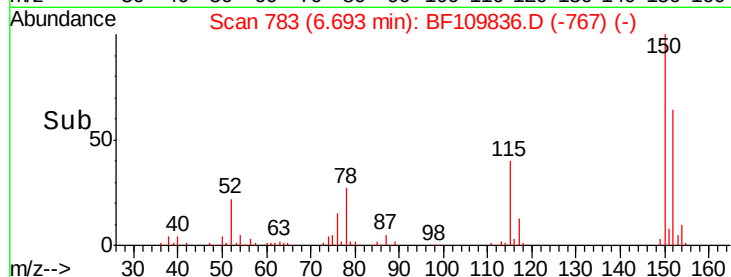



#5


2-Fluorophenol
Concen: 38.735 ng
RT: 5.31 min Scan# 548
Delta R.T. -0.01 min
Lab File: BF109836.D
Acq: 12 Oct 2018 16:24

Tgt Ion:112 Resp: 221010
Ion Ratio Lower Upper
112 100
64 59.3 44.1 66.1
63 31.9 23.7 35.5

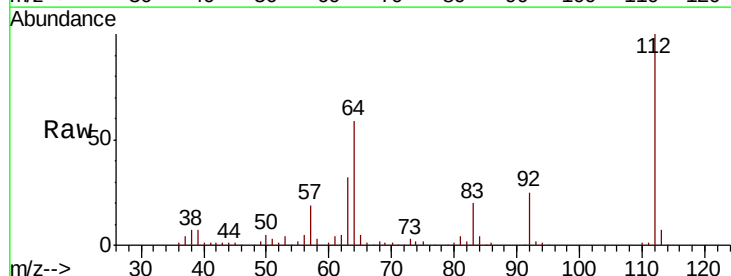

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

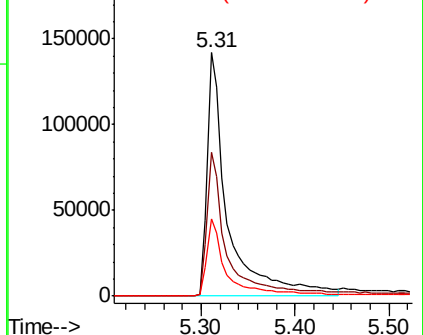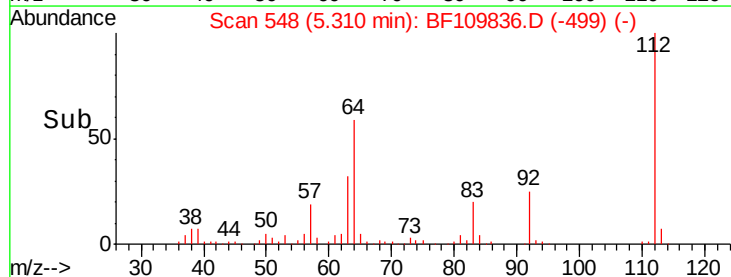

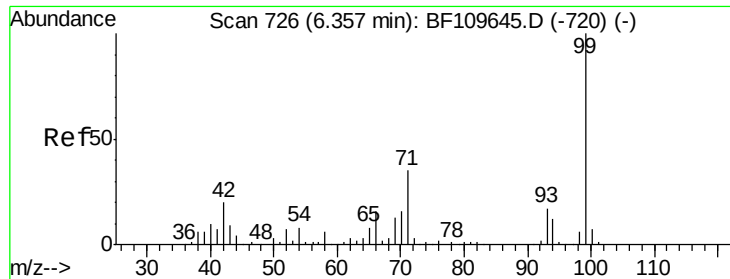

#7

Phenol-d6

Concen: 25.086 ng

RT: 6.34 min Scan# 723

Delta R.T. -0.02 min

Lab File: BF109836.D

Acq: 12 Oct 2018 16:24

Instrument :

BNA_F

ClientSampleId :

100818-SIDI-E-D-B



Tot Ion: 99 Resp: 191215

Ion Ratio Lower Upper

99 100

42 18.3 15.8 23.6



71 35.7 28.0 42.0

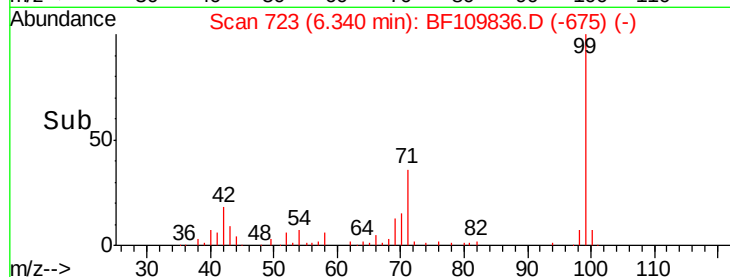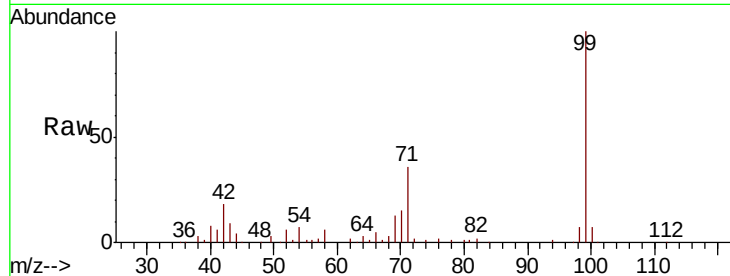

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

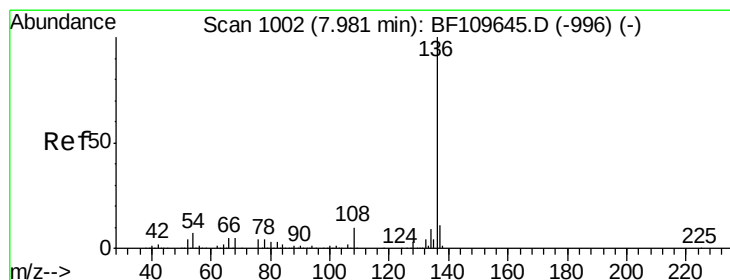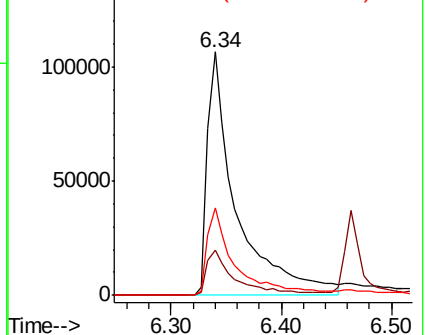

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.97 min Scan# 1001

Delta R.T. -0.01 min

Lab File: BF109836.D

Acq: 12 Oct 2018 16:24

Tgt Ion: 136 Resp: 429893



Ion Ratio Lower Upper

136 100

137 10.7 8.8 13.2

54 6.7 5.4 8.2

68 5.0 4.2 6.2

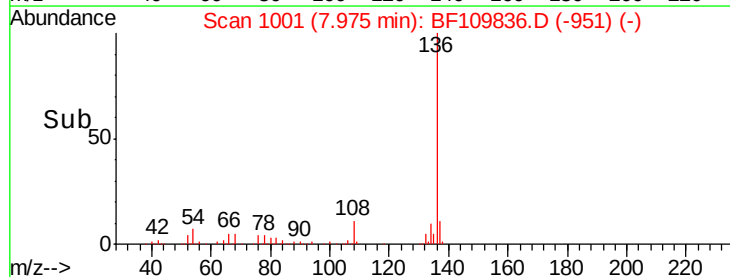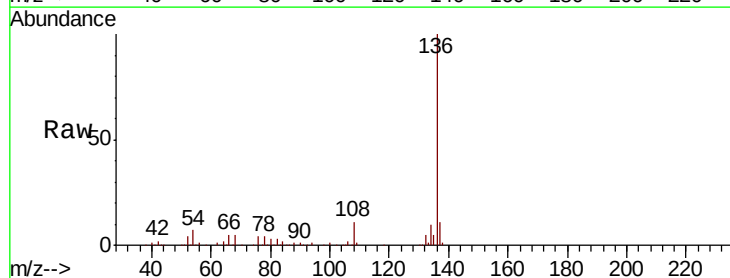



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1




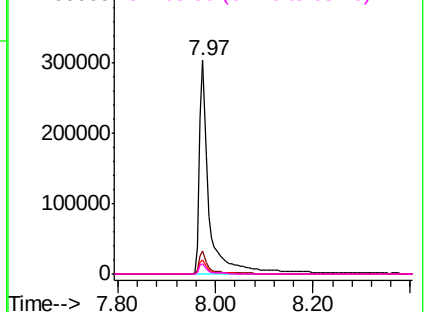


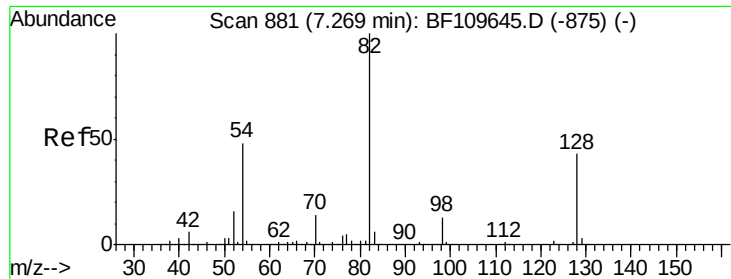

#23
 Nitrobenzene-d5
 Concen: 101.375 ng
 RT: 7.26 min Scan# 880
 Delta R.T. -0.01 min
 Lab File: BF109836.D
 Acq: 12 Oct 2018 16:24




Instrument :
 BNA_F
 ClientSampleId :
 100818-SIDI-E-D-B


Tot Ion	82	Resp	790595
Ion Ratio	Lower	Upper	
82	100		
128	43.1	34.2	51.2
54	48.6	38.6	58.0

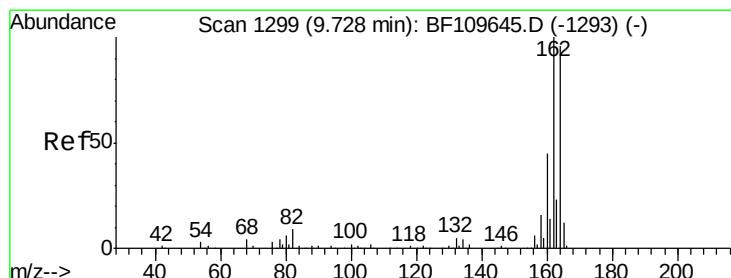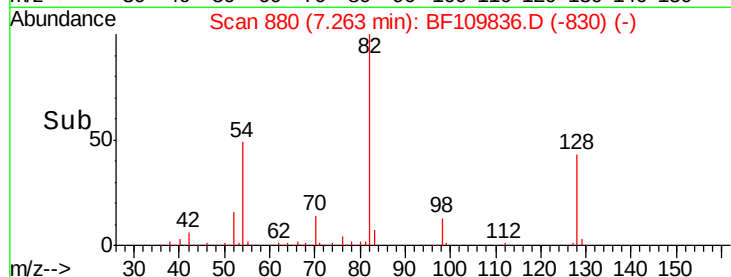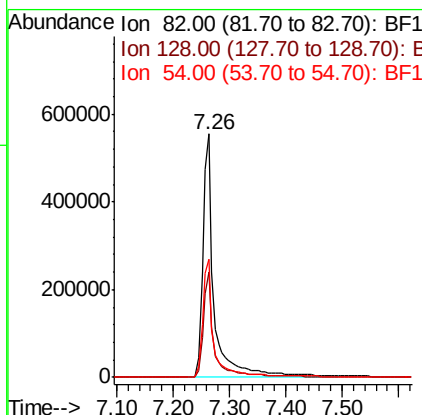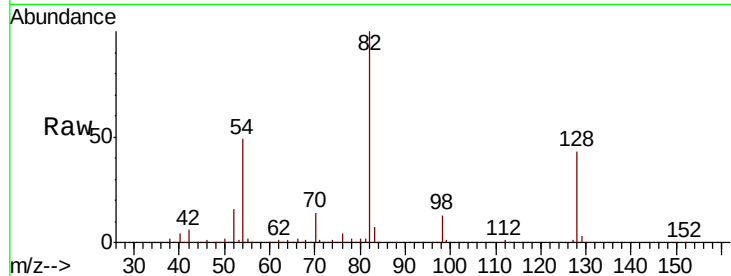

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.72 min Scan# 1298
 Delta R.T. -0.01 min
 Lab File: BF109836.D
 Acq: 12 Oct 2018 16:24

Tgt Ion	164	Resp	200694
Ion Ratio	Lower	Upper	
164	100		
162	103.4	83.0	124.6
160	47.6	37.0	55.6

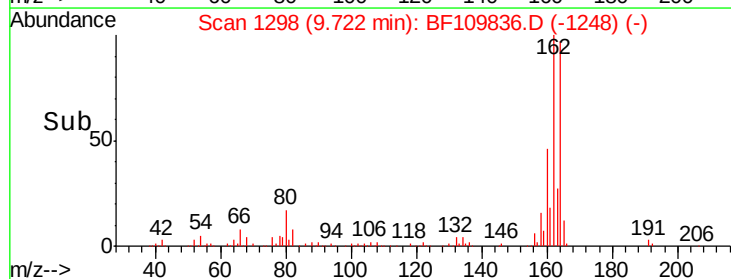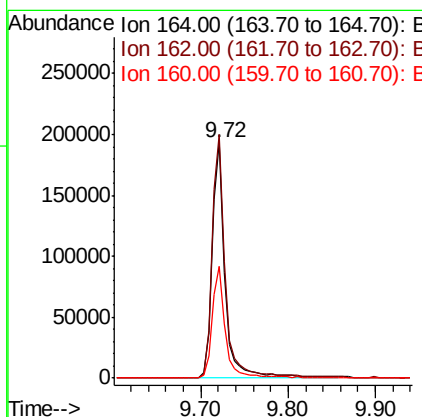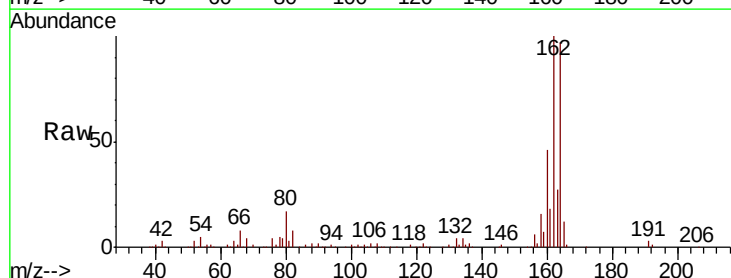


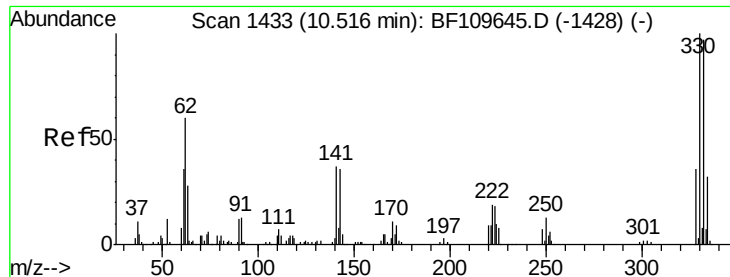




#41
 2,4,6-Tribromophenol
 Concen: 95.992 ng
 RT: 10.51 min Scan# 1432
 Delta R.T. -0.01 min
 Lab File: BF109836.D
 Acq: 12 Oct 2018 16:24

Instrument :
 BNA_F
 ClientSampleId :
 100818-SIDI-E-D-B

Tot Ion:330 Resp: 209914
 Ion Ratio Lower Upper
 330 100
 332 96.8 77.1 115.7
 141 34.8 27.0 40.4

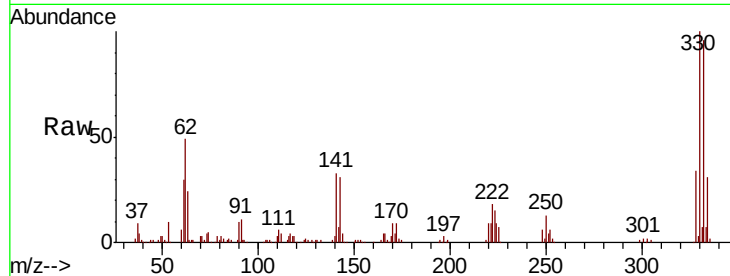


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

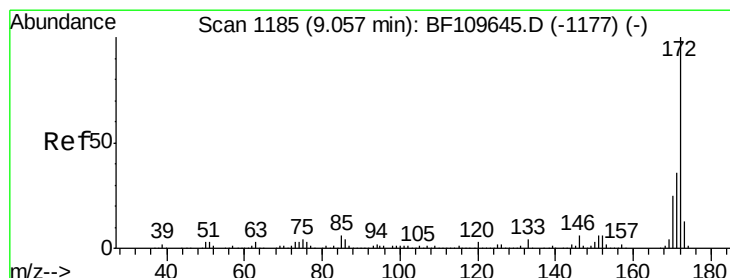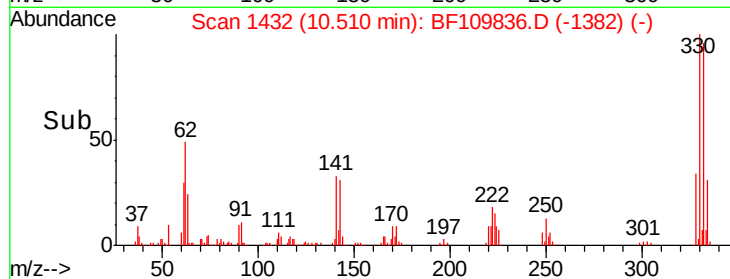
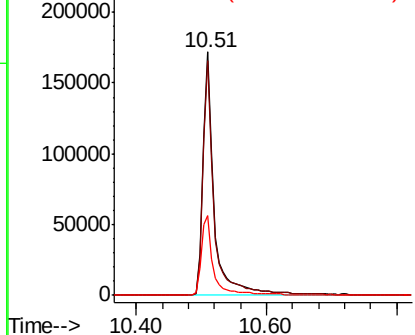



#44
 2-Fluorobiphenyl
 Concen: 95.913 ng
 RT: 9.05 min Scan# 1184
 Delta R.T. -0.01 min
 Lab File: BF109836.D
 Acq: 12 Oct 2018 16:24

Tgt Ion:172 Resp: 1397655
 Ion Ratio Lower Upper
 172 100
 171 36.3 28.6 43.0
 170 24.5 19.7 29.5

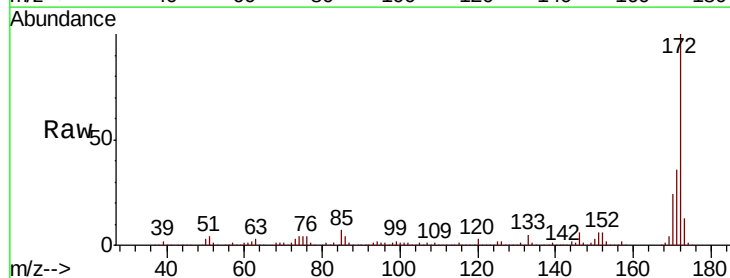

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

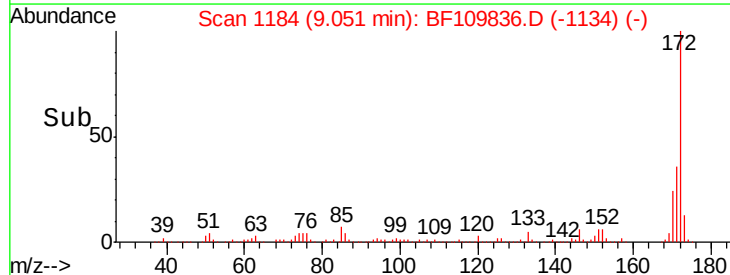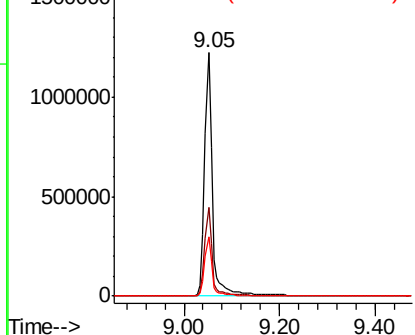

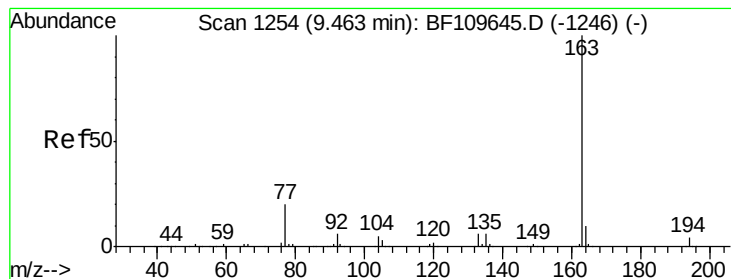

#49

Dimethylphthalate

Concen: 2.297 ng

RT: 9.45 min Scan# 1251

Delta R.T. -0.02 min

Lab File: BF109836.D

Acq: 12 Oct 2018 16:24

Instrument :

BNA_F

ClientSampleId :

100818-SIDI-E-D-B


Tot Ion:163 Resp: 33803

Ion Ratio Lower Upper

163 100

194 3.8 3.2 4.8




164 9.6 8.1 12.1

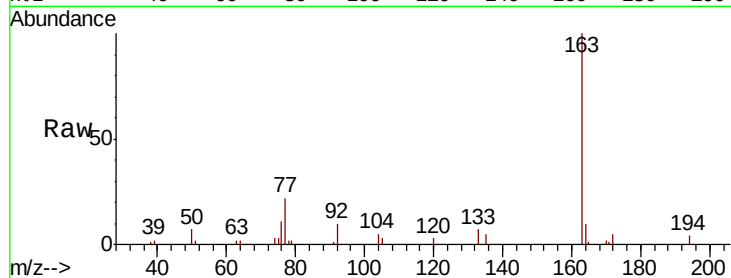

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

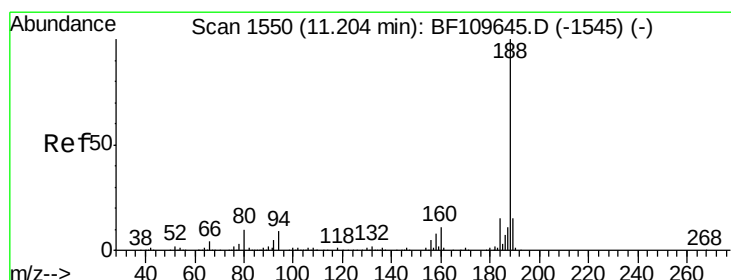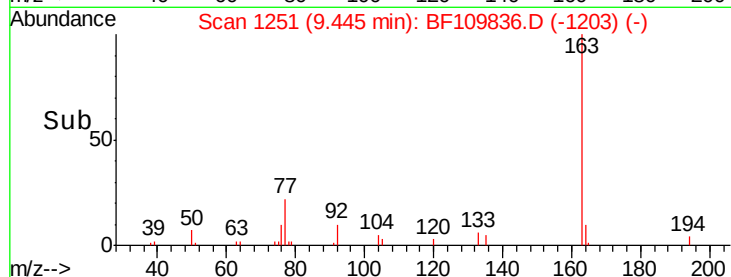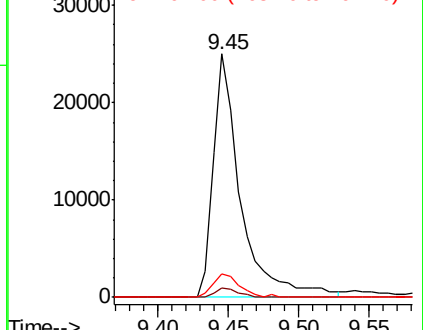

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.20 min Scan# 1549

Delta R.T. -0.01 min

Lab File: BF109836.D

Acq: 12 Oct 2018 16:24


Tgt Ion:188 Resp: 383547

Ion Ratio Lower Upper

188 100

94 8.8 7.2 10.8



80 9.9 7.9 11.9

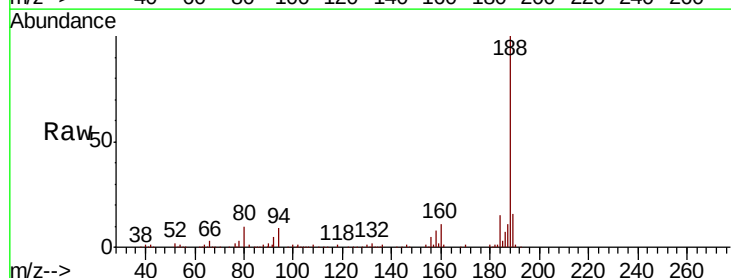


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

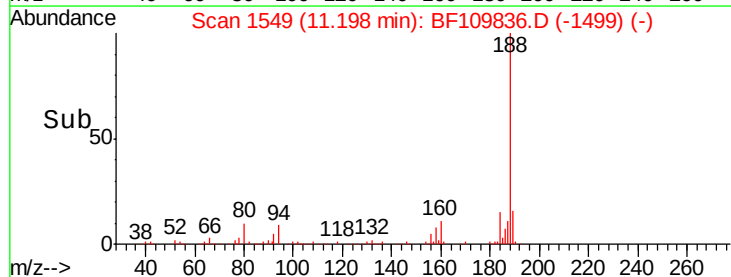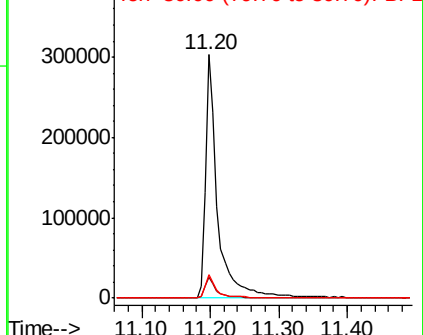

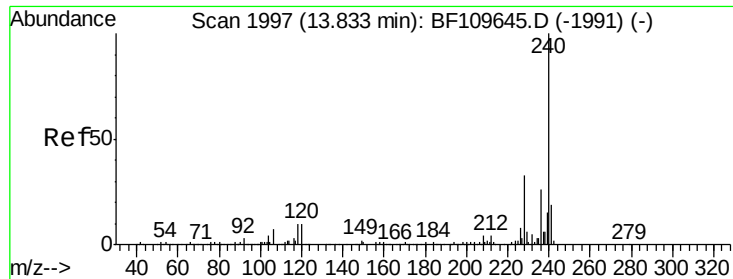

#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.83 min Scan# 1996

Delta R.T. -0.01 min

Lab File: BF109836.D

Acq: 12 Oct 2018 16:24

Instrument :

BNA_F

ClientSampleId :

100818-SIDI-E-D-B


Tot Ion:240 Resp: 243298

Ion Ratio Lower Upper

240 100

120 11.0 8.3 12.5




236 25.4 21.2 31.8

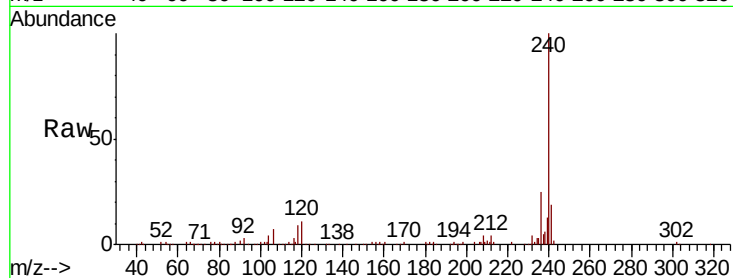

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

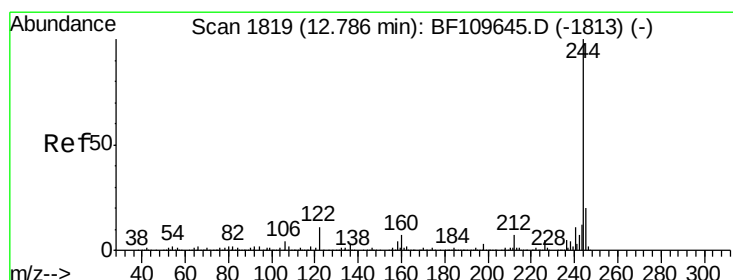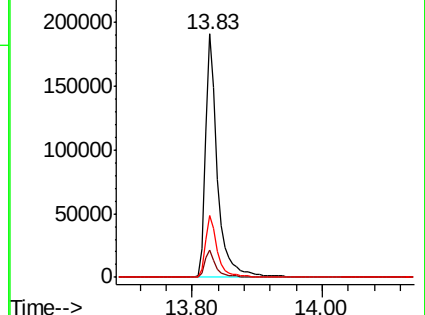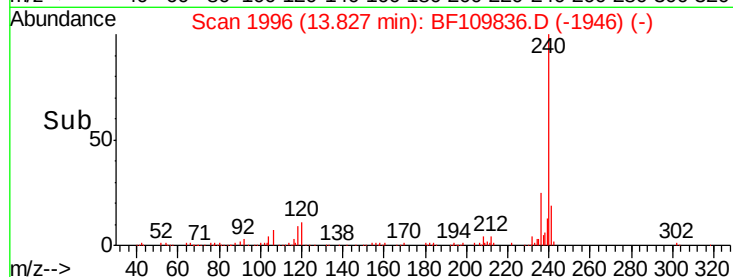

#78

Terphenyl-d14

Concen: 100.428 ng

RT: 12.79 min Scan# 1819

Delta R.T. 0.00 min

Lab File: BF109836.D

Acq: 12 Oct 2018 16:24


Tgt Ion:244 Resp: 1262187

Ion Ratio Lower Upper

244 100

212 7.0 5.8 8.8



122 11.0 8.7 13.1

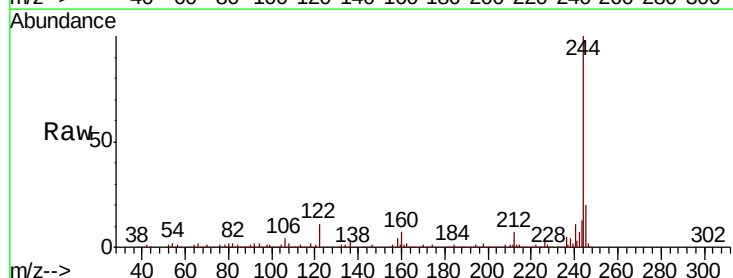


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

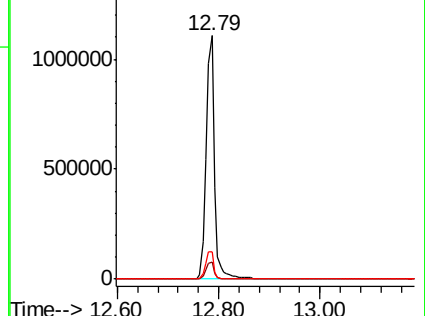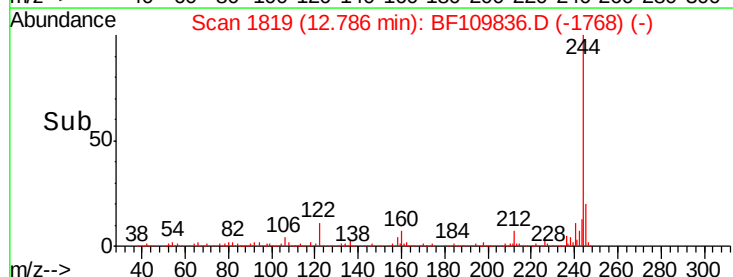

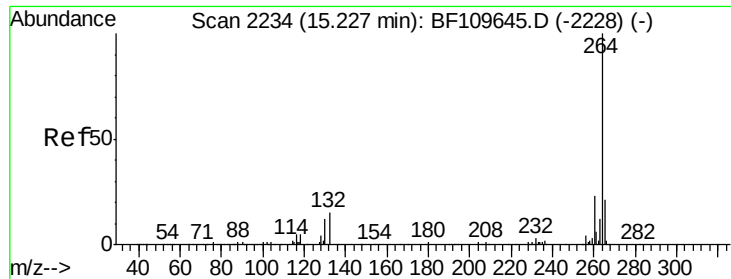

#86
Pervlene-d12
Concen: 20.000 ng
RT: 15.23 min Scan# 2234
Delta R.T. 0.00 min
Lab File: BF109836.D
Acq: 12 Oct 2018 16:24

Instrument :
BNA_F
ClientSampleId :
100818-SIDI-E-D-B

Tot Ion	Ratio	Lower	Upper
264	100		
260	22.1	18.7	28.1
265	20.8	16.7	25.1

