


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF101218\
 Data File : BF109825.D
 Acq On : 12 Oct 2018 10:53
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 08 16:02:11 2018

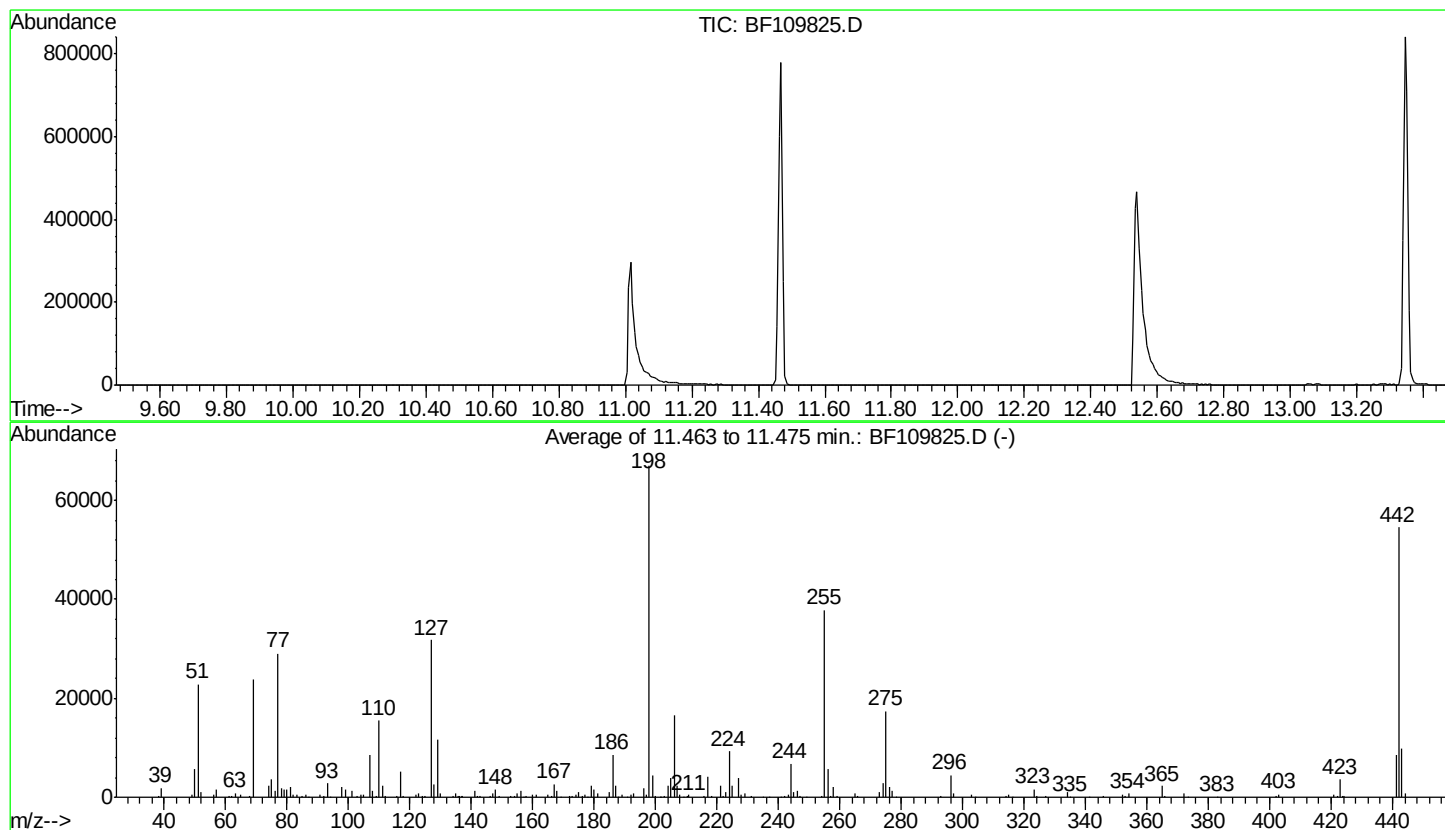

AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	22840	PASS
68	69	0.00	2	1.4	334	PASS
69	198	0.00	100	35.5	23814	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.4	31775	PASS
197	198	0.00	2	0.8	533	PASS
198	198	100	100	100.0	67045	PASS
199	198	5	9	6.6	4401	PASS
275	198	10	60	26.1	17478	PASS
365	198	1	100	3.4	2309	PASS
441	198	0.01	100	12.9	8664	PASS
442	198	50	100	81.4	54602	PASS
443	442	15	24	18.1	9877	PASS