
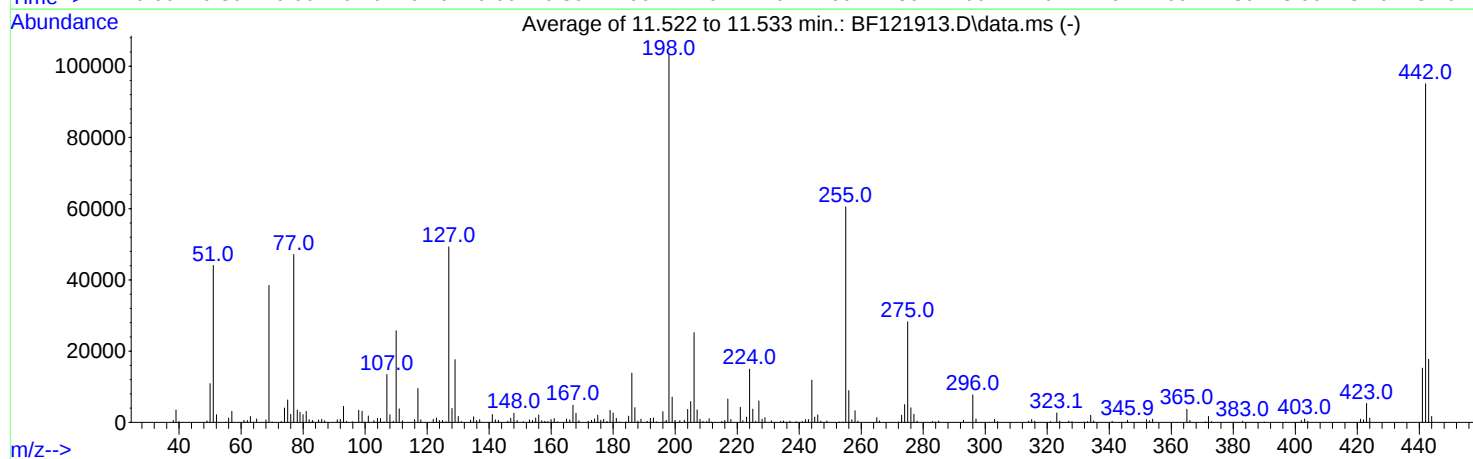


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101220\
 Data File : BF121913.D
 Acq On : 12 Oct 2020 10:24
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 12 16:22:33 2020

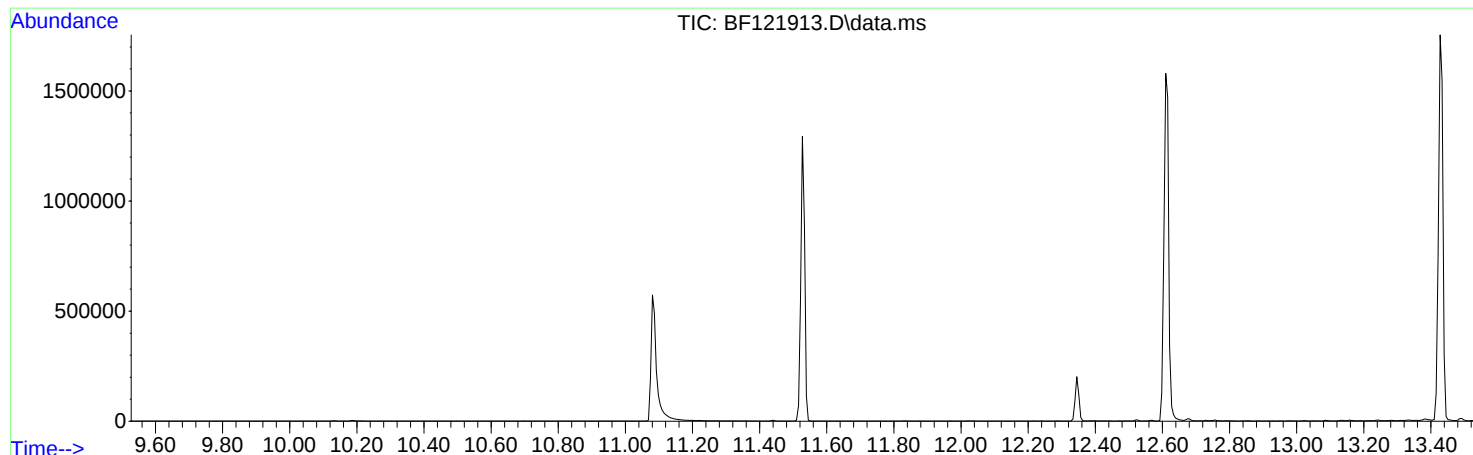

AutoFind: Scans 1604, 1605, 1606; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.7	44064	PASS
68	69	0.00	2	1.8	707	PASS
69	198	0.00	100	37.2	38445	PASS
70	69	0.00	2	0.3	130	PASS
127	198	10	80	47.7	49291	PASS
197	198	0.00	2	0.6	578	PASS
198	198	100	100	100.0	103288	PASS
199	198	5	9	6.9	7087	PASS
275	198	10	60	27.4	28263	PASS
365	198	1	100	3.6	3677	PASS
441	198	0.01	100	14.7	15218	PASS
442	198	50	100	92.0	95061	PASS
443	442	15	24	18.6	17680	PASS