
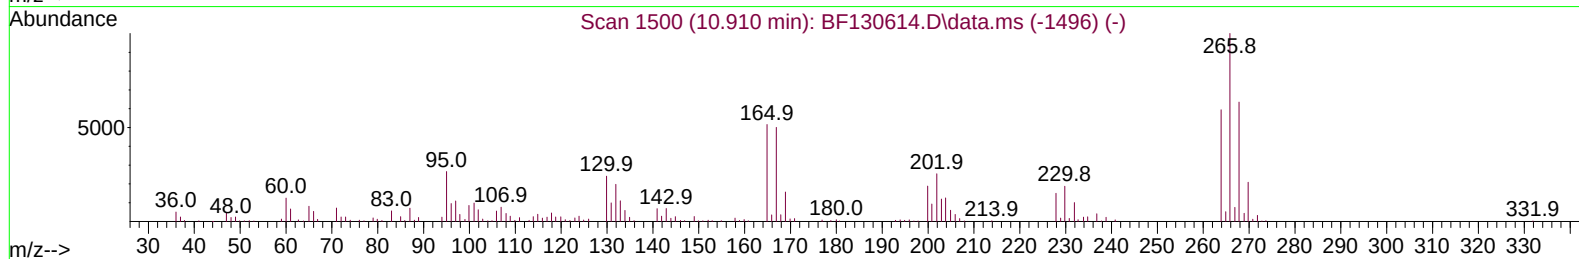
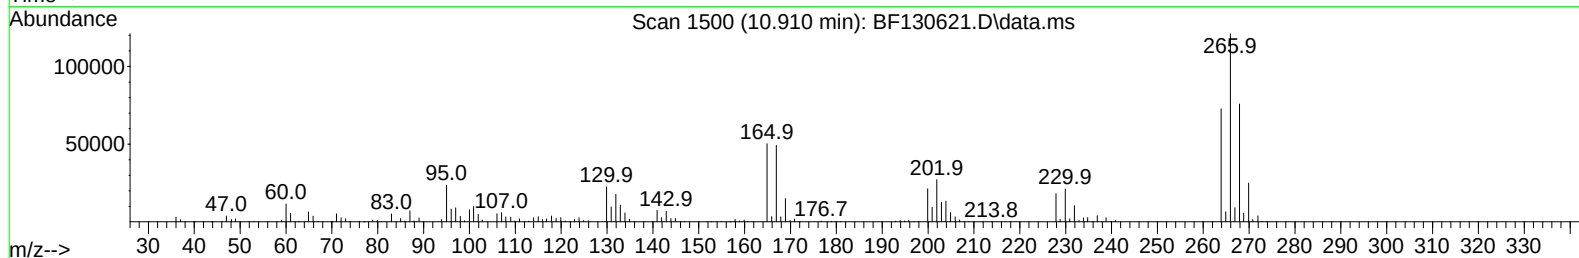


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101222\
Data File : BF130621.D
Acq On : 12 Oct 2022 09:21
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 13 07:28:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 12 06:52:52 2022
Response via : Initial Calibration

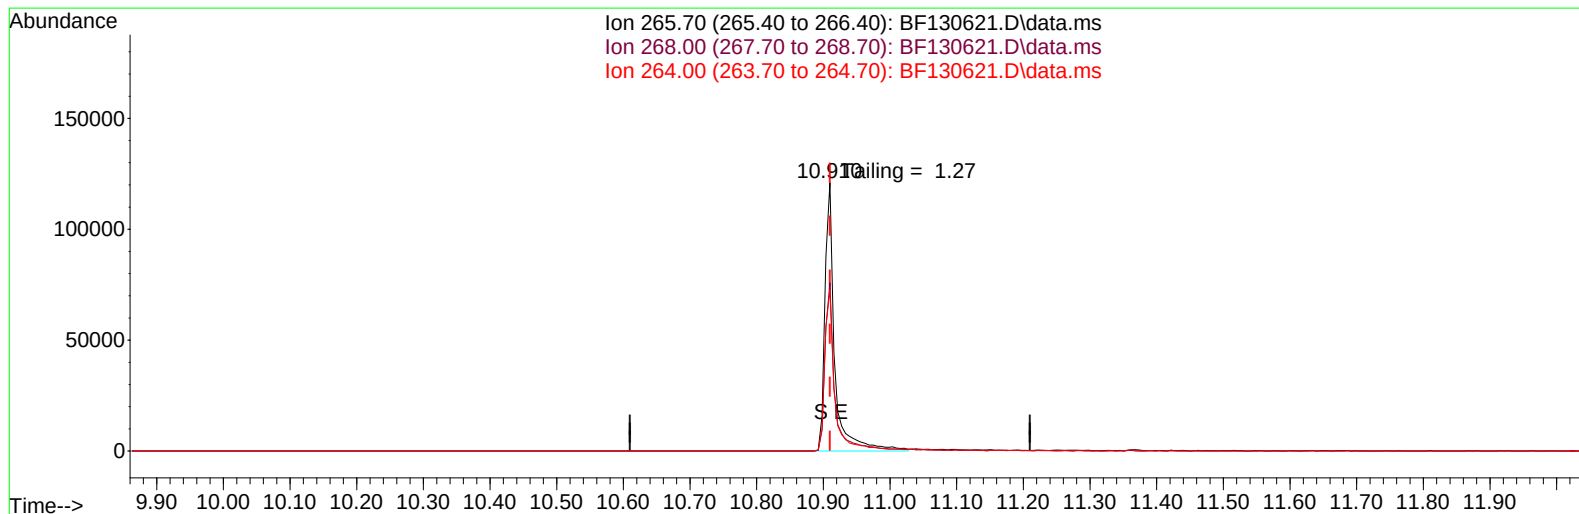

TIC: BF130621.D\data.ms




(70) Pentachlorophenol (C)

10.910min (-0.000) 172831.30 ng

response 123894

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	62.66
264.00	59.40	60.11
0.00	0.00	0.00

Quant Time: Oct 13 07:28:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 12 06:52:52 2022
Response via : Initial Calibration

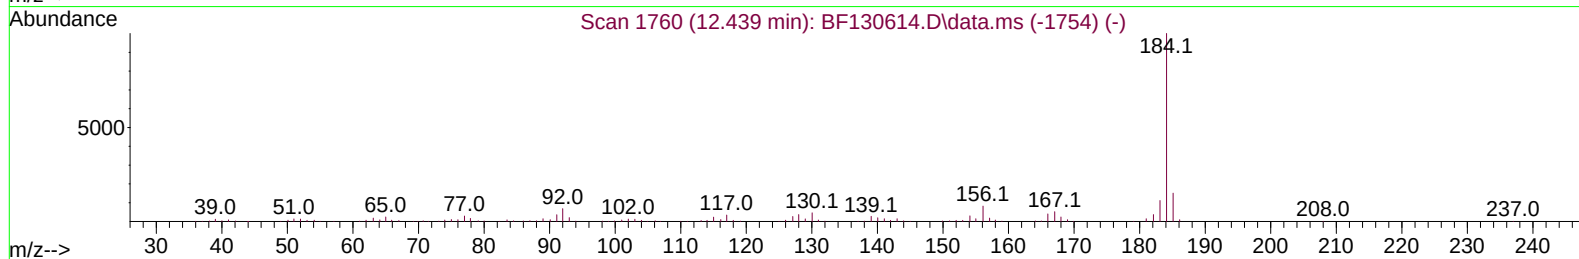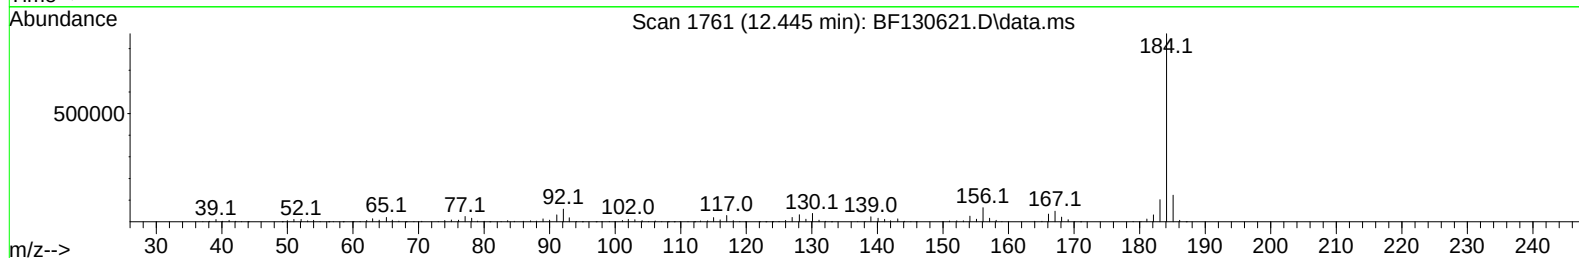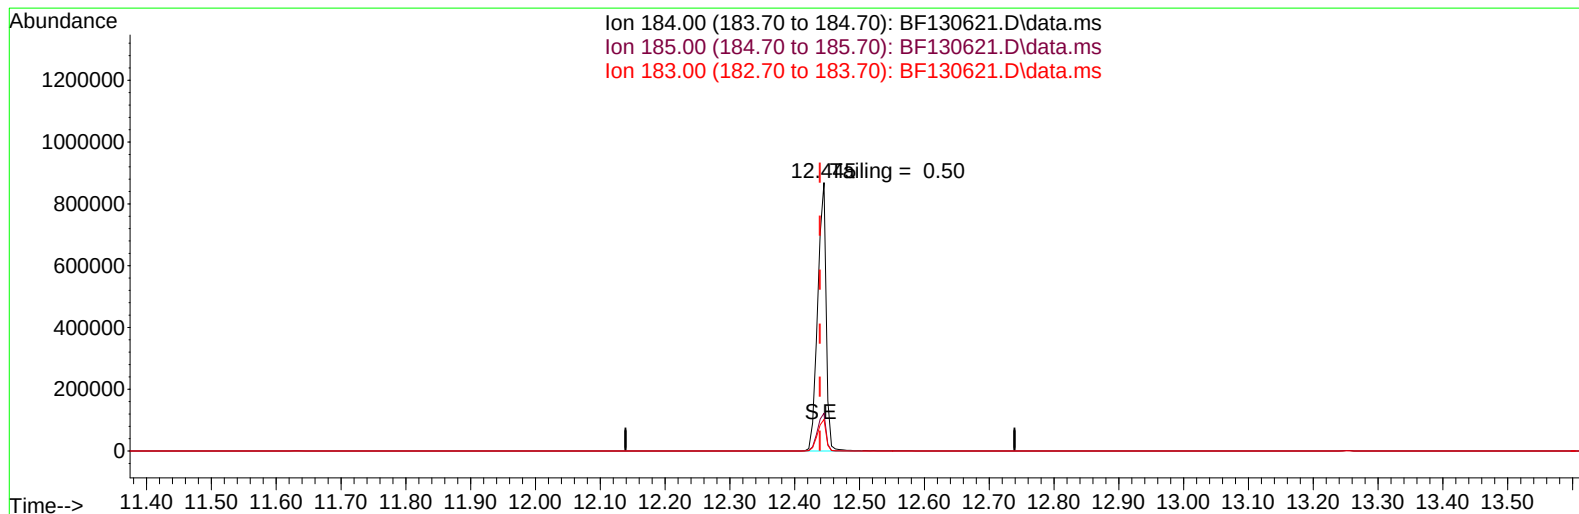

TIC: BF130621.D\data.ms

(77) Benzidine

12.445min (+ 0.006) 110415.79 ng

response **789826**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.11
183.00	11.20	11.74
0.00	0.00	0.00