

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101315\
 Data File : BF082237.D
 Acq On : 13 Oct 2015 1:58
 Operator : UM/IZ
 Sample : G3990-12
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TE-PMW(40)

Quant Time: Oct 13 06:29:24 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF101015.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 13 06:28:22 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.83	152	59557	20.00	ng	0.00
21) Naphthalene-d8	8.11	136	238368	20.00	ng	-0.01
38) Acenaphthene-d10	9.87	164	126790	20.00	ng	0.00
63) Phenanthrene-d10	11.36	188	253033	20.00	ng	0.00
75) Chrysene-d12	14.00	240	254416	20.00	ng	-0.01
86) Perylene-d12	15.44	264	194484	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.42	112	220094	74.58	ng	0.00
7) Phenol-d6	6.46	99	166342	43.32	ng	-0.01
23) Nitrobenzene-d5	7.41	82	434411	122.39	ng	0.00
41) 2,4,6-Tribromophenol	10.66	330	192578	161.96	ng	-0.01
44) 2-Fluorobiphenyl	9.20	172	865361	113.19	ng	0.00
78) Terphenyl-d14	12.95	244	898858	93.62	ng	0.00
Target Compounds						
9) Benzaldehyde	6.59	77	8745	4.46	ng	# 75
15) Benzyl Alcohol	6.98	79	6316	2.38	ng	# 52
19) n-Nitroso-di-n-propylamine	7.41	70	55489	20.58	ng	# 75
25) Isophorone	7.41	82	440747	61.52	ng	# 66
50) 2,6-Dinitrotoluene	9.87	165	15872	8.43	ng	# 30
56) 2,4-Dinitrotoluene	9.87	165	15872	6.74	ng	# 21
66) 4-Bromophenyl-phenylether	10.66	248	12212	4.82	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101315\
Data File : BF082237.D
Acq On : 13 Oct 2015 1:58
Operator : UM/IZ
Sample : G3990-12
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TE-PMW(40)

Quant Time: Oct 13 06:29:24 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 13 06:28:22 2015
Response via : Initial Calibration

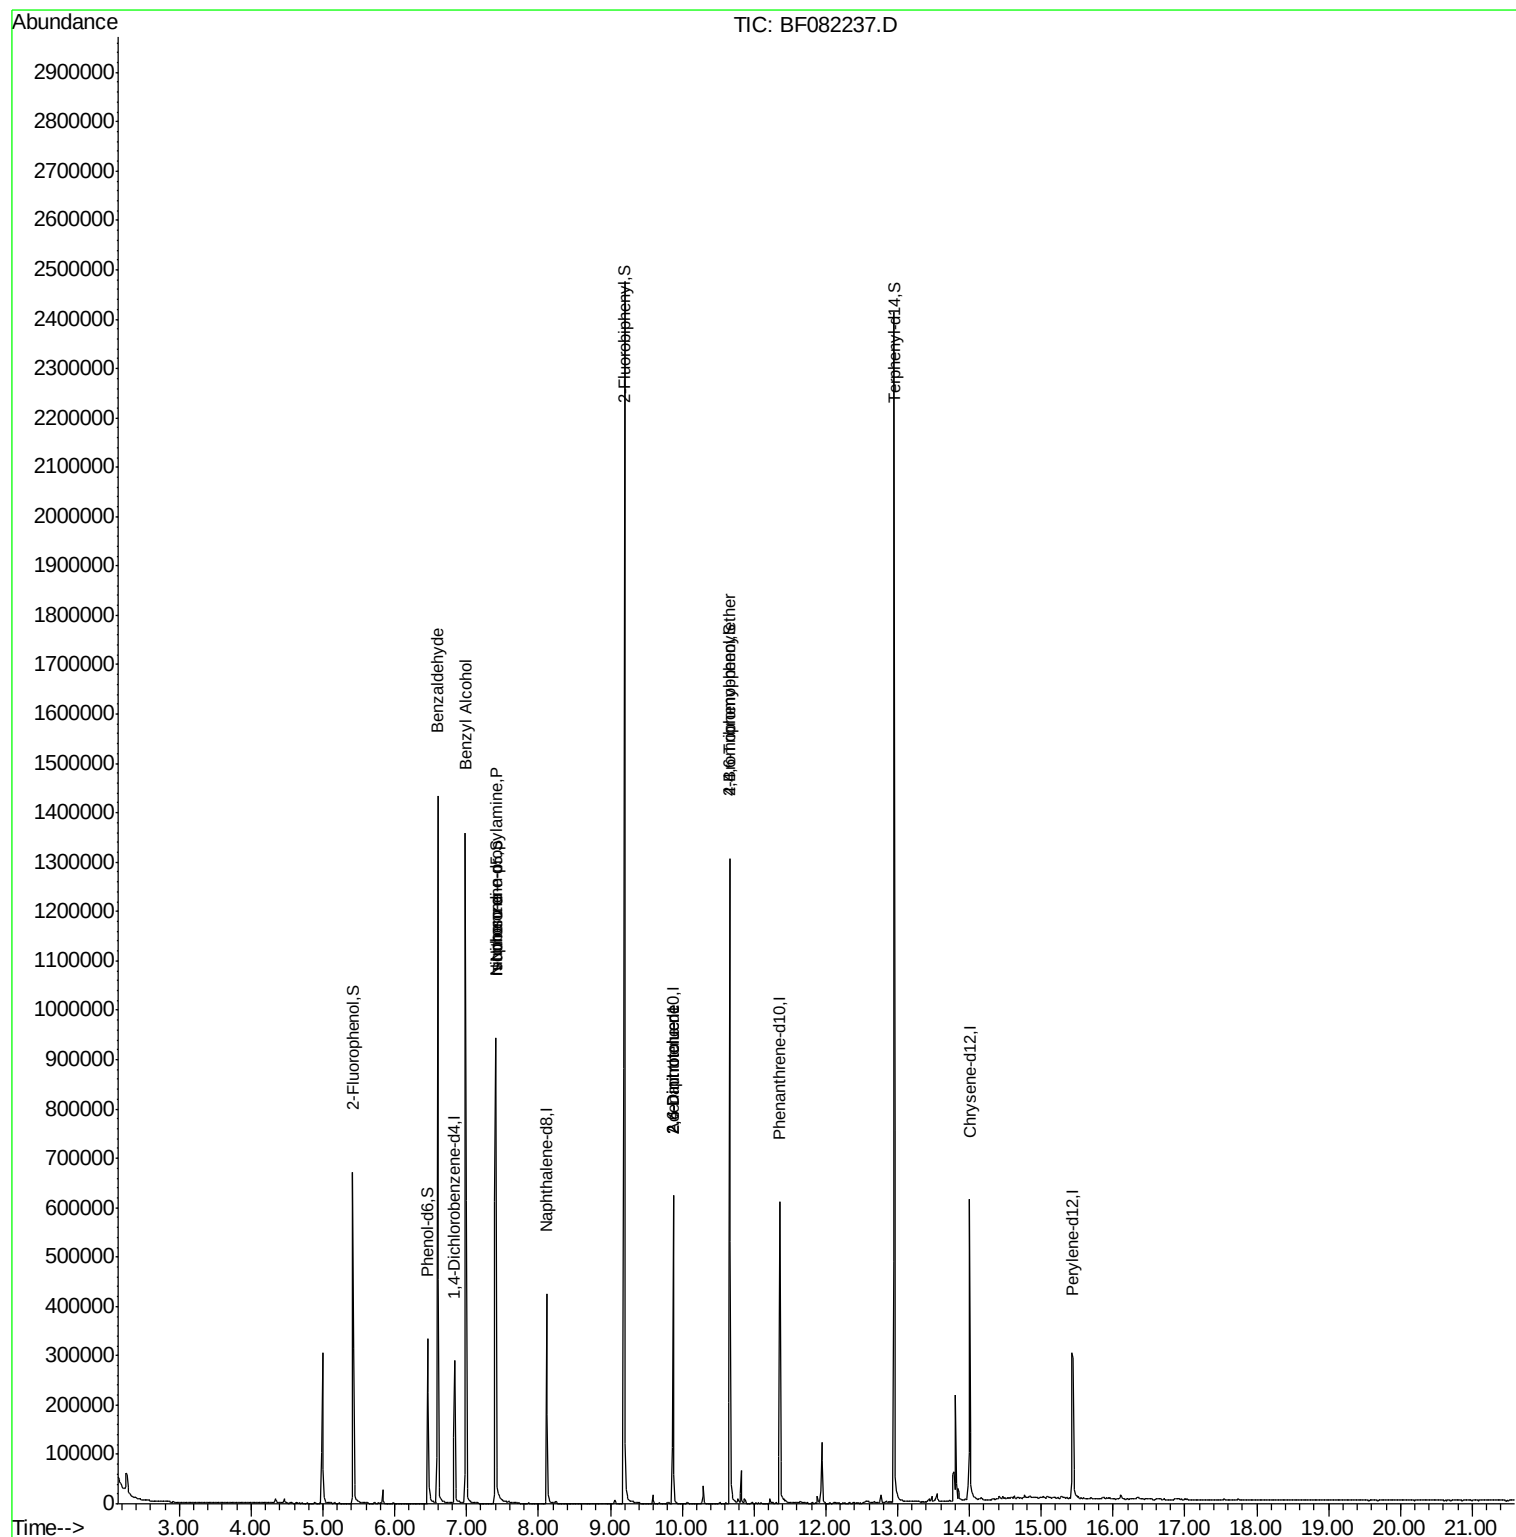

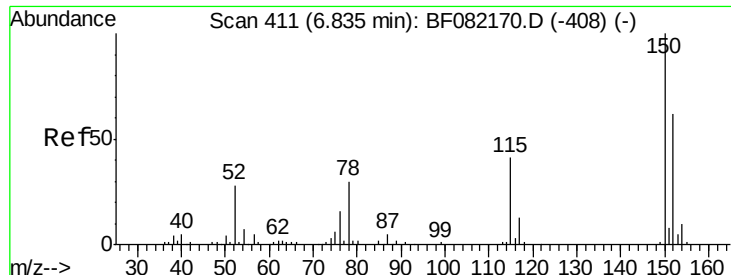

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.83 min Scan# 411

Delta R.T. 0.00 min

Lab File: BF082237.D

Acq: 13 Oct 2015 1:58

Instrument :

BNA_F

ClientSampleId :

TE-PMW(40)


Tot Ion:152 Resp: 59557

Ion Ratio Lower Upper

152 100

150 160.9 129.0 193.4




115 53.1 52.1 78.1

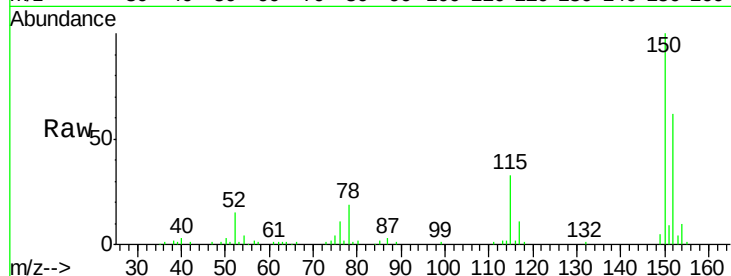

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

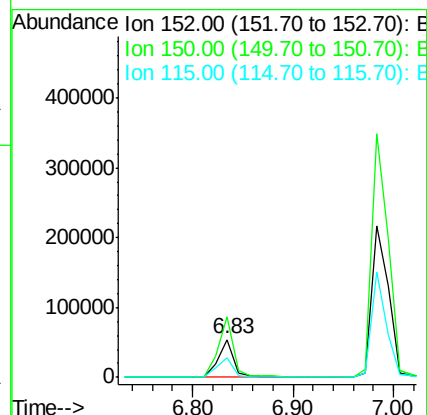

#5

2-Fluorophenol

Concen: 74.58 ng

RT: 5.42 min Scan# 287

Delta R.T. 0.00 min

Lab File: BF082237.D

Acq: 13 Oct 2015 1:58


Tgt Ion:112 Resp: 220094

Ion Ratio Lower Upper

112 100

64 68.0 48.6 73.0



63 36.3 25.1 37.7




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

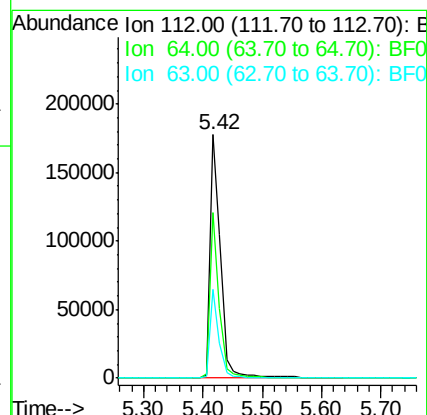

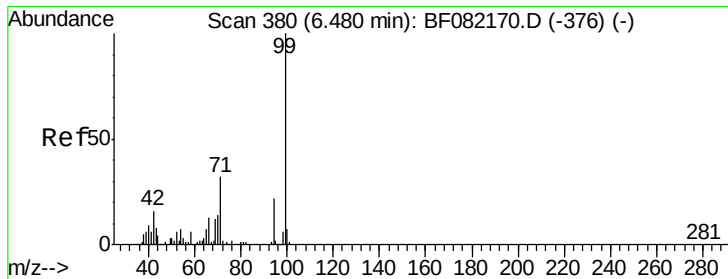

#7

Phenol-d6

Concen: 43.32 ng

RT: 6.46 min Scan# 378

Delta R.T. -0.01 min

Lab File: BF082237.D

Acq: 13 Oct 2015 1:58

Instrument :

BNA_F

ClientSampleId :

TE-PMW(40)





Tot Ion: 99 Resp: 166342

Ion Ratio Lower Upper

99 100

42 21.7 13.2 19.8#

71 36.1 25.6 38.4

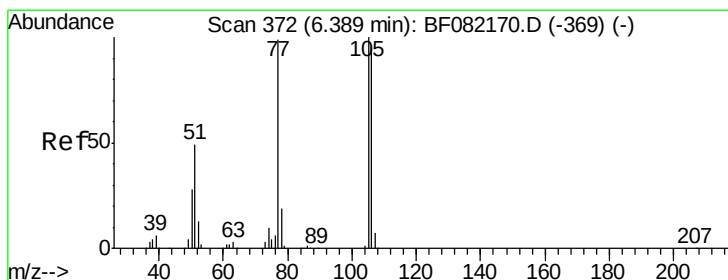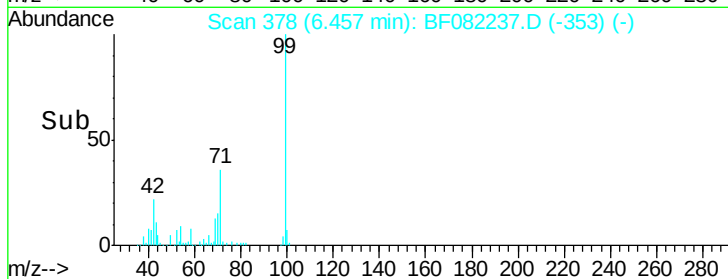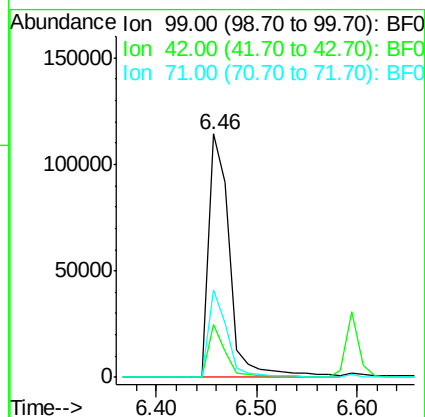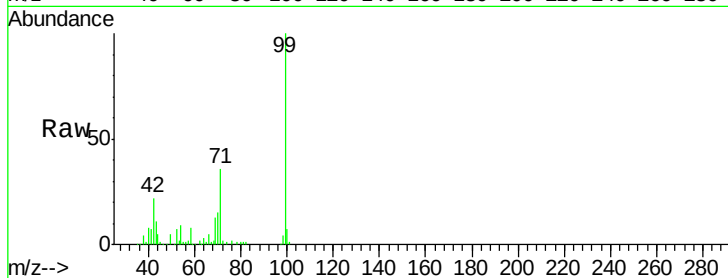

#9

Benzaldehyde

Concen: 4.46 ng

RT: 6.59 min Scan# 390

Delta R.T. 0.22 min

Lab File: BF082237.D

Acq: 13 Oct 2015 1:58




Tgt Ion: 77 Resp: 8745


Ion Ratio Lower Upper

77 100

105 79.8 80.6 120.6#

106 66.0 75.5 115.5#

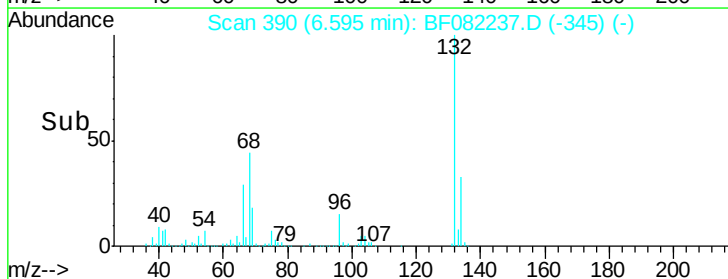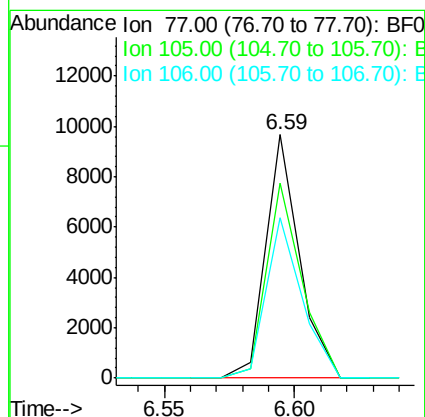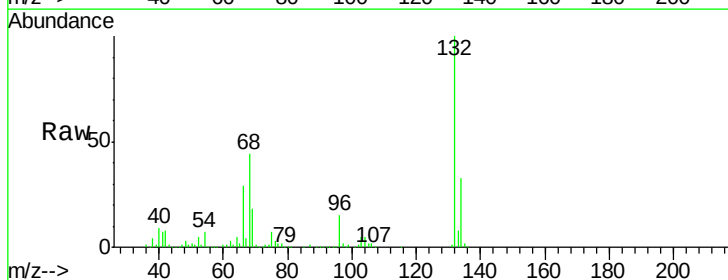



#15

Benzyl Alcohol

Concen: 2.38 ng

RT: 6.98 min Scan# 424

Delta R.T. 0.00 min

Lab File: BF082237.D

Acq: 13 Oct 2015 1:58

Instrument :

BNA_F

ClientSampleId :

TE-PMW(40)


Tot Ion: 79 Resp: 6316

Ion Ratio Lower Upper

79 100

108 27.6 58.4 87.6#




77 93.5 49.8 74.6#

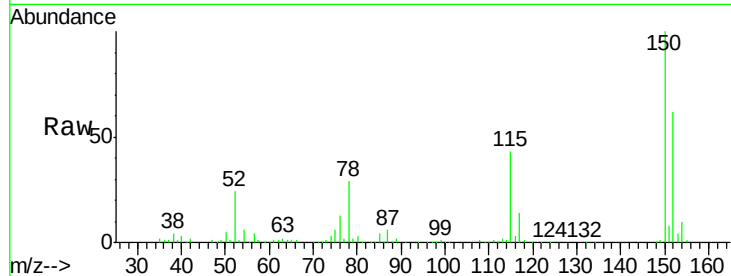

Abundance Ion 79.00 (78.70 to 79.70): BF0

Ion 108.00 (107.70 to 108.70): BF0

Ion 77.00 (76.70 to 77.70): BF0

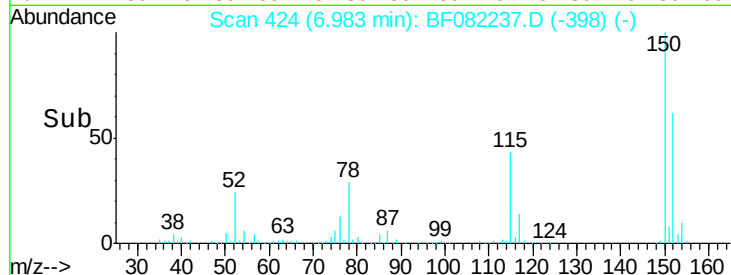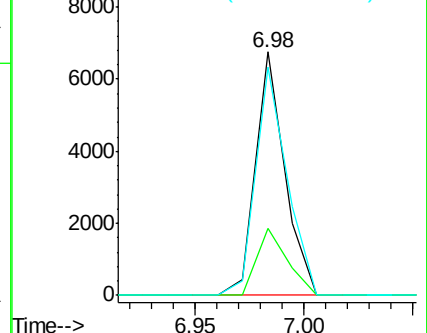

#19

n-Nitroso-di-n-propylamine

Concen: 20.58 ng

RT: 7.41 min Scan# 461

Delta R.T. 0.15 min

Lab File: BF082237.D

Acq: 13 Oct 2015 1:58

Tgt Ion: 70 Resp: 55489


Ion Ratio Lower Upper

70 100

42 40.1 39.8 59.8

101 0.0 8.6 13.0#

130 2.8 20.5 30.7#






Abundance Ion 70.00 (69.70 to 70.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 101.00 (100.70 to 101.70): BF0

Ion 130.00 (129.70 to 130.70): BF0

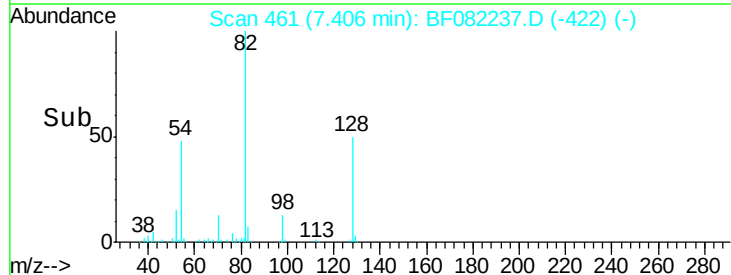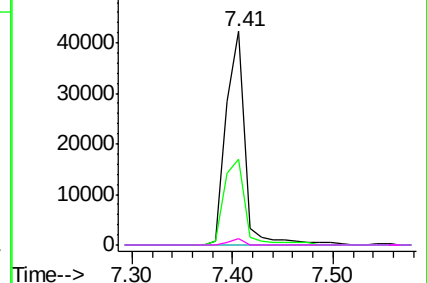

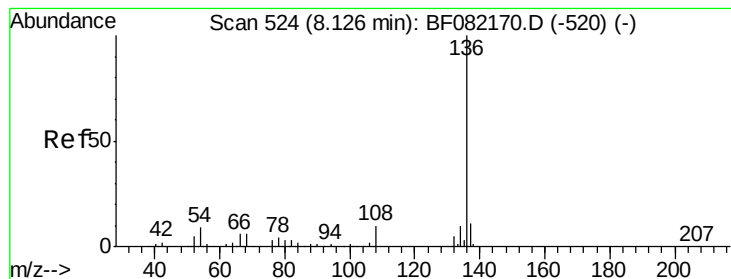

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.11 min Scan# 523

Delta R.T. -0.01 min

Lab File: BF082237.D

Acq: 13 Oct 2015 1:58

Instrument :

BNA_F

ClientSampleId :

TE-PMW(40)

Tot Ion:136 Resp: 238368


Ion Ratio Lower Upper

136 100

137 11.3 9.0 13.6

54 9.6 7.5 11.3

68 5.8 4.6 7.0






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

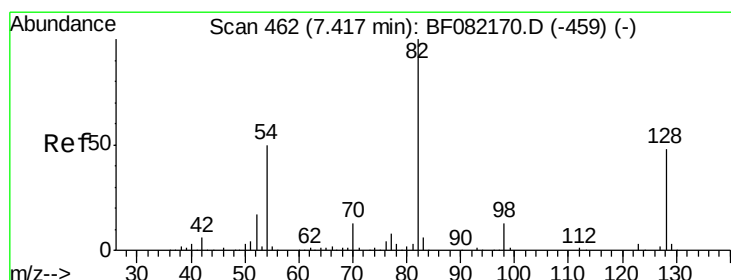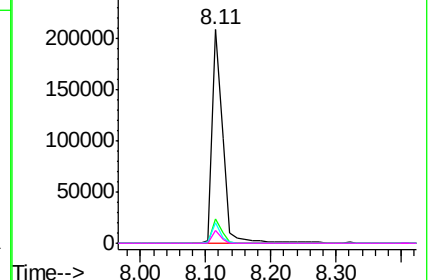

#23

Nitrobenzene-d5

Concen: 122.39 ng

RT: 7.41 min Scan# 461

Delta R.T. 0.00 min

Lab File: BF082237.D

Acq: 13 Oct 2015 1:58


Tgt Ion: 82 Resp: 434411

Ion Ratio Lower Upper

82 100

128 50.5 38.7 58.1



54 47.9 40.1 60.1




Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

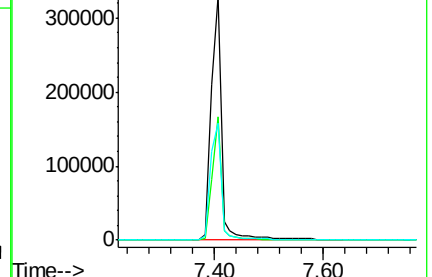



#25

Isophorone

Concen: 61.52 ng

RT: 7.41 min Scan# 461

Delta R.T. -0.25 min

Lab File: BF082237.D

Acq: 13 Oct 2015 1:58

Instrument :

BNA_F

ClientSampleId :

TE-PMW(40)


Tot Ion: 82 Resp: 440747

Ion Ratio Lower Upper




82 100

95 0.0 5.6 8.4#

138 0.0 13.6 20.4#



Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 95.00 (94.70 to 95.70): BF0
Ion 138.00 (137.70 to 138.70): BF0

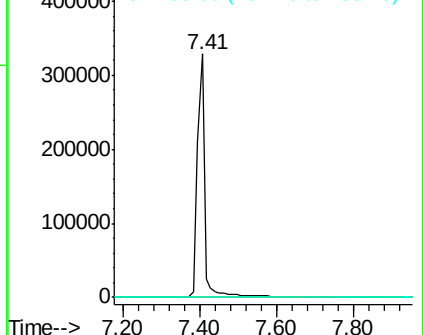

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.87 min Scan# 677

Delta R.T. 0.00 min

Lab File: BF082237.D

Acq: 13 Oct 2015 1:58


Tgt Ion: 164 Resp: 126790

Ion Ratio Lower Upper



164 100


162 102.6 81.6 122.4

160 44.4 36.4 54.6



Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E



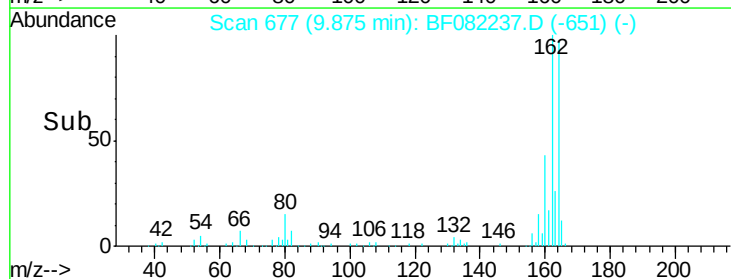
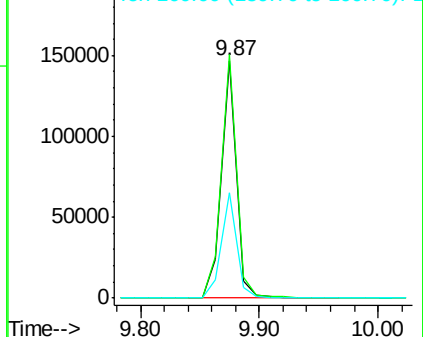




#41
 2,4,6-Tribromophenol
 Concen: 161.96 ng
 RT: 10.66 min Scan# 746
 Delta R.T. -0.01 min
 Lab File: BF082237.D
 Acq: 13 Oct 2015 1:58




Instrument :
 BNA_F
 ClientSampleId :
 TE-PMW(40)


Tot Ion:330 Resp: 192578
 Ion Ratio Lower Upper
 330 100
 332 96.1 77.1 115.7
 141 33.8 29.8 44.8

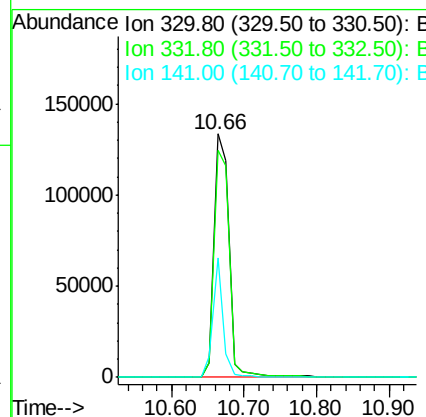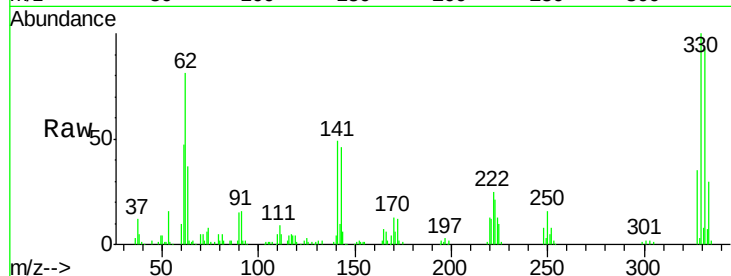

#44
 2-Fluorobiphenyl
 Concen: 113.19 ng
 RT: 9.20 min Scan# 618
 Delta R.T. 0.00 min
 Lab File: BF082237.D
 Acq: 13 Oct 2015 1:58

Tgt Ion:172 Resp: 865361
 Ion Ratio Lower Upper
 172 100
 171 36.8 28.6 42.8
 170 24.8 19.7 29.5



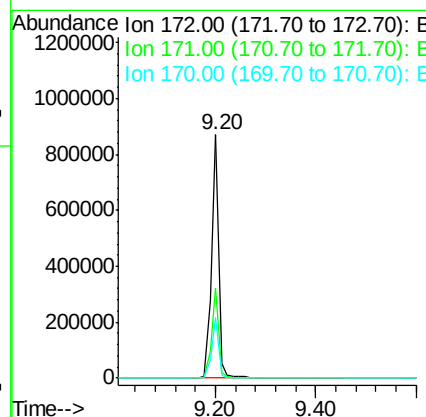



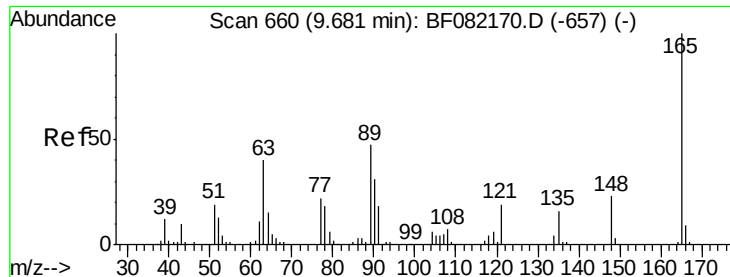

#50
 2,6-Dinitrotoluene
 Concen: 8.43 ng
 RT: 9.87 min Scan# 677
 Delta R.T. 0.21 min
 Lab File: BF082237.D
 Acq: 13 Oct 2015 1:58




Instrument :
 BNA_F
 ClientSampleId :
 TE-PMW(40)


Tot Ion	Ratio	Lower	Upper
165	100		
63	0.0	36.7	55.1#
89	0.0	37.8	56.6#

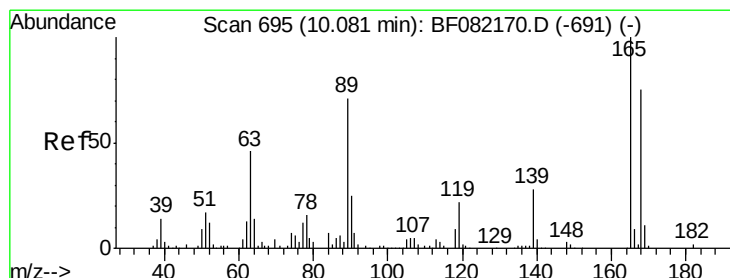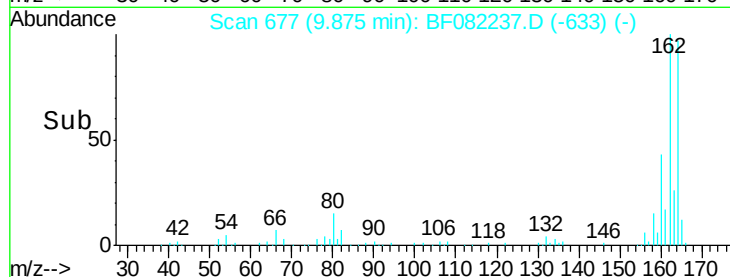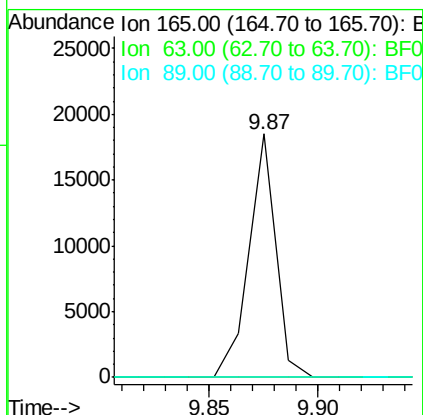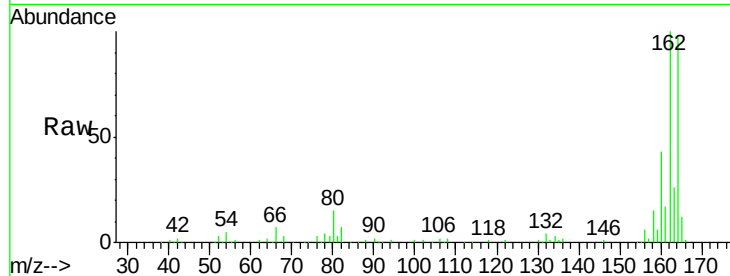

#56
 2,4-Dinitrotoluene
 Concen: 6.74 ng
 RT: 9.87 min Scan# 677
 Delta R.T. -0.19 min
 Lab File: BF082237.D
 Acq: 13 Oct 2015 1:58

Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	38.6	58.0#
89	0.0	57.0	85.6#
182	0.0	1.8	2.6#

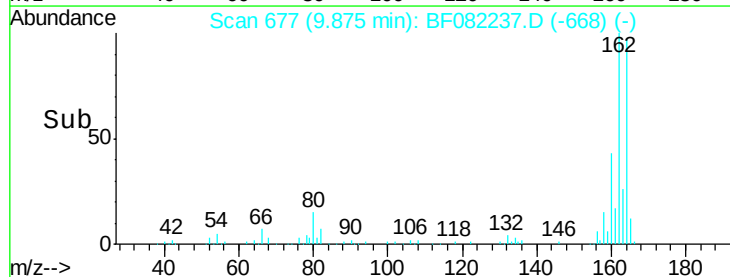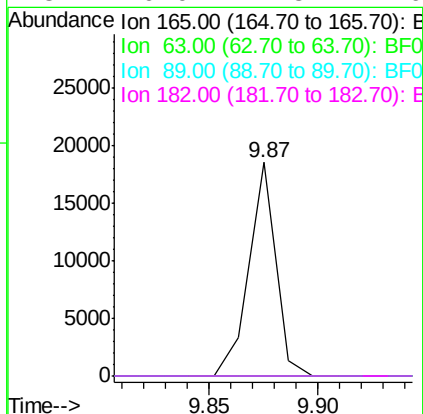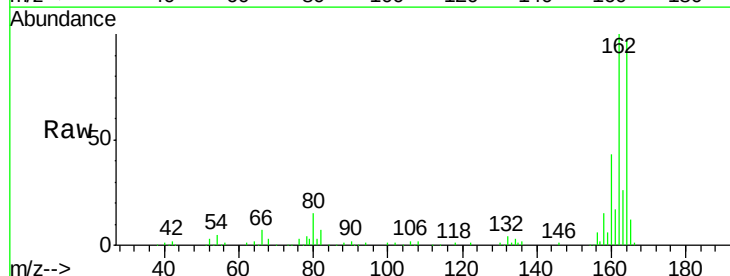

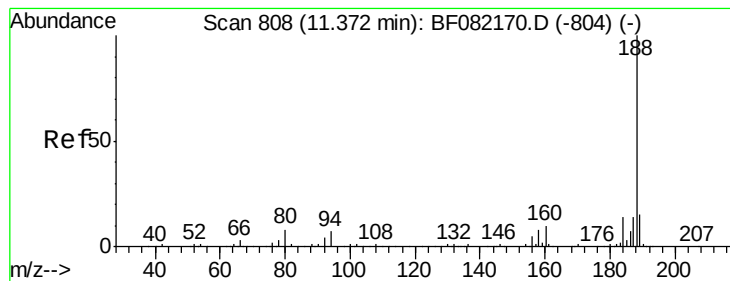

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.36 min Scan# 807

Delta R.T. 0.00 min

Lab File: BF082237.D

Acq: 13 Oct 2015 1:58

Instrument :

BNA_F

ClientSampleId :

TE-PMW(40)



Tot Ion:188 Resp: 253033

Ion Ratio Lower Upper

188 100

94 7.9 5.8 8.6



80 8.5 6.4 9.6

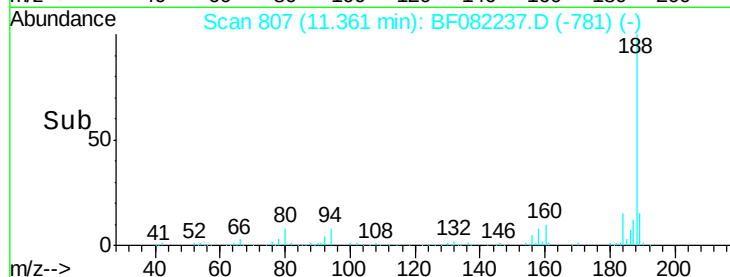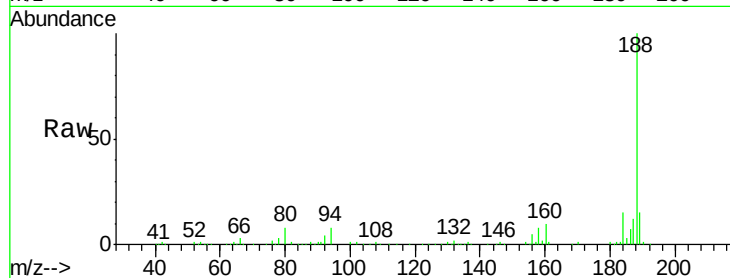

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

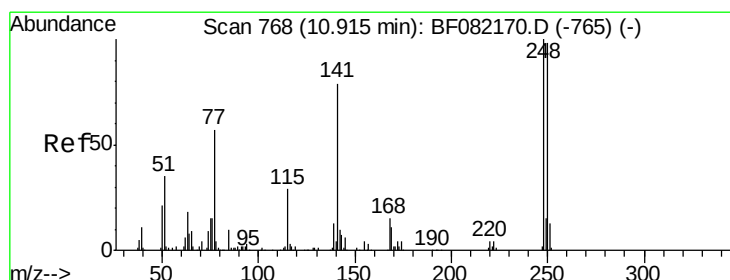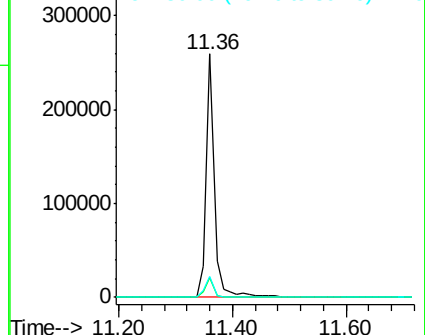

#66

4-Bromophenyl-phenylether

Concen: 4.82 ng

RT: 10.66 min Scan# 746

Delta R.T. -0.25 min

Lab File: BF082237.D

Acq: 13 Oct 2015 1:58



Tgt Ion:248 Resp: 12212

Ion Ratio Lower Upper

248 100

250 201.1 78.6 117.8#


141 599.3 63.3 94.9#

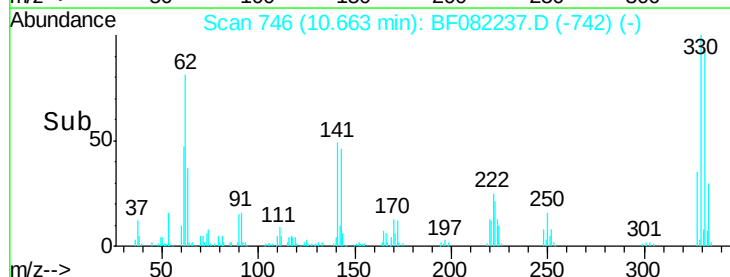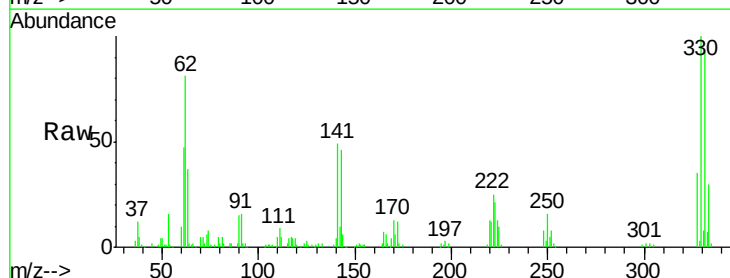


Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E




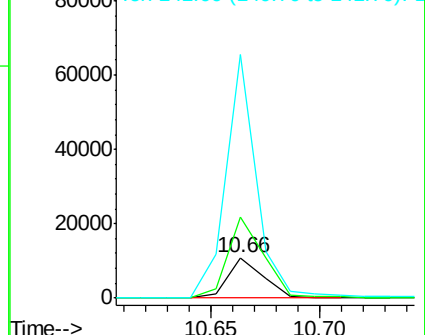


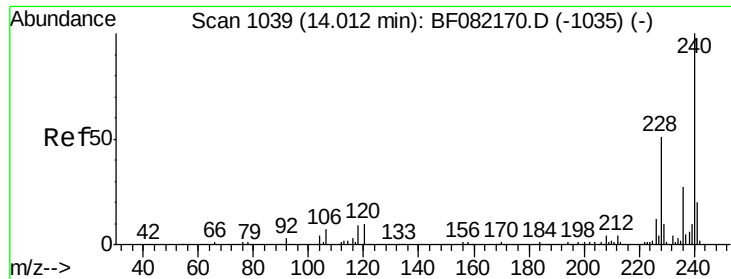

#75
 Chrysene-d12
 Concen: 20.00 ng
 RT: 14.00 min Scan# 1038
 Delta R.T. -0.01 min
 Lab File: BF082237.D
 Acq: 13 Oct 2015 1:58




Instrument :
 BNA_F
 ClientSampleId :
 TE-PMW(40)


Tot Ion:240 Resp: 254416
 Ion Ratio Lower Upper
 240 100
 120 9.7 8.1 12.1
 236 25.6 21.3 31.9

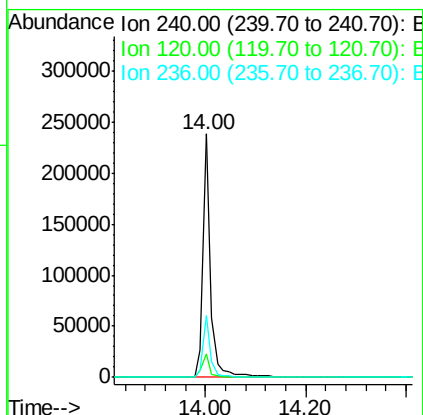

#78
 Terphenyl-d14
 Concen: 93.62 ng
 RT: 12.95 min Scan# 946
 Delta R.T. 0.00 min
 Lab File: BF082237.D
 Acq: 13 Oct 2015 1:58

Tgt Ion:244 Resp: 898858
 Ion Ratio Lower Upper
 244 100
 212 7.9 5.8 8.6
 122 12.1 5.9 8.9#

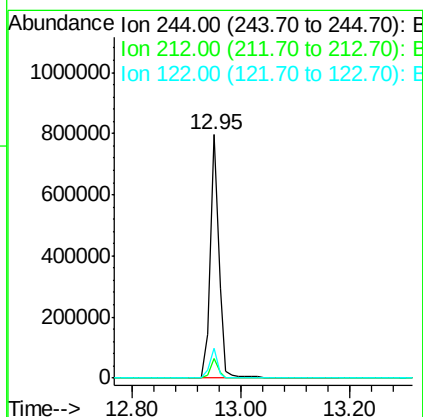


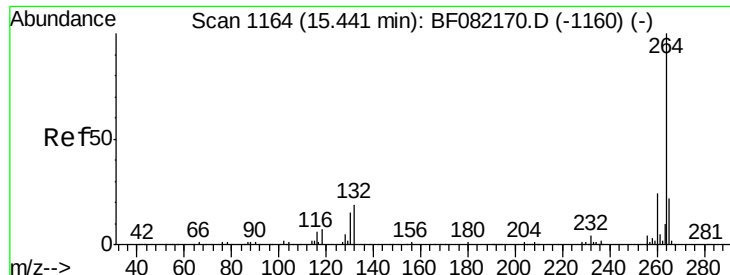

#86
Pervlene-d12
Concen: 20.00 ng
RT: 15.44 min Scan# 1164
Delta R.T. 0.00 min
Lab File: BF082237.D
Acq: 13 Oct 2015 1:58

Instrument :
BNA_F
ClientSampleId :
TE-PMW(40)

Tot Ion: 264 Resp: 194484
Ion Ratio Lower Upper
264 100
260 23.3 19.0 28.6
265 22.0 17.3 25.9

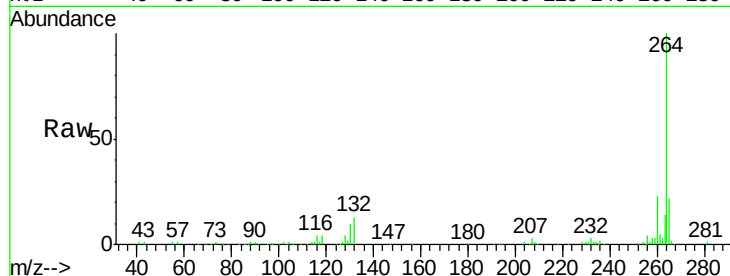

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

