


Data Path : Z:\HPCHEM1\BNA F\Data\BF101315\
 Data File : BF082235.D
 Acq On : 13 Oct 2015 00:57
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 12 01:46:21 2015

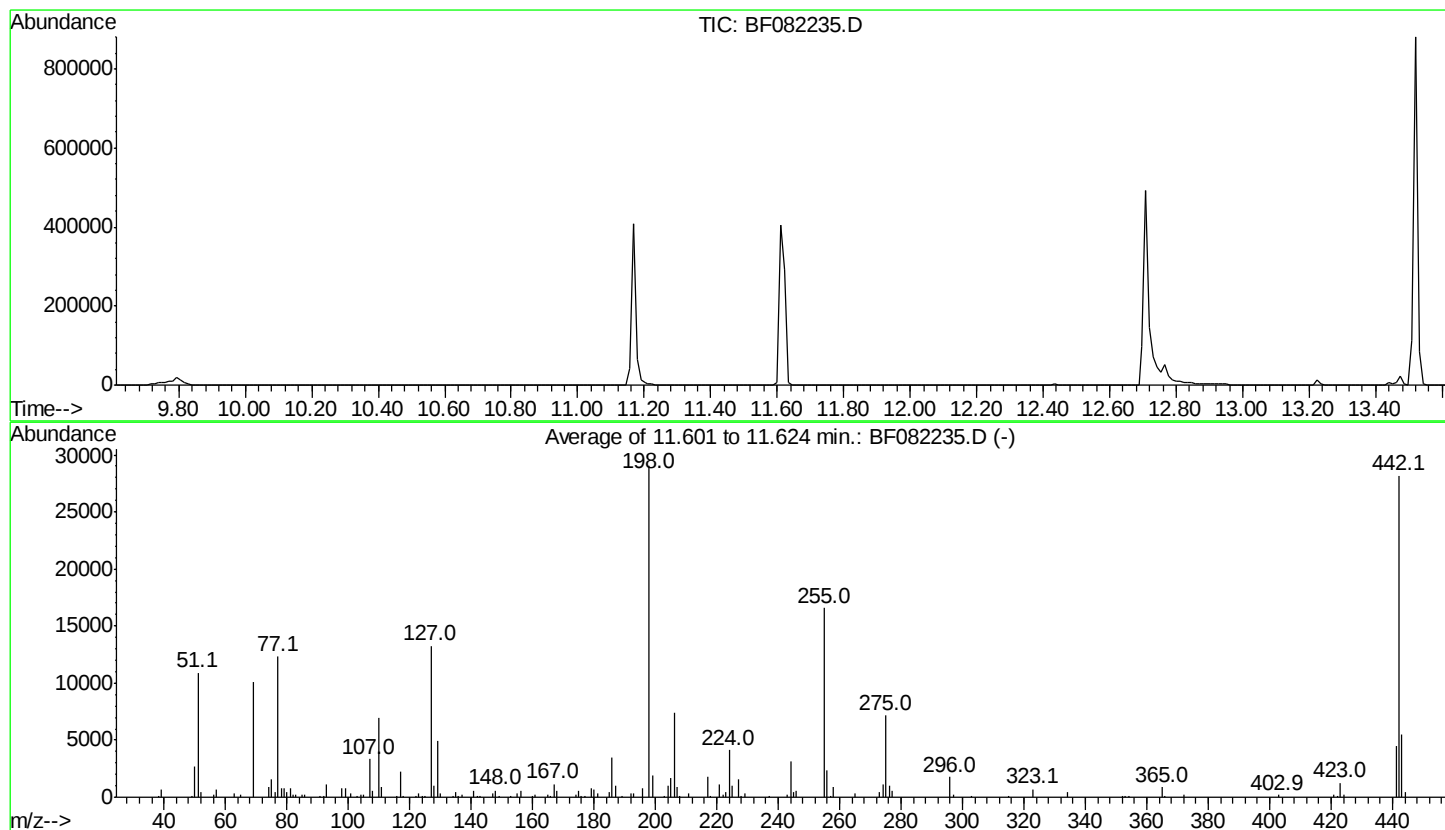

AutoFind: Scans 828, 829, 830; Background Corrected with Scan 825

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.6	10913	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.8	10106	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.6	13250	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	29054	PASS
199	198	5	9	6.7	1959	PASS
275	198	10	60	24.6	7142	PASS
365	198	1	100	3.1	888	PASS
441	442	0.01	24	16.0	4503	PASS
442	198	50	100	97.0	28172	PASS
443	442	15	24	19.7	5541	PASS