
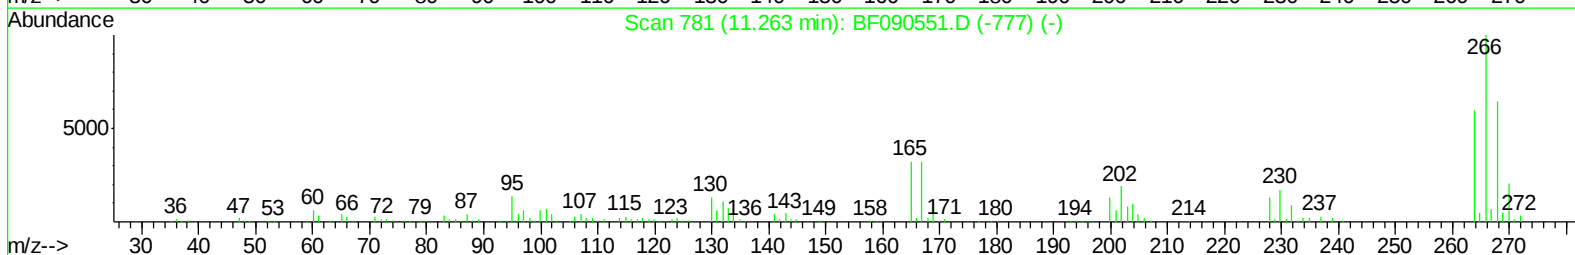
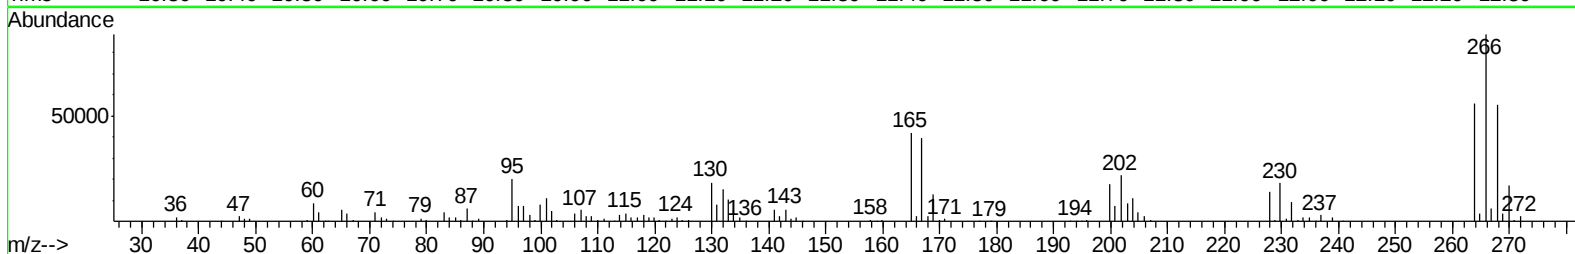


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101316\
 Data File : BF090546.D
 Acq On : 13 Oct 2016 16:59
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 14 07:14:56 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 14 02:03:28 2016
 Response via : Initial Calibration

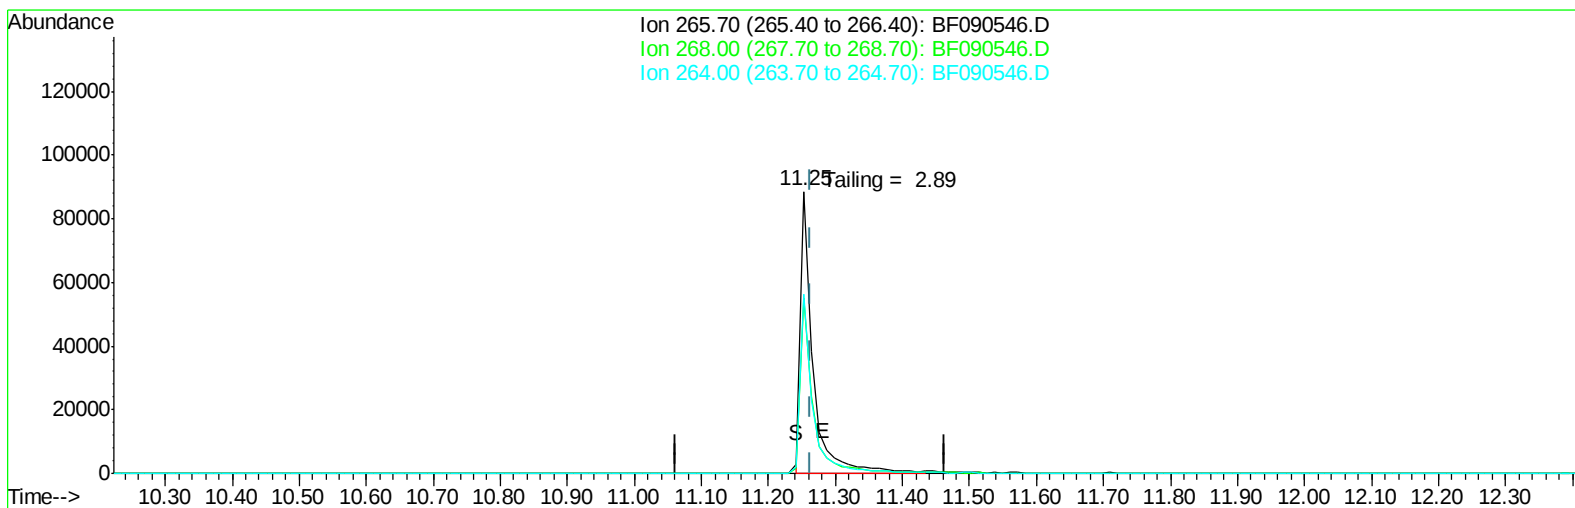

TIC: BF090546.D

(69) Pentachlorophenol (C)




11.252min (-0.011) 0.00ng m

response 116598

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	62.50
264.00	59.90	63.51
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101316\
 Data File : BF090546.D
 Acq On : 13 Oct 2016 16:59
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 14 07:14:56 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 14 02:03:28 2016
 Response via : Initial Calibration

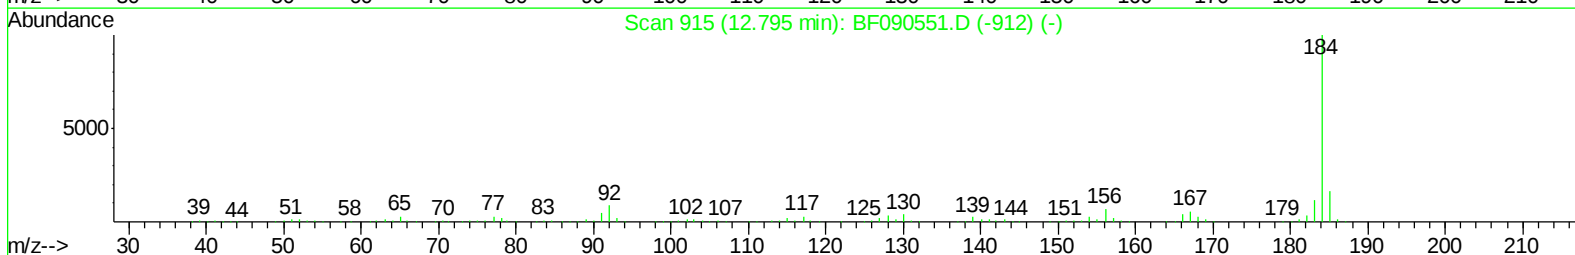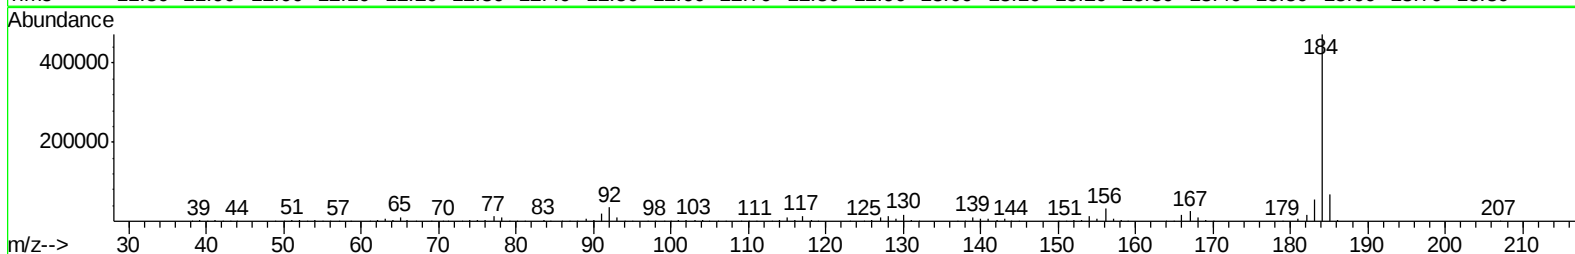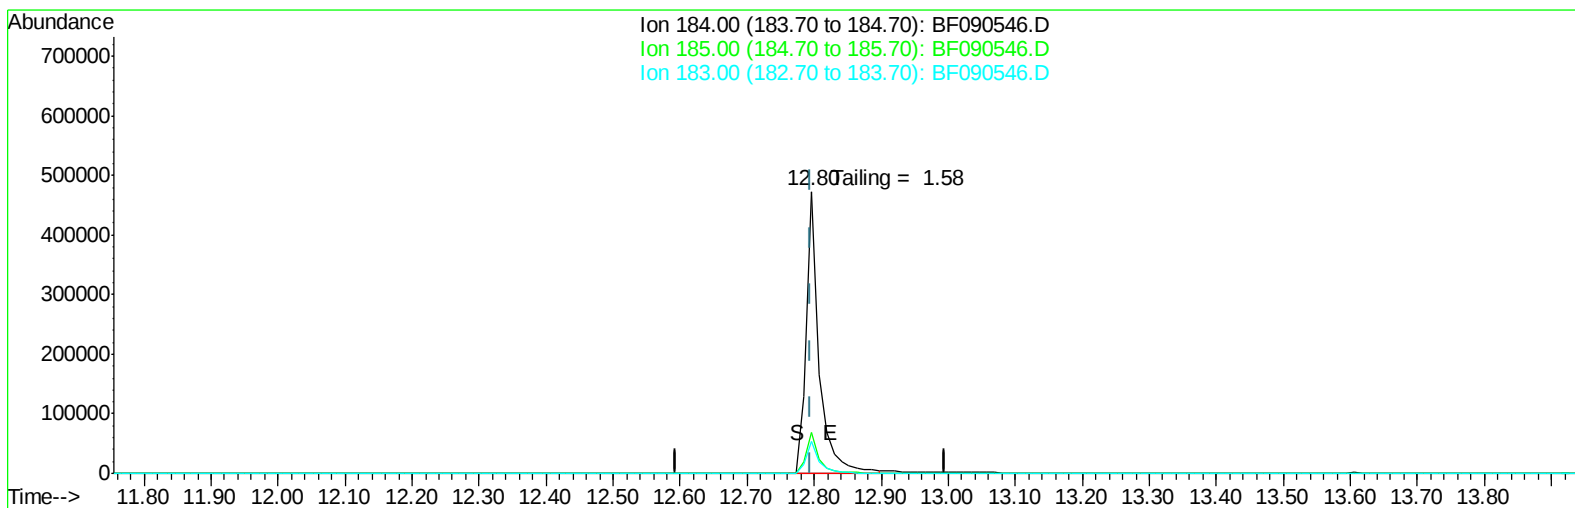

TIC: BF090546.D

(76) Benzidine

12.795min (-0.000) 0.00ng

response 645129

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.47
183.00	11.70	11.48
0.00	0.00	0.00