


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101316\
Data File : BF090546.D
Acq On : 13 Oct 2016 16:59
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101316.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Oct 14 12:44:45 2016

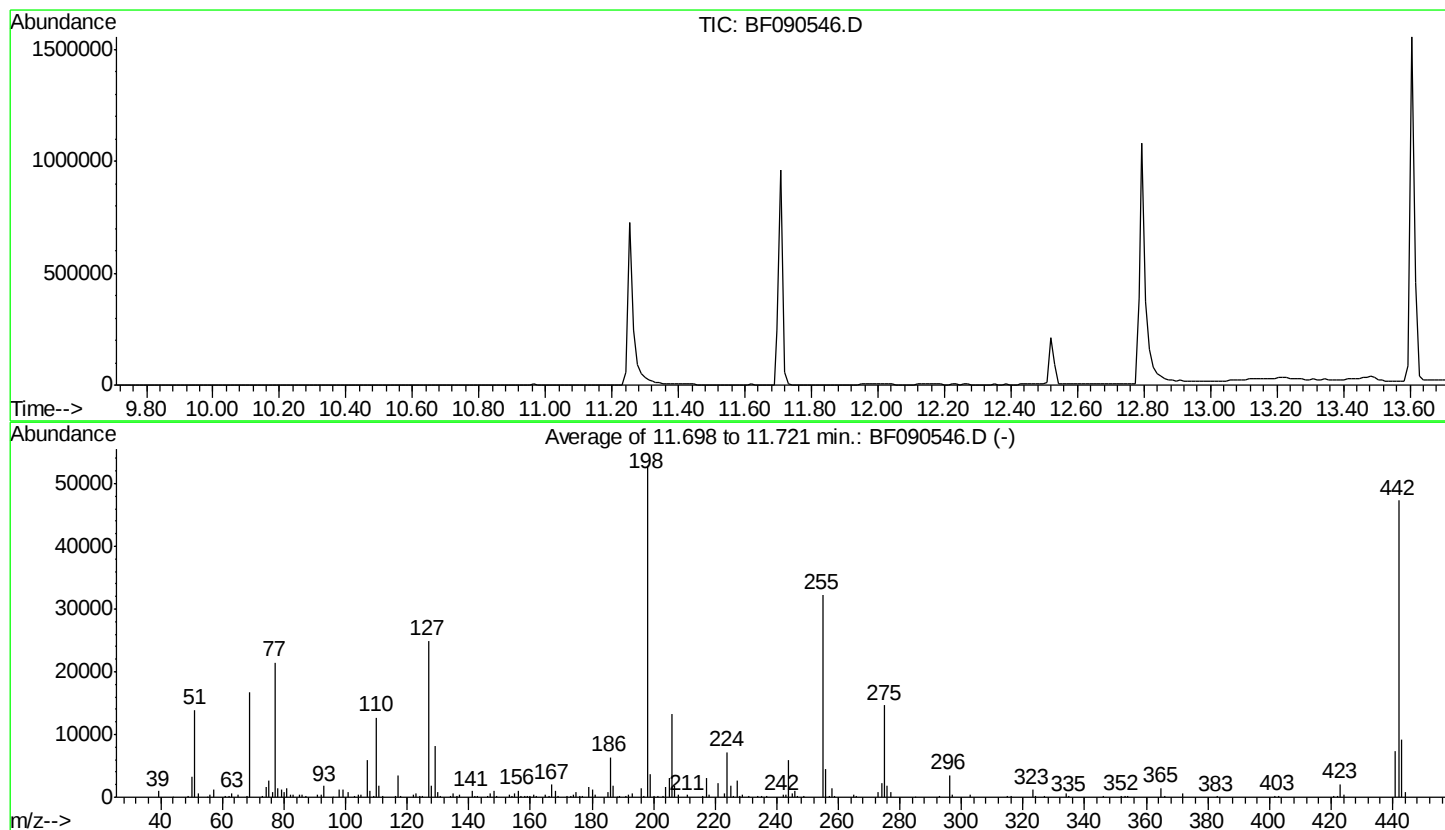

AutoFind: Scans 819, 820, 821; Background Corrected with Scan 816

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.4	13967	PASS
68	69	0.00	2	1.9	310	PASS
69	198	0.00	100	31.7	16756	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.2	24961	PASS
197	198	0.00	2	0.3	145	PASS
198	198	100	100	100.0	52868	PASS
199	198	5	9	6.9	3640	PASS
275	198	10	60	27.7	14620	PASS
365	198	1	100	2.7	1442	PASS
441	442	0.01	24	15.6	7367	PASS
442	198	50	100	89.5	47292	PASS
443	442	15	24	19.3	9141	PASS