

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101317\
 Data File : BF099456.D
 Acq On : 13 Oct 2017 23:01
 Operator : SJ/JU
 Sample : I5819-07
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Oct 14 00:04:28 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 11 16:25:21 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.85	152	90640	20.00	ng	0.00
21) Naphthalene-d8	8.13	136	354891	20.00	ng	0.00
38) Acenaphthene-d10	9.89	164	137019	20.00	ng	0.00
63) Phenanthrene-d10	11.37	188	202509	20.00	ng	0.00
75) Chrysene-d12	14.02	240	162104	20.00	ng	0.00
86) Perylene-d12	15.49	264	178208	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.47	112	403617	70.89	ng	0.00
7) Phenol-d6	6.49	99	292983	41.71	ng	0.00
23) Nitrobenzene-d5	7.42	82	564996	102.10	ng	0.00
41) 2,4,6-Tribromophenol	10.68	330	152096	135.66	ng	0.00
44) 2-Fluorobiphenyl	9.21	172	962750	117.30	ng	0.00
78) Terphenyl-d14	12.96	244	631658	88.62	ng	0.00
Target Compounds						
9) Benzaldehyde	6.63	77	12478	3.06	ng	Qvalue 87
19) n-Nitroso-di-n-propylamine	7.42	70	71920	16.04	ng	# 74
25) Isophorone	7.42	82	564992	49.38	ng	# 64
50) 2,6-Dinitrotoluene	9.89	165	17080	7.59	ng	# 24
56) 2,4-Dinitrotoluene	9.89	165	17080	5.85	ng	# 21
66) 4-Bromophenyl-phenylether	10.68	248	10244	5.17	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101317\
Data File : BF099456.D
Acq On : 13 Oct 2017 23:01
Operator : SJ/JU
Sample : I5819-07
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Oct 14 00:04:28 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 11 16:25:21 2017
Response via : Initial Calibration

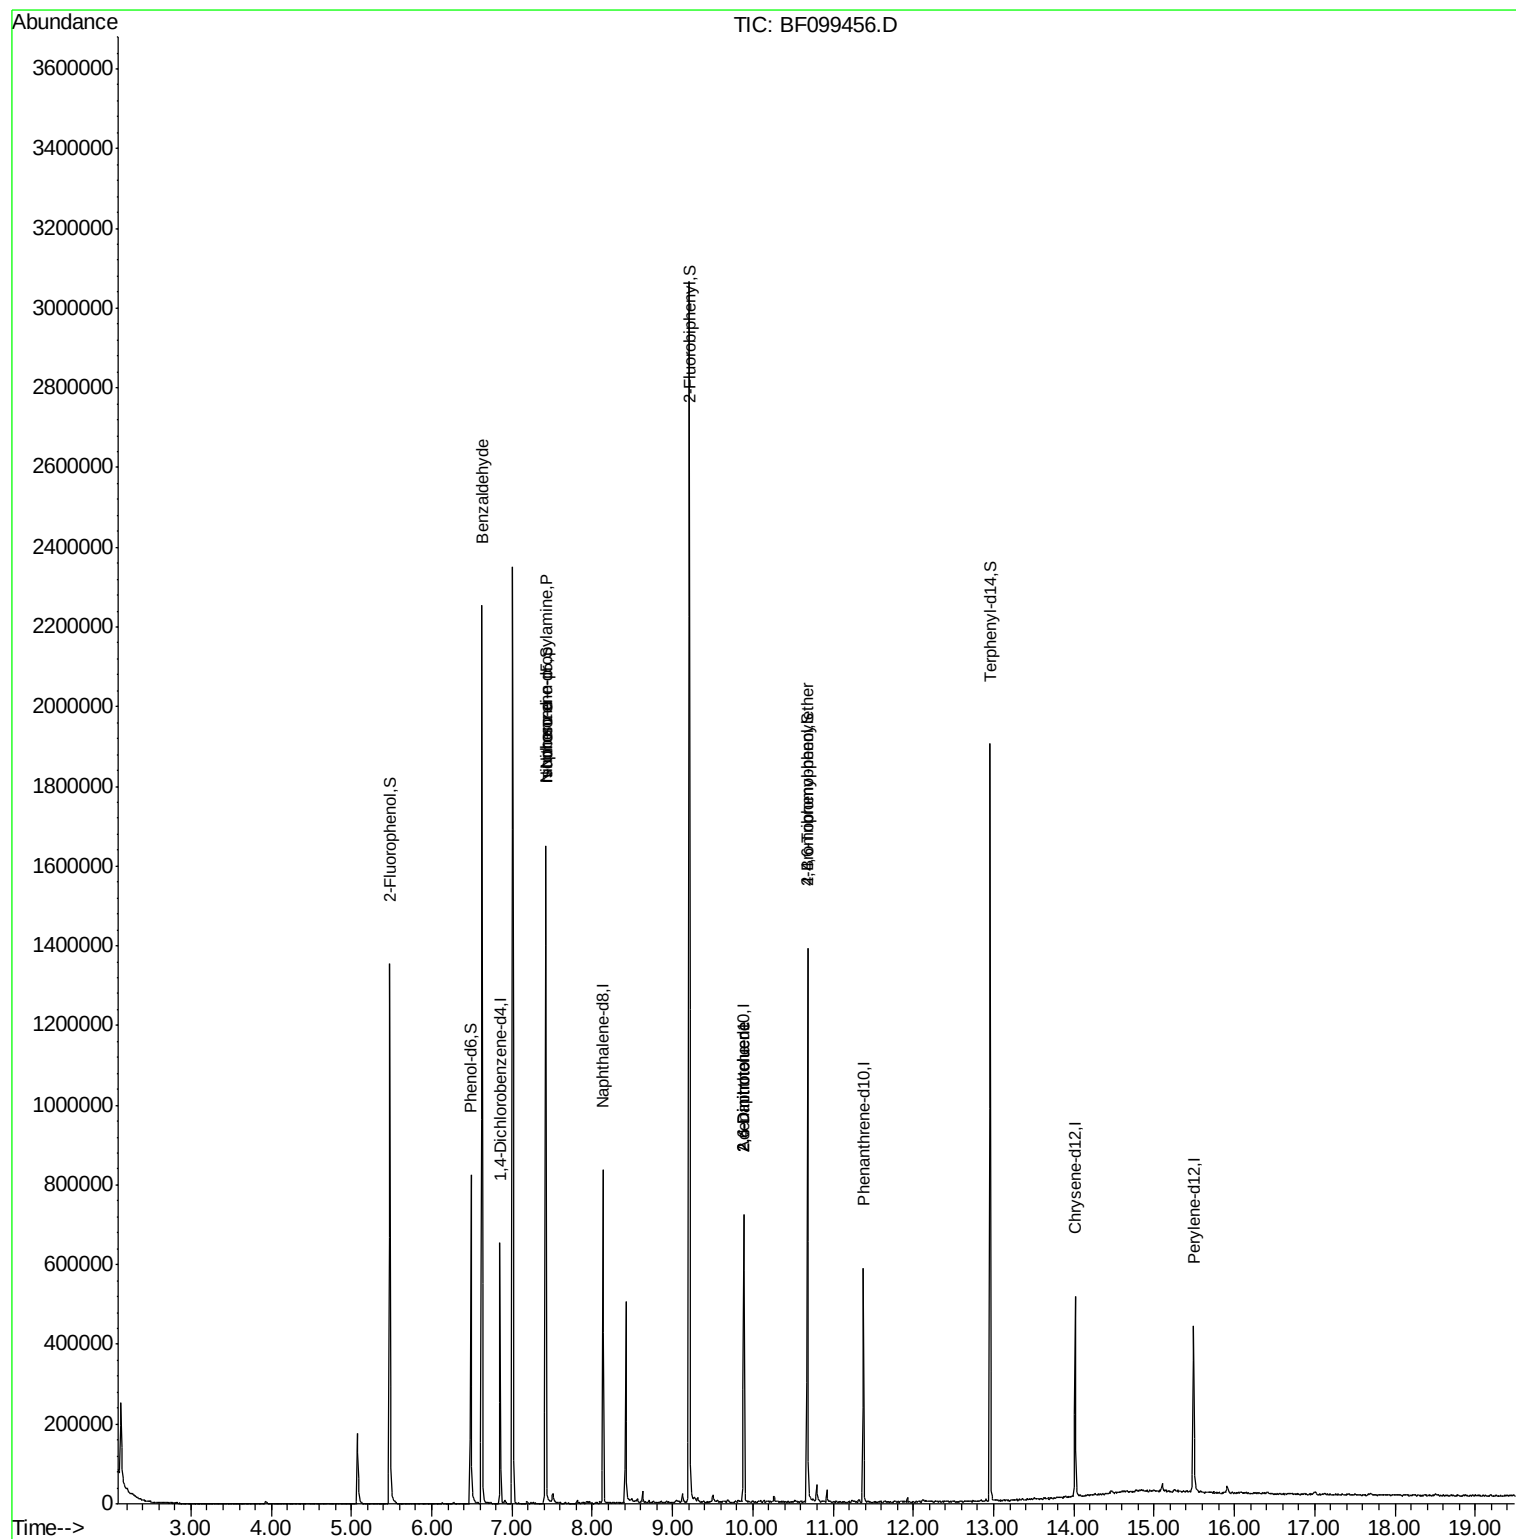

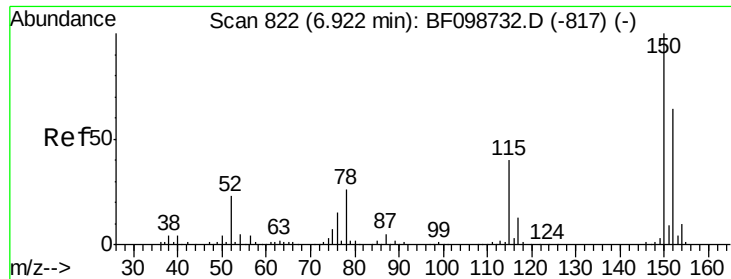


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.85 min Scan# 810
Delta R.T. 0.00 min
Lab File: BF099456.D
Acq: 13 Oct 2017 23:01

Instrument :
BNA_F
ClientSampleId :

Tot Ion:152 Resp: 90640
Ion Ratio Lower Upper
152 100
150 155.4 124.6 186.8
115 61.6 50.1 75.1

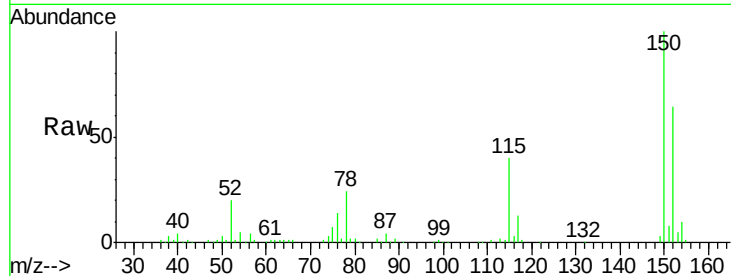


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

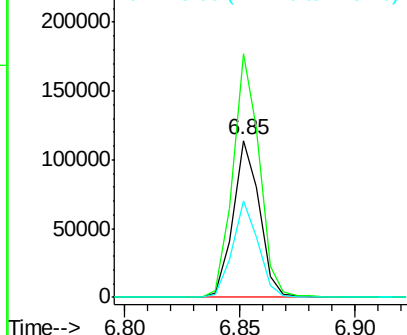



#5


2-Fluorophenol
Concen: 70.89 ng
RT: 5.47 min Scan# 576
Delta R.T. 0.01 min
Lab File: BF099456.D
Acq: 13 Oct 2017 23:01

Tgt Ion:112 Resp: 403617
Ion Ratio Lower Upper
112 100
64 56.7 47.9 71.9
63 27.5 23.7 35.5



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

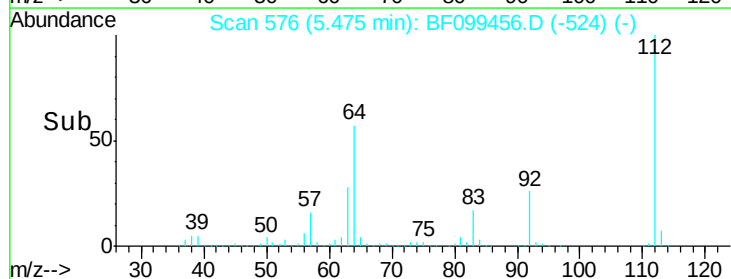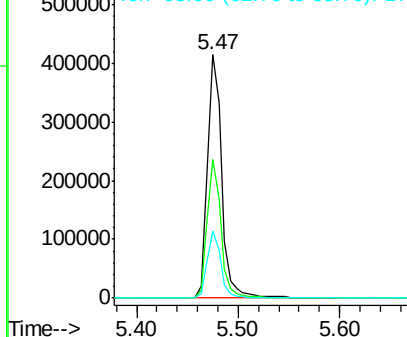

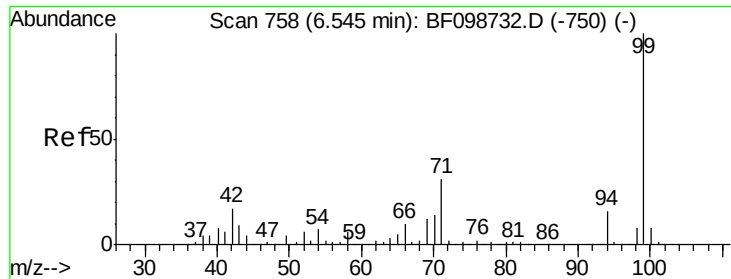

#7

Phenol-d6

Concen: 41.71 ng

RT: 6.49 min Scan# 748

Delta R.T. 0.00 min

Lab File: BF099456.D

Acq: 13 Oct 2017 23:01

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 99 Resp: 292983

Ion Ratio Lower Upper

99 100

42 15.3 14.5 21.7




71 29.5 25.4 38.0

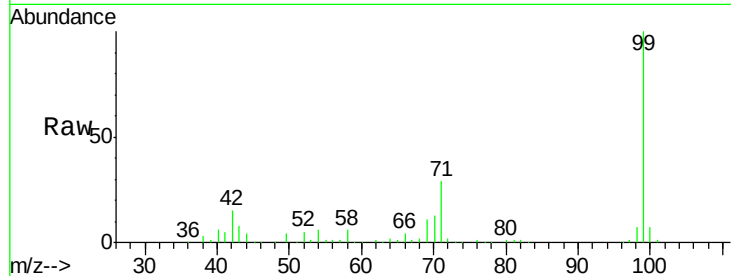

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

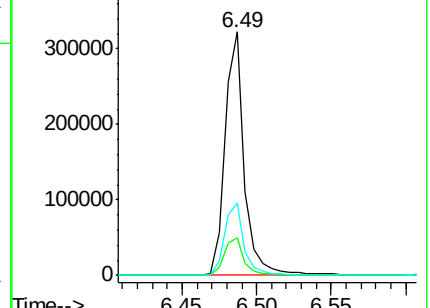

#9

Benzaldehyde

Concen: 3.06 ng

RT: 6.63 min Scan# 772

Delta R.T. 0.22 min

Lab File: BF099456.D

Acq: 13 Oct 2017 23:01


Tgt Ion: 77 Resp: 12478

Ion Ratio Lower Upper

77 100

105 82.3 81.1 121.1



106 88.7 74.5 114.5




Abundance Ion 77.00 (76.70 to 77.70): BF0

Ion 105.00 (104.70 to 105.70): E

Ion 106.00 (105.70 to 106.70): E



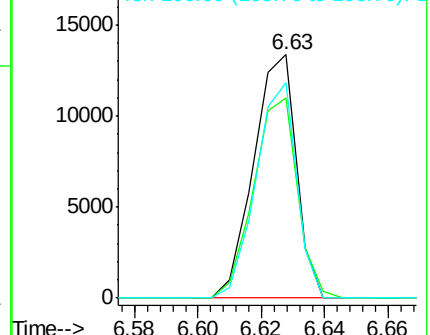





#19
n-Nitroso-di-n-propylamine
Concen: 16.04 ng
RT: 7.42 min Scan# 907
Delta R.T. 0.15 min
Lab File: BF099456.D
Acq: 13 Oct 2017 23:01




Instrument :
BNA_F
ClientSampled :


Tot Ion: 70 Resp: 71920
Ion Ratio Lower Upper
70 100
42 43.0 47.5 71.3#
101 0.0 7.4 11.2#
130 2.6 16.6 25.0#

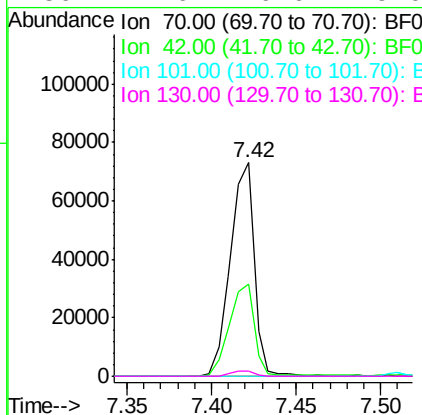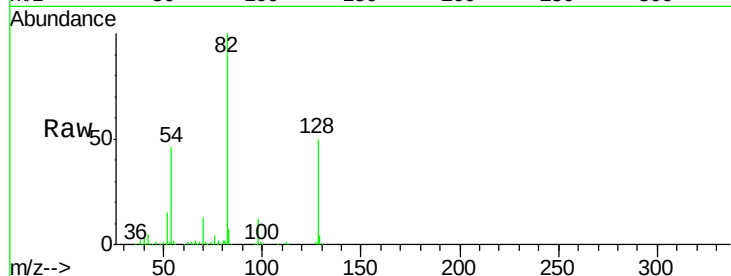

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.13 min Scan# 1028
Delta R.T. 0.00 min
Lab File: BF099456.D
Acq: 13 Oct 2017 23:01

Tgt Ion: 136 Resp: 354891
Ion Ratio Lower Upper
136 100
137 10.6 8.9 13.3
54 7.4 6.6 9.8
68 5.6 5.0 7.4



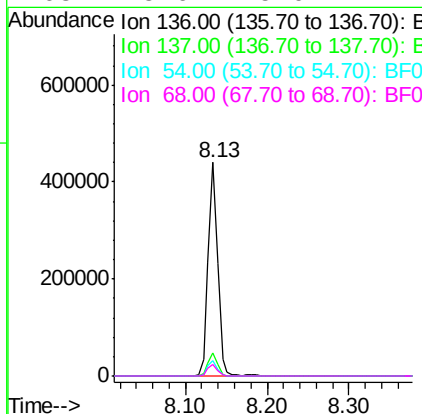



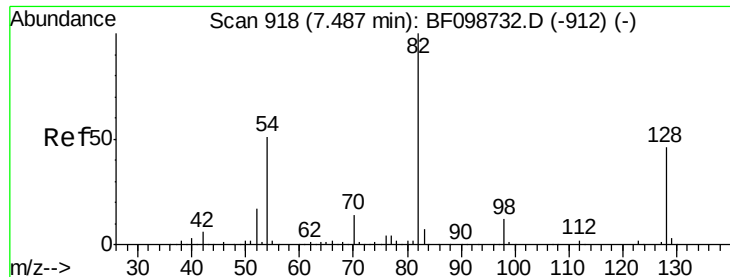

#23
Nitrobenzene-d5
Concen: 102.10 ng
RT: 7.42 min Scan# 907
Delta R.T. 0.00 min
Lab File: BF099456.D
Acq: 13 Oct 2017 23:01




Instrument :
BNA_F
ClientSampled :


Tot Ion	82	Resp	564996
Ion Ratio	100	Lower	Upper
128	49.8	36.1	54.1
54	46.2	41.4	62.2

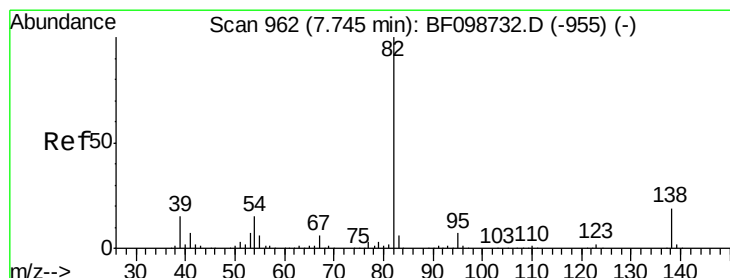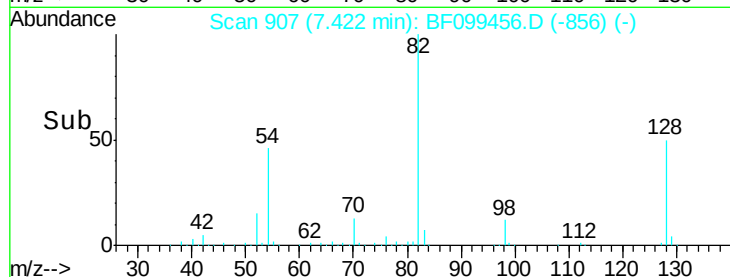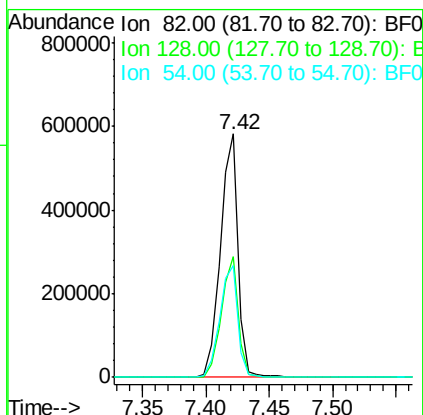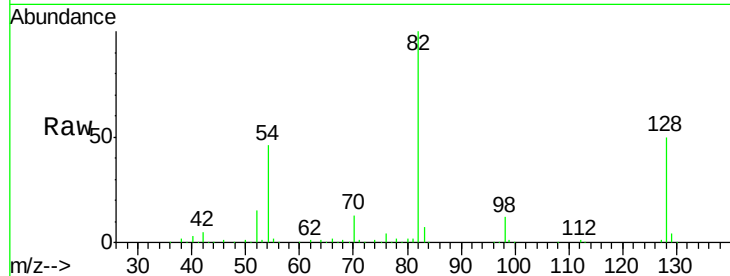

#25
Isophorone
Concen: 49.38 ng
RT: 7.42 min Scan# 907
Delta R.T. -0.25 min
Lab File: BF099456.D
Acq: 13 Oct 2017 23:01

Tgt Ion	82	Resp	564992
Ion Ratio	100	Lower	Upper
95	0.0	5.2	7.8#
138	0.0	14.9	22.3#

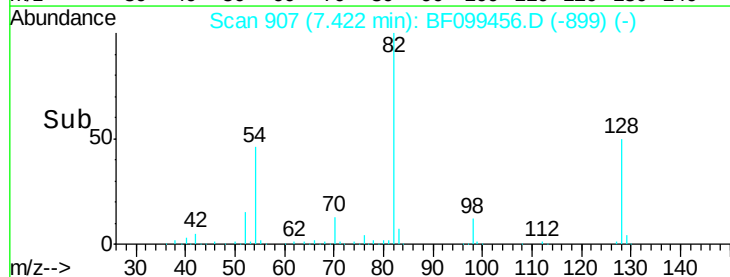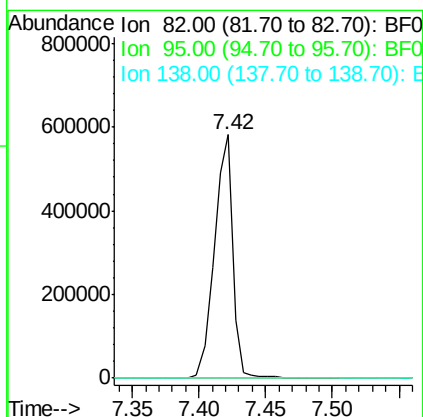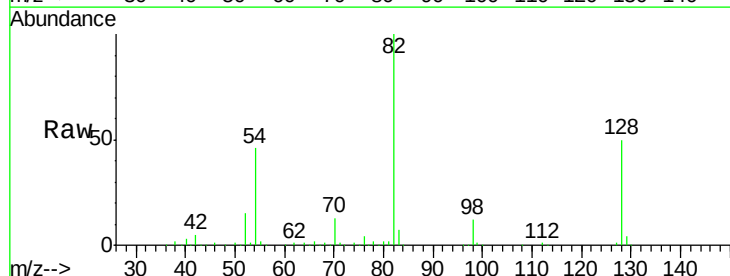

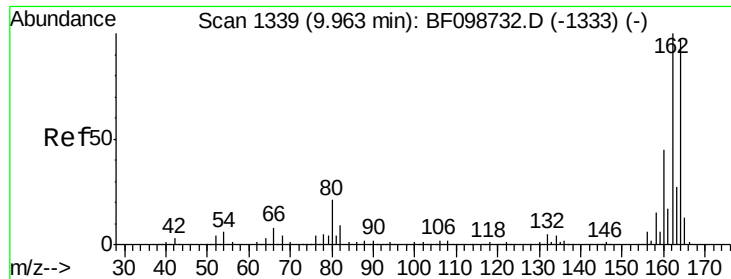

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.89 min Scan# 1326

Delta R.T. -0.01 min

Lab File: BF099456.D

Acq: 13 Oct 2017 23:01

Instrument :

BNA_F

ClientSampleId :


Tot Ion:164 Resp: 137019

Ion Ratio Lower Upper

164 100

162 103.8 86.1 129.1




160 45.8 38.3 57.5



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

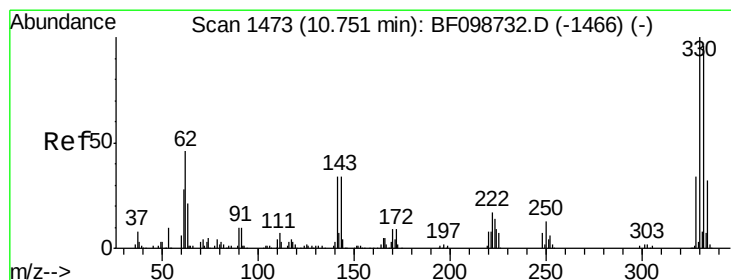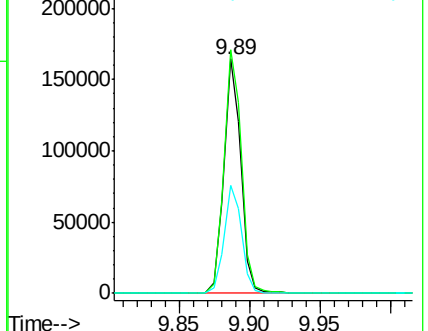

#41

2,4,6-Tribromophenol

Concen: 135.66 ng

RT: 10.68 min Scan# 1461

Delta R.T. 0.00 min

Lab File: BF099456.D

Acq: 13 Oct 2017 23:01


Tgt Ion:330 Resp: 152096

Ion Ratio Lower Upper

330 100

332 98.0 77.0 115.6



141 40.2 29.9 44.9




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

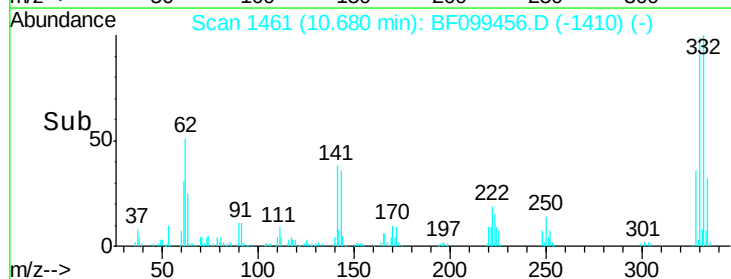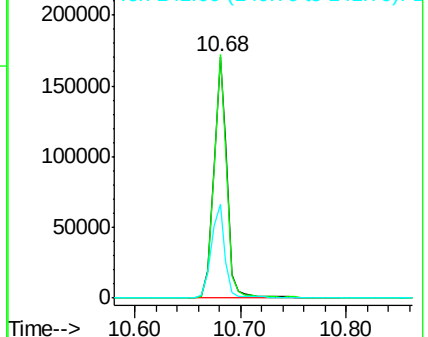







#44
 2-Fluorobiphenyl
 Concen: 117.30 ng
 RT: 9.21 min Scan# 1211
 Delta R.T. 0.00 min
 Lab File: BF099456.D
 Acq: 13 Oct 2017 23:01

Instrument :
 BNA_F
 ClientSampled :

Tot Ion:172 Resp: 962750
 Ion Ratio Lower Upper
 172 100
 171 36.7 29.7 44.5
 170 24.1 19.6 29.4




Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

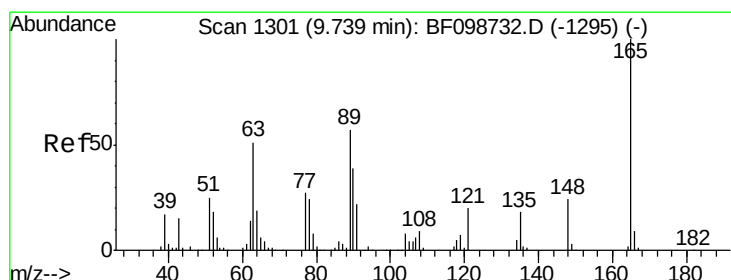
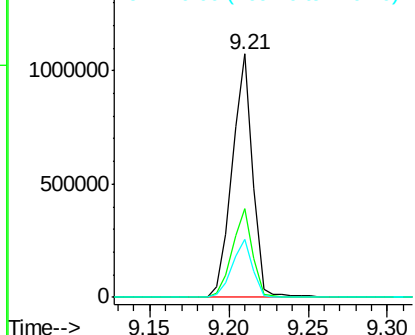



#50
 2,6-Dinitrotoluene
 Concen: 7.59 ng
 RT: 9.89 min Scan# 1326
 Delta R.T. 0.21 min
 Lab File: BF099456.D
 Acq: 13 Oct 2017 23:01

Tgt Ion:165 Resp: 17080
 Ion Ratio Lower Upper
 165 100
 63 0.0 44.7 67.1#
 89 0.0 44.0 66.0#



Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF0
 Ion 89.00 (88.70 to 89.70): BF0




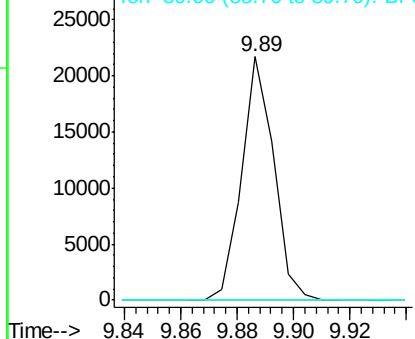


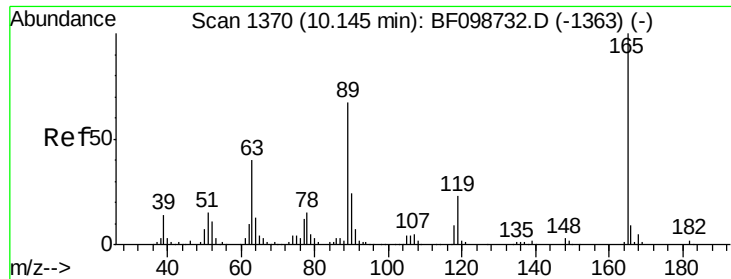

#56
 2,4-Dinitrotoluene
 Concen: 5.85 ng
 RT: 9.89 min Scan# 1326
 Delta R.T. -0.20 min
 Lab File: BF099456.D
 Acq: 13 Oct 2017 23:01




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion:165	Resp:	17080
Ion Ratio	Lower	Upper
165	100	
63	0.0	36.4 54.6#
89	0.0	57.8 86.6#
182	0.0	1.6 2.4#

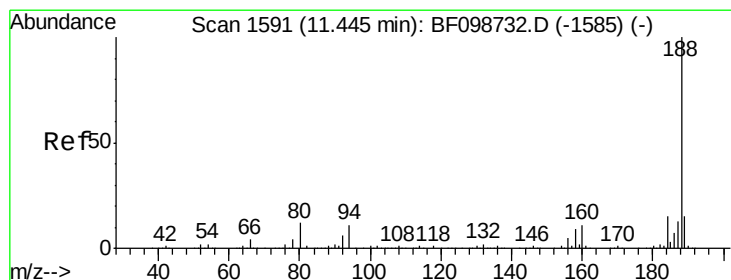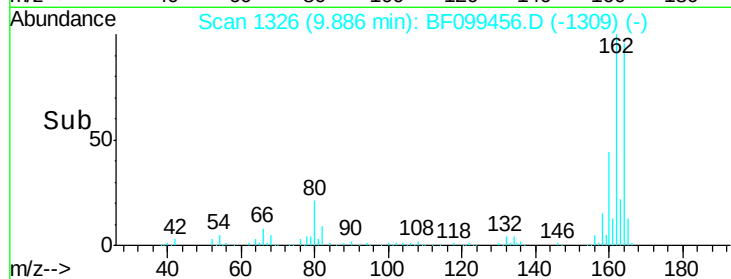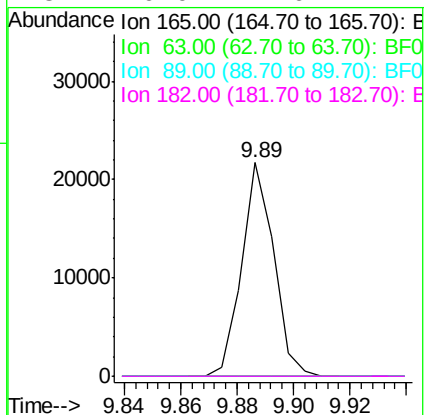

#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.37 min Scan# 1579
 Delta R.T. 0.00 min
 Lab File: BF099456.D
 Acq: 13 Oct 2017 23:01

Tgt Ion:188	Resp:	202509
Ion Ratio	Lower	Upper
188	100	
94	11.3	8.5 12.7
80	11.8	9.2 13.8

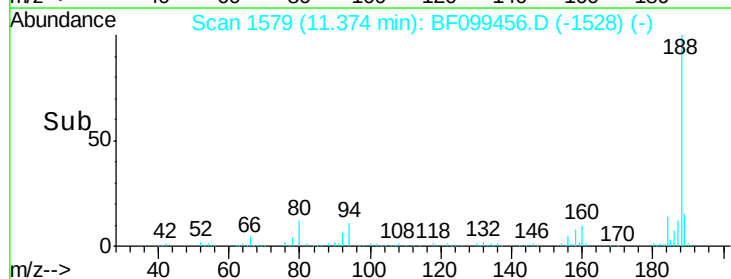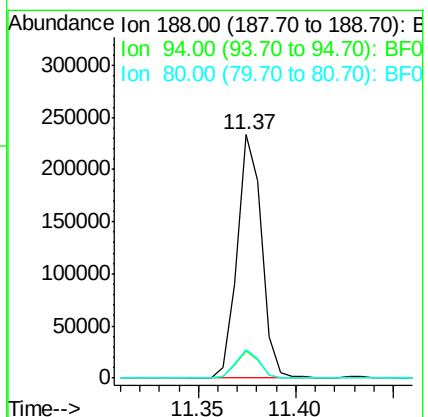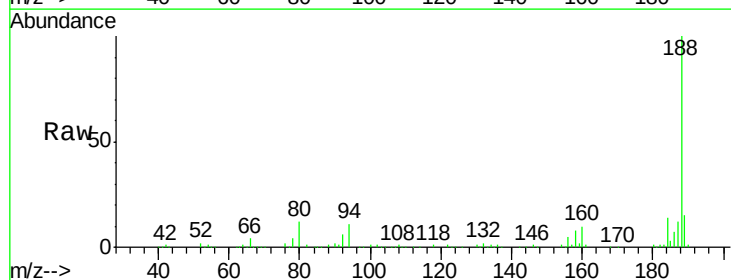


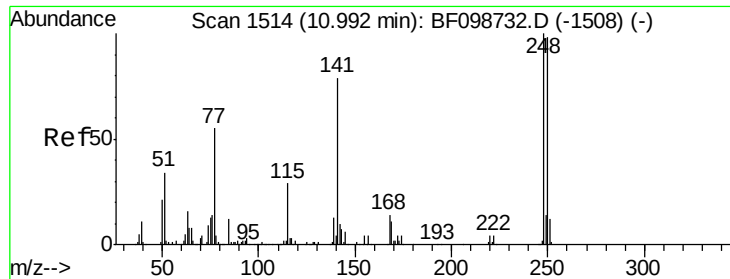




#66
4-Bromophenyl-phenylether
Concen: 5.17 ng
RT: 10.68 min Scan# 1461
Delta R.T. -0.24 min
Lab File: BF099456.D
Acq: 13 Oct 2017 23:01

Instrument :
BNA_F
ClientSampled :

Tot Ion:248 Resp: 10244
Ion Ratio Lower Upper
248 100
250 200.1 76.9 115.3#
141 549.6 74.4 111.6#

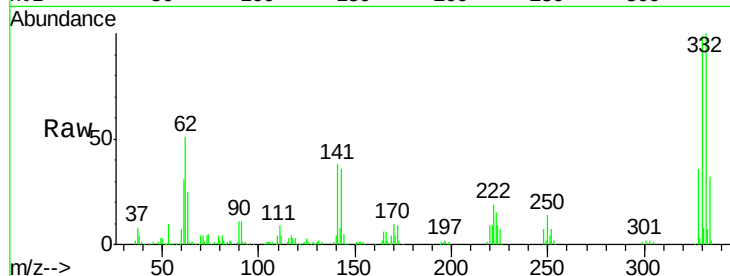


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

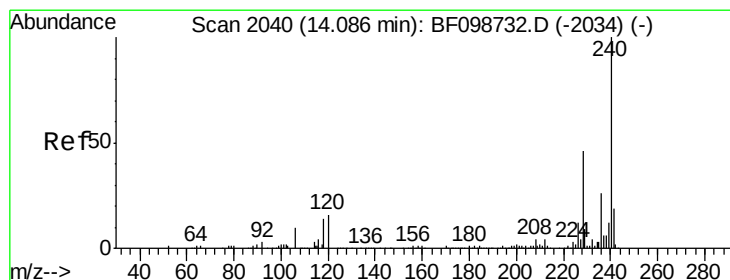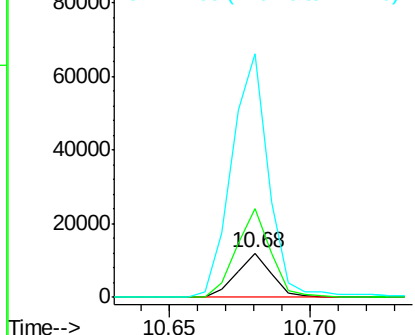
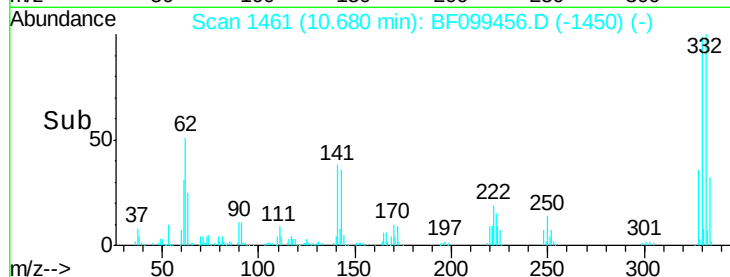



#75
Chrysene-d12
Concen: 20.00 ng
RT: 14.02 min Scan# 2028
Delta R.T. 0.00 min
Lab File: BF099456.D
Acq: 13 Oct 2017 23:01

Tgt Ion:240 Resp: 162104
Ion Ratio Lower Upper
240 100
120 14.9 9.5 14.3#
236 24.5 20.7 31.1

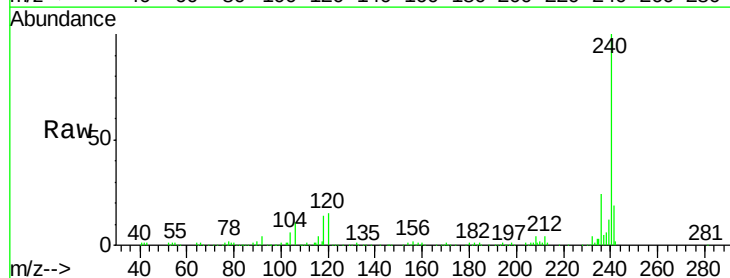

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

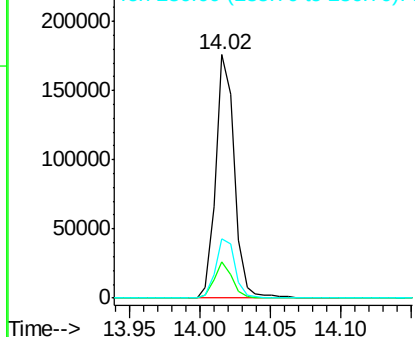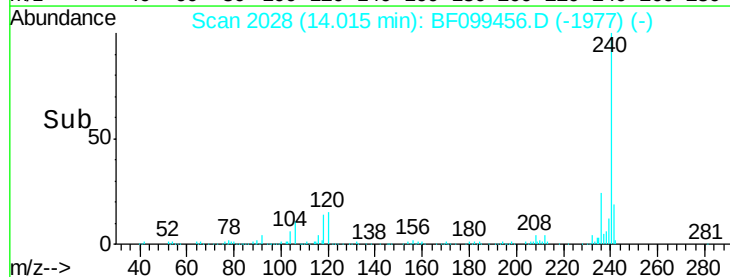

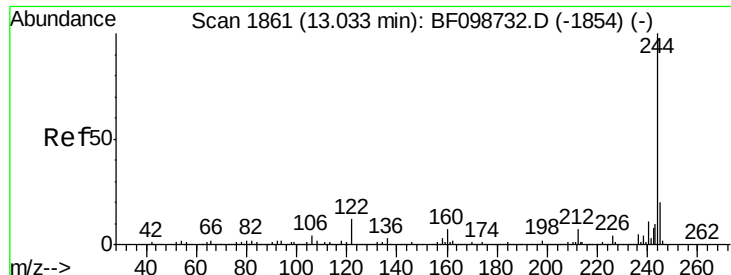

#78

Terphenyl-d14

Concen: 88.62 ng

RT: 12.96 min Scan# 1848

Delta R.T. 0.00 min

Lab File: BF099456.D

Acq: 13 Oct 2017 23:01

Instrument :

BNA_F

ClientSampleId :


Tot Ion:244 Resp: 631658

Ion Ratio Lower Upper

244 100

212 7.5 5.4 8.0




122 15.1 11.0 16.4



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

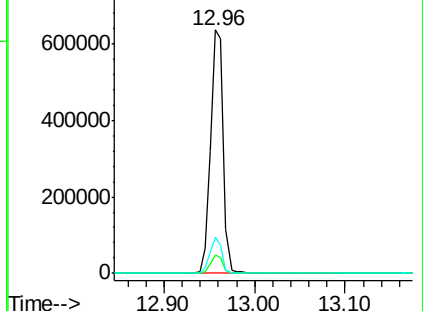

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.49 min Scan# 2279

Delta R.T. 0.01 min

Lab File: BF099456.D

Acq: 13 Oct 2017 23:01


Tgt Ion:264 Resp: 178208

Ion Ratio Lower Upper

264 100

260 23.2 19.2 28.8

265 21.4 17.5 26.3



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

