
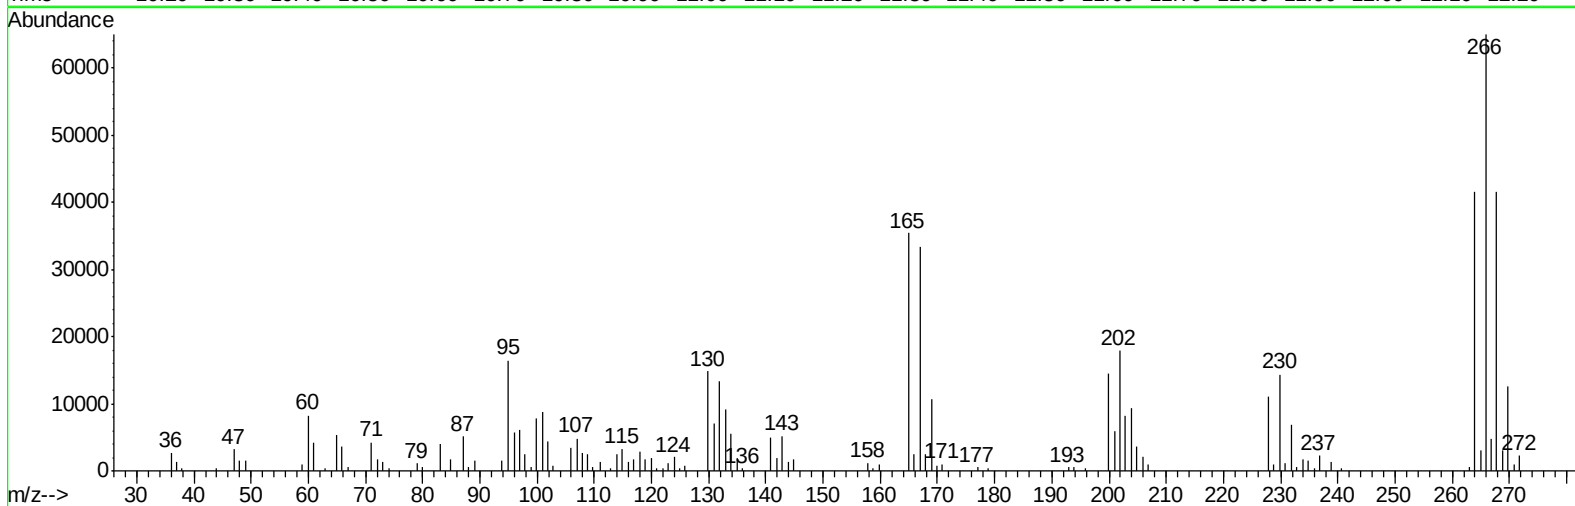


Data Path : Z:\HPCHEM1\BNA F\DATA\BF101317\
Data File : BF099438.D
Acq On : 13 Oct 2017 13:55
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 13 23:46:35 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 11 16:25:21 2017
Response via : Initial Calibration

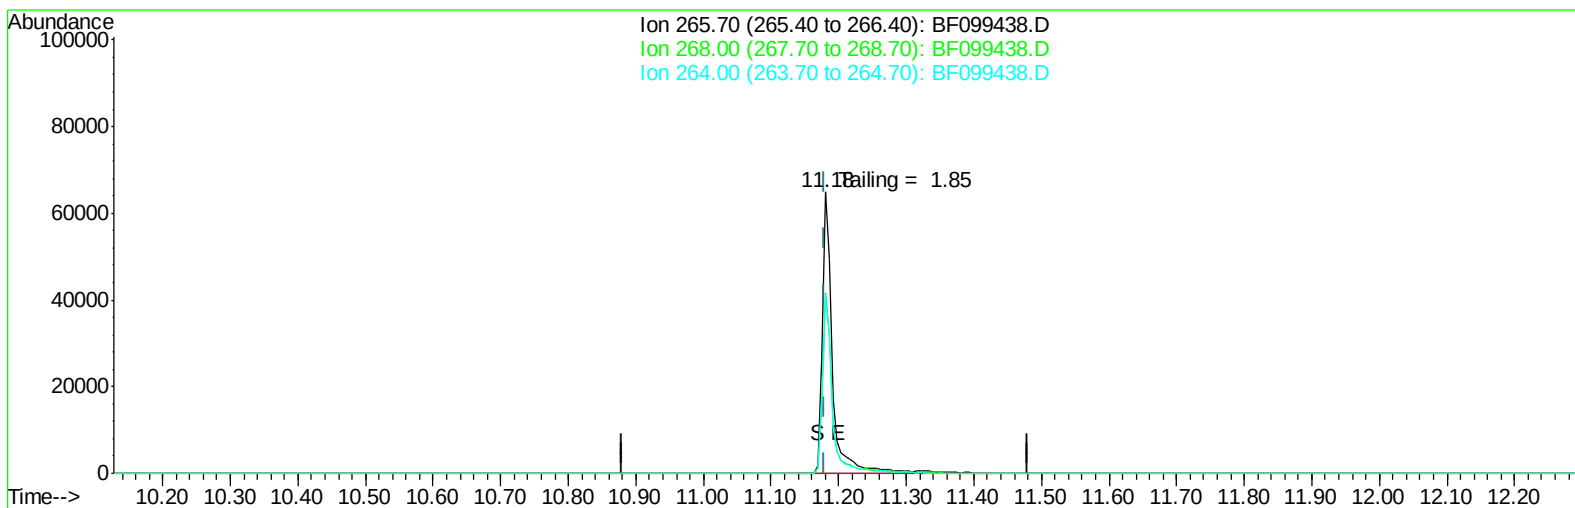

TIC: BF099438.D

(69) Pentachlorophenol (C)



11.181min (+0.000) 9153.37ng

response 68310

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.01
264.00	61.90	63.82
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101317\
Data File : BF099438.D
Acq On : 13 Oct 2017 13:55
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 13 23:46:35 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 11 16:25:21 2017
Response via : Initial Calibration

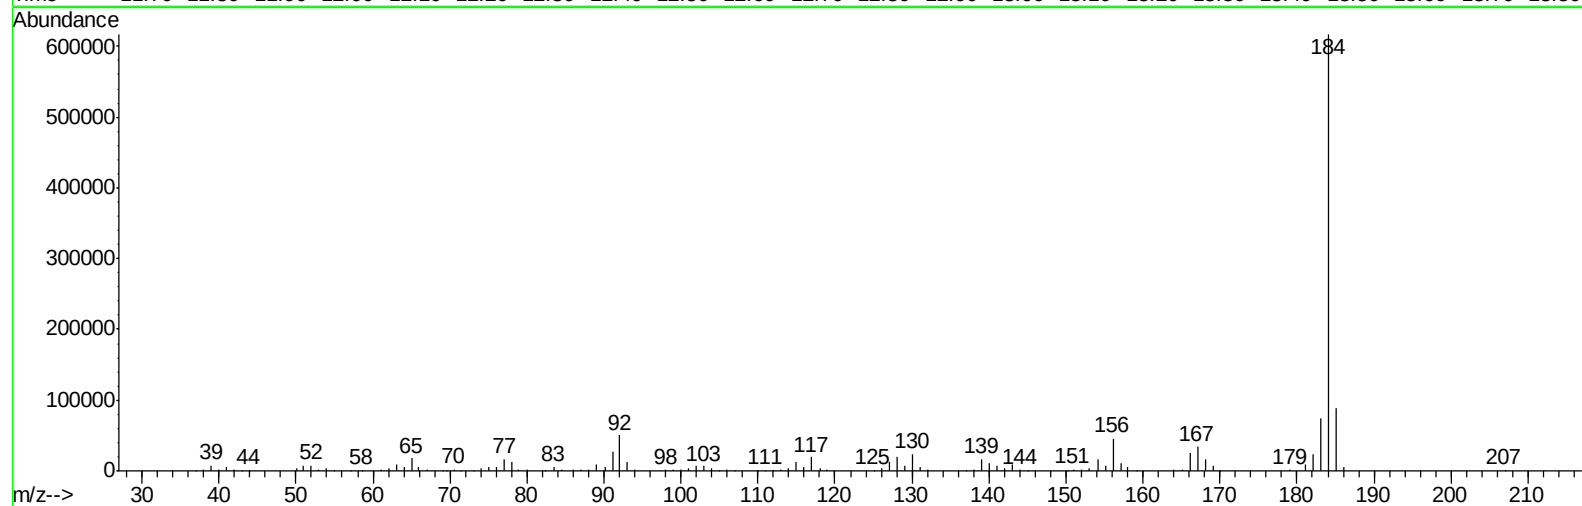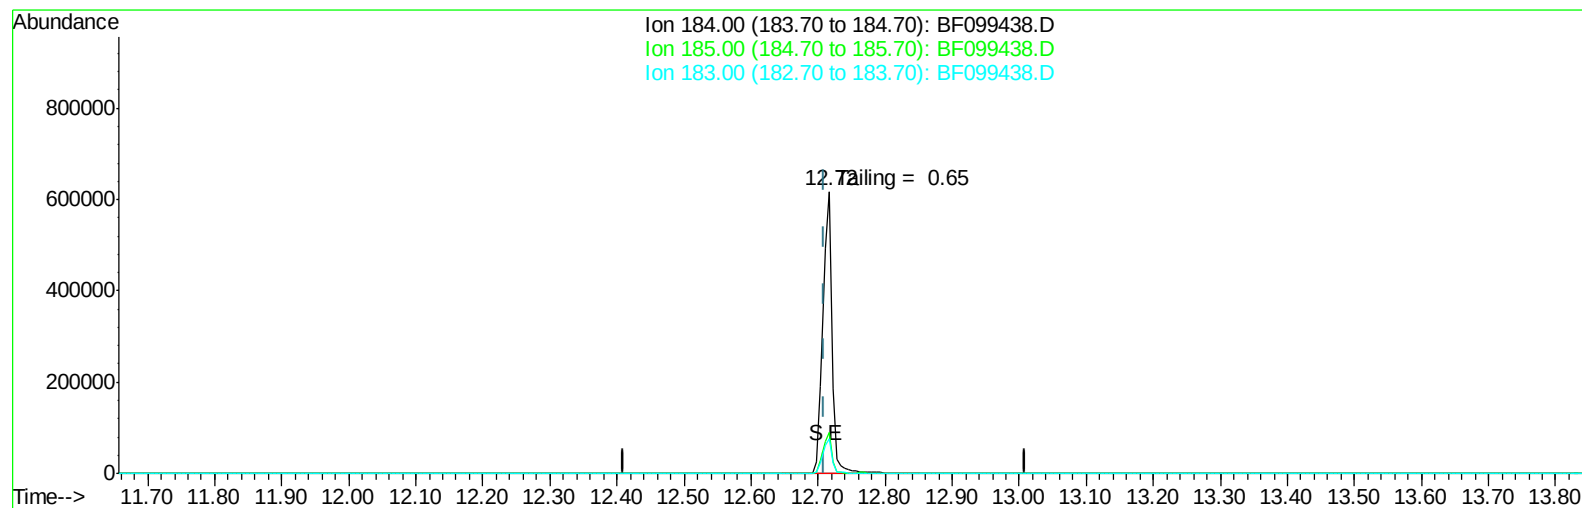

TIC: BF099438.D

(76) Benzidine

12.716min (+0.006) 15081.32ng

response 567846

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.34
183.00	11.60	12.11
0.00	0.00	0.00