
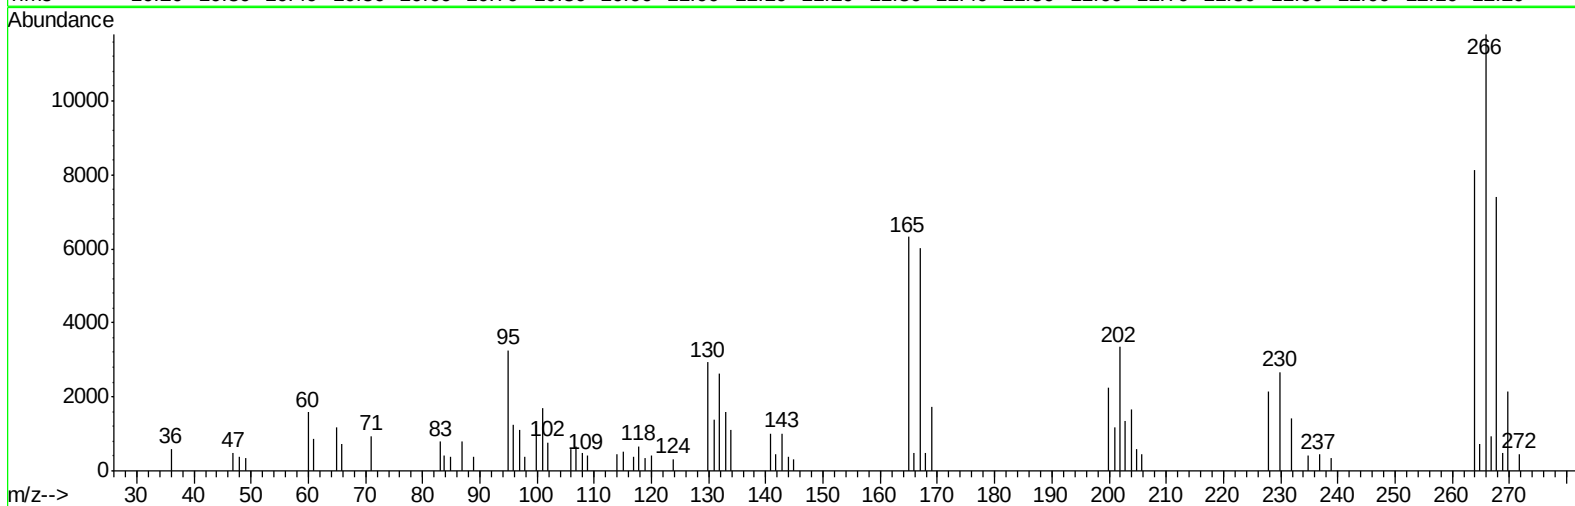


Data Path : Z:\HPCHEM1\BNA F\DATA\BF101317\
Data File : BF099463.D
Acq On : 14 Oct 2017 2:45
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 14 04:16:07 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 11 16:25:21 2017
Response via : Initial Calibration

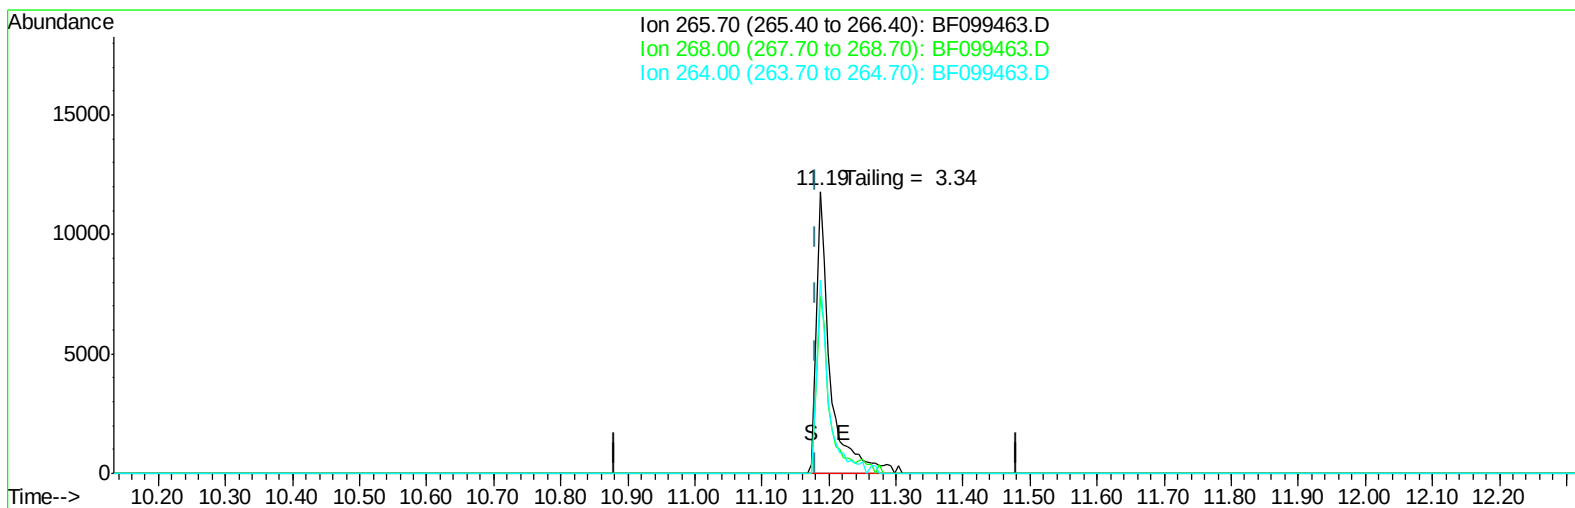

TIC: BF099463.D

(69) Pentachlorophenol (C)



11.186min (+0.006) 20537.20ng

response 16302

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.83
264.00	61.90	68.86
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101317\
Data File : BF099463.D
Acq On : 14 Oct 2017 2:45
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 14 04:16:07 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 11 16:25:21 2017
Response via : Initial Calibration

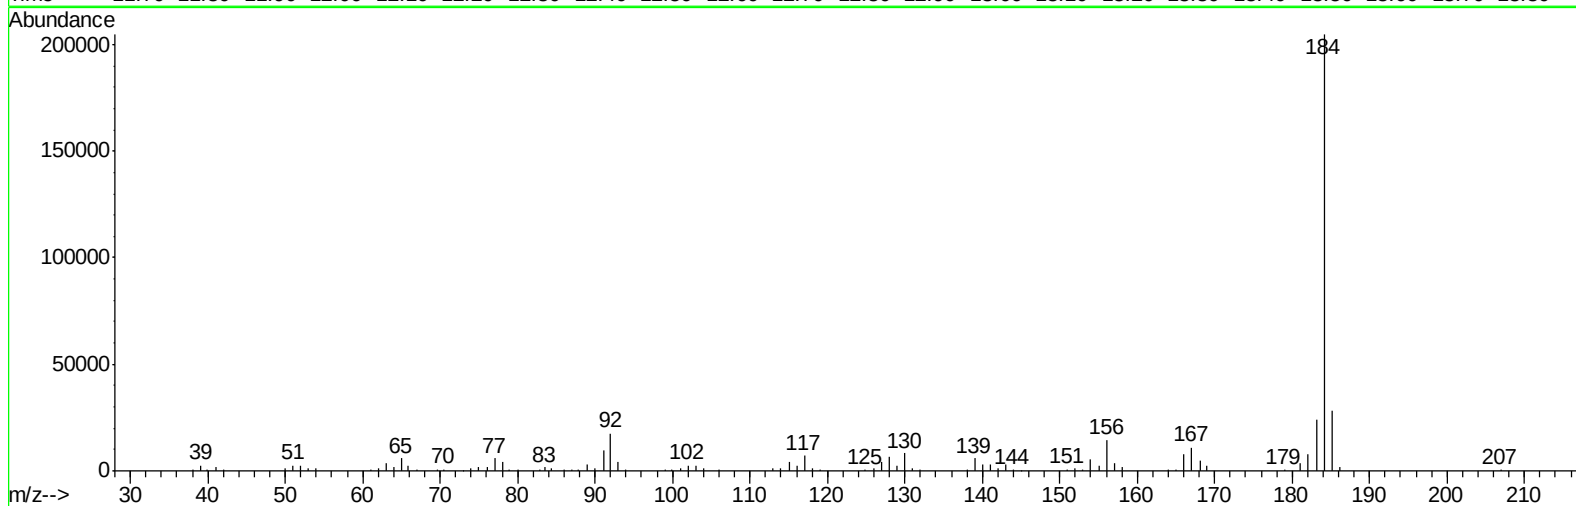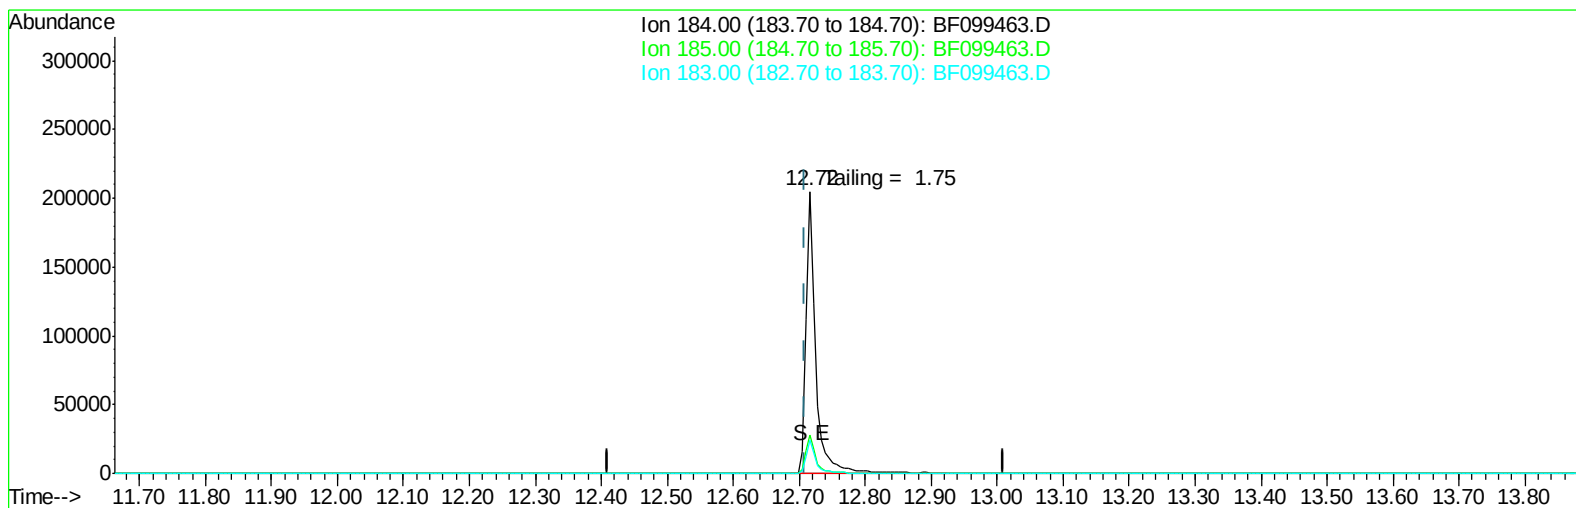

TIC: BF099463.D

(76) Benzidine

12.716min (+0.006) 0.00ng

response 212289

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.69
183.00	11.60	11.77
0.00	0.00	0.00