

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101317\
 Data File : BF099452.D
 Acq On : 13 Oct 2017 21:08
 Operator : SJ/JU
 Sample : I5819-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 3904-PP2

Quant Time: Oct 13 23:39:53 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 11 16:25:21 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.85	152	86855	20.00	ng	0.00
21) Naphthalene-d8	8.13	136	328888	20.00	ng	0.00
38) Acenaphthene-d10	9.89	164	126771	20.00	ng	0.00
63) Phenanthrene-d10	11.37	188	183716	20.00	ng	0.00
75) Chrysene-d12	14.02	240	144910	20.00	ng	0.00
86) Perylene-d12	15.49	264	165818	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.47	112	393915	72.20	ng	0.00
7) Phenol-d6	6.48	99	280706	41.71	ng	0.00
23) Nitrobenzene-d5	7.42	82	586210	114.31	ng	0.00
41) 2,4,6-Tribromophenol	10.68	330	149447	144.07	ng	0.00
44) 2-Fluorobiphenyl	9.21	172	1005951	132.47	ng	0.00
78) Terphenyl-d14	12.96	244	616608	96.77	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101317\
Data File : BF099452.D
Acq On : 13 Oct 2017 21:08
Operator : SJ/JU
Sample : I5819-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
3904-PP2

Quant Time: Oct 13 23:39:53 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 11 16:25:21 2017
Response via : Initial Calibration

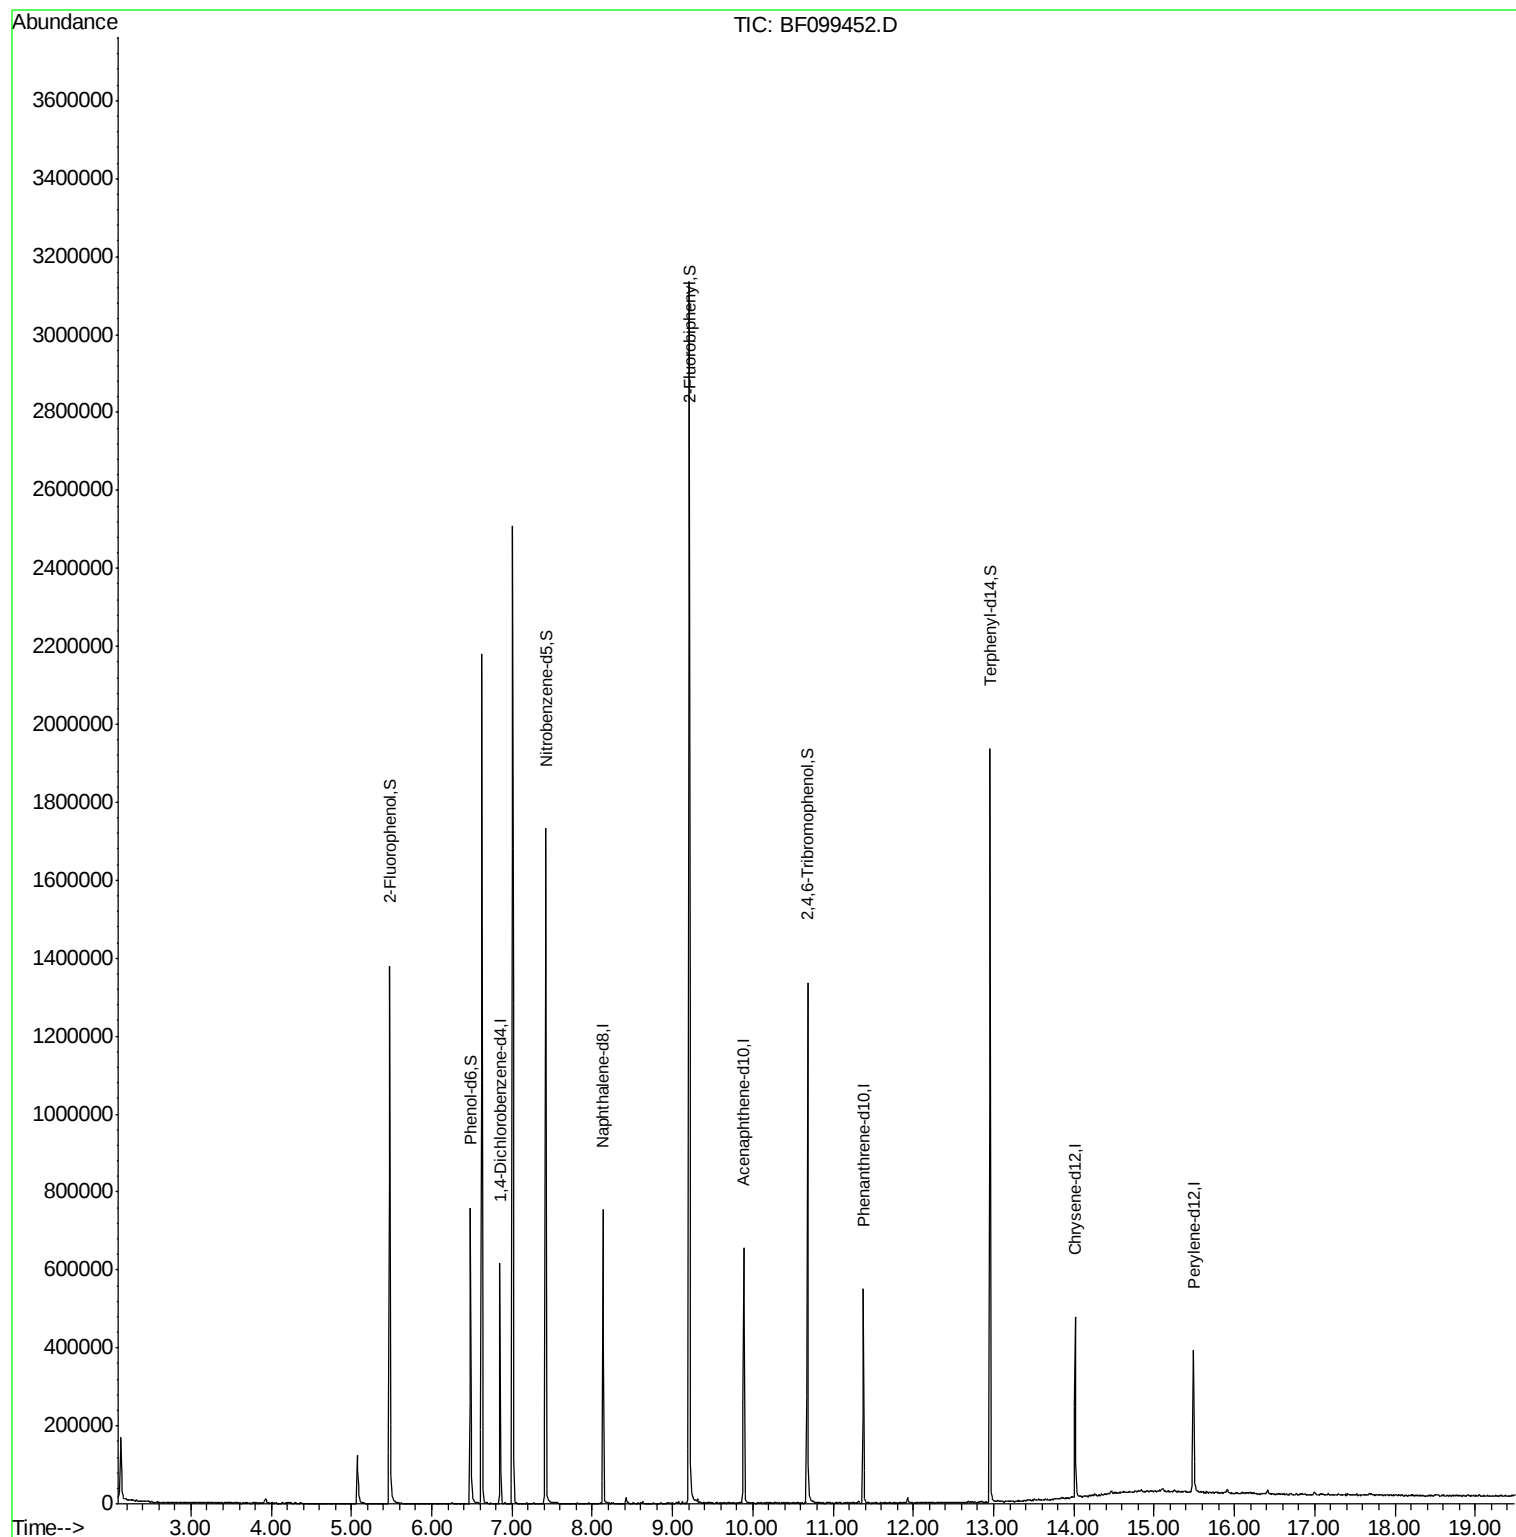

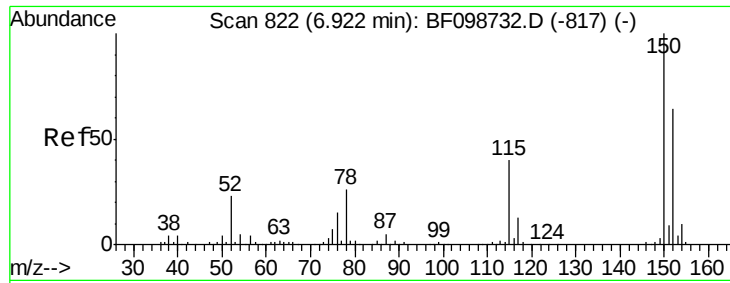

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.85 min Scan# 810

Delta R.T. -0.00 min

Lab File: BF099452.D

Acq: 13 Oct 2017 21:08

Instrument :

BNA_F

ClientSampleId :

3904-PP2


Tgt Ion:152 Resp: 86855

Ion Ratio Lower Upper

152 100

150 158.9 124.6 186.8




115 60.8 50.1 75.1



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

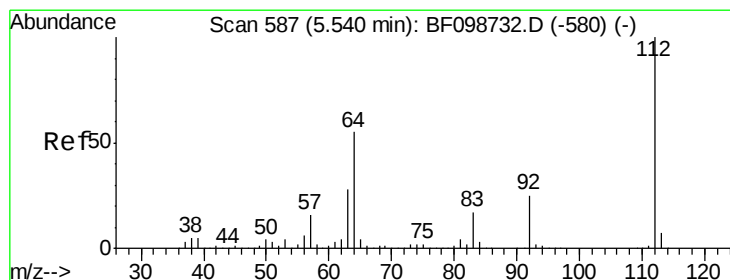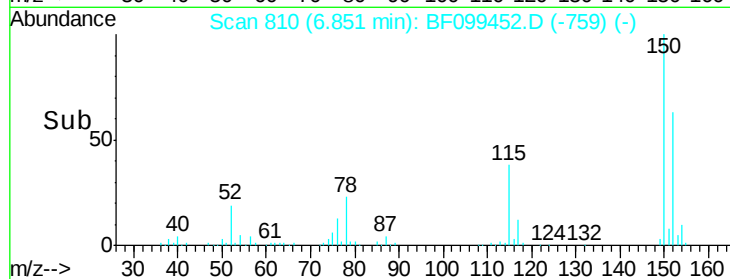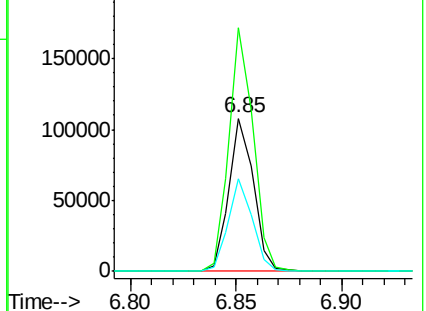

#5

2-Fluorophenol

Concen: 72.20 ng

RT: 5.47 min Scan# 576

Delta R.T. 0.01 min

Lab File: BF099452.D

Acq: 13 Oct 2017 21:08


Tgt Ion:112 Resp: 393915

Ion Ratio Lower Upper

112 100

64 54.8 47.9 71.9



63 26.6 23.7 35.5




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

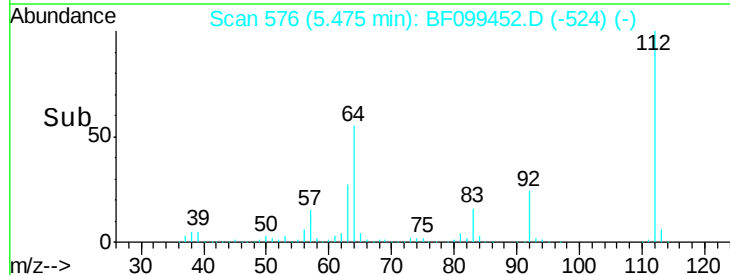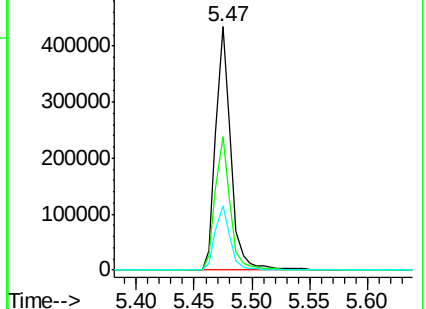

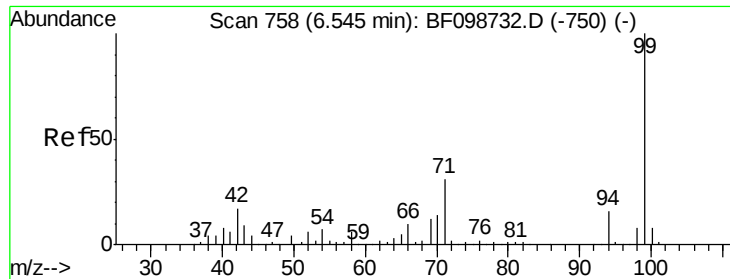

#7

Phenol-d6

Concen: 41.71 ng

RT: 6.48 min Scan# 747

Delta R.T. -0.01 min

Lab File: BF099452.D

Acq: 13 Oct 2017 21:08

Instrument :

BNA_F

ClientSampleId :

3904-PP2


Tgt Ion: 99 Resp: 280706

Ion Ratio Lower Upper

99 100

42 15.9 14.5 21.7




71 31.0 25.4 38.0

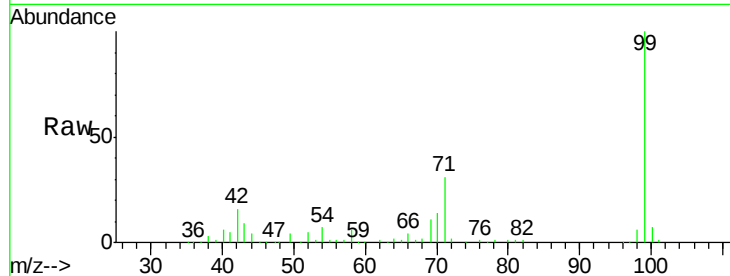

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

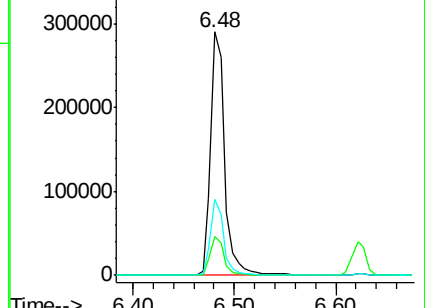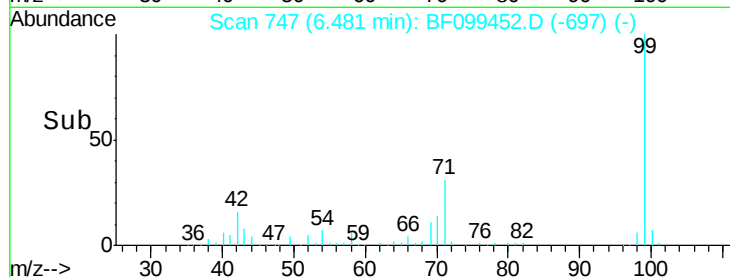

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.13 min Scan# 1028

Delta R.T. -0.00 min

Lab File: BF099452.D

Acq: 13 Oct 2017 21:08

Tgt Ion: 136 Resp: 328888


Ion Ratio Lower Upper

136 100

137 10.9 8.9 13.3

54 7.0 6.6 9.8

68 6.0 5.0 7.4






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

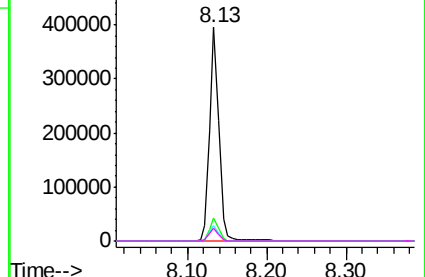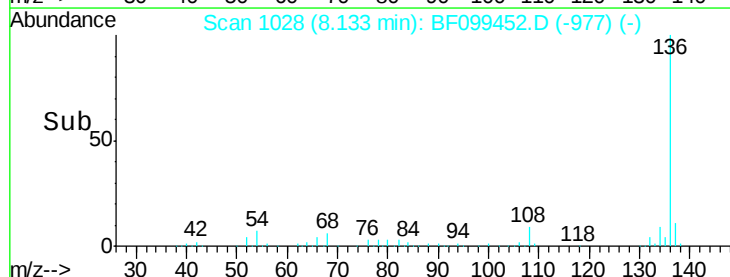

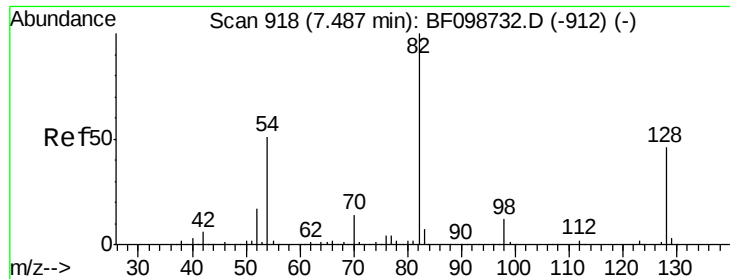

#23

Nitrobenzene-d5

Concen: 114.31 ng

RT: 7.42 min Scan# 907

Delta R.T. -0.00 min

Lab File: BF099452.D

Acq: 13 Oct 2017 21:08

Instrument :

BNA_F

ClientSampleId :

3904-PP2


Tgt Ion: 82 Resp: 586210

Ion Ratio Lower Upper




82 100

128 49.6 36.1 54.1

54 46.1 41.4 62.2

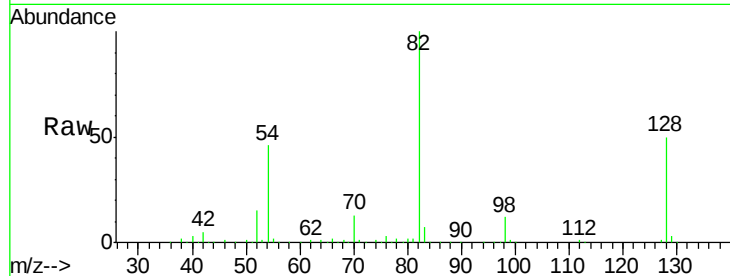

Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): B
Ion 54.00 (53.70 to 54.70): BF0

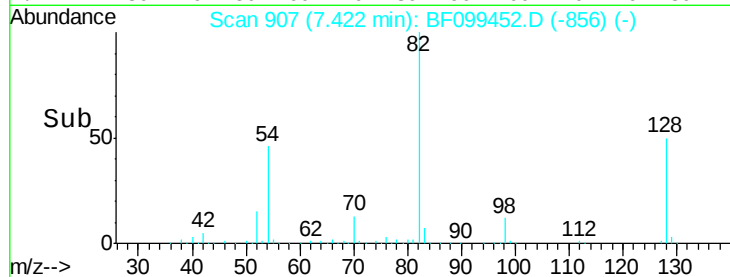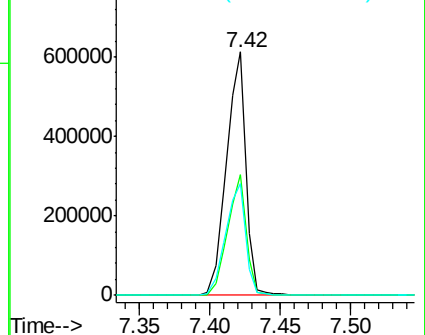

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.89 min Scan# 1326

Delta R.T. -0.01 min

Lab File: BF099452.D

Acq: 13 Oct 2017 21:08


Tgt Ion: 164 Resp: 126771

Ion Ratio Lower Upper



164 100


162 103.4 86.1 129.1

160 45.5 38.3 57.5



Abundance Ion 164.00 (163.70 to 164.70): B
Ion 162.00 (161.70 to 162.70): B
Ion 160.00 (159.70 to 160.70): B

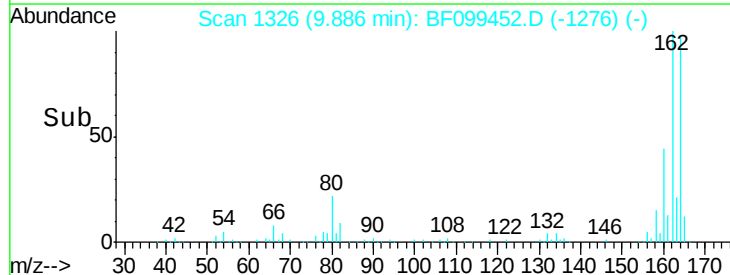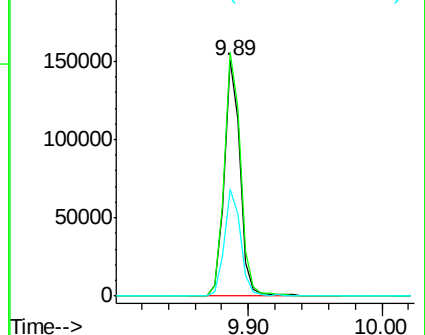


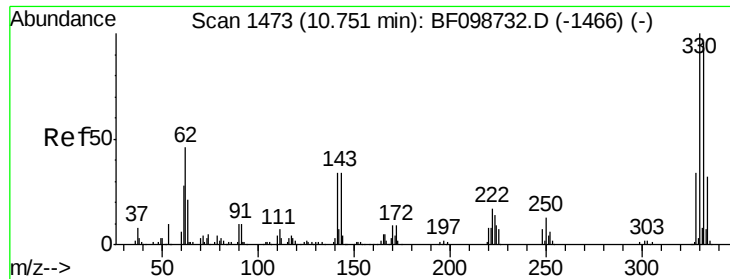




#41
 2,4,6-Tribromophenol
 Concen: 144.07 ng
 RT: 10.68 min Scan# 1461
 Delta R.T. -0.00 min
 Lab File: BF099452.D
 Acq: 13 Oct 2017 21:08

Instrument :
 BNA_F
 ClientSampleId :
 3904-PP2

Tgt Ion:330 Resp: 149447
 Ion Ratio Lower Upper
 330 100
 332 95.0 77.0 115.6
 141 39.3 29.9 44.9




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

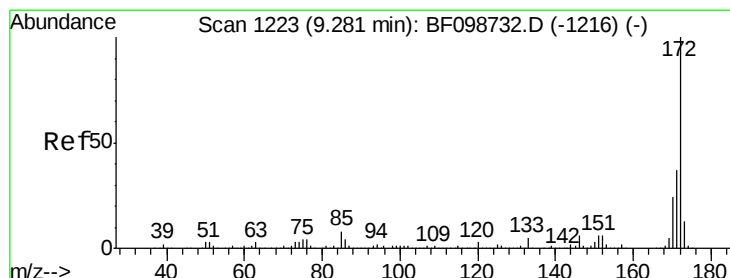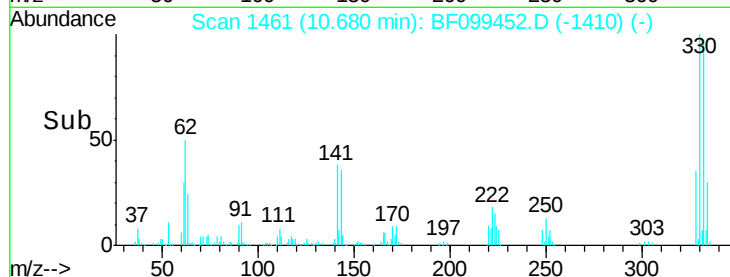
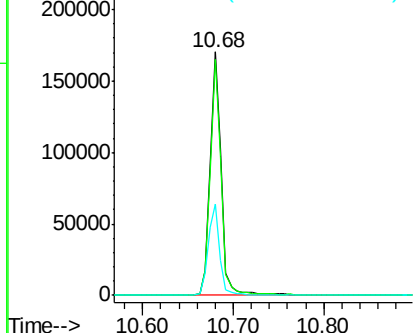



#44
 2-Fluorobiphenyl
 Concen: 132.47 ng
 RT: 9.21 min Scan# 1211
 Delta R.T. -0.00 min
 Lab File: BF099452.D
 Acq: 13 Oct 2017 21:08

Tgt Ion:172 Resp: 1005951
 Ion Ratio Lower Upper
 172 100
 171 36.7 29.7 44.5
 170 24.2 19.6 29.4



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



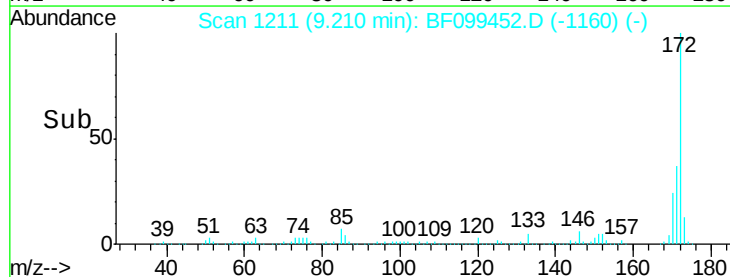
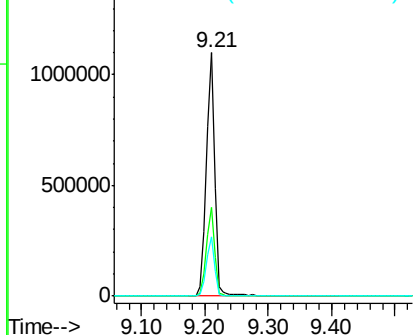


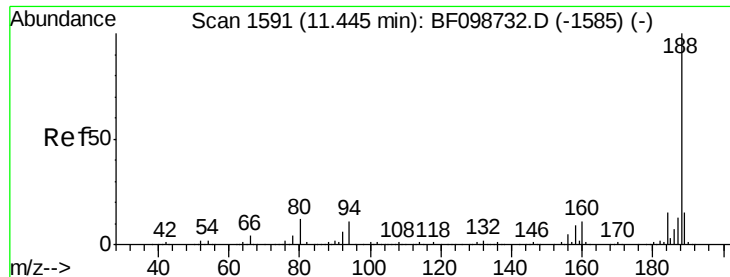

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.37 min Scan# 1579
Delta R.T. -0.00 min
Lab File: BF099452.D
Acq: 13 Oct 2017 21:08




Instrument :
BNA_F
ClientSampleId :
3904-PP2


Tgt Ion:188 Resp: 183716
Ion Ratio Lower Upper
188 100
94 10.8 8.5 12.7
80 11.9 9.2 13.8

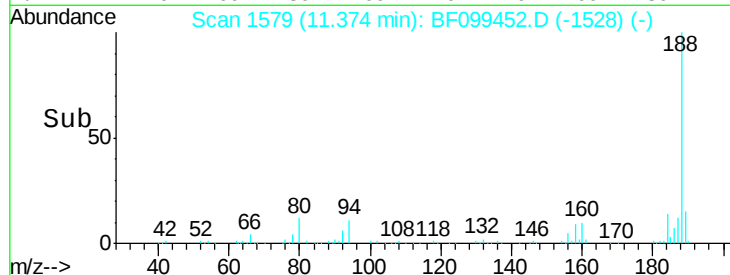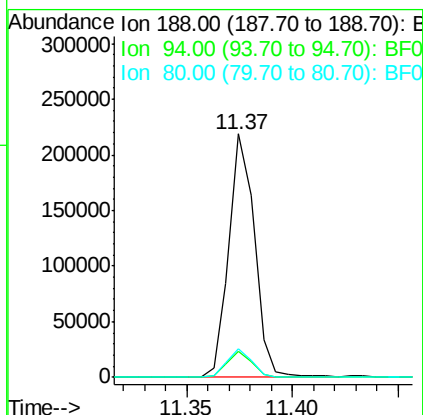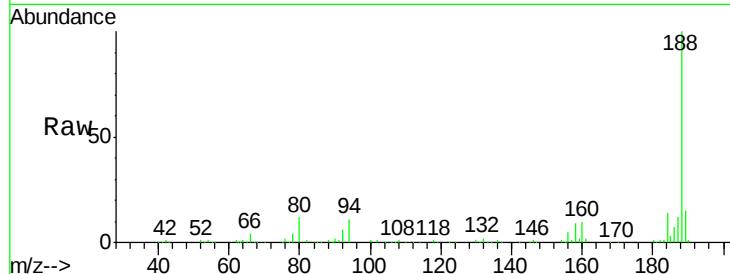

#75
Chrysene-d12
Concen: 20.00 ng
RT: 14.02 min Scan# 2028
Delta R.T. -0.00 min
Lab File: BF099452.D
Acq: 13 Oct 2017 21:08

Tgt Ion:240 Resp: 144910
Ion Ratio Lower Upper
240 100
120 16.2 9.5 14.3#
236 25.4 20.7 31.1


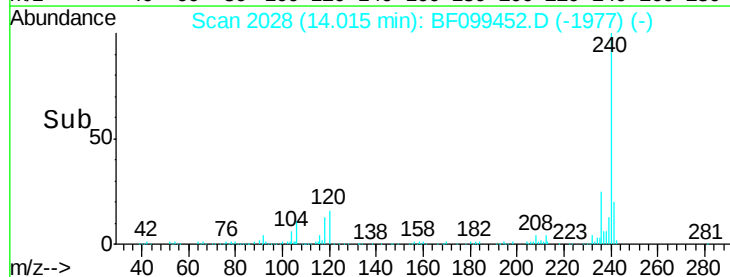
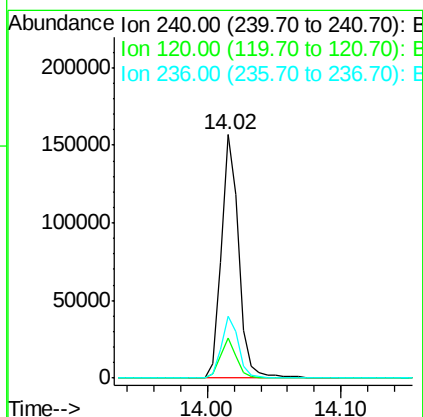
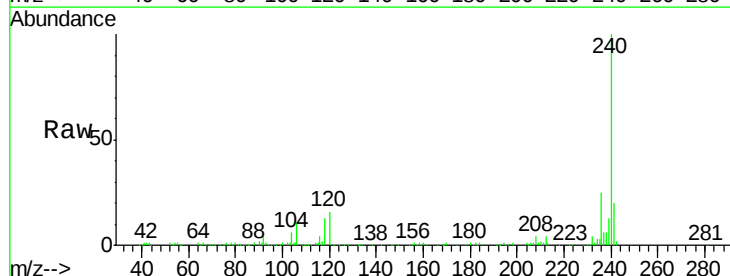


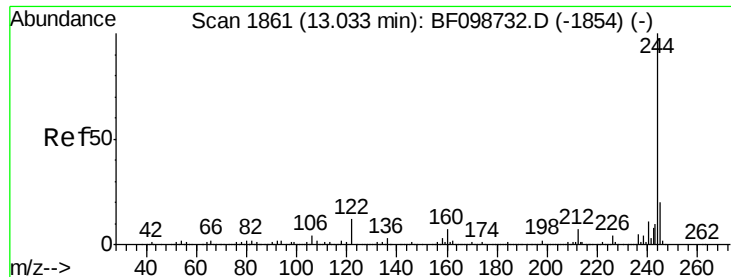

#78
 Terphenyl-d14
 Concen: 96.77 ng
 RT: 12.96 min Scan# 1848
 Delta R.T. -0.00 min
 Lab File: BF099452.D
 Acq: 13 Oct 2017 21:08

Instrument :
 BNA_F
 ClientSampleId :
 3904-PP2

Tgt Ion:244 Resp: 616608
 Ion Ratio Lower Upper
 244 100
 212 7.3 5.4 8.0
 122 15.0 11.0 16.4

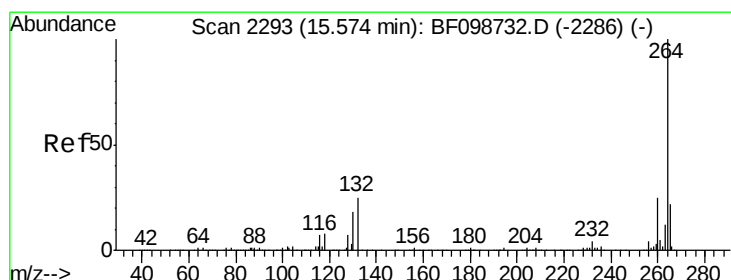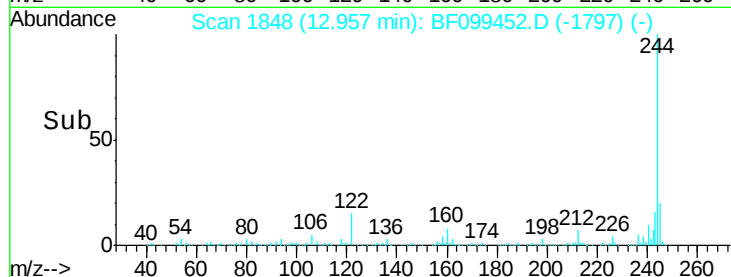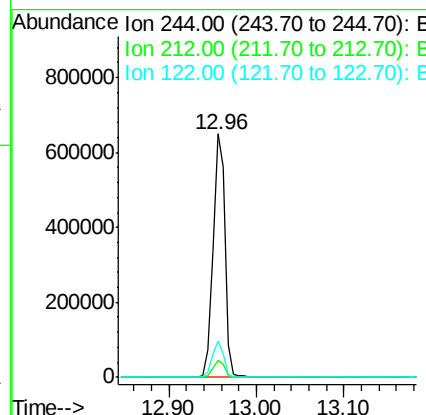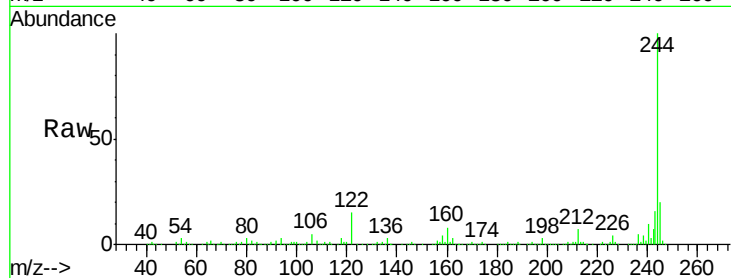

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.49 min Scan# 2279
 Delta R.T. 0.01 min
 Lab File: BF099452.D
 Acq: 13 Oct 2017 21:08

Tgt Ion:264 Resp: 165818
 Ion Ratio Lower Upper
 264 100
 260 24.3 19.2 28.8
 265 21.7 17.5 26.3

