

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101317\
 Data File : BF099457.D
 Acq On : 13 Oct 2017 23:29
 Operator : SJ/JU
 Sample : I5819-08
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 3909-SPP2-DUP

Quant Time: Oct 14 00:11:00 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 11 16:25:21 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.85	152	96328	20.00	ng	0.00
21) Naphthalene-d8	8.13	136	368355	20.00	ng	0.00
38) Acenaphthene-d10	9.89	164	145565	20.00	ng	0.00
63) Phenanthrene-d10	11.37	188	207117	20.00	ng	0.00
75) Chrysene-d12	14.02	240	166946	20.00	ng	0.00
86) Perylene-d12	15.49	264	187654	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.47	112	449953	74.36	ng	0.00
7) Phenol-d6	6.49	99	329413	44.13	ng	0.00
23) Nitrobenzene-d5	7.42	82	656576	114.31	ng	0.00
41) 2,4,6-Tribromophenol	10.68	330	173336	145.52	ng	0.00
44) 2-Fluorobiphenyl	9.21	172	1098186	125.95	ng	0.00
78) Terphenyl-d14	12.96	244	704205	95.93	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101317\
Data File : BF099457.D
Acq On : 13 Oct 2017 23:29
Operator : SJ/JU
Sample : I5819-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
3909-SPP2-DUP

Quant Time: Oct 14 00:11:00 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 11 16:25:21 2017
Response via : Initial Calibration

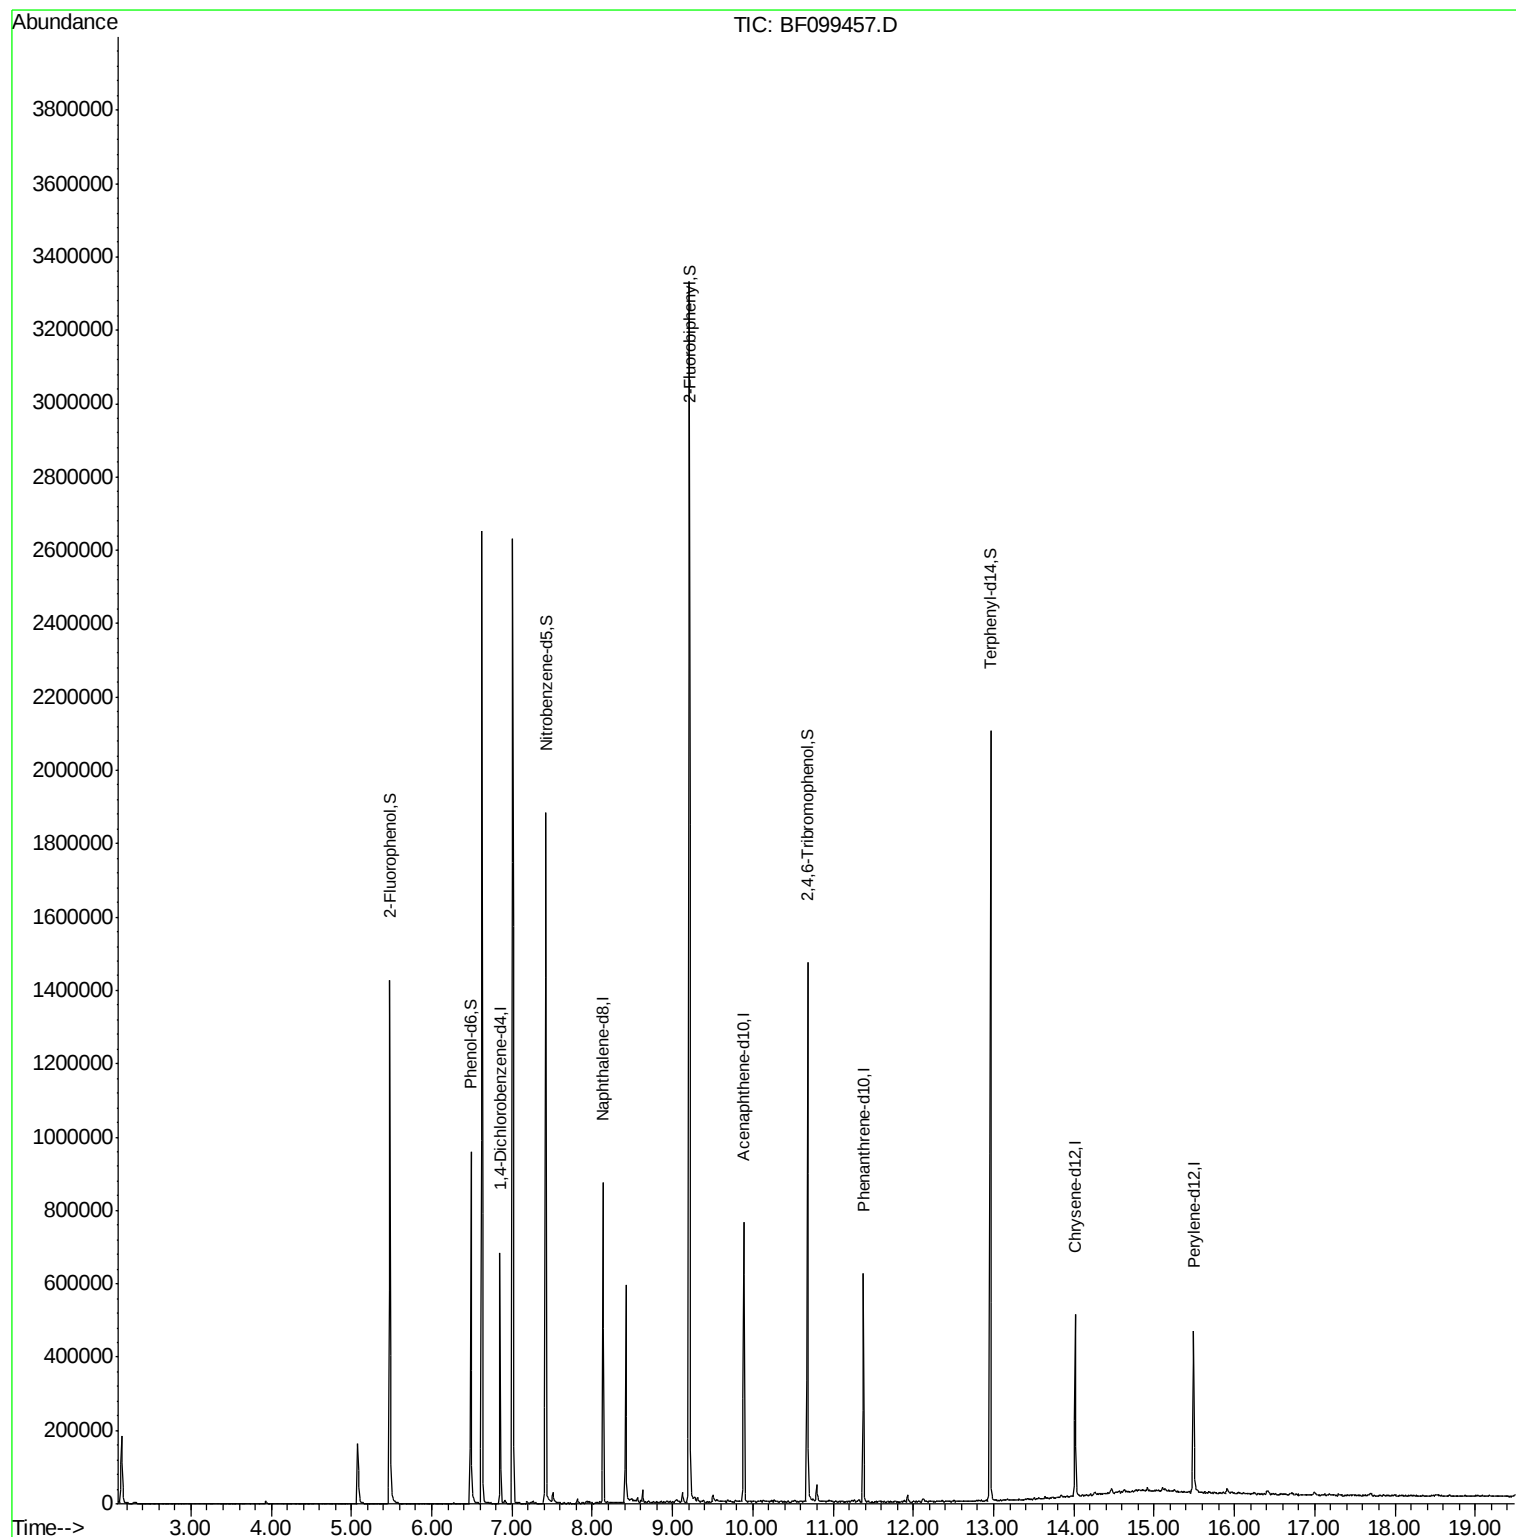


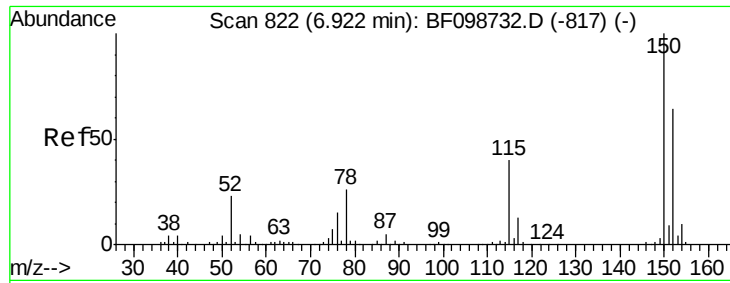




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 6.85 min Scan# 810
 Delta R.T. 0.00 min
 Lab File: BF099457.D
 Acq: 13 Oct 2017 23:29

Instrument :
 BNA_F
 ClientSampleId :
 3909-SPP2-DUP

Tgt Ion:152 Resp: 96328
 Ion Ratio Lower Upper
 152 100
 150 158.4 124.6 186.8
 115 60.2 50.1 75.1

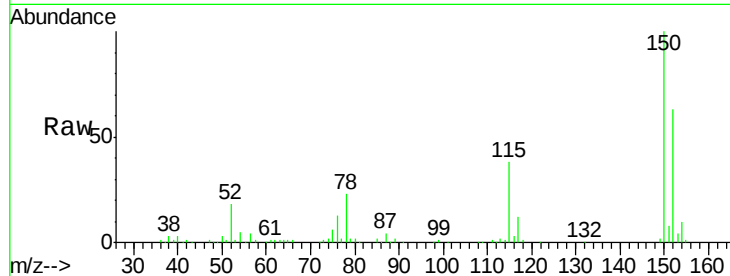


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

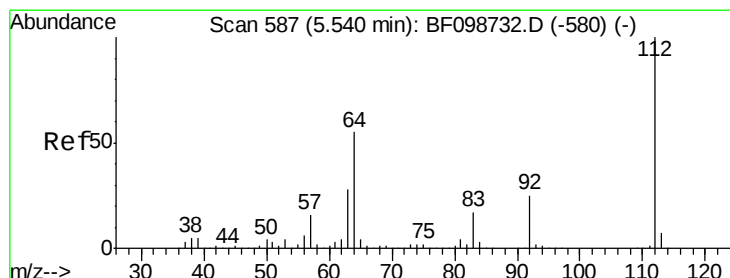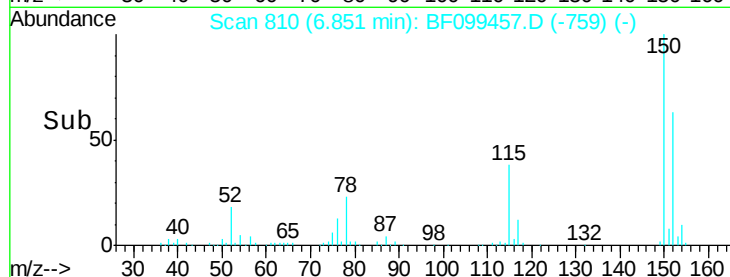
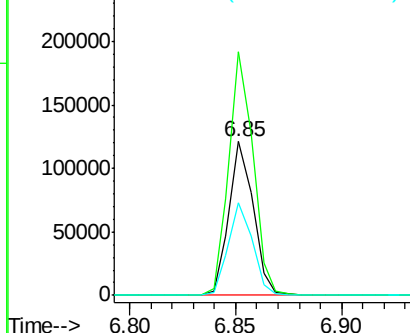



#5
 2-Fluorophenol
 Concen: 74.36 ng
 RT: 5.47 min Scan# 576
 Delta R.T. 0.01 min
 Lab File: BF099457.D
 Acq: 13 Oct 2017 23:29

Tgt Ion:112 Resp: 449953
 Ion Ratio Lower Upper
 112 100
 64 56.7 47.9 71.9
 63 27.3 23.7 35.5

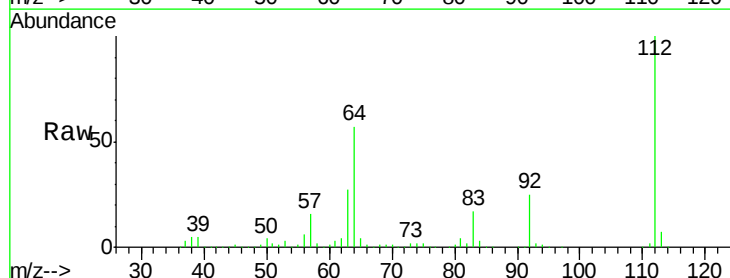

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

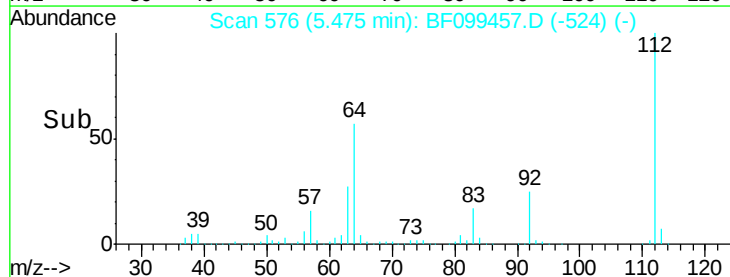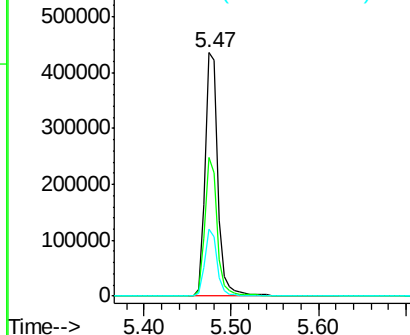

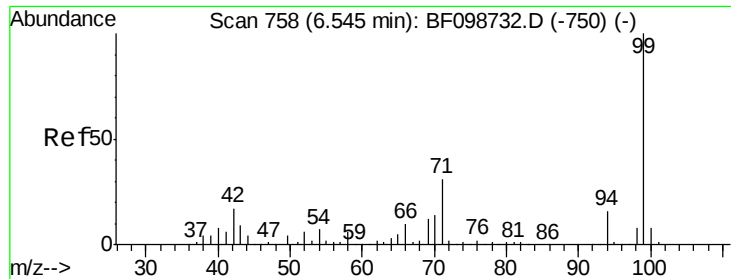

#7

Phenol-d6

Concen: 44.13 ng

RT: 6.49 min Scan# 748

Delta R.T. 0.00 min

Lab File: BF099457.D

Acq: 13 Oct 2017 23:29

Instrument :

BNA_F

ClientSampleId :

3909-SPP2-DUP


Tgt Ion: 99 Resp: 329413

Ion Ratio Lower Upper

99 100

42 15.1 14.5 21.7




71 29.9 25.4 38.0

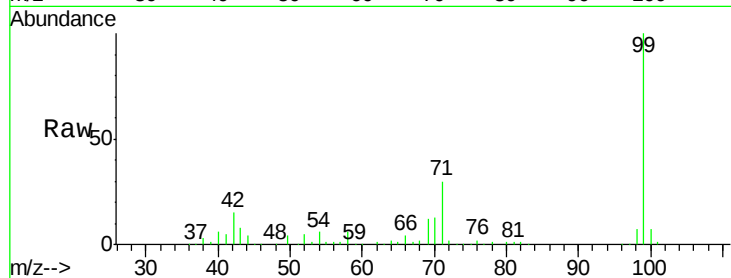

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

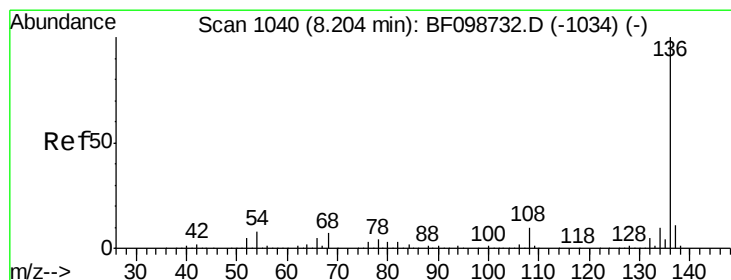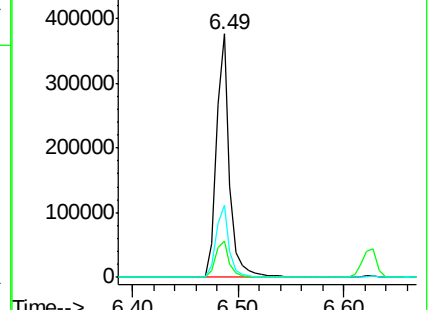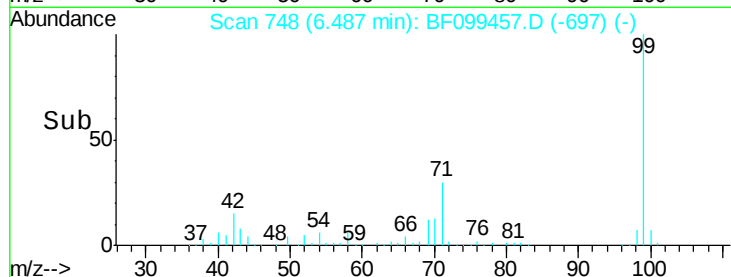

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.13 min Scan# 1028

Delta R.T. 0.00 min

Lab File: BF099457.D

Acq: 13 Oct 2017 23:29

Tgt Ion: 136 Resp: 368355


Ion Ratio Lower Upper

136 100

137 10.9 8.9 13.3

54 7.1 6.6 9.8

68 5.7 5.0 7.4


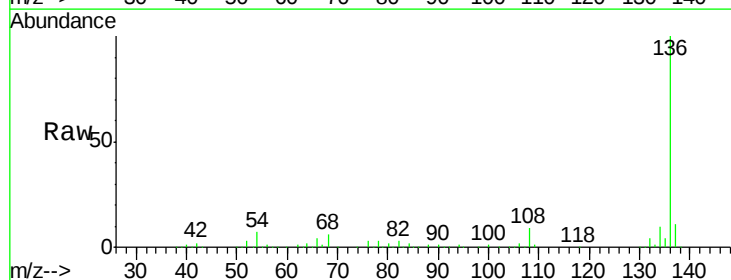



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



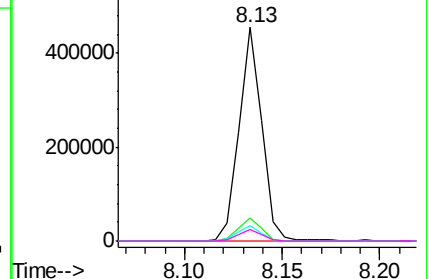
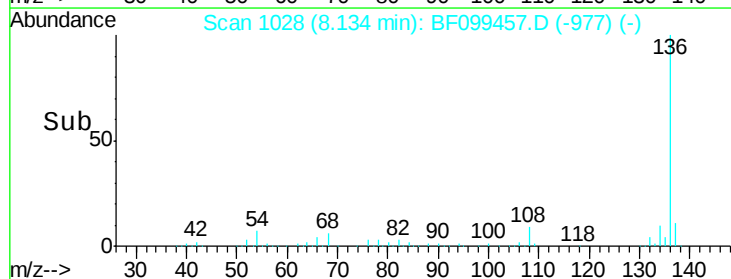


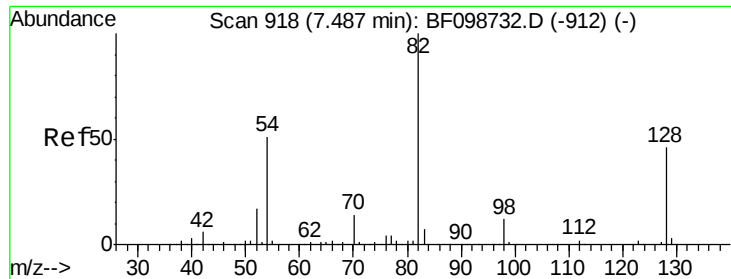

#23
 Nitrobenzene-d5
 Concen: 114.31 ng
 RT: 7.42 min Scan# 907
 Delta R.T. 0.00 min
 Lab File: BF099457.D
 Acq: 13 Oct 2017 23:29




Instrument :
 BNA_F
 ClientSampleId :
 3909-SPP2-DUP


Tgt Ion: 82 Resp: 656576
 Ion Ratio Lower Upper
 82 100
 128 48.1 36.1 54.1
 54 46.2 41.4 62.2

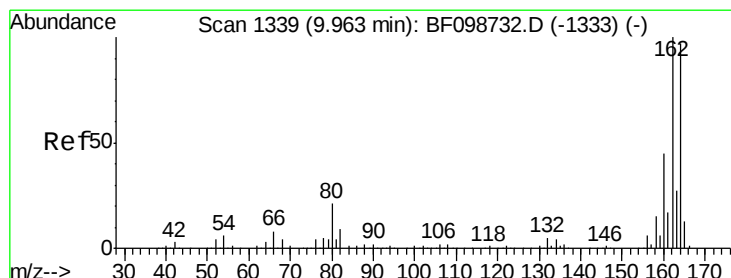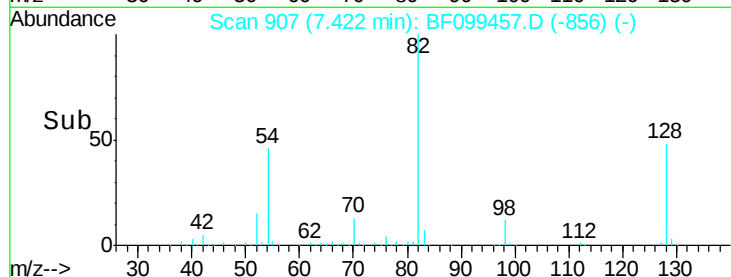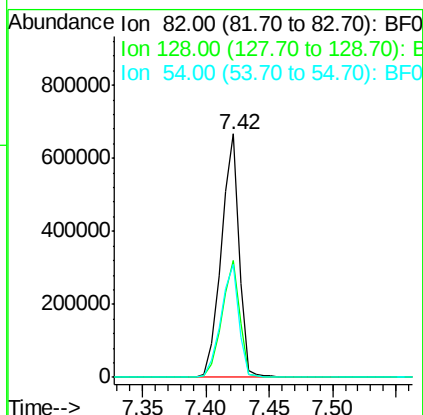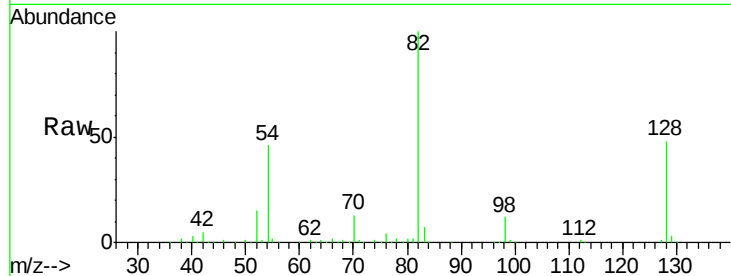

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.89 min Scan# 1326
 Delta R.T. -0.01 min
 Lab File: BF099457.D
 Acq: 13 Oct 2017 23:29

Tgt Ion:164 Resp: 145565
 Ion Ratio Lower Upper
 164 100
 162 103.4 86.1 129.1
 160 45.9 38.3 57.5


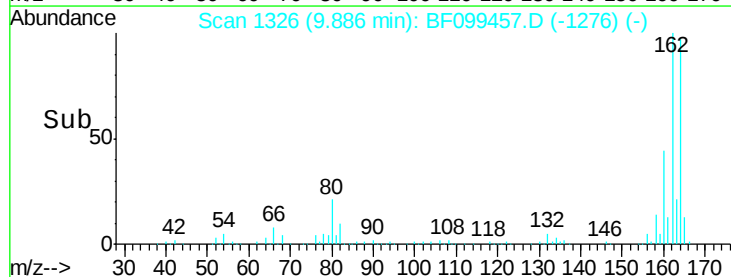
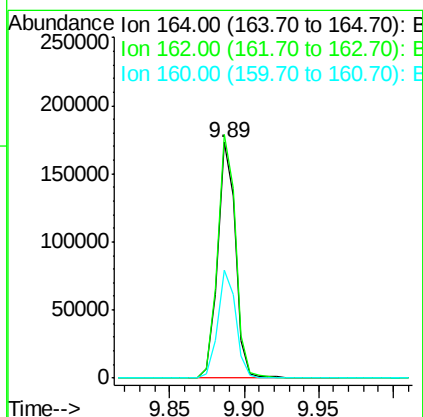
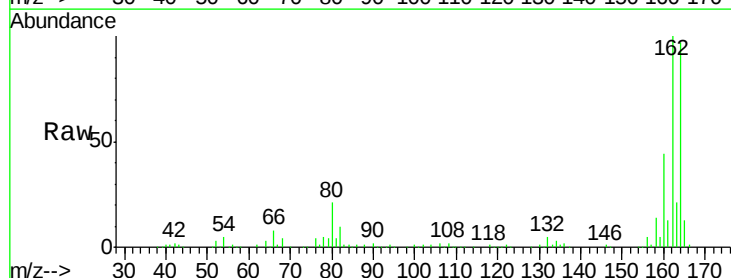


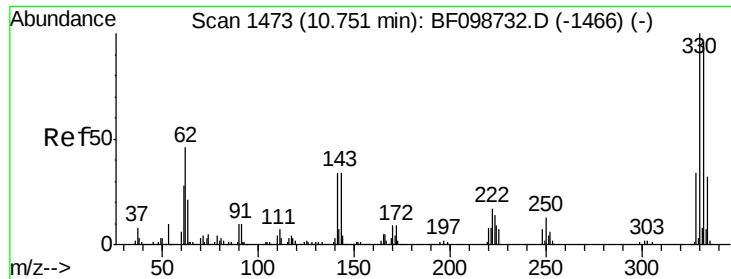

#41
 2,4,6-Tribromophenol
 Concen: 145.52 ng
 RT: 10.68 min Scan# 1461
 Delta R.T. 0.00 min
 Lab File: BF099457.D
 Acq: 13 Oct 2017 23:29




Instrument :
 BNA_F
 ClientSampleId :
 3909-SPP2-DUP


Tgt Ion	Ratio	Lower	Upper
330	100		
332	97.3	77.0	115.6
141	39.5	29.9	44.9

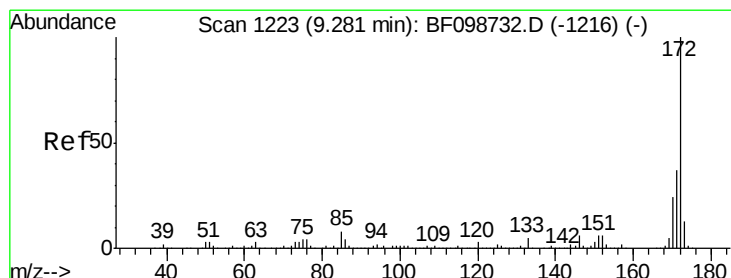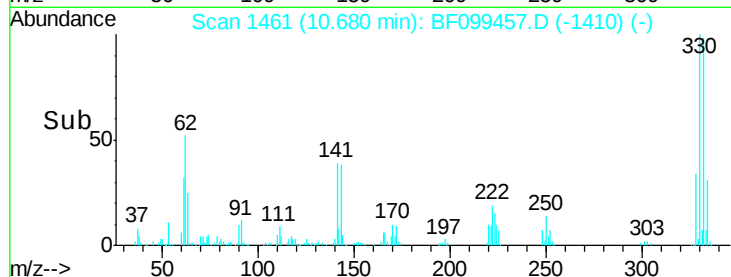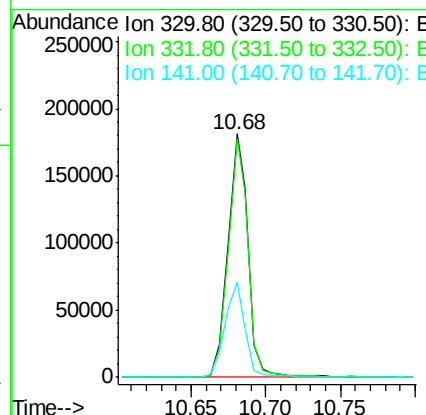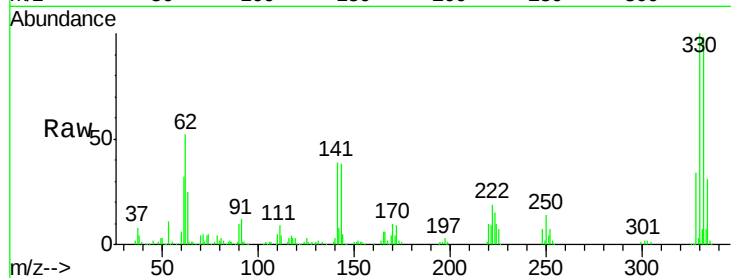

#44
 2-Fluorobiphenyl
 Concen: 125.95 ng
 RT: 9.21 min Scan# 1211
 Delta R.T. 0.00 min
 Lab File: BF099457.D
 Acq: 13 Oct 2017 23:29

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.9	29.7	44.5
170	24.0	19.6	29.4


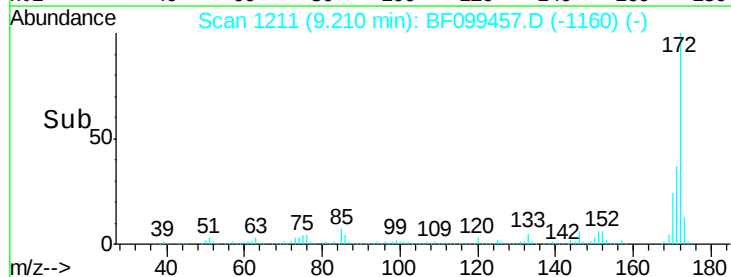
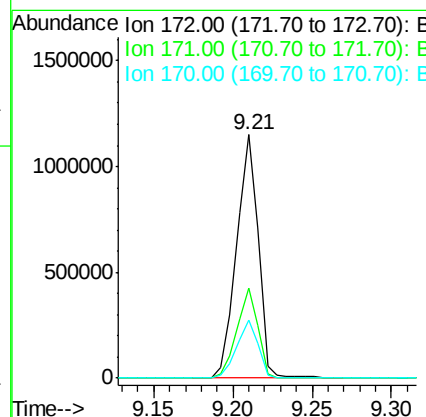
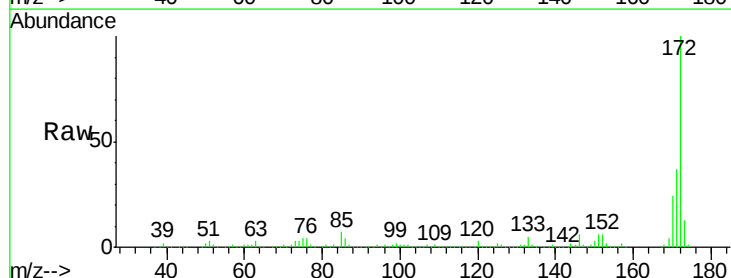


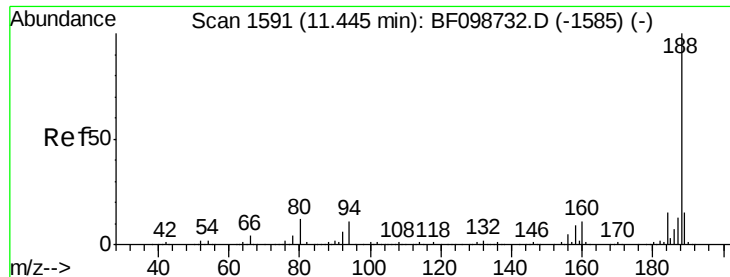

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.37 min Scan# 1579
Delta R.T. 0.00 min
Lab File: BF099457.D
Acq: 13 Oct 2017 23:29




Instrument :
BNA_F
ClientSampleId :
3909-SPP2-DUP


Tgt Ion:188 Resp: 207117
Ion Ratio Lower Upper
188 100
94 11.1 8.5 12.7
80 11.8 9.2 13.8

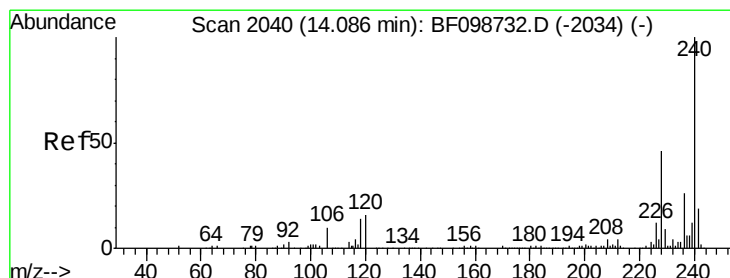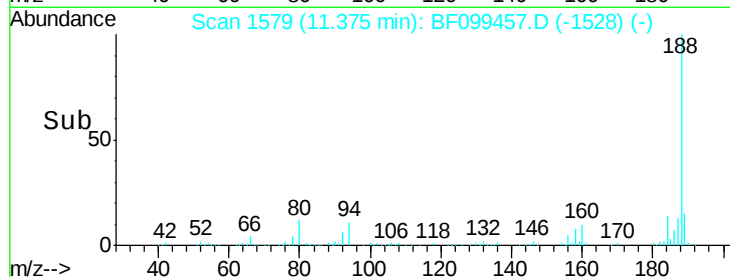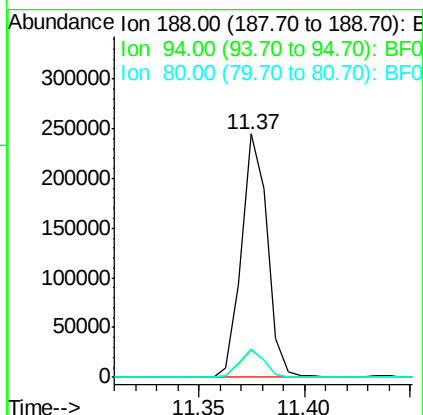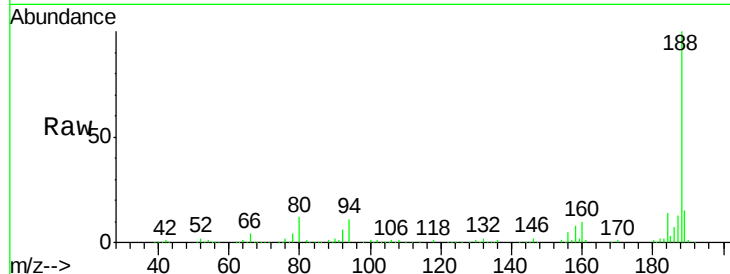

#75
Chrysene-d12
Concen: 20.00 ng
RT: 14.02 min Scan# 2028
Delta R.T. 0.00 min
Lab File: BF099457.D
Acq: 13 Oct 2017 23:29

Tgt Ion:240 Resp: 166946
Ion Ratio Lower Upper
240 100
120 15.7 9.5 14.3#
236 25.9 20.7 31.1


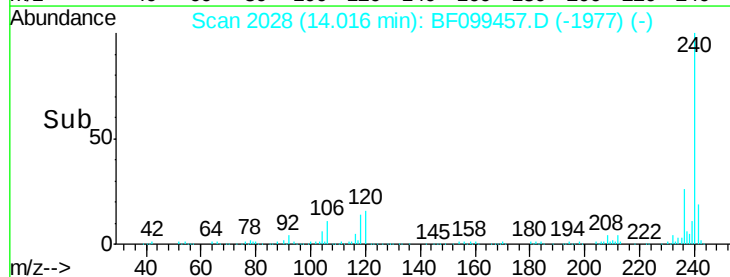
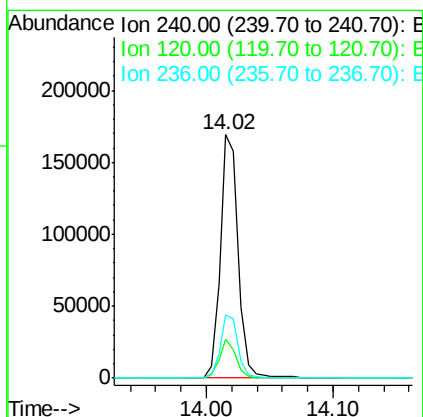
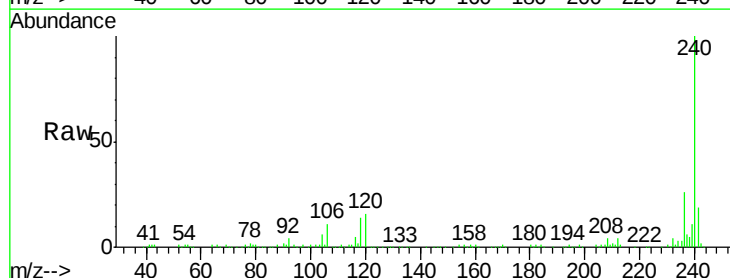


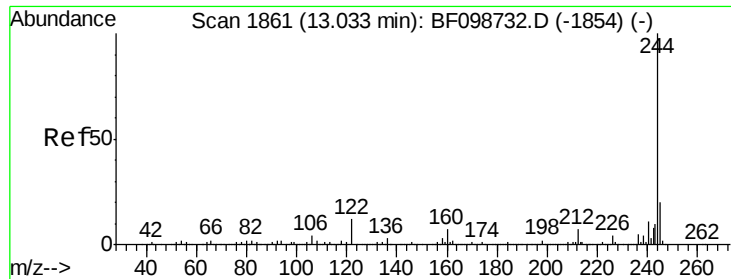

#78
 Terphenyl-d14
 Concen: 95.93 ng
 RT: 12.96 min Scan# 1849
 Delta R.T. 0.01 min
 Lab File: BF099457.D
 Acq: 13 Oct 2017 23:29

Instrument :
 BNA_F
 ClientSampleId :
 3909-SPP2-DUP

Tgt Ion: 244 Resp: 704205
 Ion Ratio Lower Upper
 244 100
 212 6.9 5.4 8.0
 122 12.7 11.0 16.4

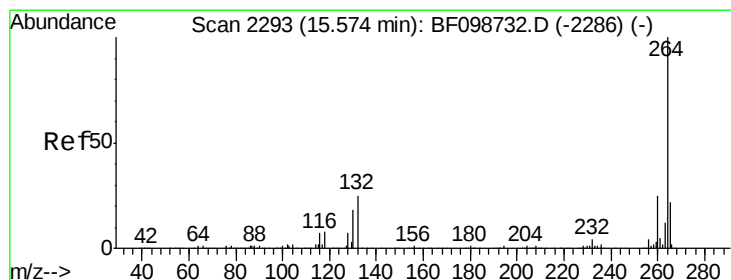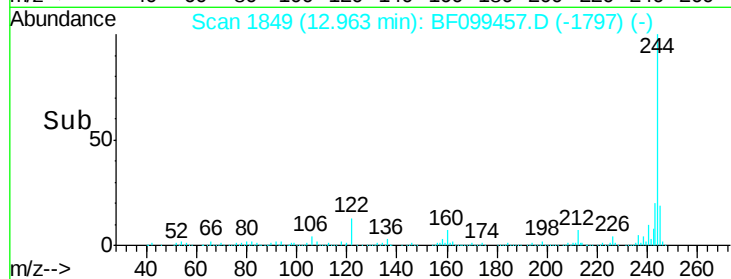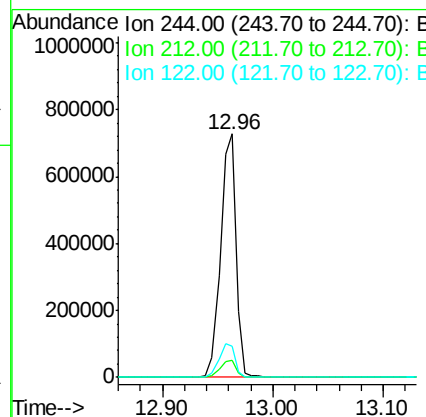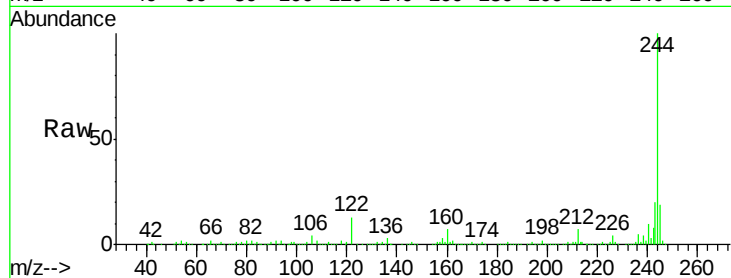

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.49 min Scan# 2279
 Delta R.T. 0.01 min
 Lab File: BF099457.D
 Acq: 13 Oct 2017 23:29

Tgt Ion: 264 Resp: 187654
 Ion Ratio Lower Upper
 264 100
 260 24.4 19.2 28.8
 265 21.6 17.5 26.3

