

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101317\
 Data File : BF099465.D
 Acq On : 14 Oct 2017 3:41
 Operator : SJ/JU
 Sample : PB103194BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB103194BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.092	507	511	527	rBV	291519	384883	16.37%	2.090%
2	5.487	574	578	596	rBV	2205573	2205157	93.79%	11.977%
3	6.492	744	749	752	rBV	2026422	2062547	87.73%	11.202%
4	6.628	768	772	775	rBV	2531817	2209000	93.95%	11.997%
5	6.851	807	810	817	rVB	681109	568054	24.16%	3.085%
6	7.010	833	837	840	rBV	2073678	1814834	77.19%	9.857%
7	7.422	902	907	910	rBV	1326991	1334849	56.77%	7.250%
8	8.133	1024	1028	1044	rBV	848737	737677	31.38%	4.006%
9	9.210	1206	1211	1214	rBV	2666917	2351126	100.00%	12.769%
10	9.886	1323	1326	1340	rVB	705993	694136	29.52%	3.770%
11	10.680	1457	1461	1476	rBV	1095610	997725	42.44%	5.419%
12	11.374	1576	1579	1588	rBV	563664	542503	23.07%	2.946%
13	12.957	1844	1848	1852	rBV	1606463	1490618	63.40%	8.096%
14	14.021	2025	2029	2041	rBV	493496	484473	20.61%	2.631%
15	15.492	2274	2279	2292	rVB2	402739	534657	22.74%	2.904%


Sum of corrected areas: 18412239

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101317\
Data File : BF099465.D
Acq On : 14 Oct 2017 3:41
Operator : SJ/JU
Sample : PB103194BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB103194BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

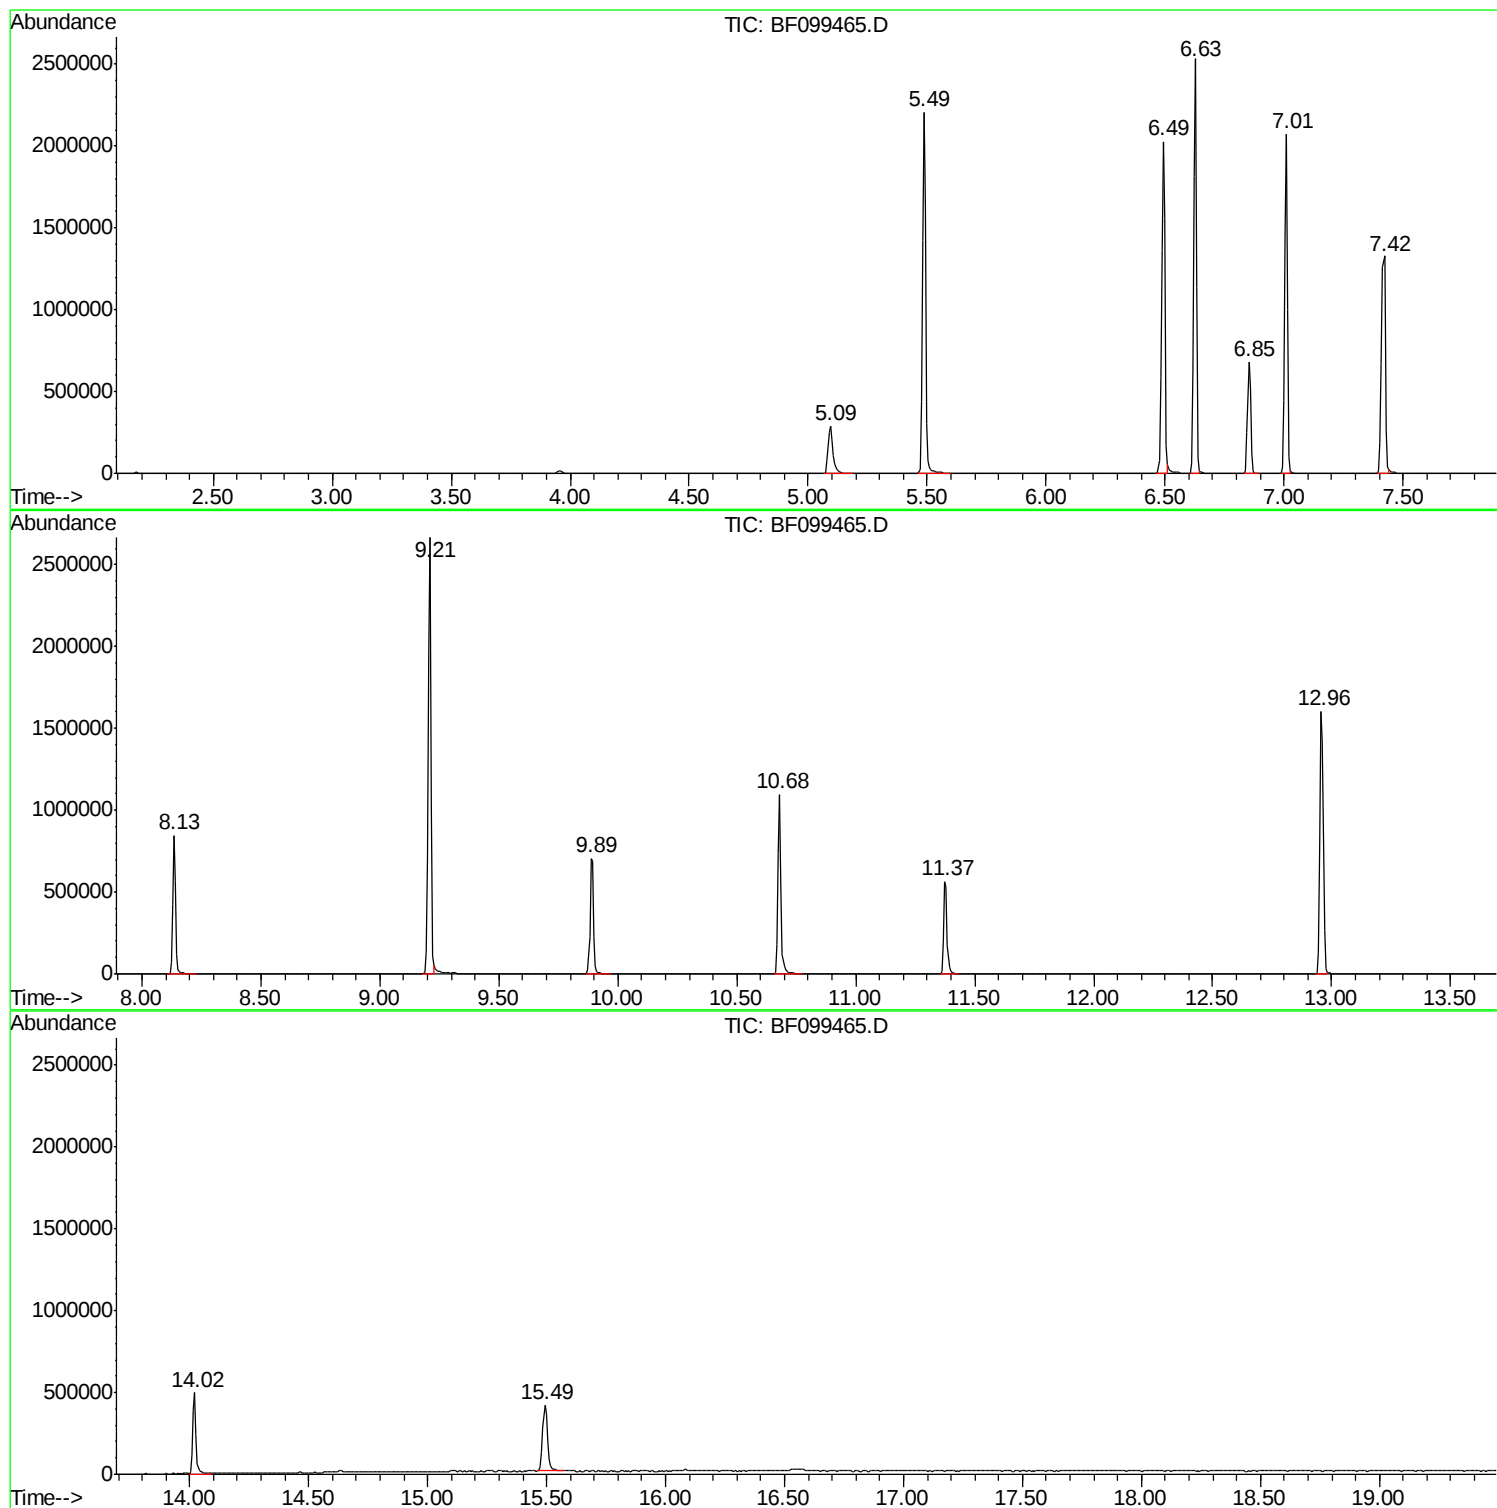

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101317\
Data File : BF099465.D
Acq On : 14 Oct 2017 3:41
Operator : SJ/JU
Sample : PB103194BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB103194BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.09	13.55 ng	384883	1,4-Dichlorobenzene-d4	6.85

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64
2		Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23
3		2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9
4		Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9
5		Acetone	58	C3H6O	000067-64-1	9

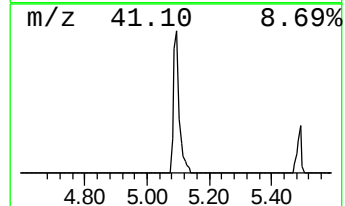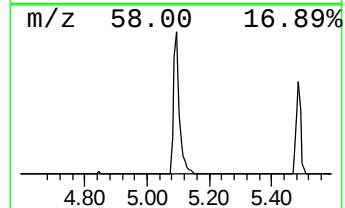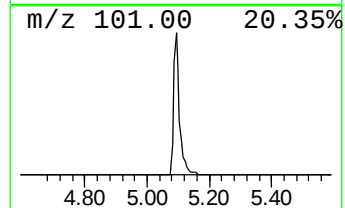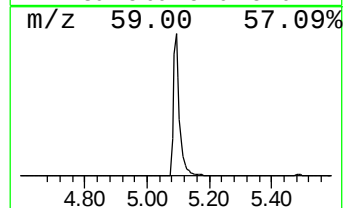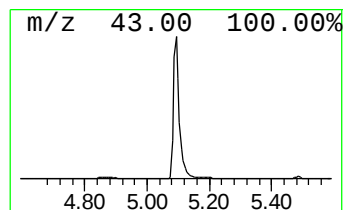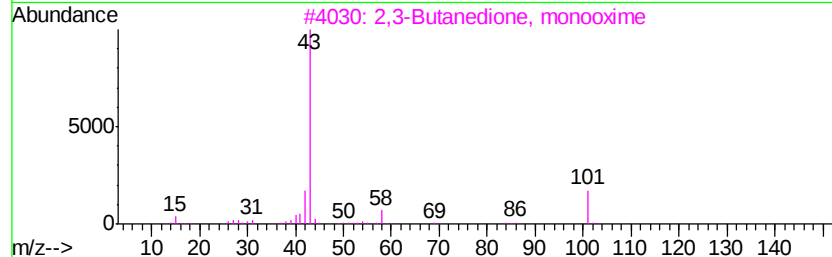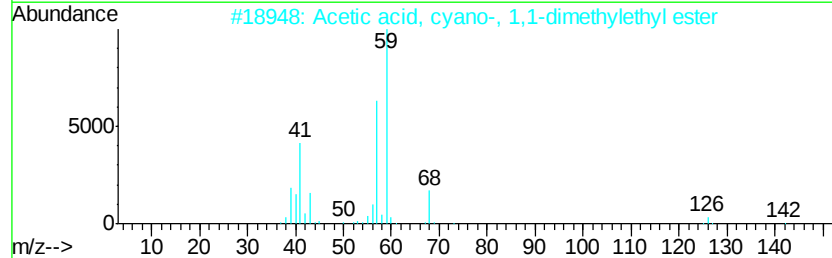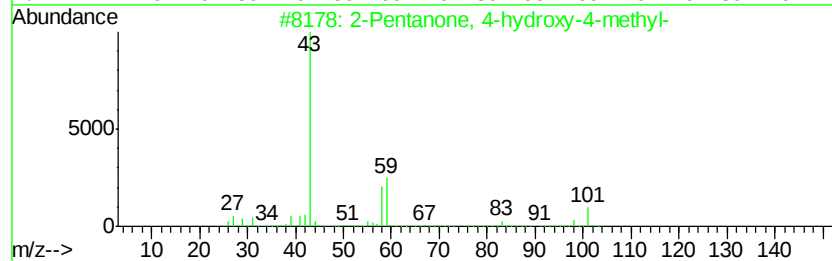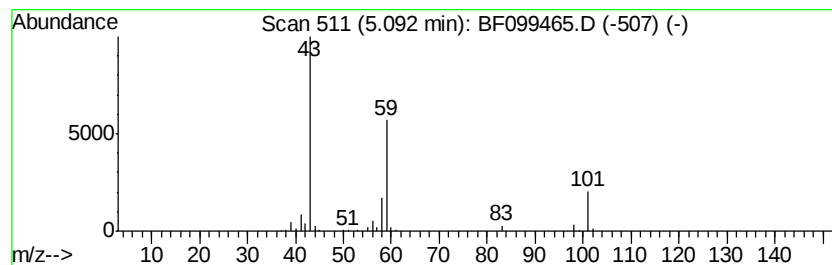

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101317\
Data File : BF099465.D
Acq On : 14 Oct 2017 3:41
Operator : SJ/JU
Sample : PB103194BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB103194BL







Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.63 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.63	77.77 ng	2209000	1,4-Dichlorobenzene-d4	6.85

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		Xenon	132	Xe	007440-63-3	9
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

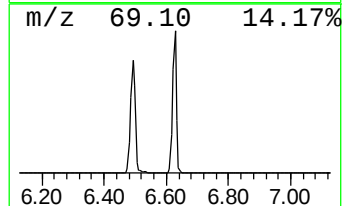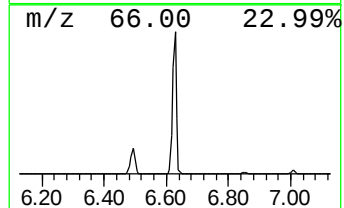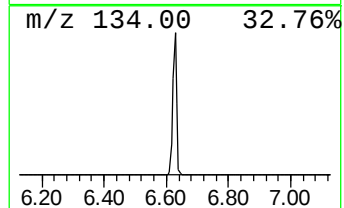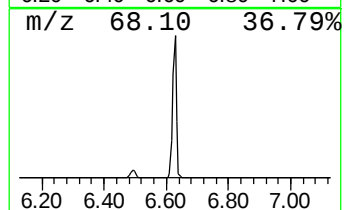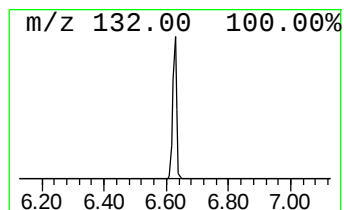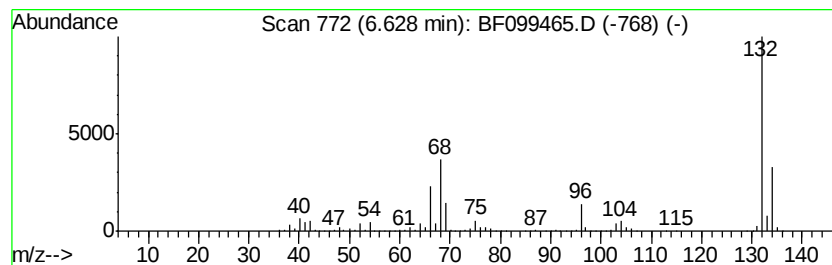

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101317\
Data File : BF099465.D
Acq On : 14 Oct 2017 3:41
Operator : SJ/JU
Sample : PB103194BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB103194BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.09	13.6	ng	384883	1	6.85	568054	20.0
unknown6.63	6.63	77.8	ng	2209000	1	6.85	568054	20.0