


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101317\
 Data File : BF099438.D
 Acq On : 13 Oct 2017 13:55
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 11 16:25:21 2017

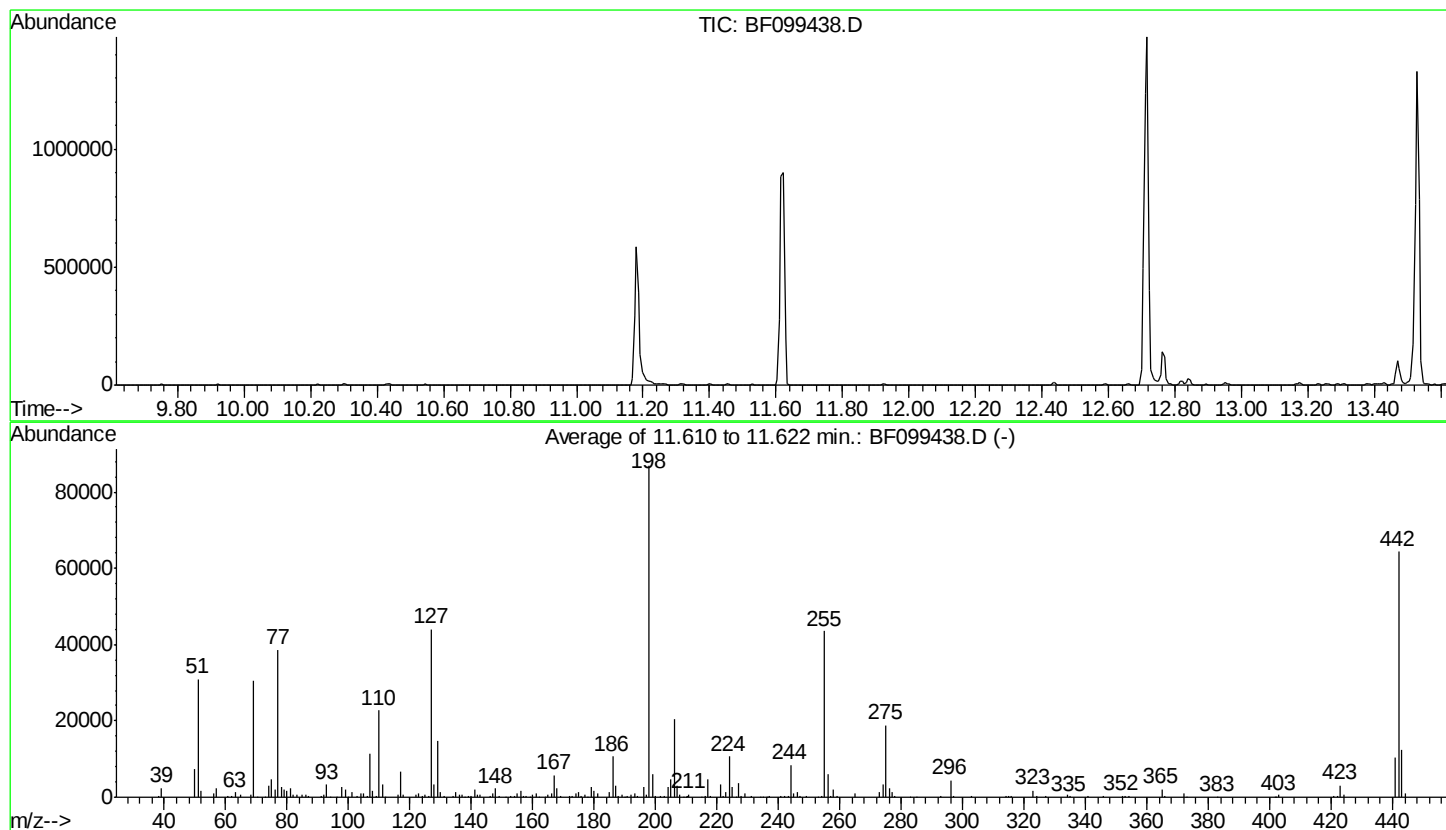

AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.7	30989	PASS
68	69	0.00	2	1.7	527	PASS
69	198	0.00	100	35.1	30538	PASS
70	69	0.00	2	0.3	100	PASS
127	198	10	80	50.7	44080	PASS
197	198	0.00	2	0.6	538	PASS
198	198	100	100	100.0	86904	PASS
199	198	5	9	6.9	5965	PASS
275	198	10	60	21.6	18814	PASS
365	198	1	100	2.3	2029	PASS
441	442	0.01	24	16.3	10472	PASS
442	198	50	100	74.0	64323	PASS
443	442	15	24	19.3	12421	PASS