


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101317\
Data File : BF099463.D
Acq On : 14 Oct 2017 2:45
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 11 16:25:21 2017

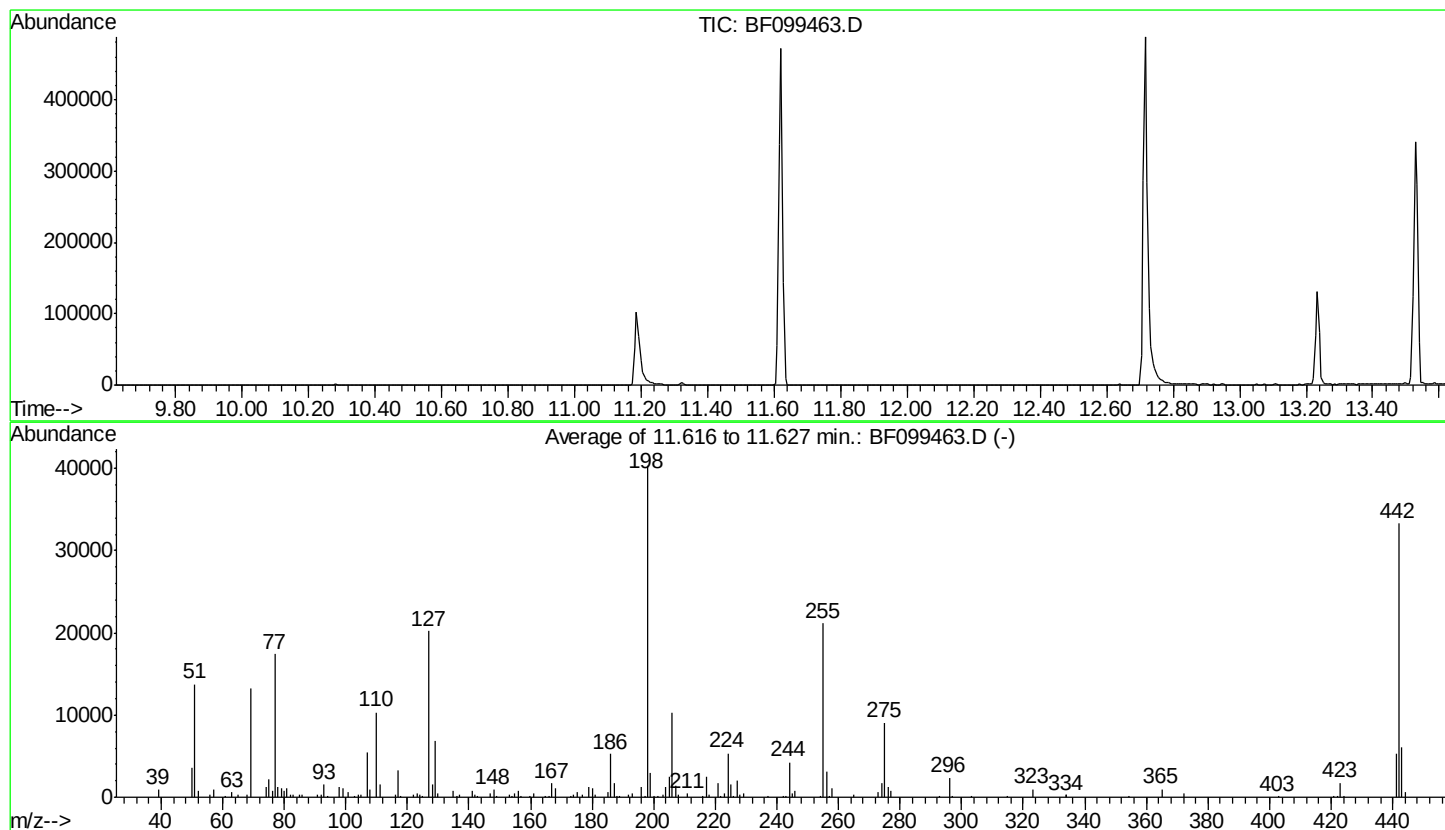

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	13763	PASS
68	69	0.00	2	2.0	259	PASS
69	198	0.00	100	32.8	13221	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.0	20196	PASS
197	198	0.00	2	0.4	152	PASS
198	198	100	100	100.0	40354	PASS
199	198	5	9	7.2	2902	PASS
275	198	10	60	22.6	9102	PASS
365	198	1	100	2.5	1006	PASS
441	442	0.01	24	15.9	5282	PASS
442	198	50	100	82.5	33282	PASS
443	442	15	24	18.5	6143	PASS