
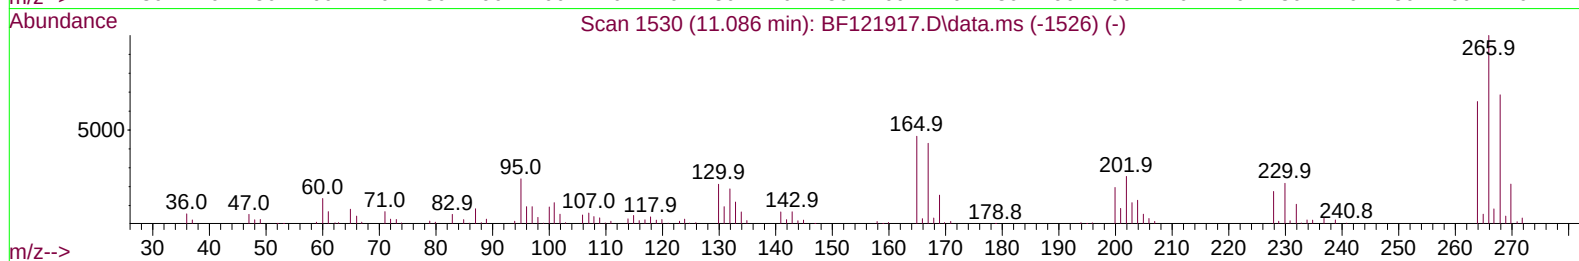
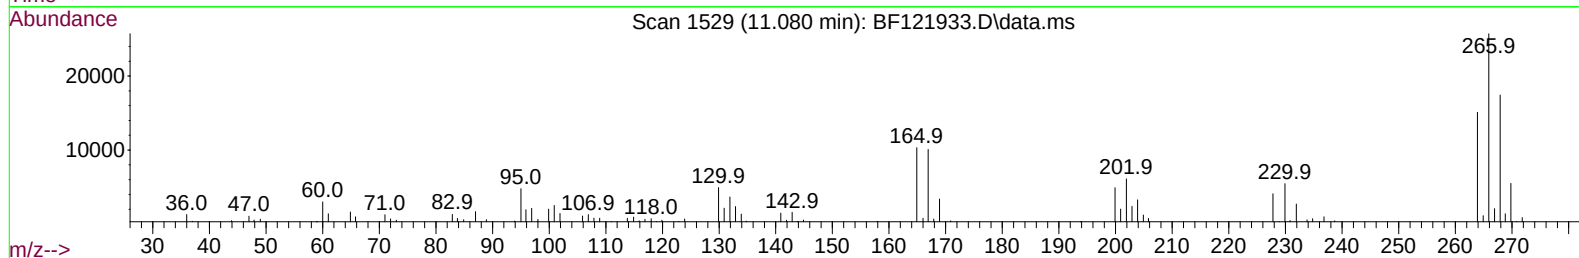


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101320\
Data File : BF121933.D
Acq On : 13 Oct 2020 11:52
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 13 17:57:25 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 12 16:22:33 2020
Response via : Initial Calibration

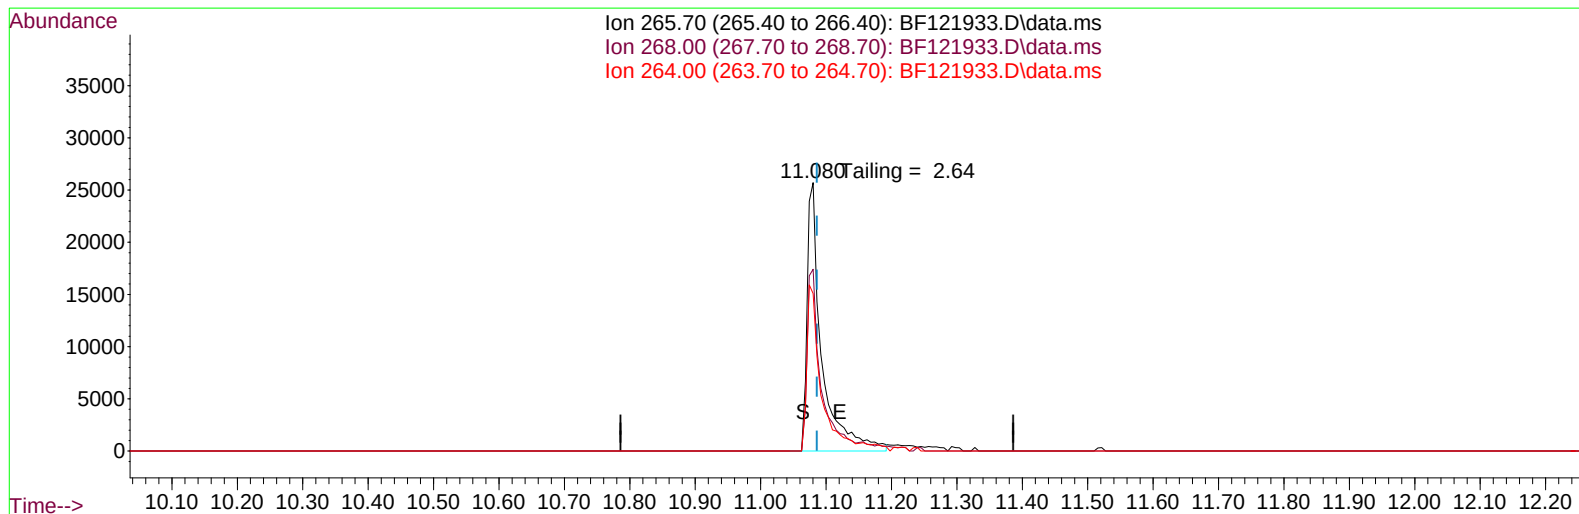

TIC: BF121933.D\data.ms

(70) Pentachlorophenol (C)




11.080min (-0.006) 30977.73 ng

response 41899

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.50	67.77
264.00	62.40	58.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101320\
Data File : BF121933.D
Acq On : 13 Oct 2020 11:52
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 13 17:57:25 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 12 16:22:33 2020
Response via : Initial Calibration

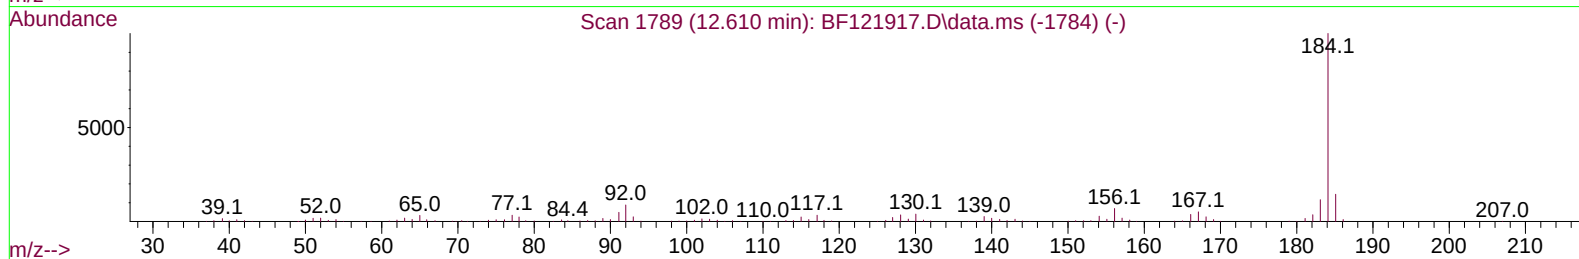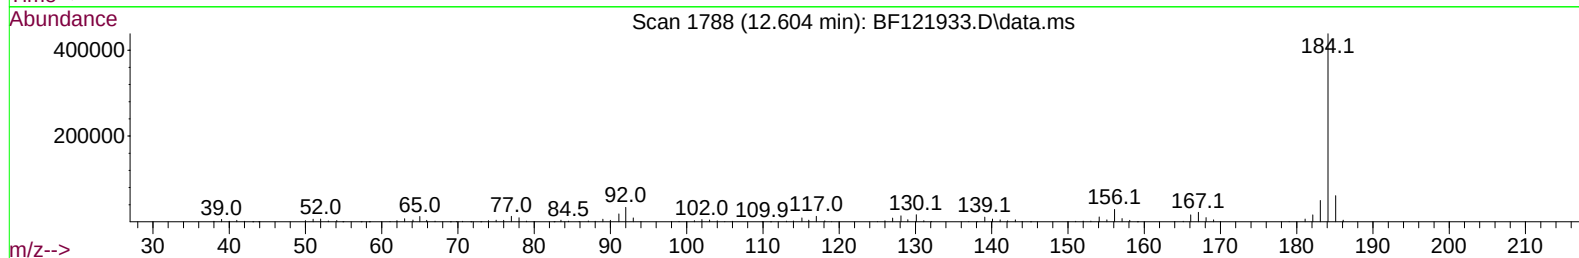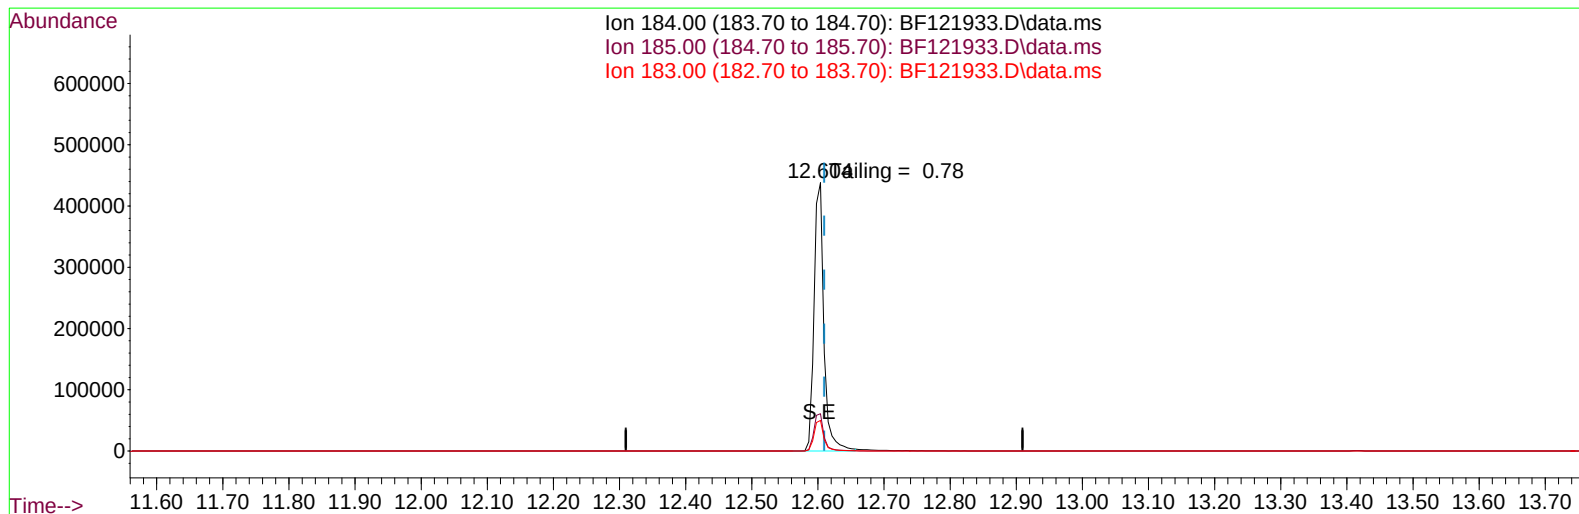

TIC: BF121933.D\data.ms

(77) Benzidine

12.604min (-0.006) 0.00 ng

response 457543

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.93
183.00	11.70	11.42
0.00	0.00	0.00