

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101320\
 Data File : BF121948.D
 Acq On : 13 Oct 2020 20:21
 Operator : JU/CG
 Sample : L4372-01 5X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-HADLEY

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF121948.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.716	273	277	284	rVB2	4961	8985	1.09%	0.133%
2	5.363	554	557	582	rBV	279334	347878	42.05%	5.167%
3	6.387	728	731	748	rBV	256814	347143	41.96%	5.156%
4	6.745	788	792	805	rVB	593071	559554	67.64%	8.312%
5	7.310	884	888	899	rBV	193310	222184	26.86%	3.300%
6	8.028	1006	1010	1027	rVB	694131	652807	78.91%	9.697%
7	9.098	1189	1192	1202	rBV	444535	392599	47.46%	5.832%
8	9.498	1256	1260	1269	rBV	41593	38793	4.69%	0.576%
9	9.775	1304	1307	1319	rVB	649670	641961	77.60%	9.536%
10	10.569	1439	1442	1453	rVB	182048	173628	20.99%	2.579%
11	10.680	1457	1461	1467	rBV3	11122	14998	1.81%	0.223%
12	11.263	1556	1560	1563	rBV	699771	614433	74.27%	9.127%
13	11.875	1660	1664	1667	rBV2	7052	8698	1.05%	0.129%
14	12.474	1763	1766	1770	rBV	133446	108509	13.12%	1.612%
15	12.704	1799	1805	1811	rBV	110195	114877	13.89%	1.706%
16	12.839	1825	1828	1832	rBV	475766	432499	52.28%	6.424%
17	13.033	1855	1861	1865	rBV	15848	29501	3.57%	0.438%
18	13.074	1865	1868	1870	rBV3	8118	10172	1.23%	0.151%
19	13.133	1875	1878	1885	rVV6	8127	18429	2.23%	0.274%
20	13.651	1964	1966	1969	rBV	21313	19692	2.38%	0.293%
21	13.763	1981	1985	1993	rBV5	28658	57538	6.96%	0.855%
22	13.904	2004	2009	2012	rBV	800247	827254	100.00%	12.288%
23	13.927	2012	2013	2020	rVB	79204	58080	7.02%	0.863%
24	14.927	2180	2183	2190	rVB	84995	134673	16.28%	2.000%
25	15.215	2230	2232	2237	rVB	53091	54236	6.56%	0.806%
26	15.280	2240	2243	2248	rVB	56391	65800	7.95%	0.977%
27	15.339	2248	2253	2261	rBV	637675	777342	93.97%	11.547%




Sum of corrected areas: 6732263

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101320\
Data File : BF121948.D
Acq On : 13 Oct 2020 20:21
Operator : JU/CG
Sample : L4372-01 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-HADLEY

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

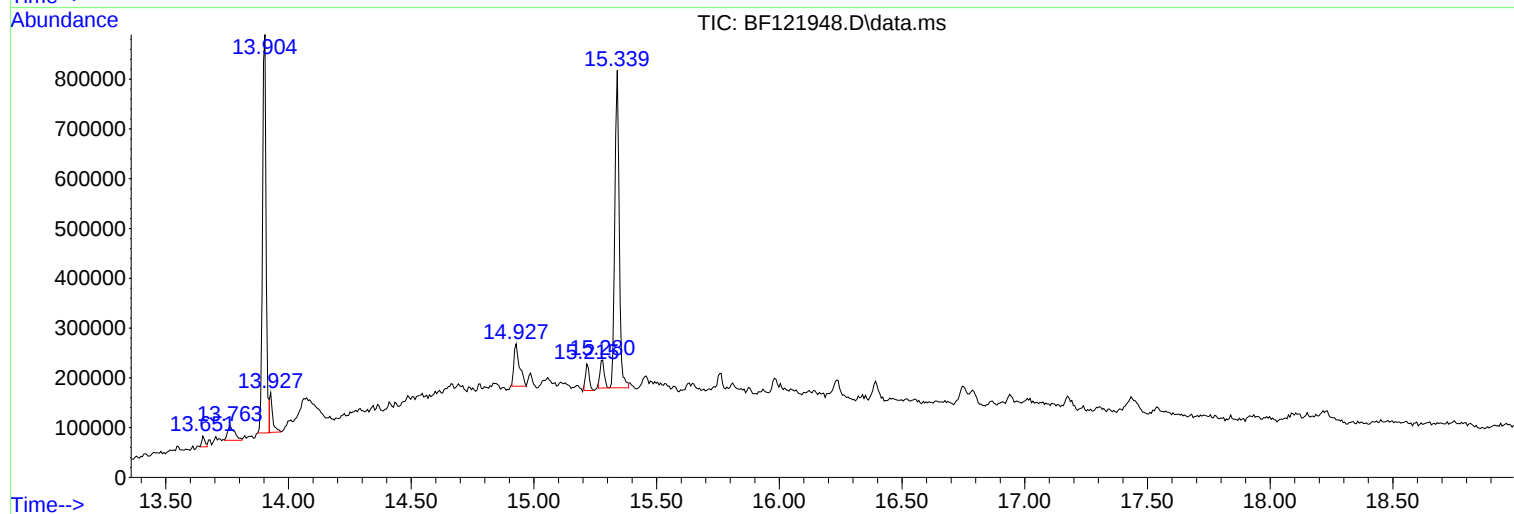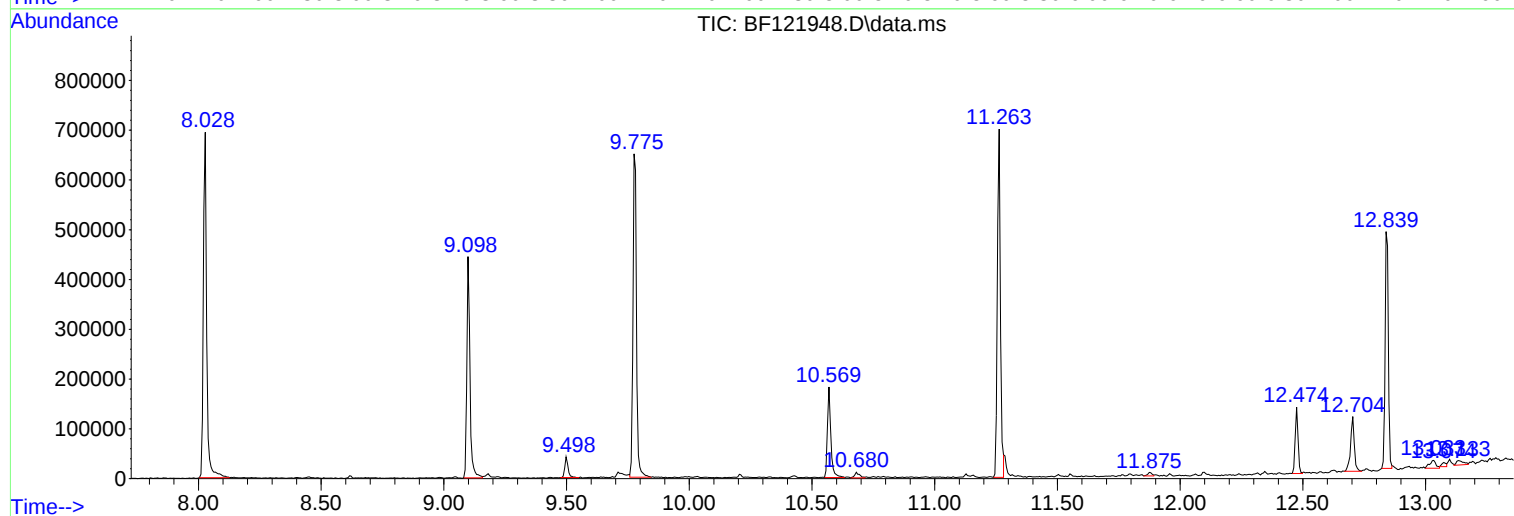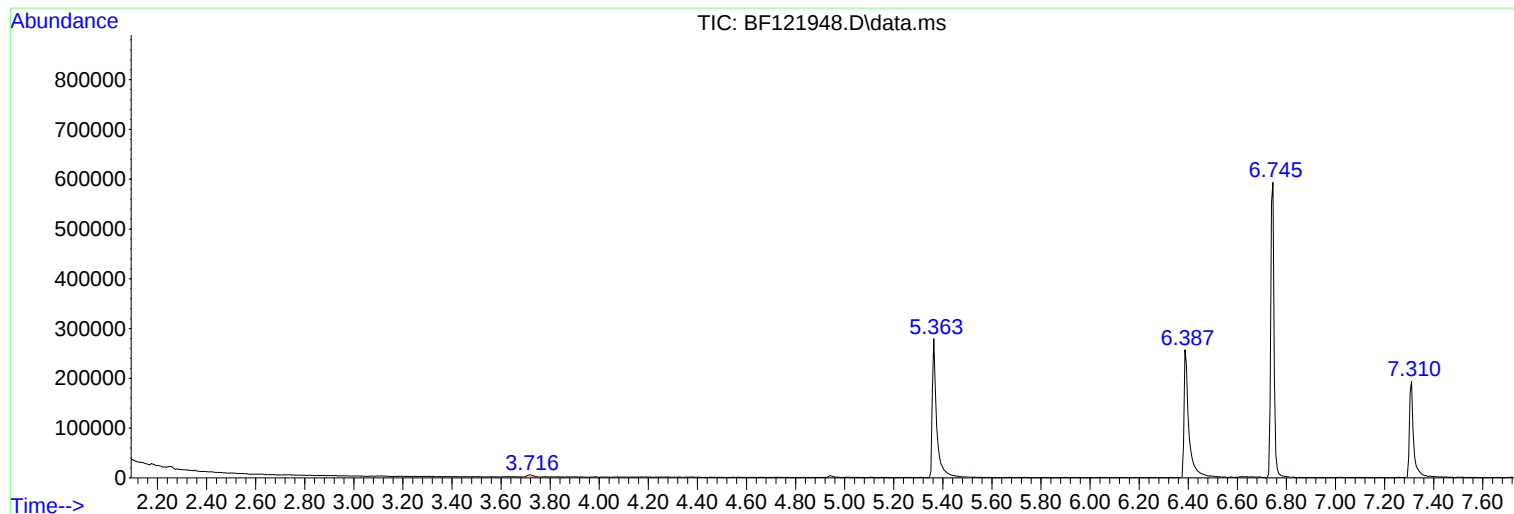

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101320\
Data File : BF121948.D
Acq On : 13 Oct 2020 20:21
Operator : JU/CG
Sample : L4372-01 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-HADLEY

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101320\
Data File : BF121948.D
Acq On : 13 Oct 2020 20:21
Operator : JU/CG
Sample : L4372-01 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-HADLEY

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc