
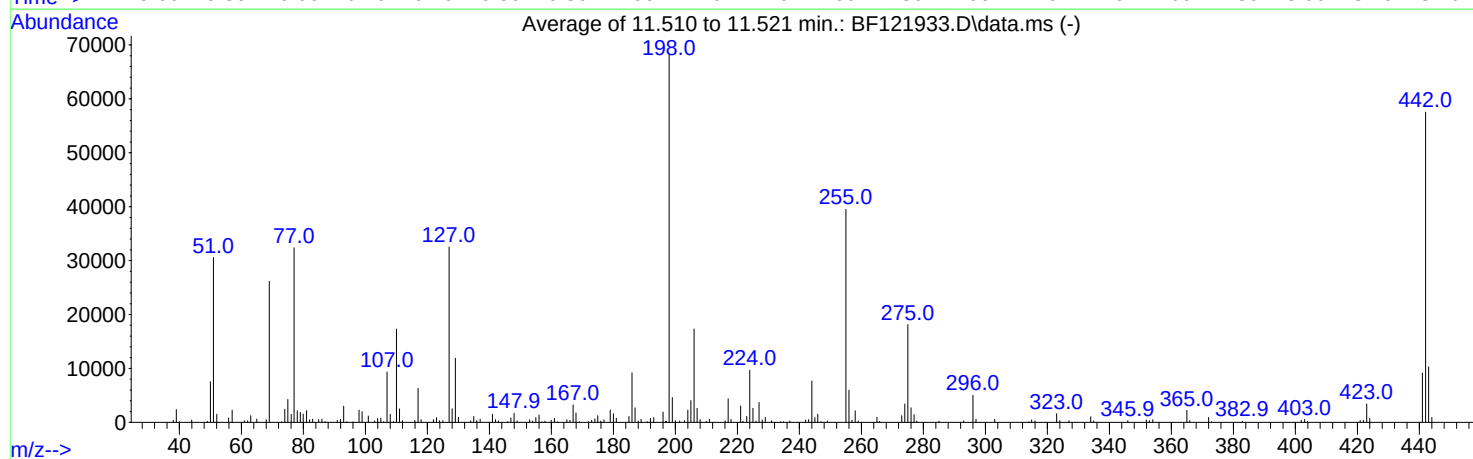


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101320\
 Data File : BF121933.D
 Acq On : 13 Oct 2020 11:52
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 12 16:22:33 2020

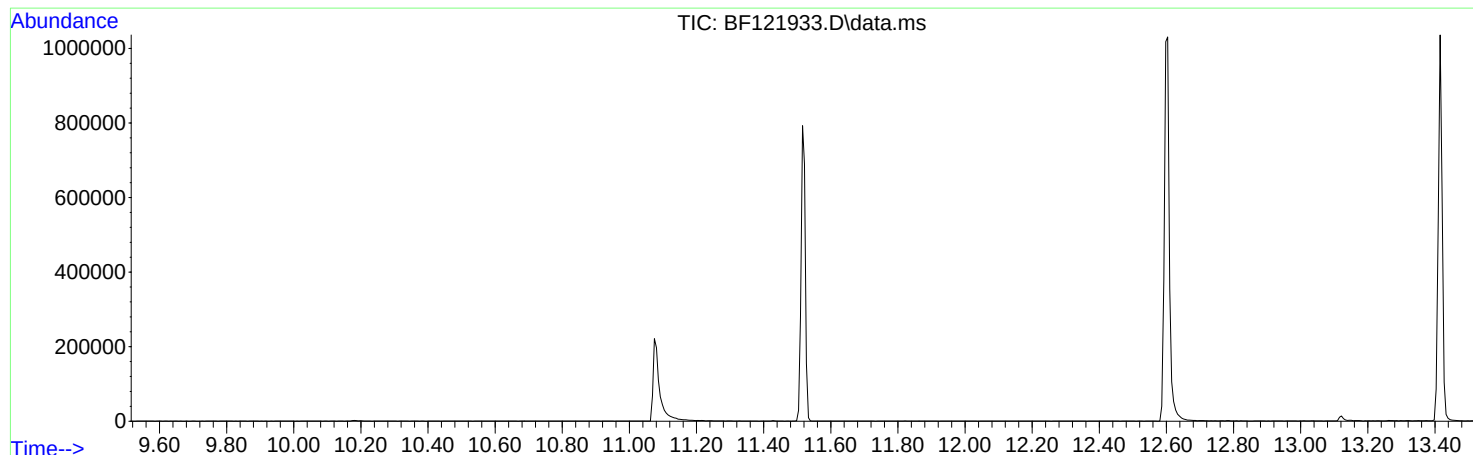

AutoFind: Scans 1602, 1603, 1604; Background Corrected with Scan 1597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.8	30568	PASS
68	69	0.00	2	1.9	506	PASS
69	198	0.00	100	38.3	26160	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.7	32523	PASS
197	198	0.00	2	0.3	198	PASS
198	198	100	100	100.0	68227	PASS
199	198	5	9	6.7	4600	PASS
275	198	10	60	26.6	18138	PASS
365	198	1	100	3.3	2224	PASS
441	198	0.01	100	13.4	9140	PASS
442	198	50	100	84.3	57538	PASS
443	442	15	24	17.9	10306	PASS