
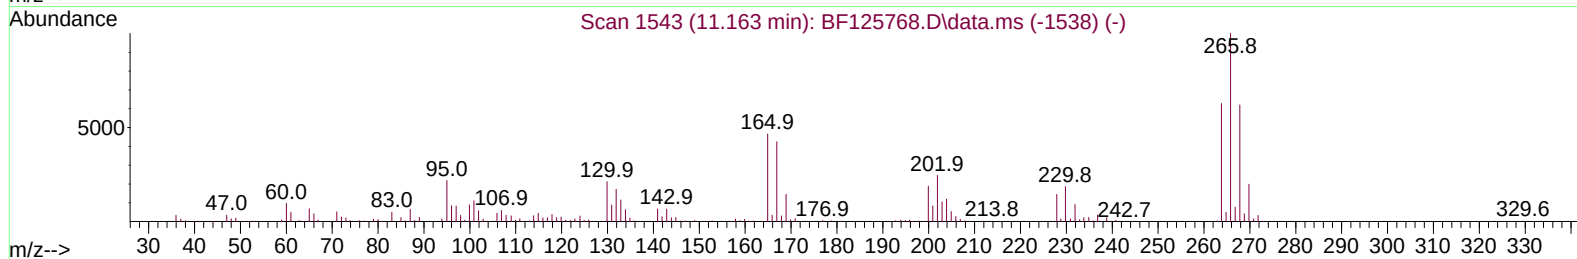
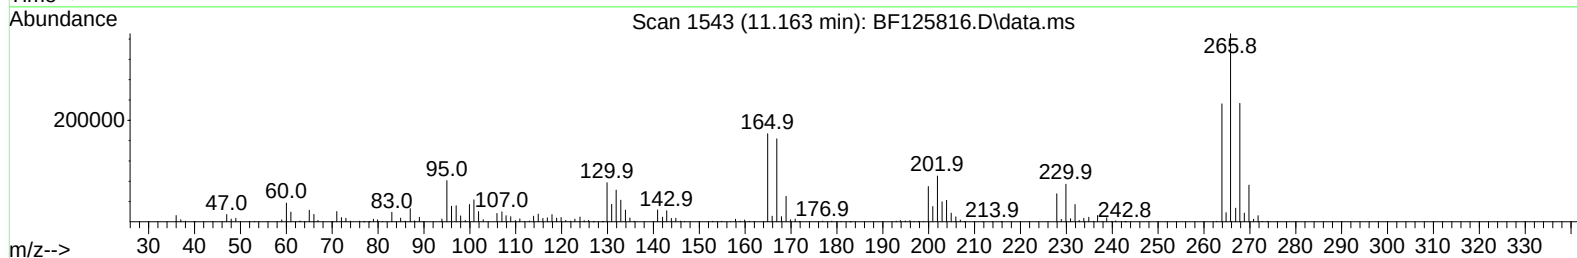


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101321\
Data File : BF125816.D
Acq On : 13 Oct 2021 9:16
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 14 04:24:36 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 13 13:23:32 2021
Response via : Initial Calibration

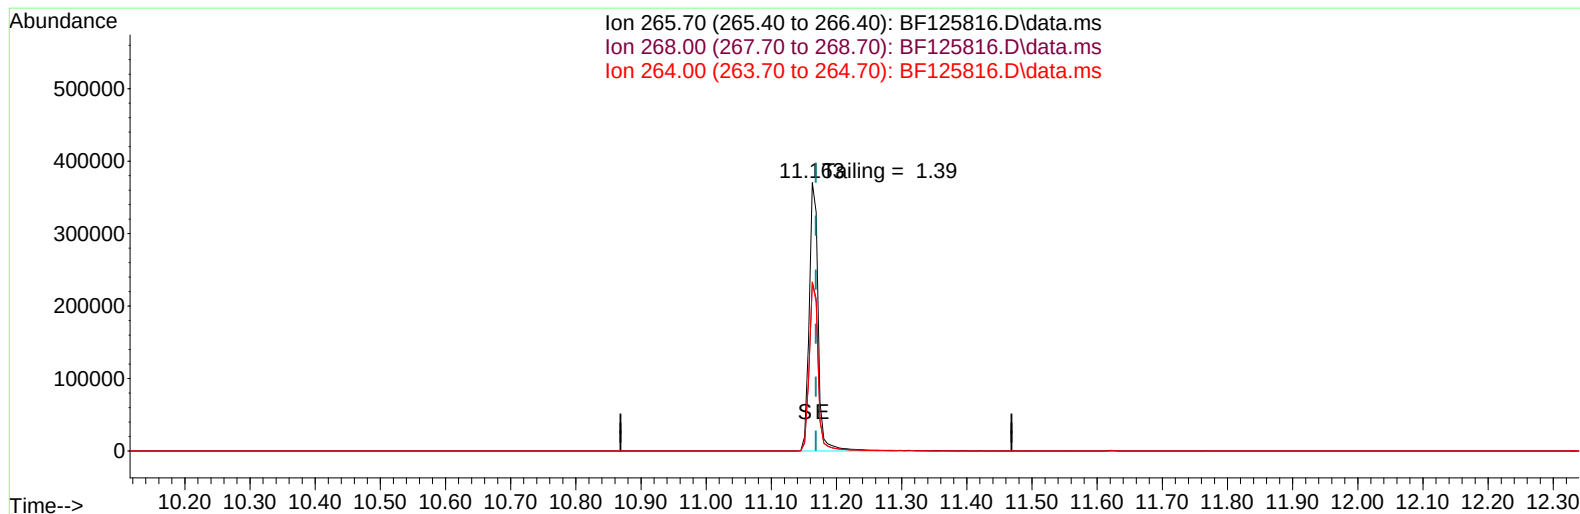

TIC: BF125816.D\data.ms

(70) Pentachlorophenol (C)




11.163min (-0.006) 33482.51 ng

response 356946

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	63.04
264.00	69.90	62.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101321\
 Data File : BF125816.D
 Acq On : 13 Oct 2021 9:16
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 14 04:24:36 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 13 13:23:32 2021
 Response via : Initial Calibration

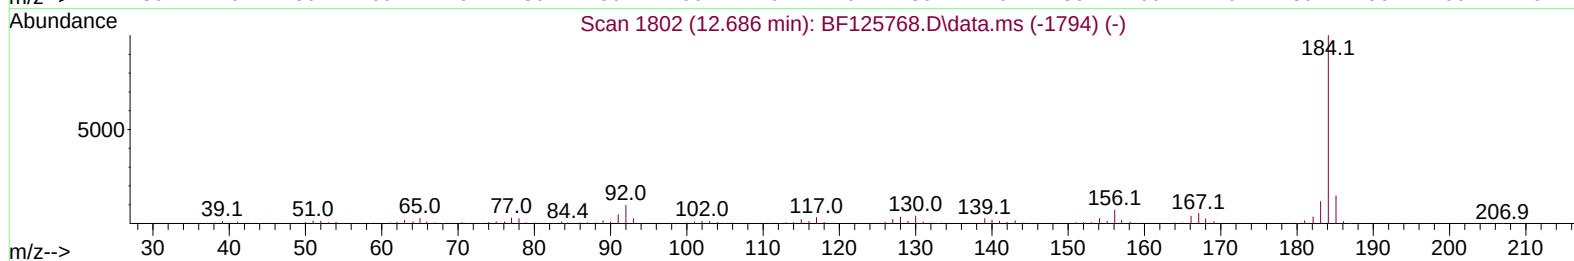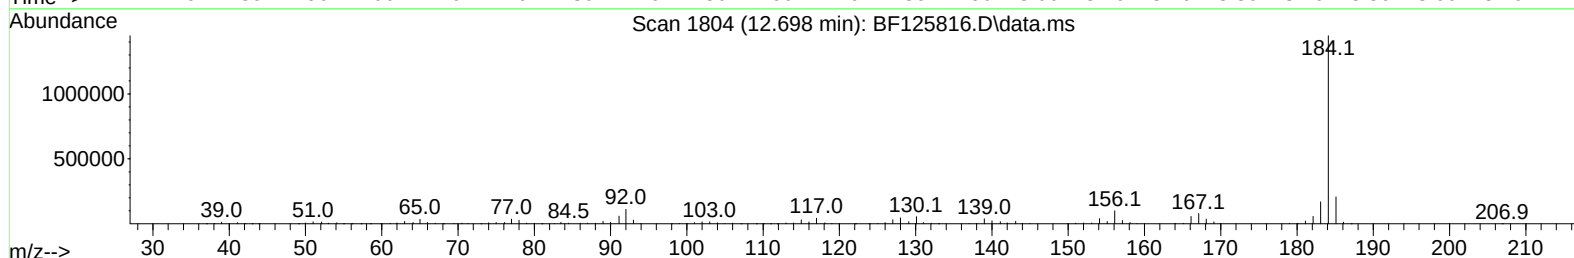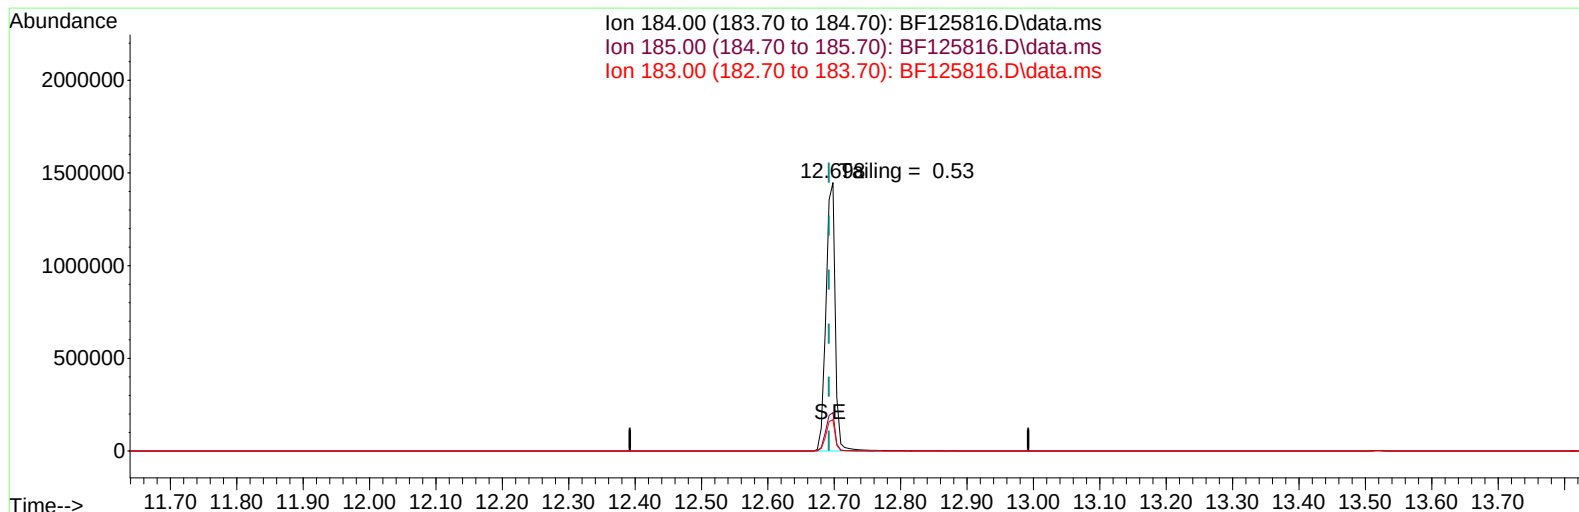

TIC: BF125816.D\data.ms

(77) Benzidine

12.698min (+ 0.006) 0.00 ng

response 1408071

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.30
183.00	10.10	11.68
0.00	0.00	0.00