

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101321\
 Data File : BF125835.D
 Acq On : 13 Oct 2021 19:53
 Operator : JU/CG
 Sample : M4172-01 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OK-3-101121

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF125835.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.899	303	308	313	rVB	12727	17133	1.39%	0.200%
2	5.451	568	572	582	rBV	463796	394357	32.09%	4.606%
3	6.463	741	744	755	rVB	481892	384144	31.26%	4.486%
4	6.845	805	809	812	rBV	1326047	999336	81.32%	11.671%
5	7.398	900	903	908	rBV	290386	215889	17.57%	2.521%
6	8.028	1006	1010	1015	rBV	68838	63920	5.20%	0.747%
7	8.128	1023	1027	1030	rBV	1569037	1228867	100.00%	14.352%
8	9.198	1205	1209	1212	rBV	587367	430841	35.06%	5.032%
9	9.881	1321	1325	1328	rBV	1416923	1170947	95.29%	13.675%
10	10.663	1454	1458	1462	rBV	269179	216304	17.60%	2.526%
11	10.786	1475	1479	1483	rBV3	21446	32808	2.67%	0.383%
12	11.233	1552	1555	1557	rBV2	18410	18526	1.51%	0.216%
13	11.263	1557	1560	1564	rVB5	18323	17107	1.39%	0.200%
14	11.363	1573	1577	1580	rBV	1426859	1170184	95.22%	13.666%
15	11.386	1580	1581	1583	rVB	48502	23617	1.92%	0.276%
16	11.886	1663	1666	1671	rVB5	39379	41312	3.36%	0.482%
17	12.574	1780	1783	1785	rBV	87169	76106	6.19%	0.889%
18	12.804	1819	1822	1824	rBV	69458	59370	4.83%	0.693%
19	12.945	1842	1846	1849	rBV	511618	438593	35.69%	5.122%
20	13.998	2021	2025	2028	rBV	1033632	905401	73.68%	10.574%
21	15.457	2269	2273	2278	rBV2	571178	657743	53.52%	7.682%




Sum of corrected areas: 8562505

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101321\
Data File : BF125835.D
Acq On : 13 Oct 2021 19:53
Operator : JU/CG
Sample : M4172-01 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-3-101121

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

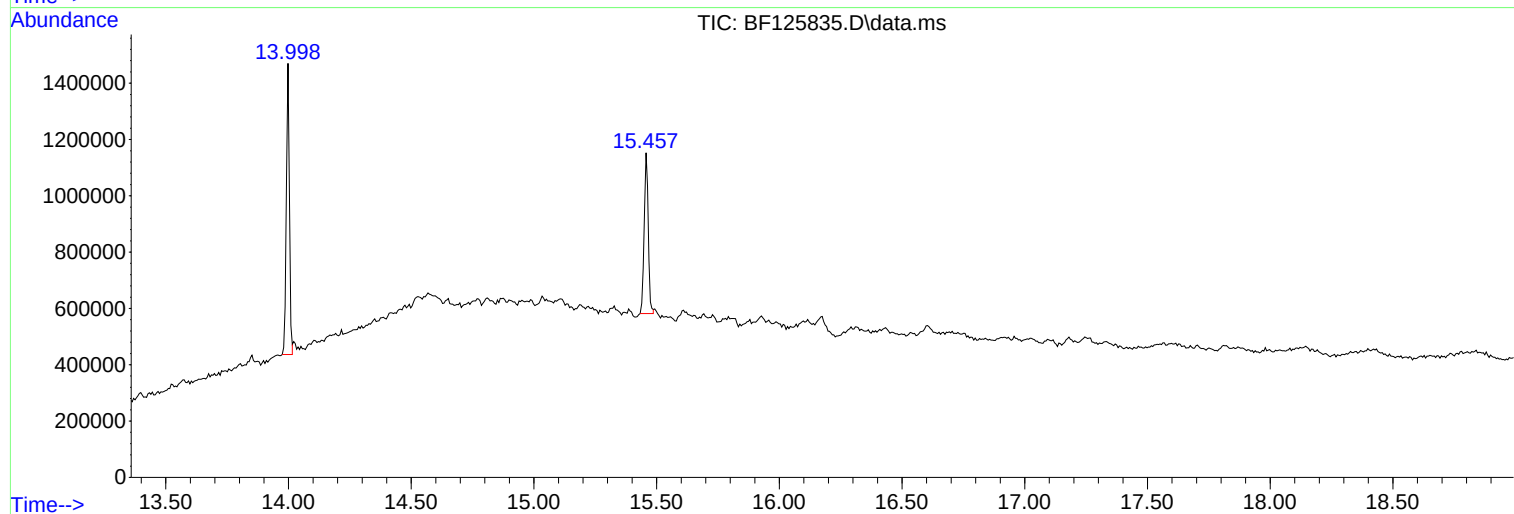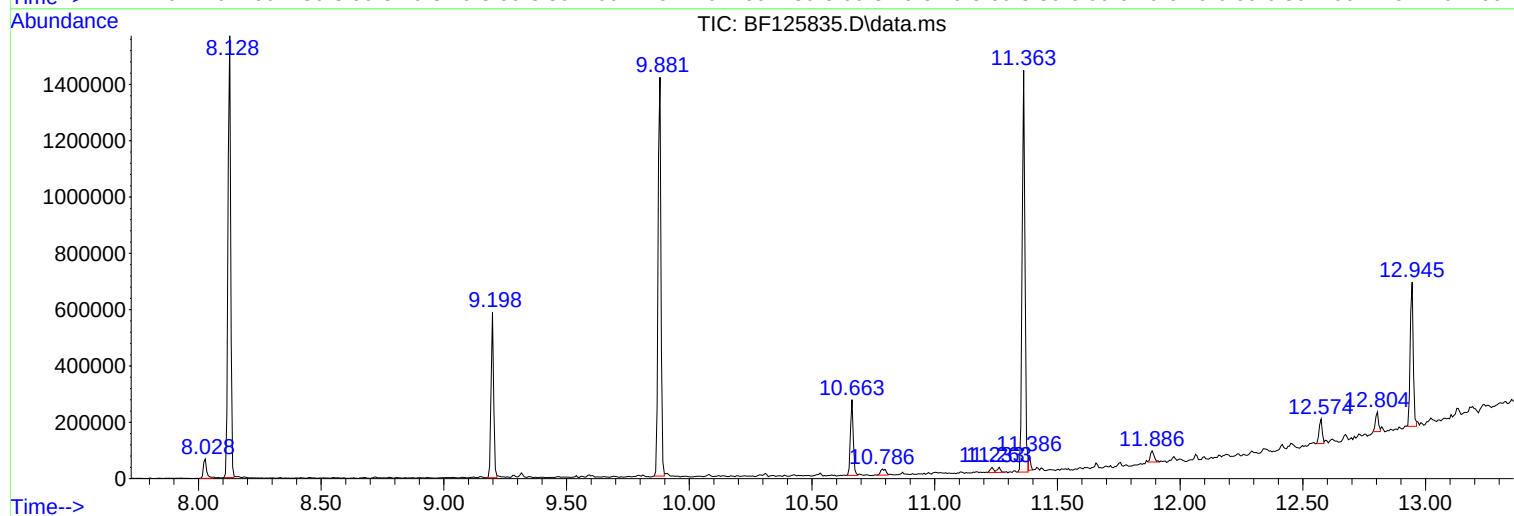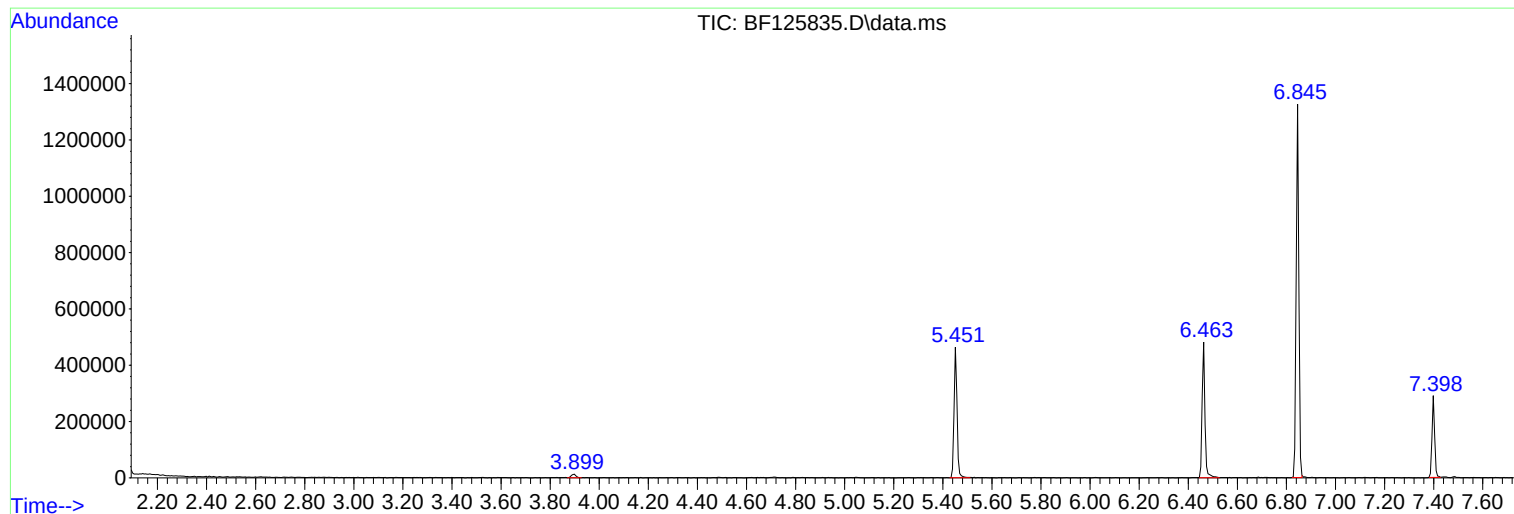

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101321\
Data File : BF125835.D
Acq On : 13 Oct 2021 19:53
Operator : JU/CG
Sample : M4172-01 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-3-101121

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101321\
Data File : BF125835.D
Acq On : 13 Oct 2021 19:53
Operator : JU/CG
Sample : M4172-01 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-3-101121

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------