
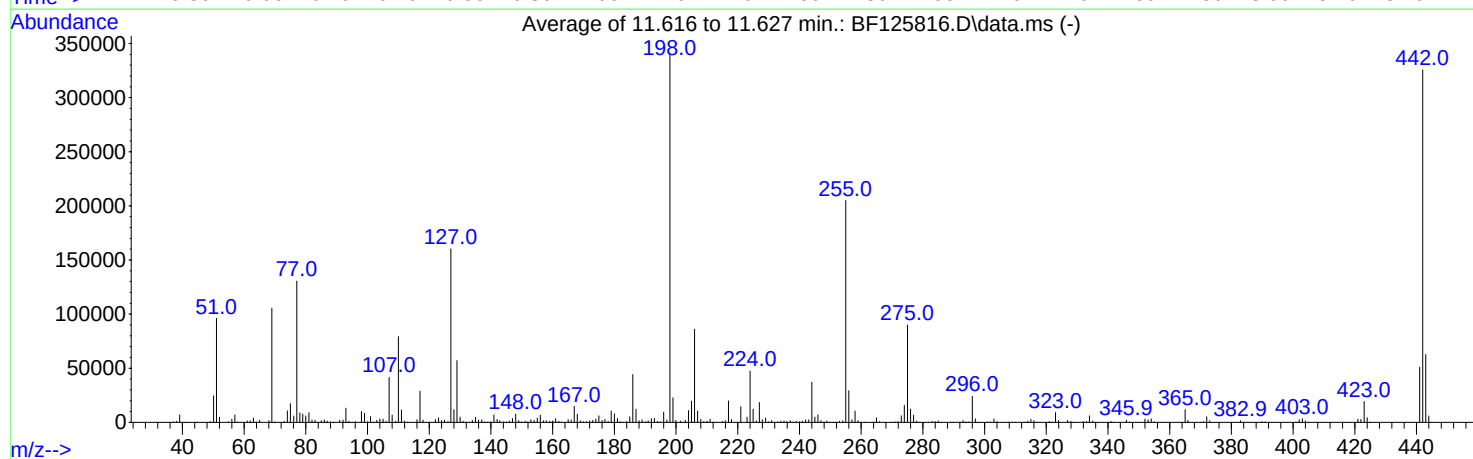


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101321\
 Data File : BF125816.D
 Acq On : 13 Oct 2021 9:16
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 13 13:23:32 2021

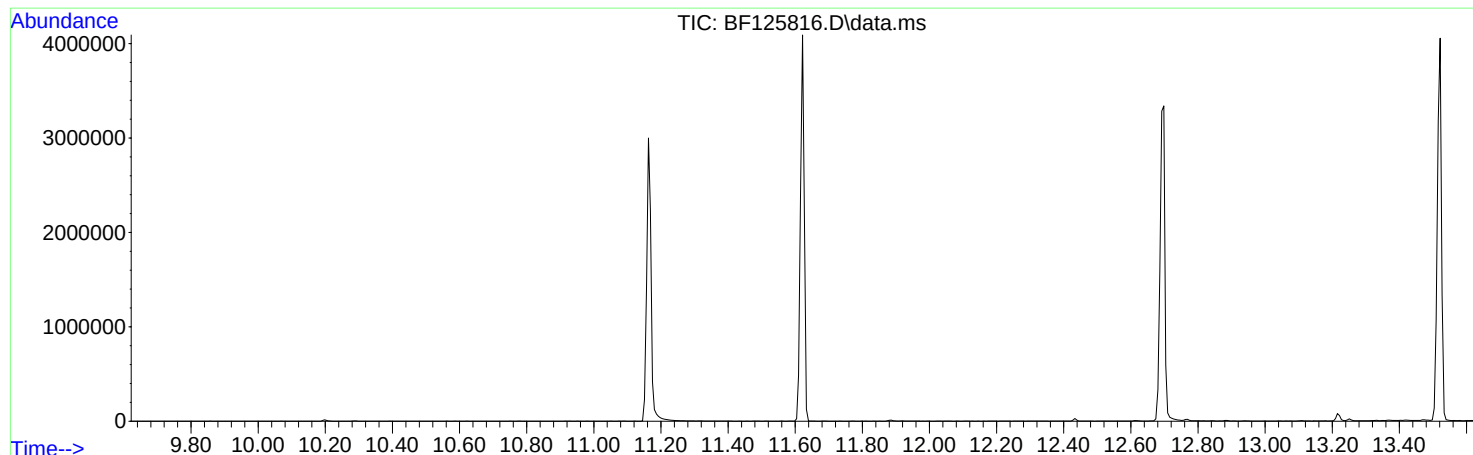




AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.3	96013	PASS
68	69	0.00	2	1.5	1590	PASS
69	198	0.00	100	31.1	105531	PASS
70	69	0.00	2	0.4	444	PASS
127	198	10	80	47.1	160189	PASS
197	198	0.00	2	0.6	2193	PASS
198	198	100	100	100.0	339797	PASS
199	198	5	9	6.7	22812	PASS
275	198	10	60	26.5	89944	PASS
365	198	1	100	3.5	11848	PASS
441	198	0.01	100	15.0	51043	PASS
442	442	50	100	100.0	325568	PASS
443	442	15	24	19.3	62747	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101321\
Data File : BF125816.D
Acq On : 13 Oct 2021 9:16
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 14 04:24:36 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 13 13:23:32 2021
Response via : Initial Calibration

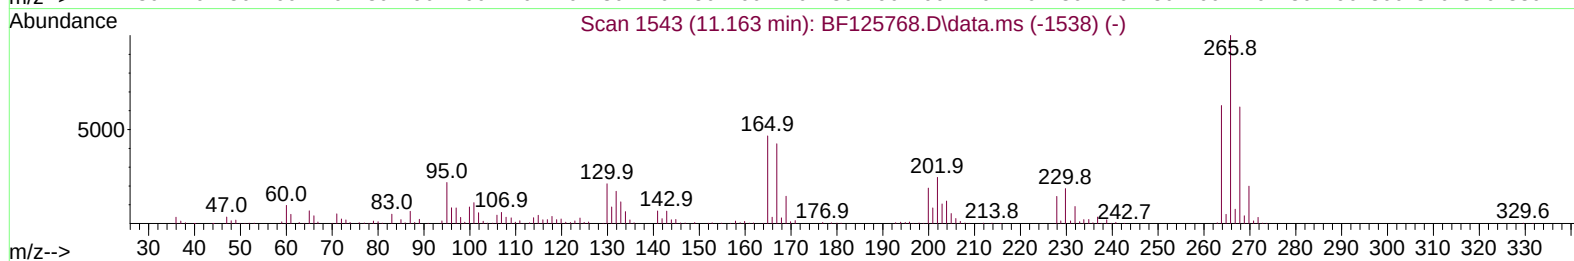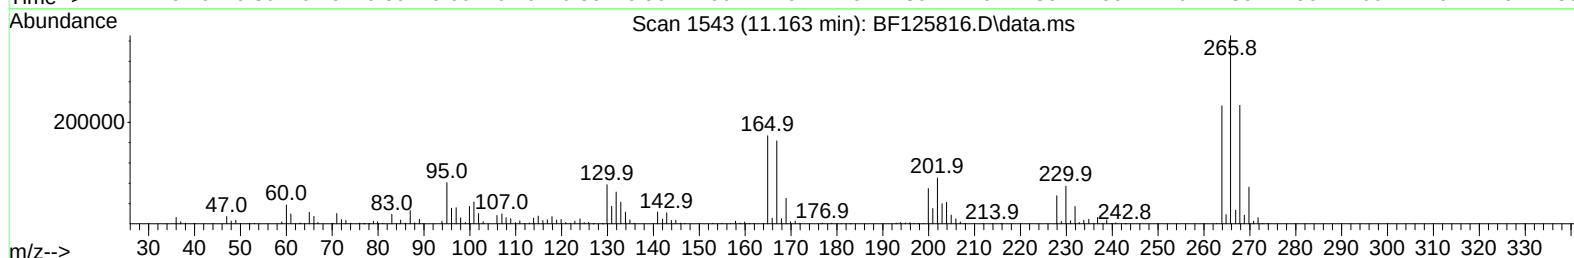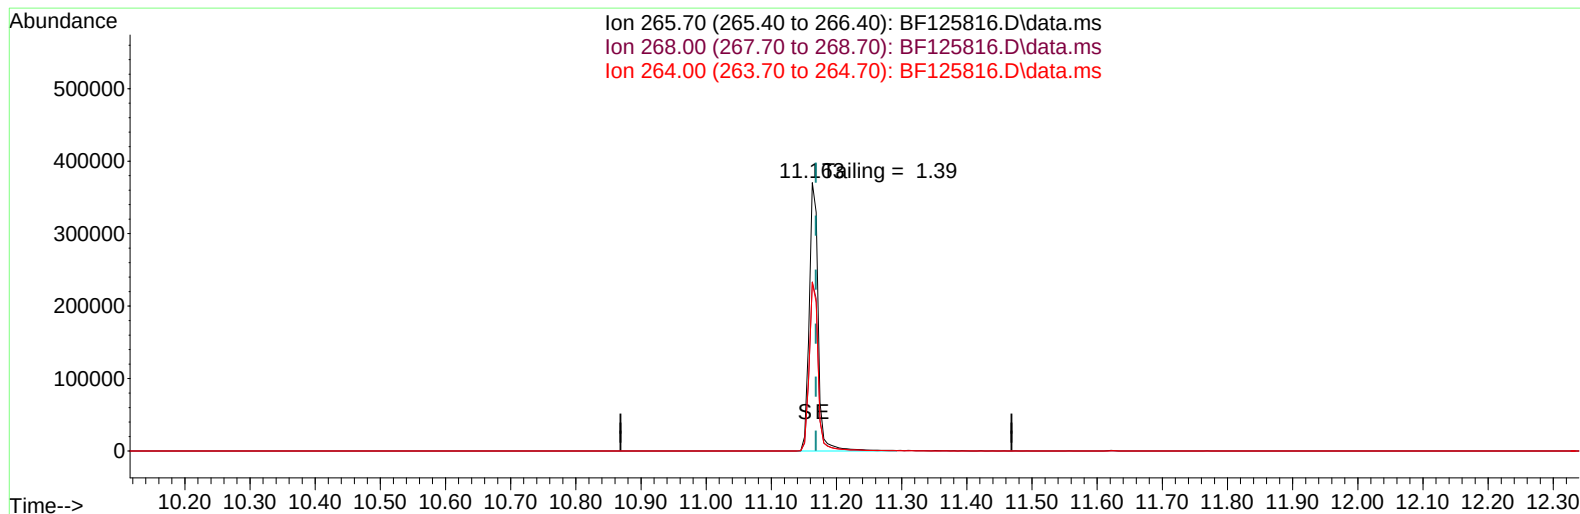

TIC: BF125816.D\data.ms

(70) Pentachlorophenol (C)

11.163min (-0.006) 33482.51 ng




response 356946

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	63.04
264.00	69.90	62.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101321\
Data File : BF125816.D
Acq On : 13 Oct 2021 9:16
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 14 04:24:36 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 13 13:23:32 2021
Response via : Initial Calibration

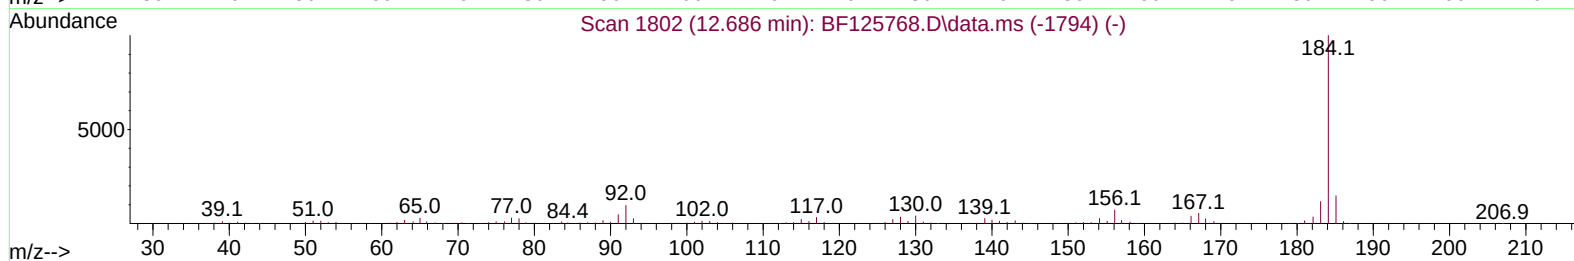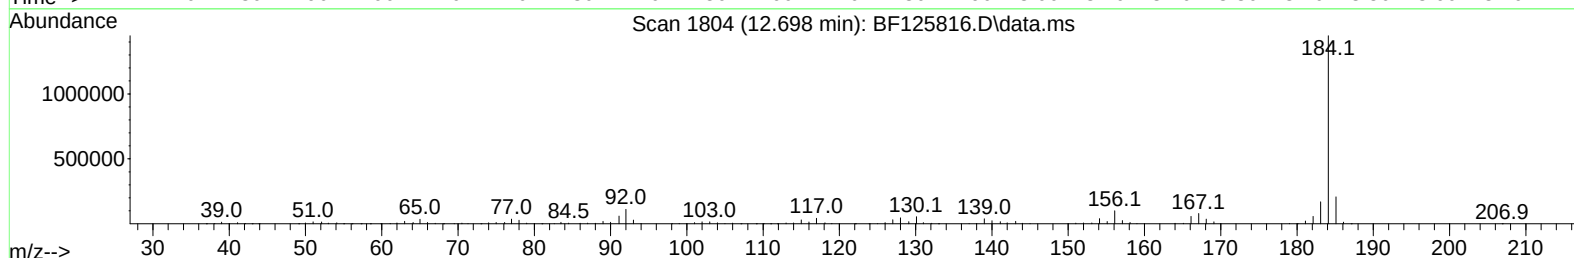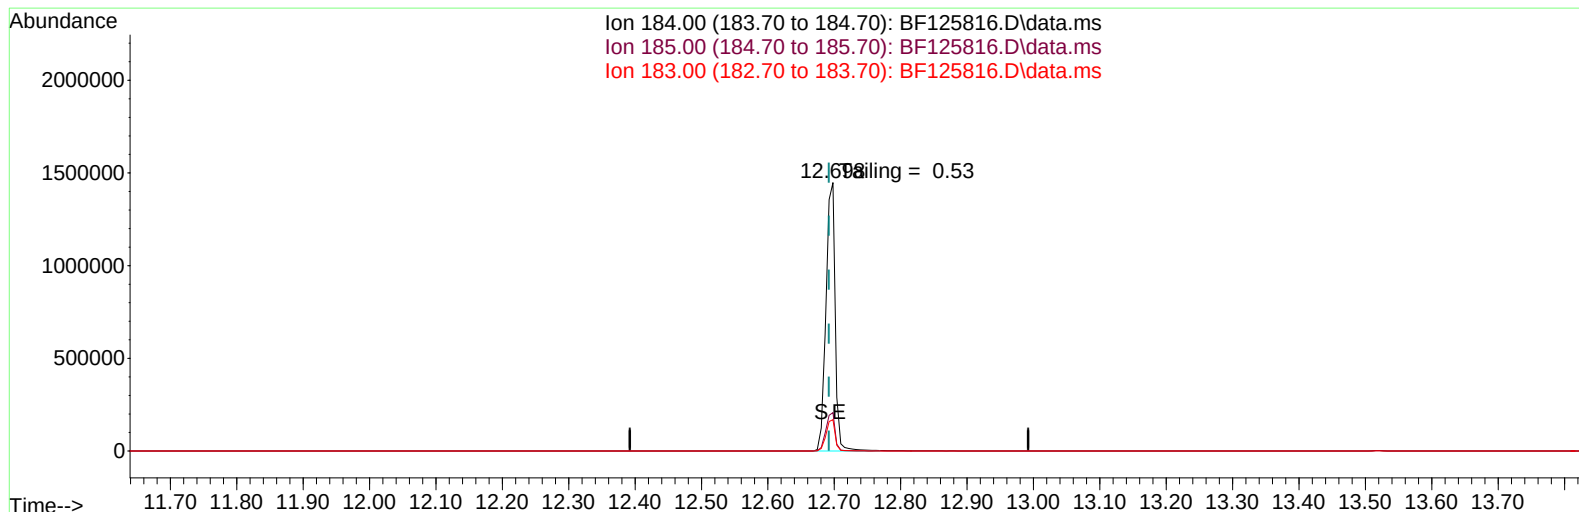

TIC: BF125816.D\data.ms

(77) Benzidine

12.698min (+ 0.006) 0.00 ng

response 1408071

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.30
183.00	10.10	11.68
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/13/2021	BNA_F	<u>BF125816.D</u>
Compound Name	Response	Retention Time
DDT	712861	13.521
DDD	18904	13.216
DDE	1458	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20362	733223	2.78