

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101322\
 Data File : BF130655.D
 Acq On : 13 Oct 2022 19:33
 Operator : CG\JU
 Sample : N5111-01 2X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130655.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.746	449	452	466	rBV	153991	196361	21.63%	2.305%
2	5.187	523	527	544	rBV	759660	832866	91.73%	9.775%
3	6.234	701	705	722	rBV	901782	830113	91.43%	9.743%
4	6.587	762	765	776	rVB	609680	485465	53.47%	5.698%
5	7.151	858	861	872	rBV	559215	520511	57.33%	6.109%
6	7.869	979	983	989	rVB	802511	600175	66.10%	7.044%
7	8.945	1162	1166	1169	rBV	1178435	907958	100.00%	10.656%
8	9.616	1276	1280	1283	rBV	757683	566572	62.40%	6.650%
9	10.398	1410	1413	1423	rBV	460485	436174	48.04%	5.119%
10	11.092	1528	1531	1534	rBV	563971	468615	51.61%	5.500%
11	11.116	1534	1535	1539	rVB	89393	64235	7.07%	0.754%
12	11.175	1539	1545	1549	rBV	21661	21653	2.38%	0.254%
13	11.598	1612	1617	1619	rBV	21591	21624	2.38%	0.254%
14	11.627	1619	1622	1627	rVB2	25938	30841	3.40%	0.362%
15	11.704	1632	1635	1638	rVV	33758	36492	4.02%	0.428%
16	11.727	1638	1639	1647	rVB2	15733	14876	1.64%	0.175%
17	12.145	1707	1710	1713	rBV	24747	25925	2.86%	0.304%
18	12.180	1713	1716	1718	rVV4	13701	15833	1.74%	0.186%
19	12.233	1722	1725	1728	rBV3	12519	15187	1.67%	0.178%
20	12.304	1733	1737	1741	rBV	144719	134236	14.78%	1.575%
21	12.527	1770	1775	1778	rBV	140498	143511	15.81%	1.684%
22	12.586	1782	1785	1788	rBV2	16202	20455	2.25%	0.240%
23	12.674	1797	1800	1804	rBV	776772	679729	74.86%	7.978%
24	12.751	1810	1813	1819	rVB4	13083	16867	1.86%	0.198%
25	12.857	1825	1831	1835	rBV2	30807	49233	5.42%	0.578%
26	12.927	1837	1843	1845	rBV2	20435	25738	2.83%	0.302%
27	12.963	1845	1849	1852	rBV2	23493	25582	2.82%	0.300%
28	13.051	1861	1864	1866	rBV2	17532	15200	1.67%	0.178%
29	13.086	1867	1870	1872	rBV	17283	14724	1.62%	0.173%
30	13.374	1916	1919	1920	rBV3	15078	15187	1.67%	0.178%
31	13.474	1934	1936	1939	rBV	17073	15978	1.76%	0.188%
32	13.580	1952	1954	1962	rVB6	33903	50551	5.57%	0.593%
33	13.721	1974	1978	1981	rBV2	527757	545736	60.11%	6.405%
34	13.751	1981	1983	1991	rVB	69138	72632	8.00%	0.852%
35	14.480	2105	2107	2108	rBV2	28566	23746	2.62%	0.279%
36	14.727	2146	2149	2156	rVB	62369	88624	9.76%	1.040%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101322\
Data File : BF130655.D
Acq On : 13 Oct 2022 19:33
Operator : CG\JU
Sample : N5111-01 2X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-3

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	15.045	2201	2203	2208	rBV	50976	58162	6.41%	0.683%
38	15.098	2209	2212	2220	rVB	351301	433057	47.70%	5.083%




Sum of corrected areas: 8520424

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101322\
Data File : BF130655.D
Acq On : 13 Oct 2022 19:33
Operator : CG\JU
Sample : N5111-01 2X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

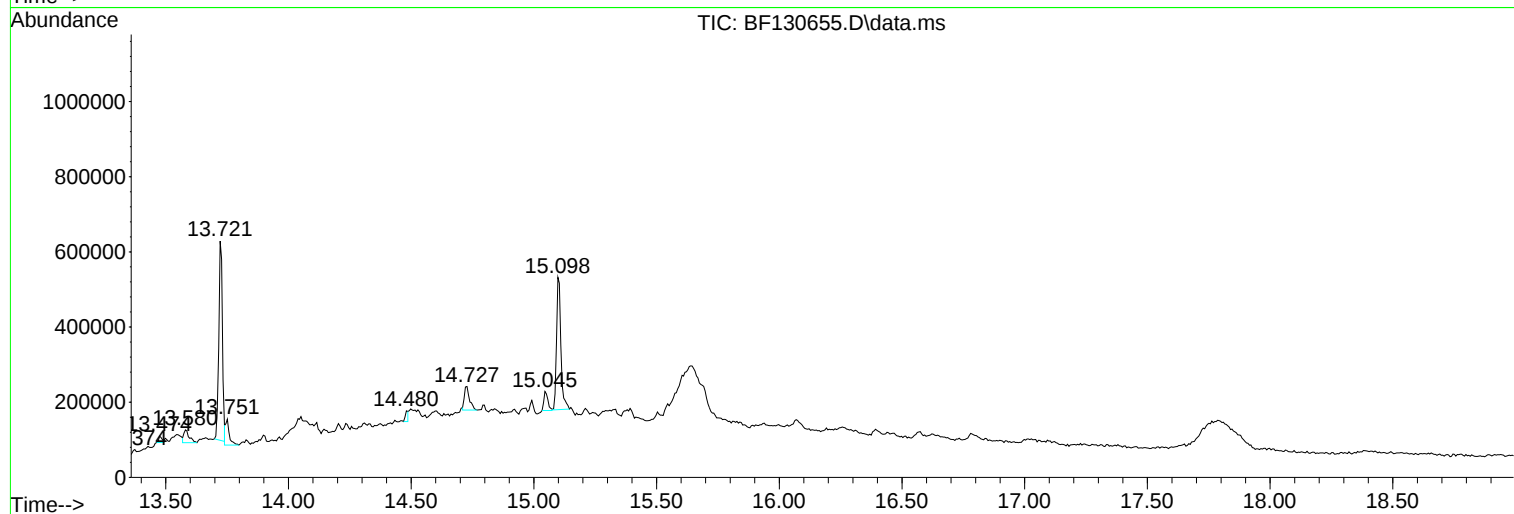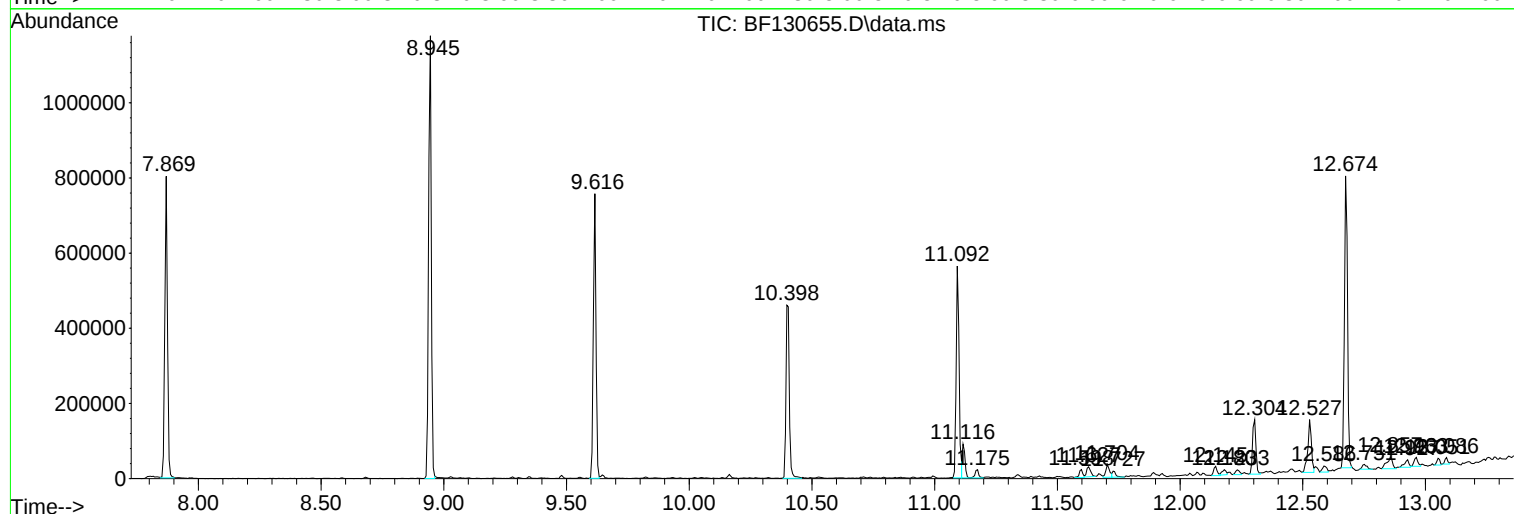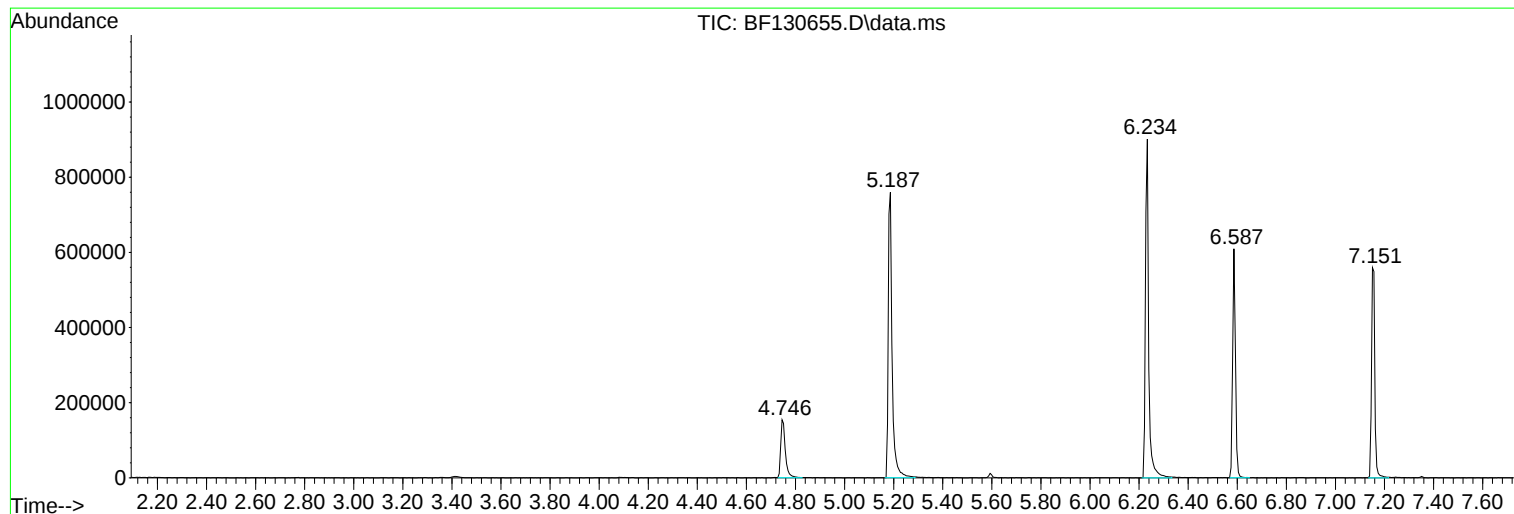

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101322\
Data File : BF130655.D
Acq On : 13 Oct 2022 19:33
Operator : CG\JU
Sample : N5111-01 2X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-3












Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.746	8.09 ng	196361	1,4-Dichlorobenzene-d4	6.587

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56		
2	Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	50		
3	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	17		
4	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		
5	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9		

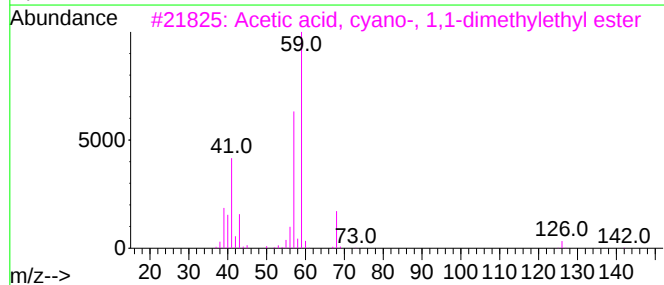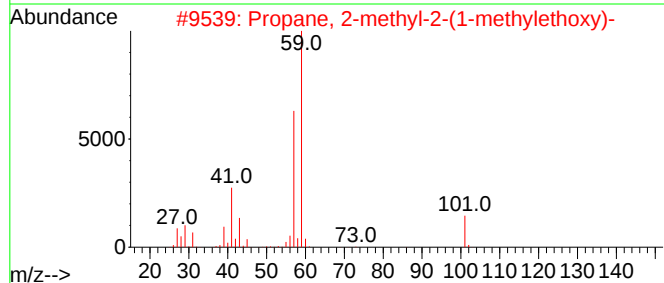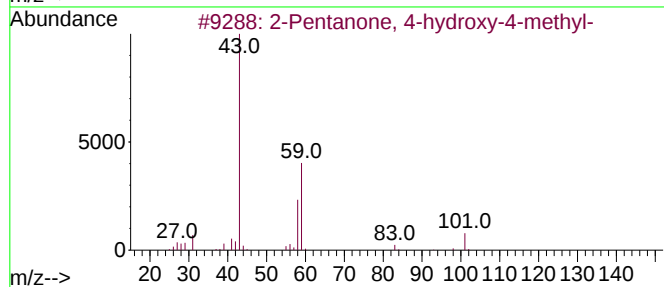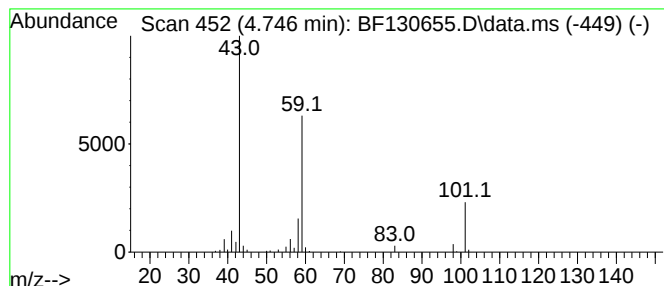

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101322\
Data File : BF130655.D
Acq On : 13 Oct 2022 19:33
Operator : CG\JU
Sample : N5111-01 2X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.746	8.1	ng	196361	1	6.587	485465	20.0