
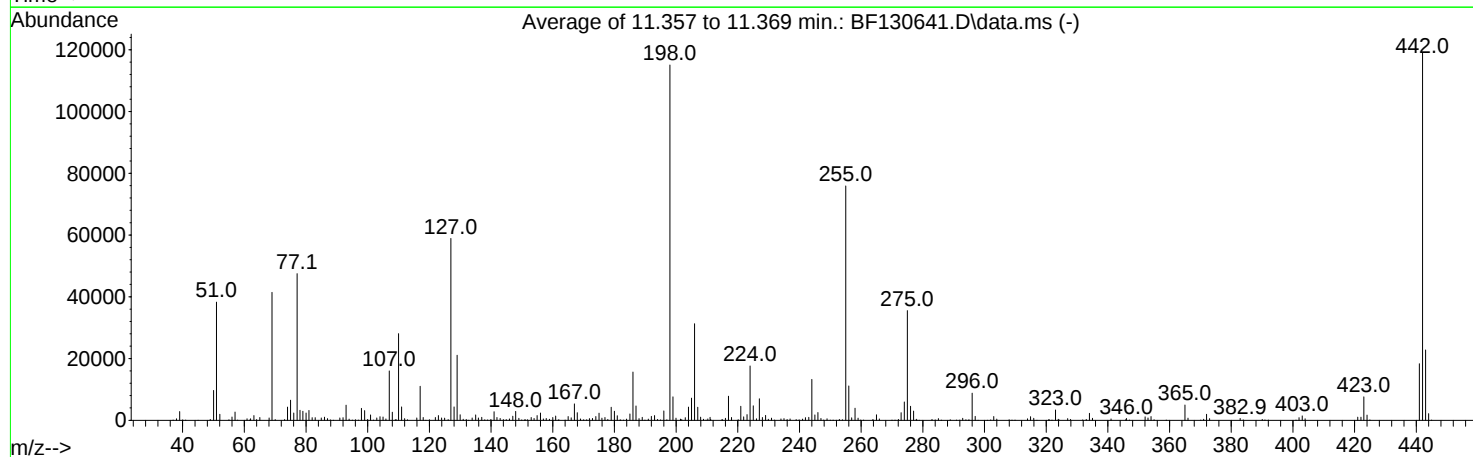


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101322\
 Data File : BF130641.D
 Acq On : 13 Oct 2022 11:14
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 12 06:52:52 2022

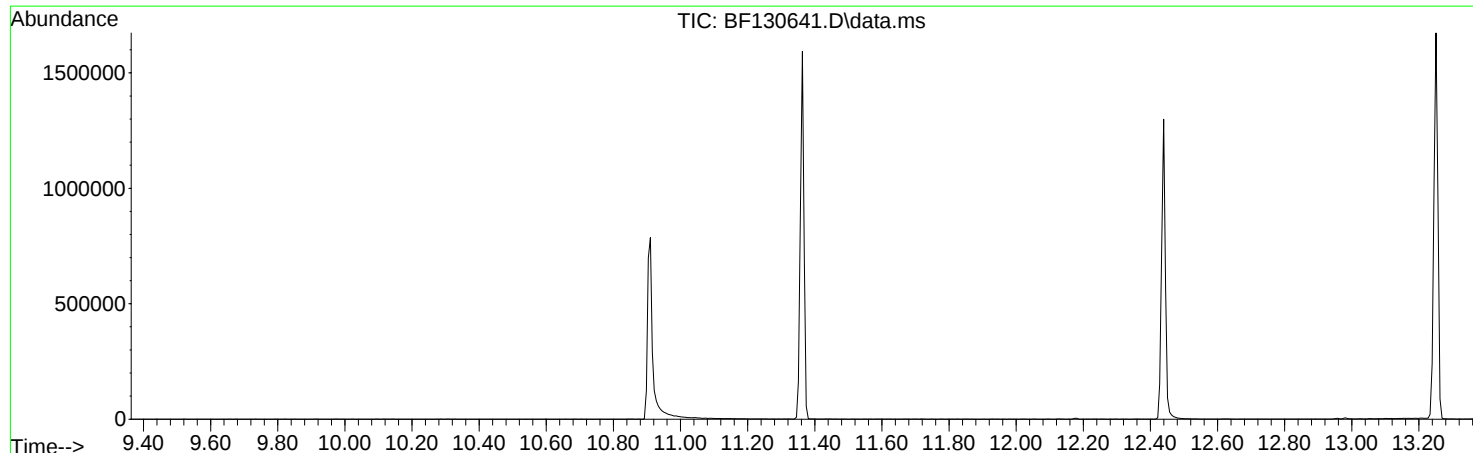




AutoFind: Scans 1576, 1577, 1578; Background Corrected with Scan 1571

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	38249	PASS
68	69	0.00	2	1.9	770	PASS
69	198	0.00	100	36.0	41423	PASS
70	69	0.00	2	0.6	257	PASS
127	198	10	80	51.2	58917	PASS
197	198	0.00	2	0.2	204	PASS
198	198	100	100	100.0	115088	PASS
199	198	5	9	6.6	7596	PASS
275	198	10	60	30.9	35539	PASS
365	198	1	100	4.3	4936	PASS
441	198	0.01	100	15.9	18301	PASS
442	442	50	100	100.0	119139	PASS
443	442	15	24	19.1	22756	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101322\
Data File : BF130641.D
Acq On : 13 Oct 2022 11:14
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 14 09:14:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 12 06:52:52 2022
Response via : Initial Calibration

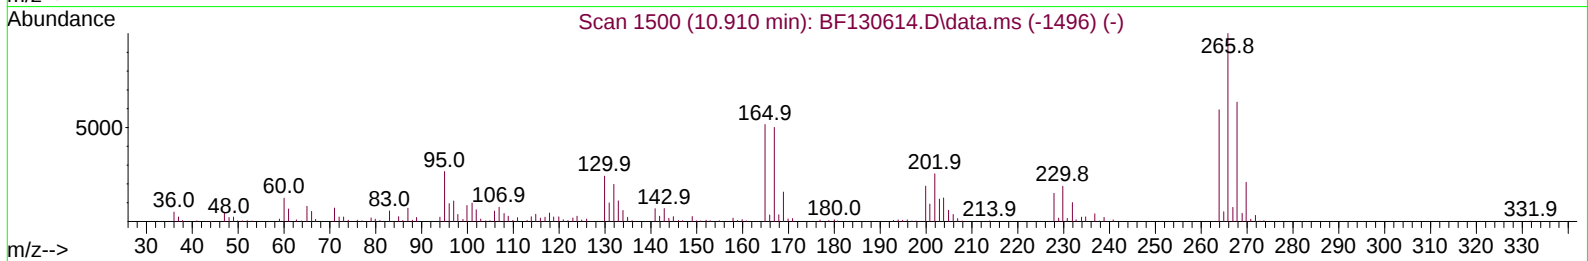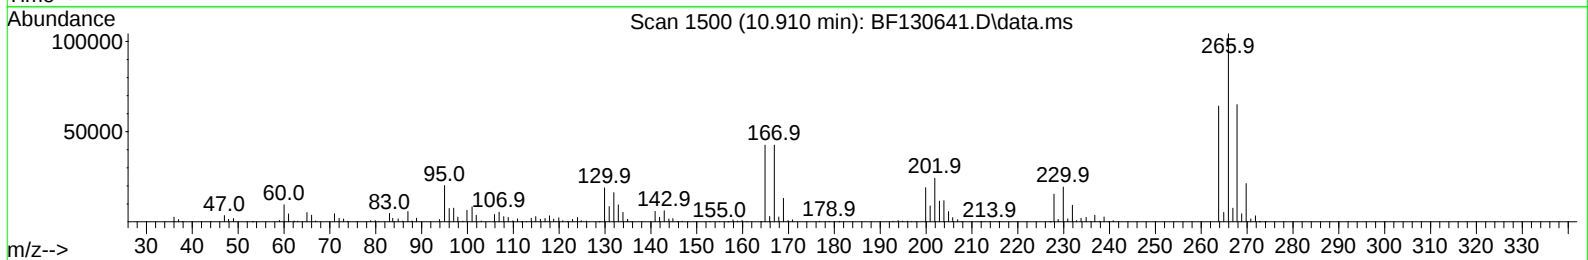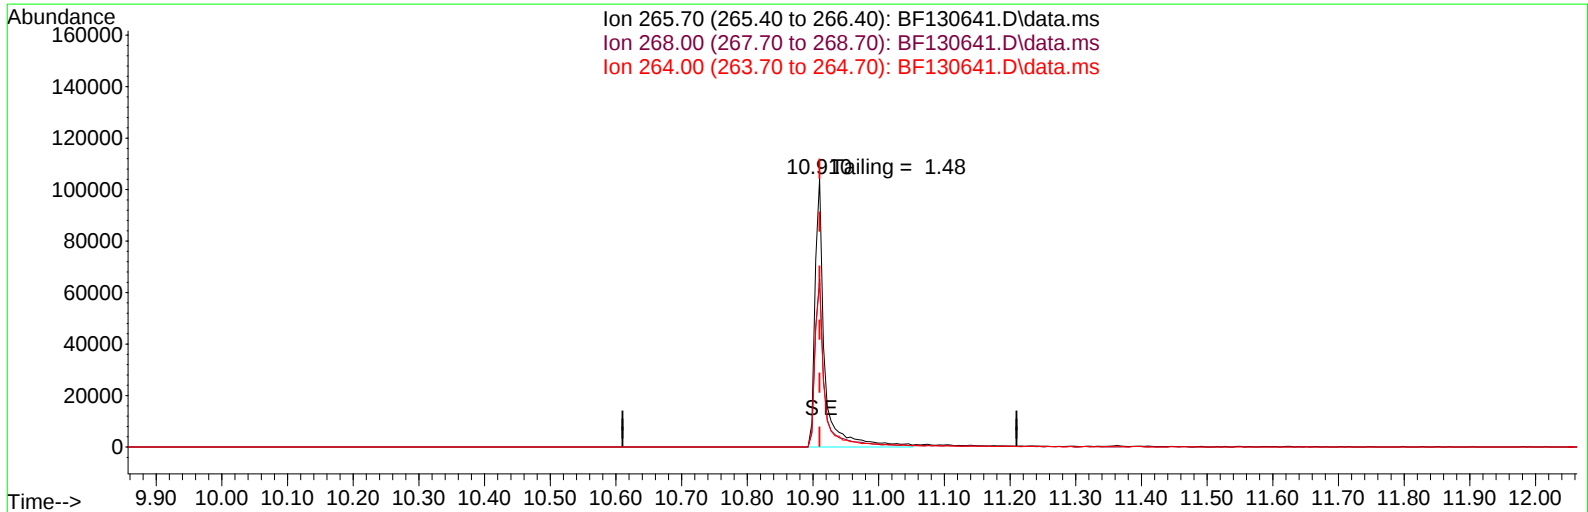

TIC: BF130641.D\data.ms

(70) Pentachlorophenol (C)

10.910min (-0.000) 37501.58 ng




response 108092

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	62.36
264.00	59.40	61.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101322\
 Data File : BF130641.D
 Acq On : 13 Oct 2022 11:14
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 14 09:14:05 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 12 06:52:52 2022
 Response via : Initial Calibration

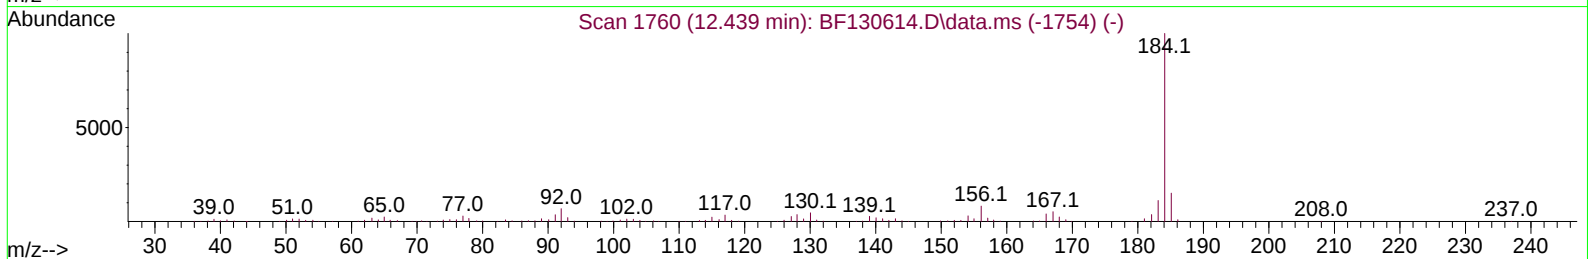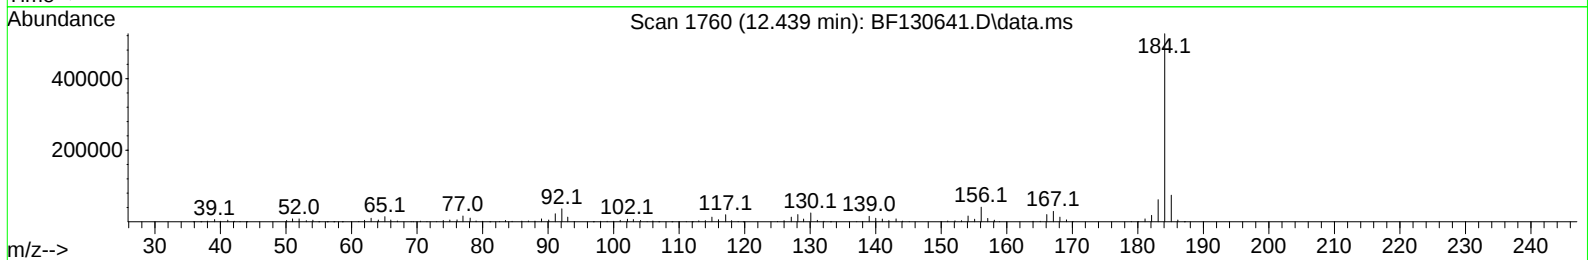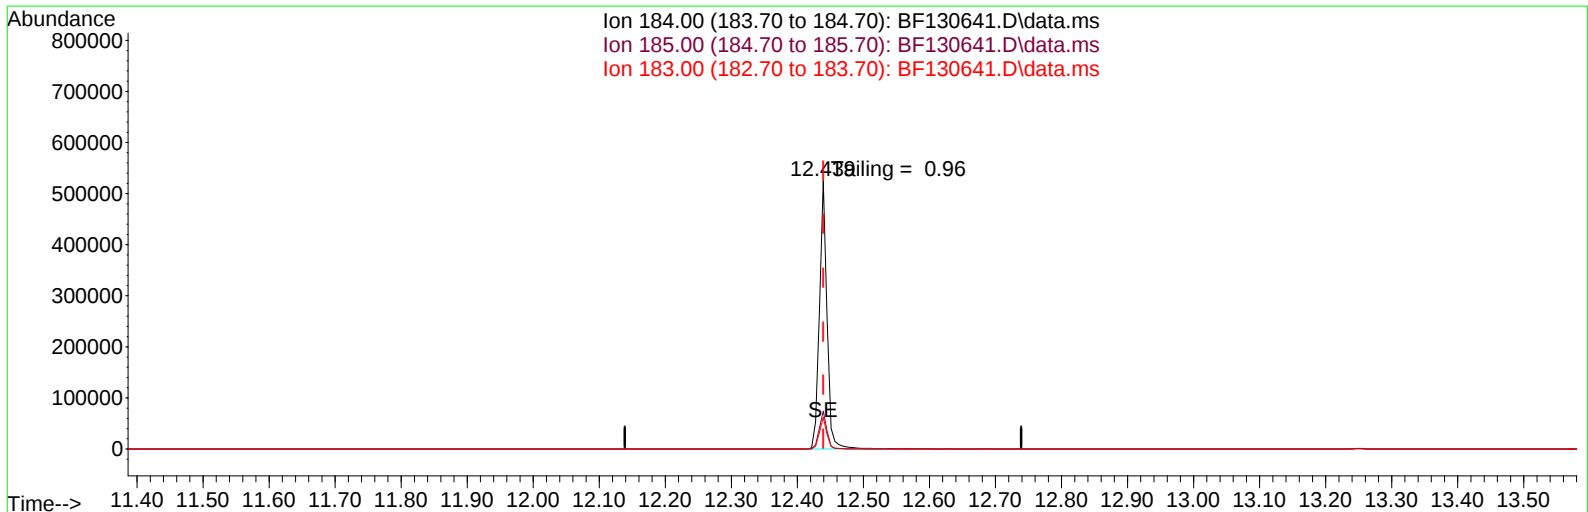

TIC: BF130641.D\data.ms

(77) Benzidine

12.439min (+ 0.000) 0.00 ng

response 423037

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.13
183.00	11.20	11.80
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/13/2022	BNA_F	<u>BF130641.D</u>
Compound Name	Response	Retention Time
DDT	273912	13.251
DDD	2420	12.98
DDE	344	12.622
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2764	276676	1.00

Instrument :
BNA_F
ClientSampleId :
DFTPP