
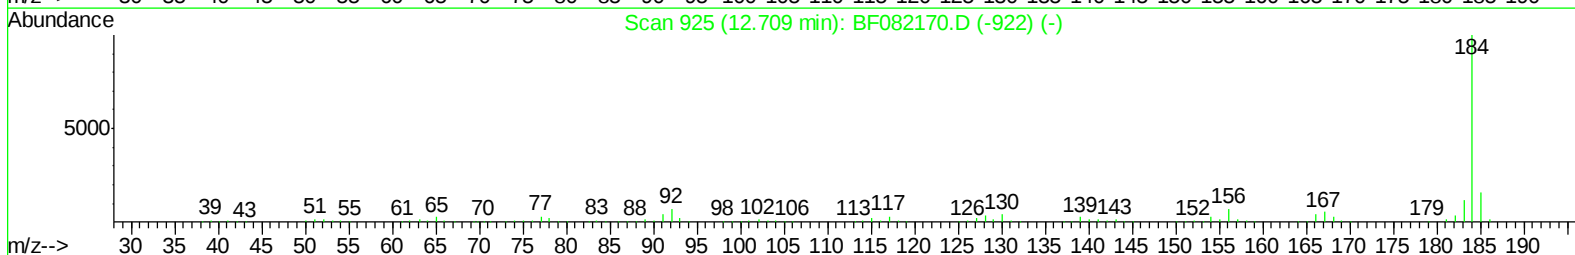
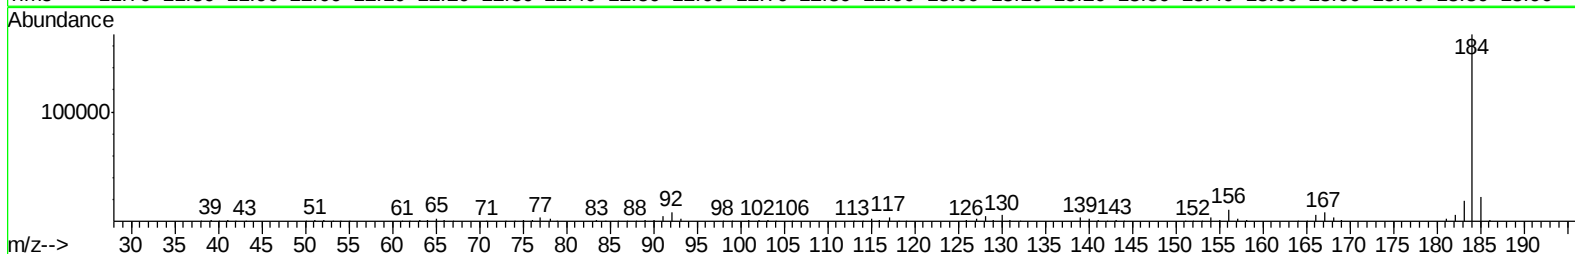


Data Path : Z:\HPCHEM1\BNA F\DATA\BF101415\  
Data File : BF082252.D  
Acq On : 13 Oct 2015 13:28  
Operator : UM/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 14 03:01:01 2015  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF101015.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Oct 14 01:15:23 2015  
Response via : Initial Calibration

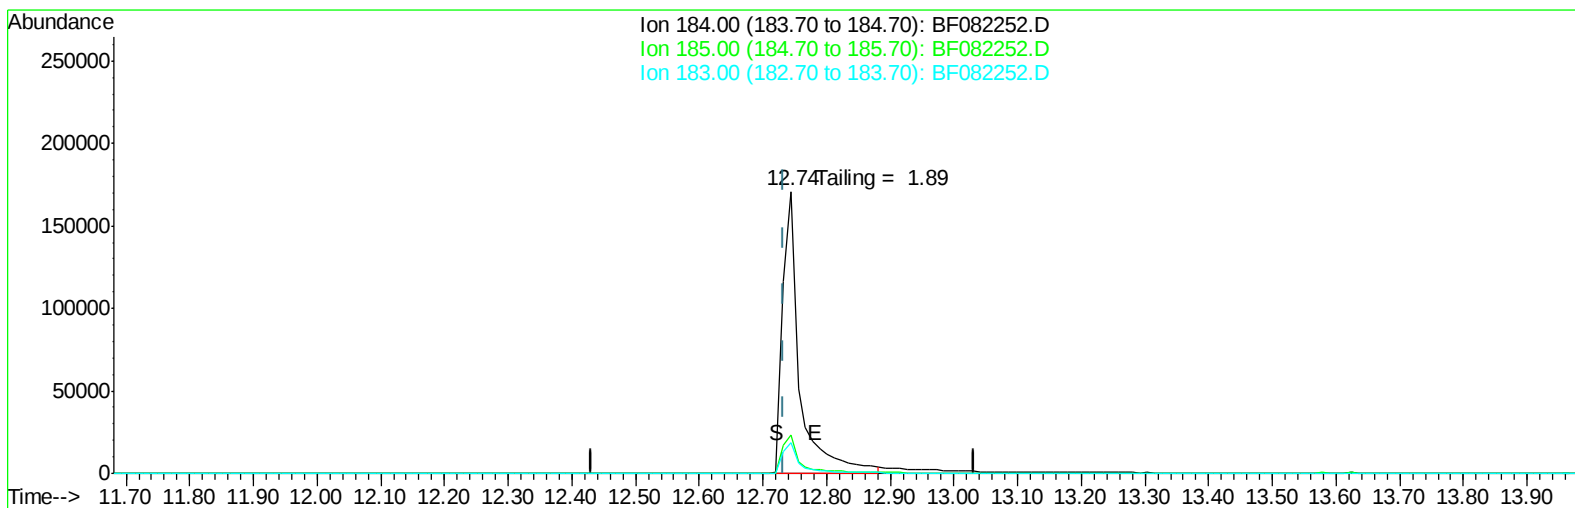

TIC: BF082252.D

(76) Benzidine




12.744min (+0.011) 0.00ng

response 327403

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.60 | 13.51 |
| 183.00 | 11.40 | 10.98 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101415\  
Data File : BF082252.D  
Acq On : 13 Oct 2015 13:28  
Operator : UM/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 14 03:01:01 2015  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF101015.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Oct 14 01:15:23 2015  
Response via : Initial Calibration

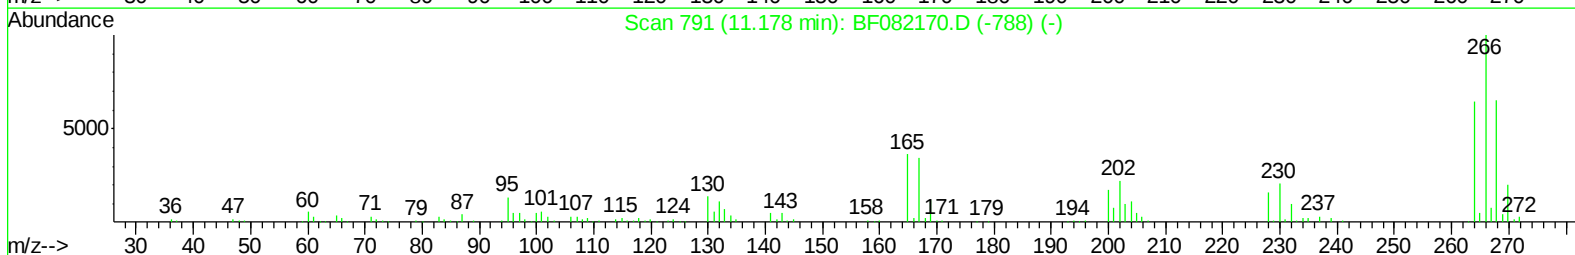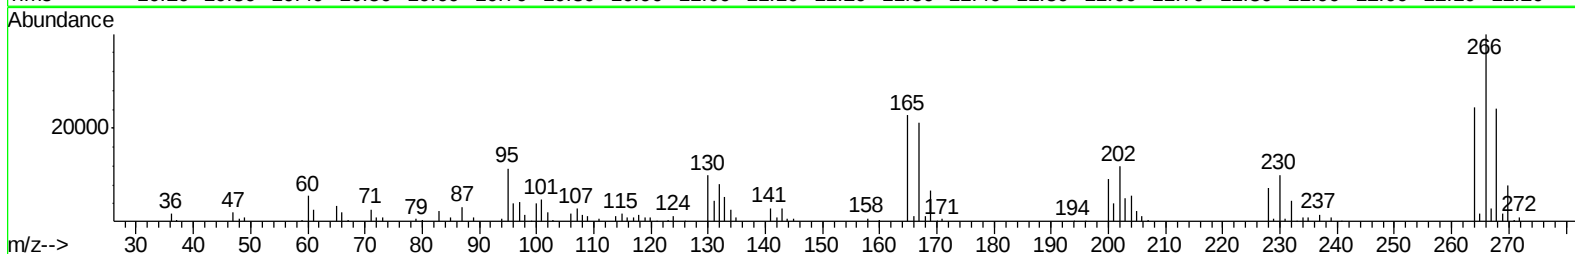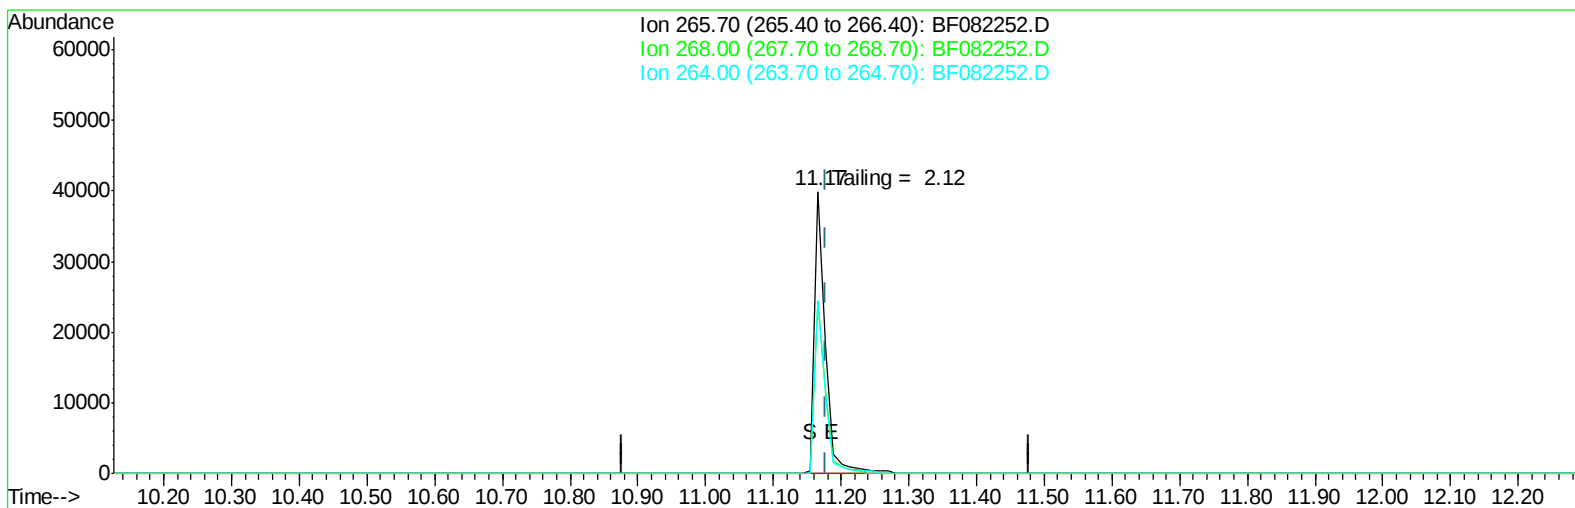

TIC: BF082252.D

(69) Pentachlorophenol (C)

11.166min (-0.011) 0.00ng

response 44972

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 65.00 | 60.82 |
| 264.00 | 64.20 | 61.52 |
| 0.00   | 0.00  | 0.00  |