
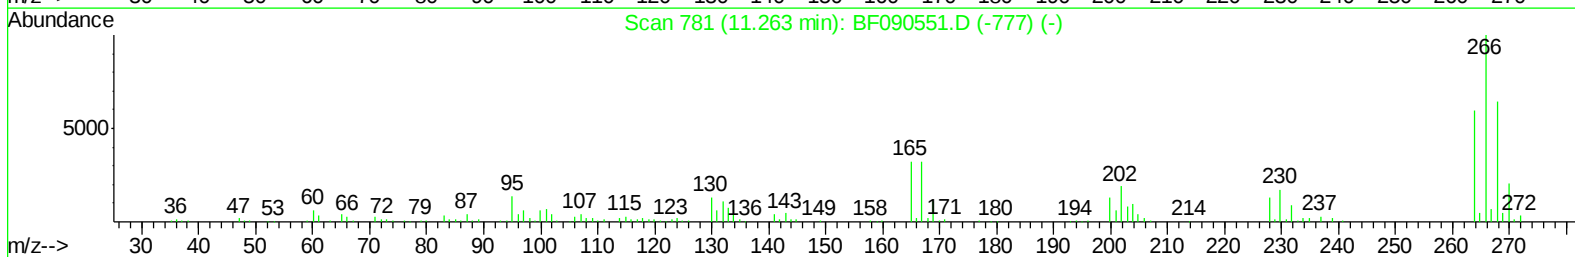
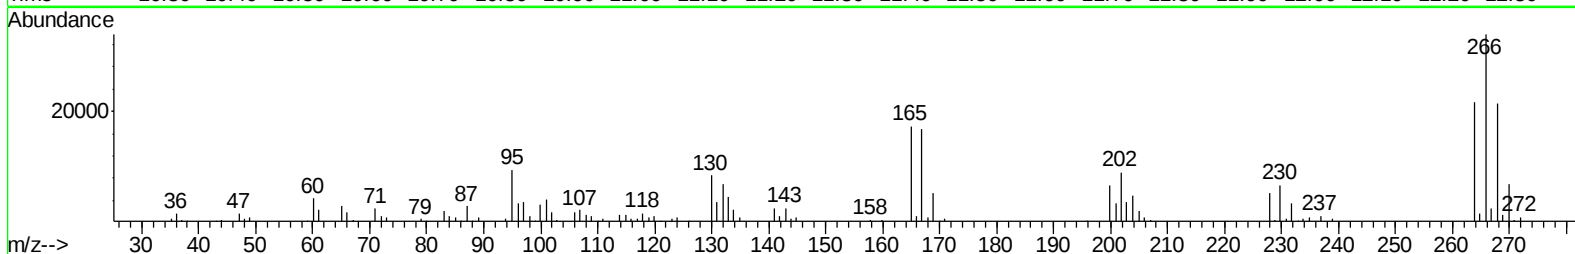


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101416\
Data File : BF090580.D
Acq On : 14 Oct 2016 22:29
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 17 02:08:20 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 14 12:44:45 2016
Response via : Initial Calibration

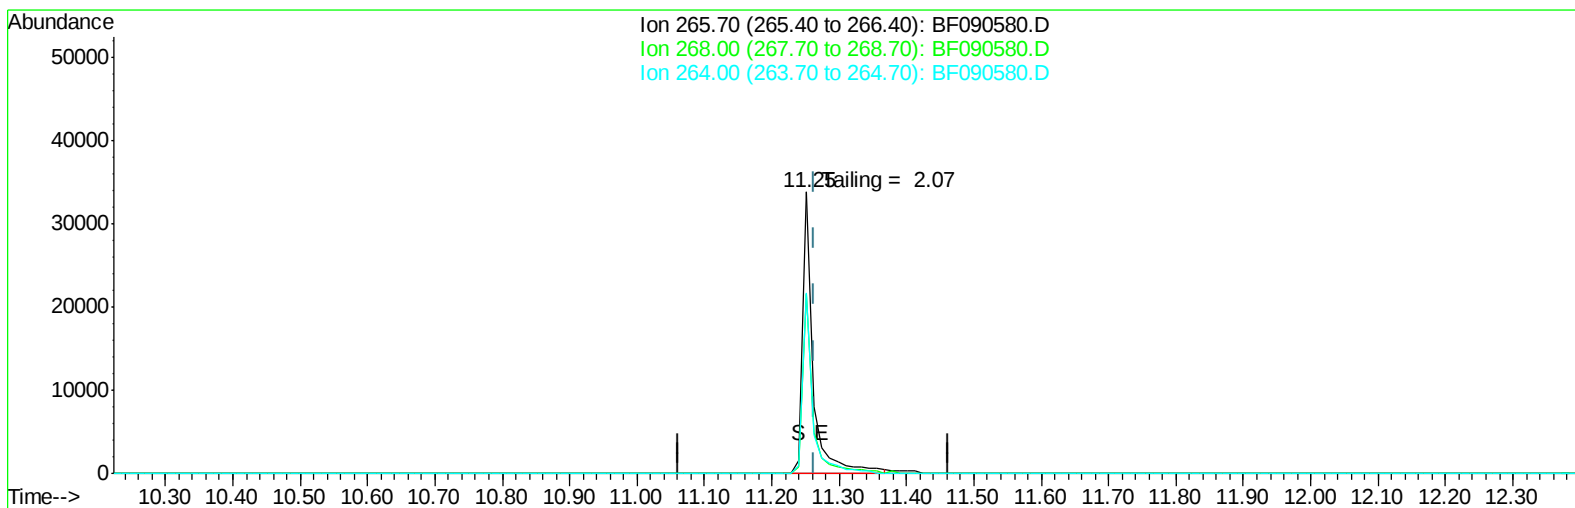

TIC: BF090580.D

(69) Pentachlorophenol (C)




11.252min (-0.011) 0.00ng

response 37482

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	63.64
264.00	59.90	63.91
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101416\
Data File : BF090580.D
Acq On : 14 Oct 2016 22:29
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 17 02:08:20 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 14 12:44:45 2016
Response via : Initial Calibration

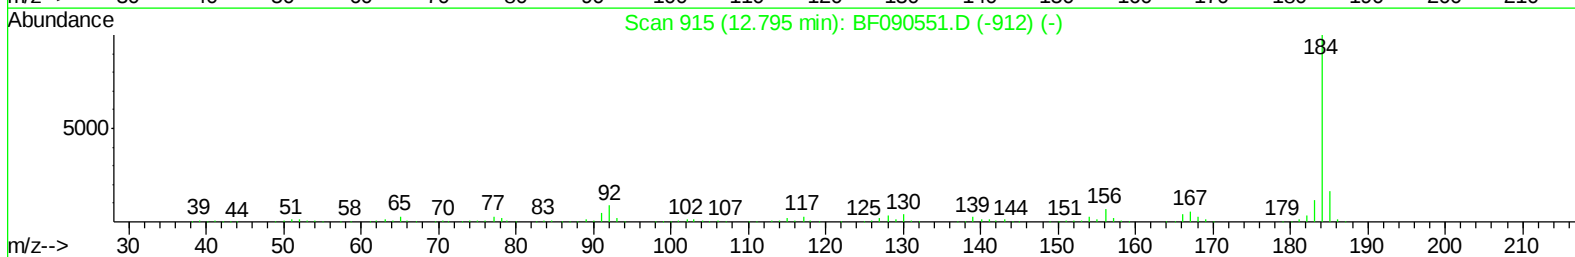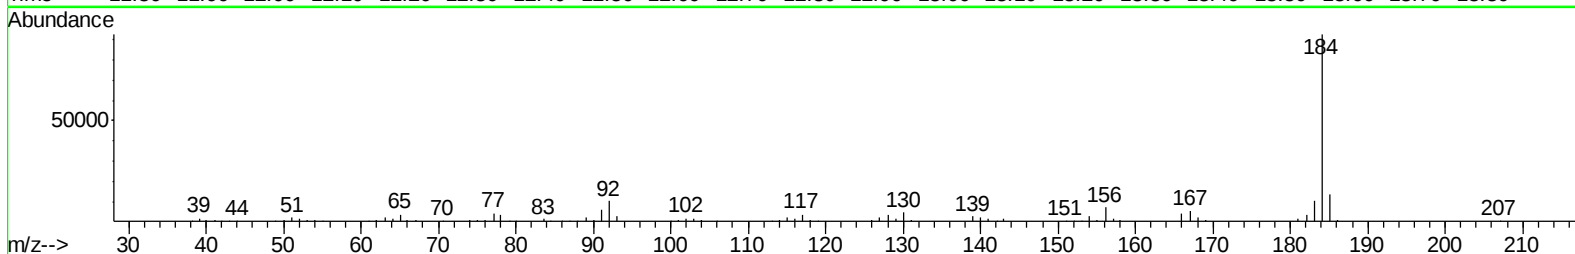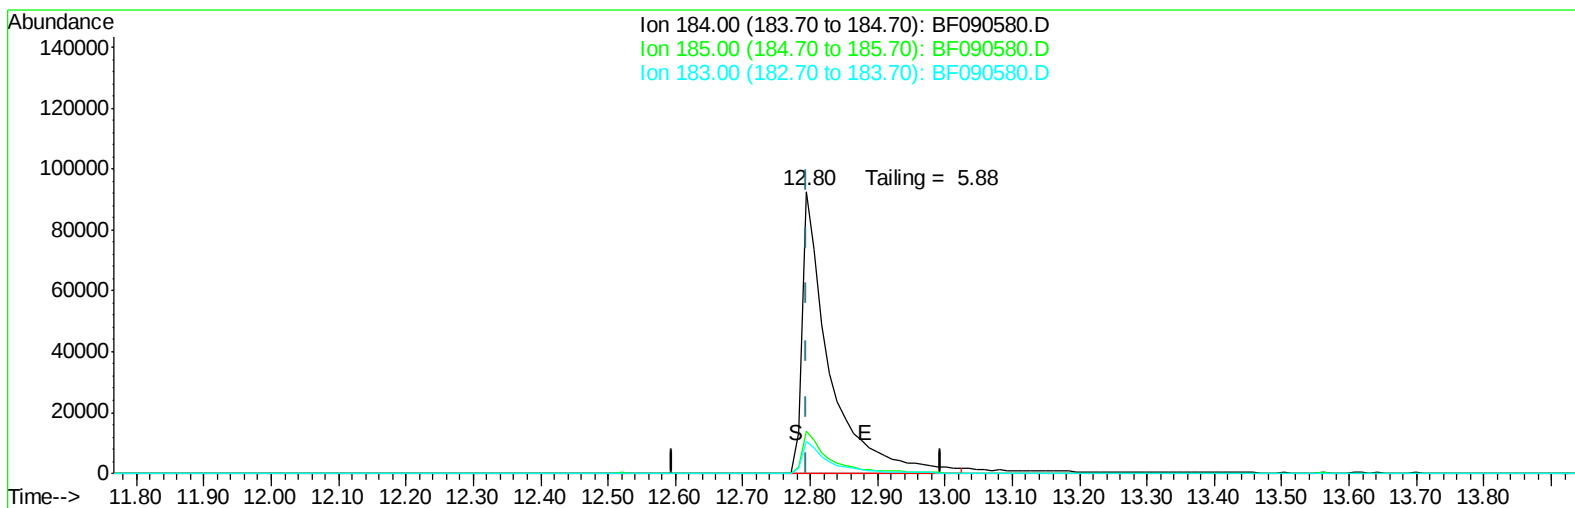

TIC: BF090580.D

(76) Benzidine

12.795min (+0.000) 0.00ng

response 247011

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.82
183.00	11.70	11.33
0.00	0.00	0.00