

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101416\
 Data File : BF090582.D
 Acq On : 15 Oct 2016 3:05
 Operator : UM/SJ
 Sample : PB94073BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB94073BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.114	240	243	253	rBV	1033796	1514890	23.02%	2.949%
2	5.526	276	279	282	rBV	3969536	5588125	84.91%	10.879%
3	6.554	366	369	378	rBV	4512207	5793615	88.03%	11.279%
4	6.691	378	381	383	rBV	4944379	6205894	94.30%	12.081%
5	6.920	398	401	412	rBV	881720	1127477	17.13%	2.195%
6	7.069	412	414	417	rBV	3413554	4685662	71.20%	9.122%
7	7.480	447	450	471	rBV	2869831	4175163	63.44%	8.128%
8	8.200	511	513	522	rBV	1231505	1580894	24.02%	3.078%
9	8.314	522	523	537	rVB2	28769	89048	1.35%	0.173%
10	9.286	605	608	610	rBV	6471991	6581288	100.00%	12.812%
11	9.960	665	667	670	rBV	1853472	1651433	25.09%	3.215%
12	10.749	734	736	739	rBV2	2594459	3278546	49.82%	6.382%
13	11.446	795	797	810	rBV	1119532	1503691	22.85%	2.927%
14	13.035	934	936	939	rBV	3761040	5643603	85.75%	10.987%
15	14.086	1026	1028	1042	rBV	598126	988430	15.02%	1.924%
16	15.549	1153	1156	1169	rBV	562988	960179	14.59%	1.869%




Sum of corrected areas: 51367938

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101416\
Data File : BF090582.D
Acq On : 15 Oct 2016 3:05
Operator : UM/SJ
Sample : PB94073BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB94073BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

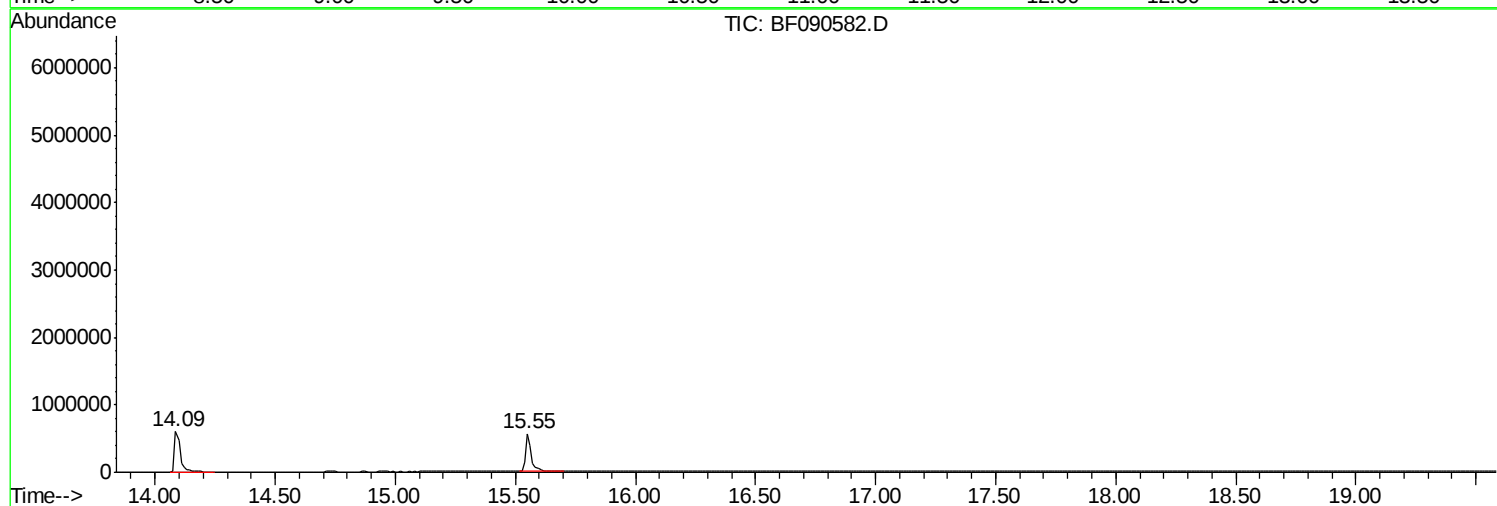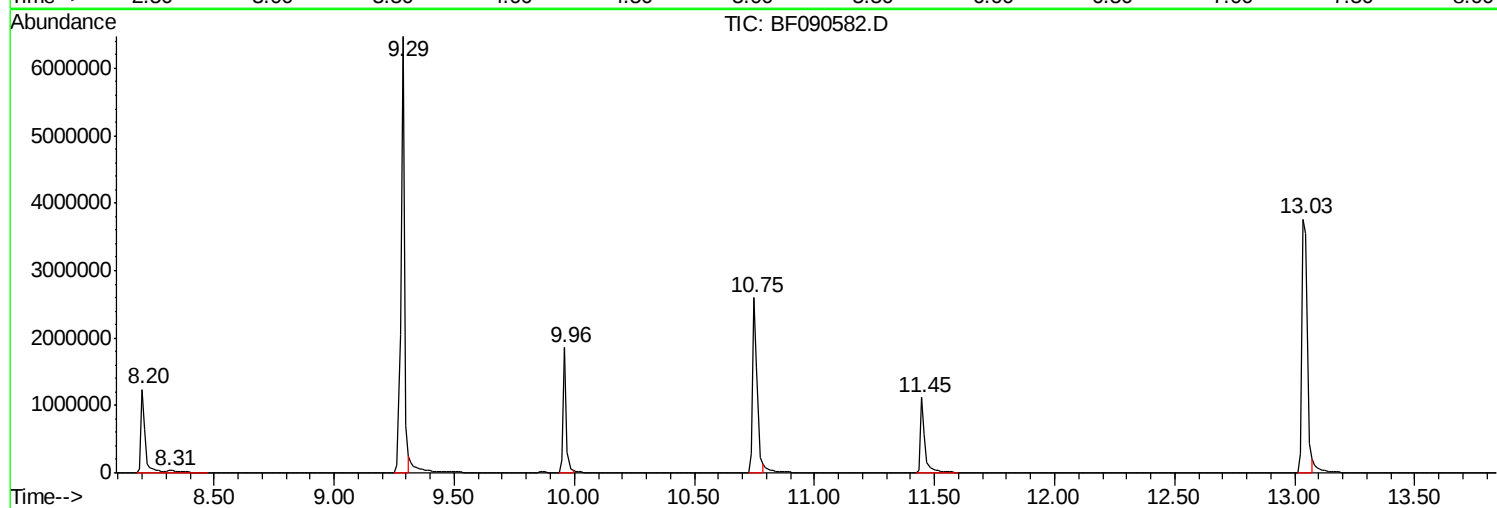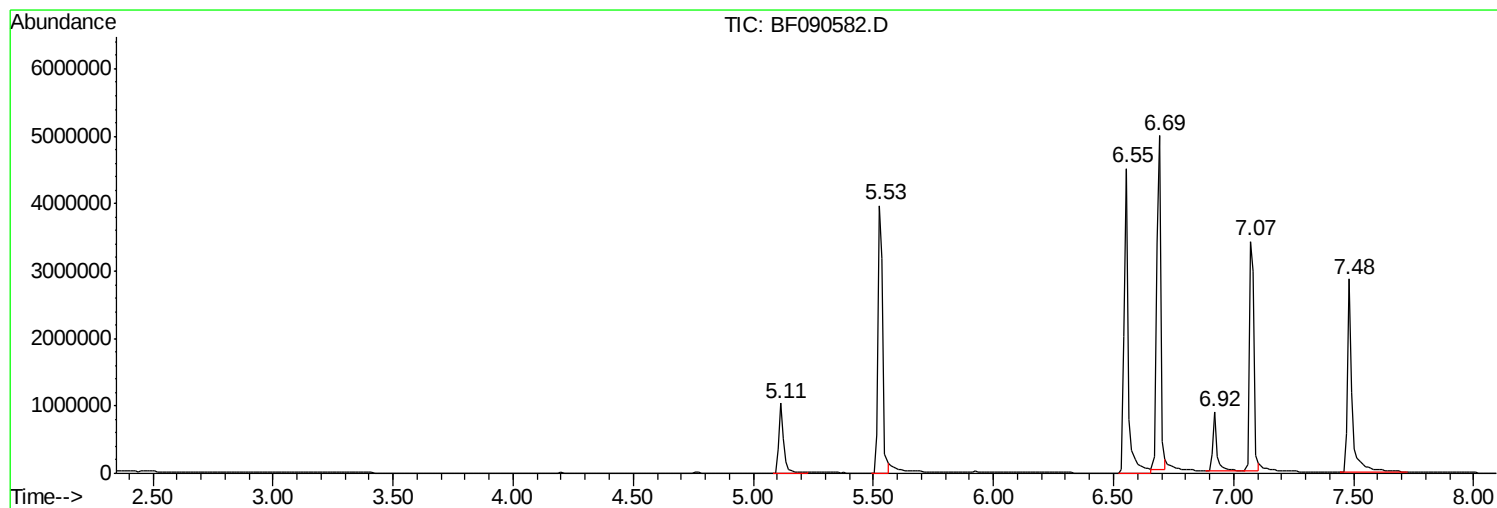

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101416\
Data File : BF090582.D
Acq On : 15 Oct 2016 3:05
Operator : UM/SJ
Sample : PB94073BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB94073BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.11	26.87 ng	1514890	1,4-Dichlorobenzene-d4	6.92

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64
2		Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	28
3		Acetic acid, cyano-, 1,1-dimethyl...	141	C7H11NO2	001116-98-9	23
4		Acetone	58	C3H6O	000067-64-1	9
5		5-Hexen-2-one	98	C6H10O	000109-49-9	9

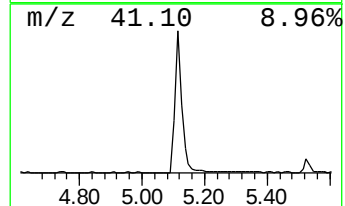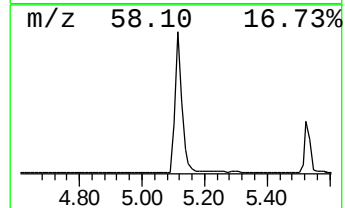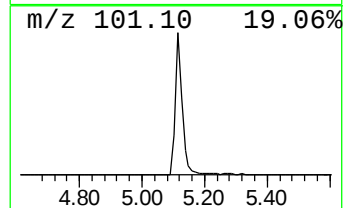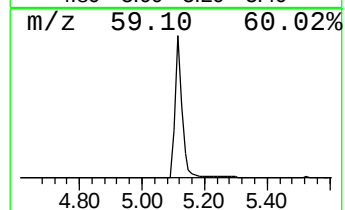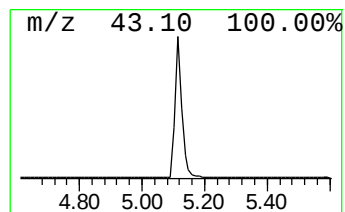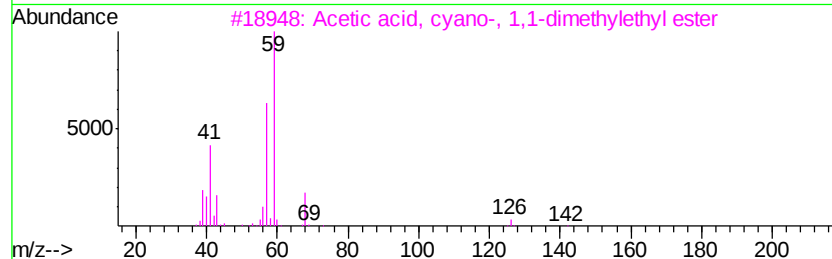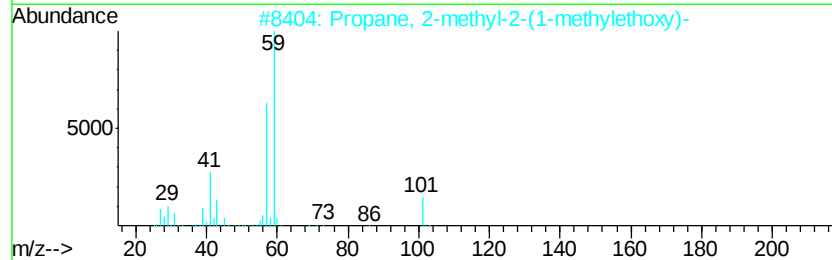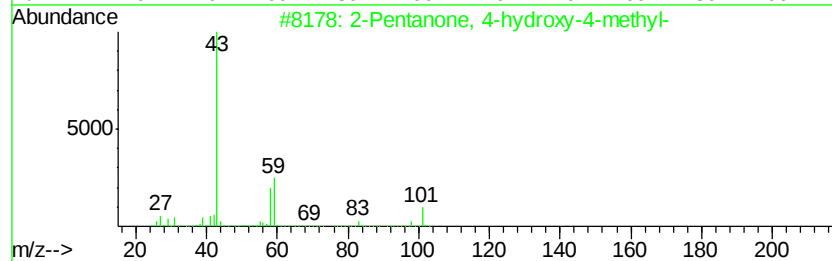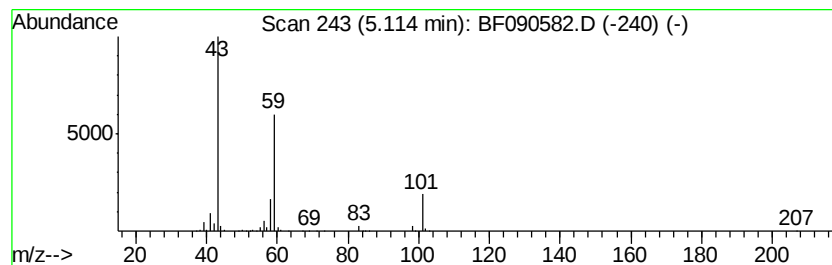

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101416\
Data File : BF090582.D
Acq On : 15 Oct 2016 3:05
Operator : UM/SJ
Sample : PB94073BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB94073BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.69 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.69	110.09 ng	6205890	1,4-Dichlorobenzene-d4	6.92

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
2	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
3	Amphetaminil	250	C17H18N2	017590-01-1	10
4	2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9
5	4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9

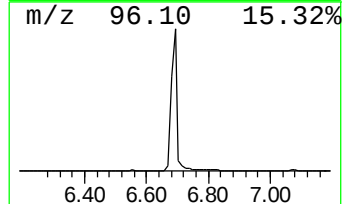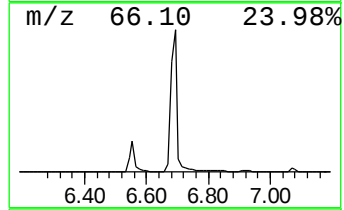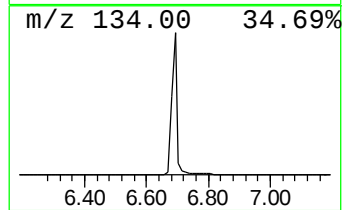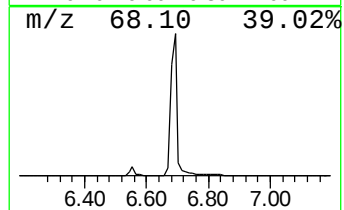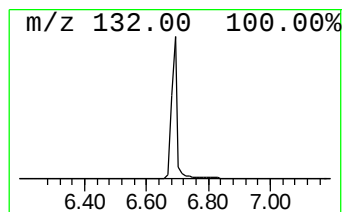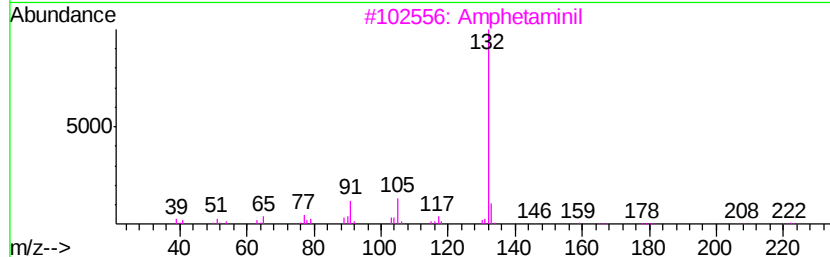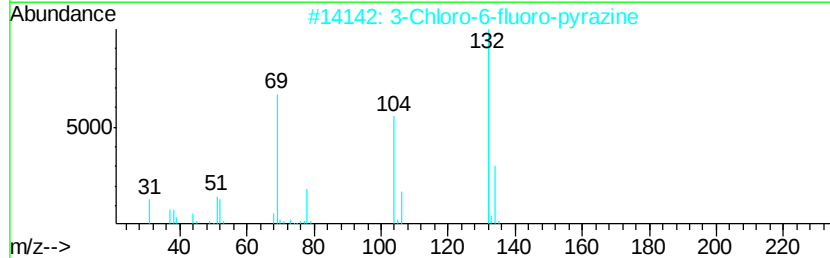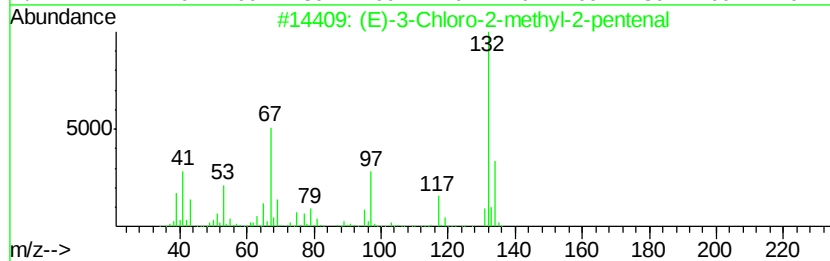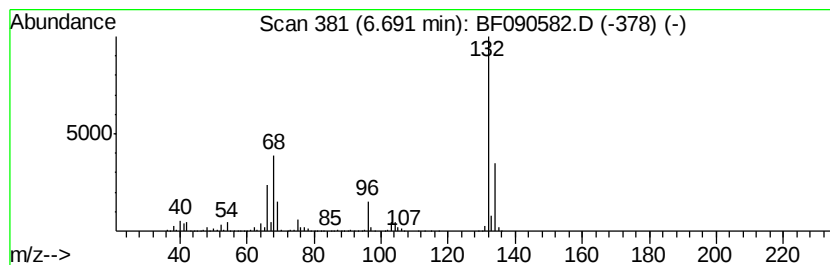

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101416\
Data File : BF090582.D
Acq On : 15 Oct 2016 3:05
Operator : UM/SJ
Sample : PB94073BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB94073BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.11	26.9	ng	1514890	1	6.92	1127480	20.0
unknown6.69	6.69	110.1	ng	6205890	1	6.92	1127480	20.0