


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101416\
 Data File : BF090580.D
 Acq On : 14 Oct 2016 22:29
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 14 12:44:45 2016

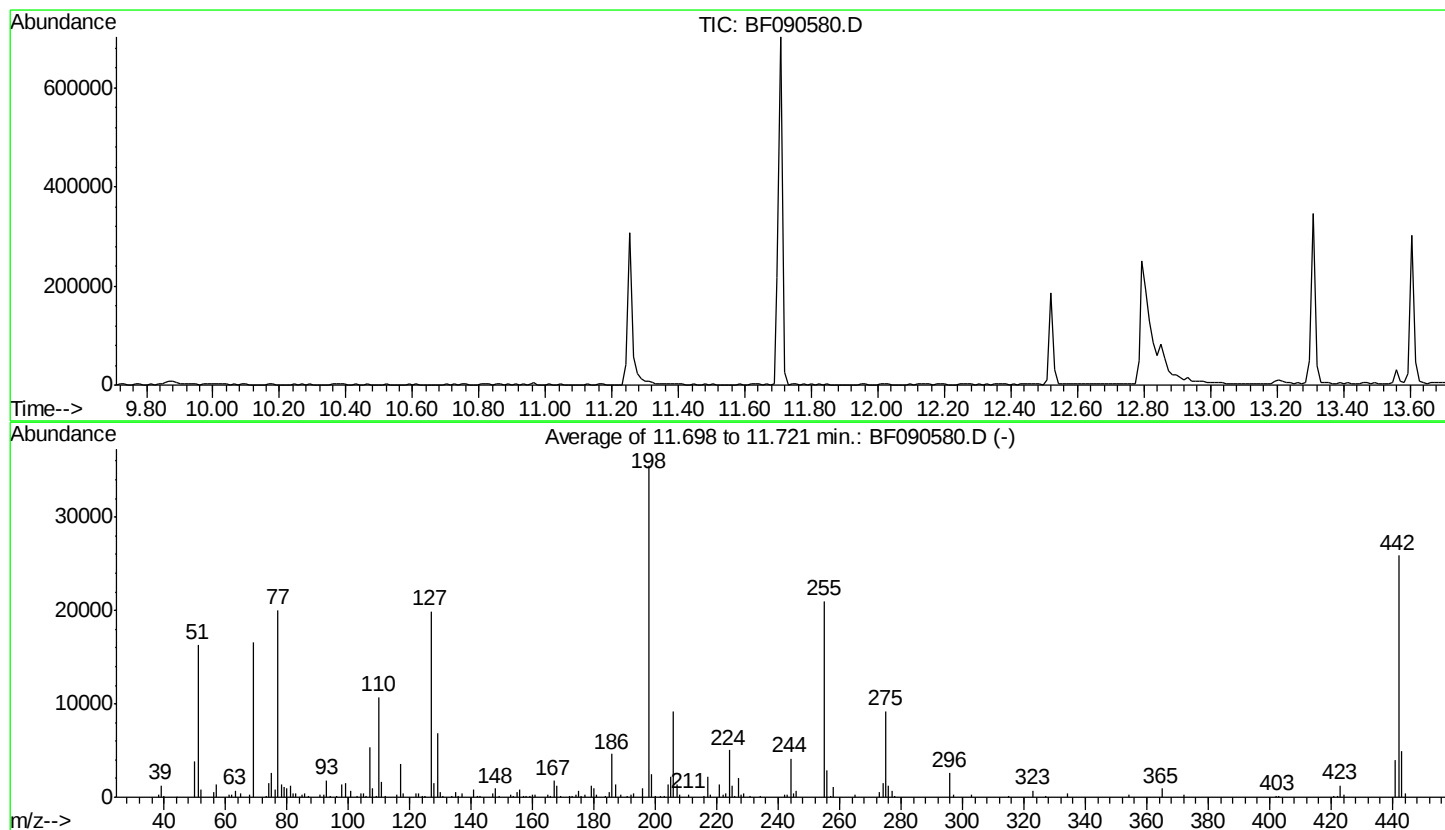

AutoFind: Scans 819, 820, 821; Background Corrected with Scan 816

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.0	16347	PASS
68	69	0.00	2	1.7	286	PASS
69	198	0.00	100	46.6	16539	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	56.0	19903	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	35514	PASS
199	198	5	9	6.8	2413	PASS
275	198	10	60	25.9	9193	PASS
365	198	1	100	2.7	949	PASS
441	442	0.01	24	15.6	4034	PASS
442	198	50	100	72.8	25849	PASS
443	442	15	24	19.0	4907	PASS