

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF101417\
 Data File : BF099485.D
 Acq On : 14 Oct 2017 19:09
 Operator : SJ/JU
 Sample : I5865-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Oct 14 22:08:10 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 11 16:25:21 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.85	152	87198	20.00	ng	0.00
21) Naphthalene-d8	8.13	136	362918	20.00	ng	0.00
38) Acenaphthene-d10	9.89	164	164570	20.00	ng	0.00
63) Phenanthrene-d10	11.37	188	288784	20.00	ng	0.00
75) Chrysene-d12	14.02	240	176505	20.00	ng	0.00
86) Perylene-d12	15.49	264	138875	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.48	112	574926	104.96	ng	0.01
7) Phenol-d6	6.49	99	697172	103.17	ng	0.00
23) Nitrobenzene-d5	7.42	82	413064	72.99	ng	0.00
41) 2,4,6-Tribromophenol	10.68	330	134090	99.57	ng	0.00
44) 2-Fluorobiphenyl	9.21	172	796268	80.77	ng	0.00
78) Terphenyl-d14	12.96	244	655263	84.43	ng	0.00
Target Compounds						
9) Benzaldehyde	6.63	77	11584	2.955	ng	85
10) Phenol	6.50	94	37066	4.905	ng	85
19) n-Nitroso-di-n-propylamine	7.42	70	52557	12.182	ng	# 74
25) Isophorone	7.42	82	413059	35.304	ng	# 64
49) Dimethylphthalate	9.60	163	181689	14.628	ng	99
56) 2,4-Dinitrotoluene	9.89	165	20771	5.919	ng	# 22
62) Azobenzene	10.60	77	33680	3.018	ng	# 1
66) 4-Bromophenyl-phenylether	10.68	248	8724	3.086	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF101417\
Data File : BF099485.D
Acq On : 14 Oct 2017 19:09
Operator : SJ/JU
Sample : I5865-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Oct 14 22:08:10 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 11 16:25:21 2017
Response via : Initial Calibration

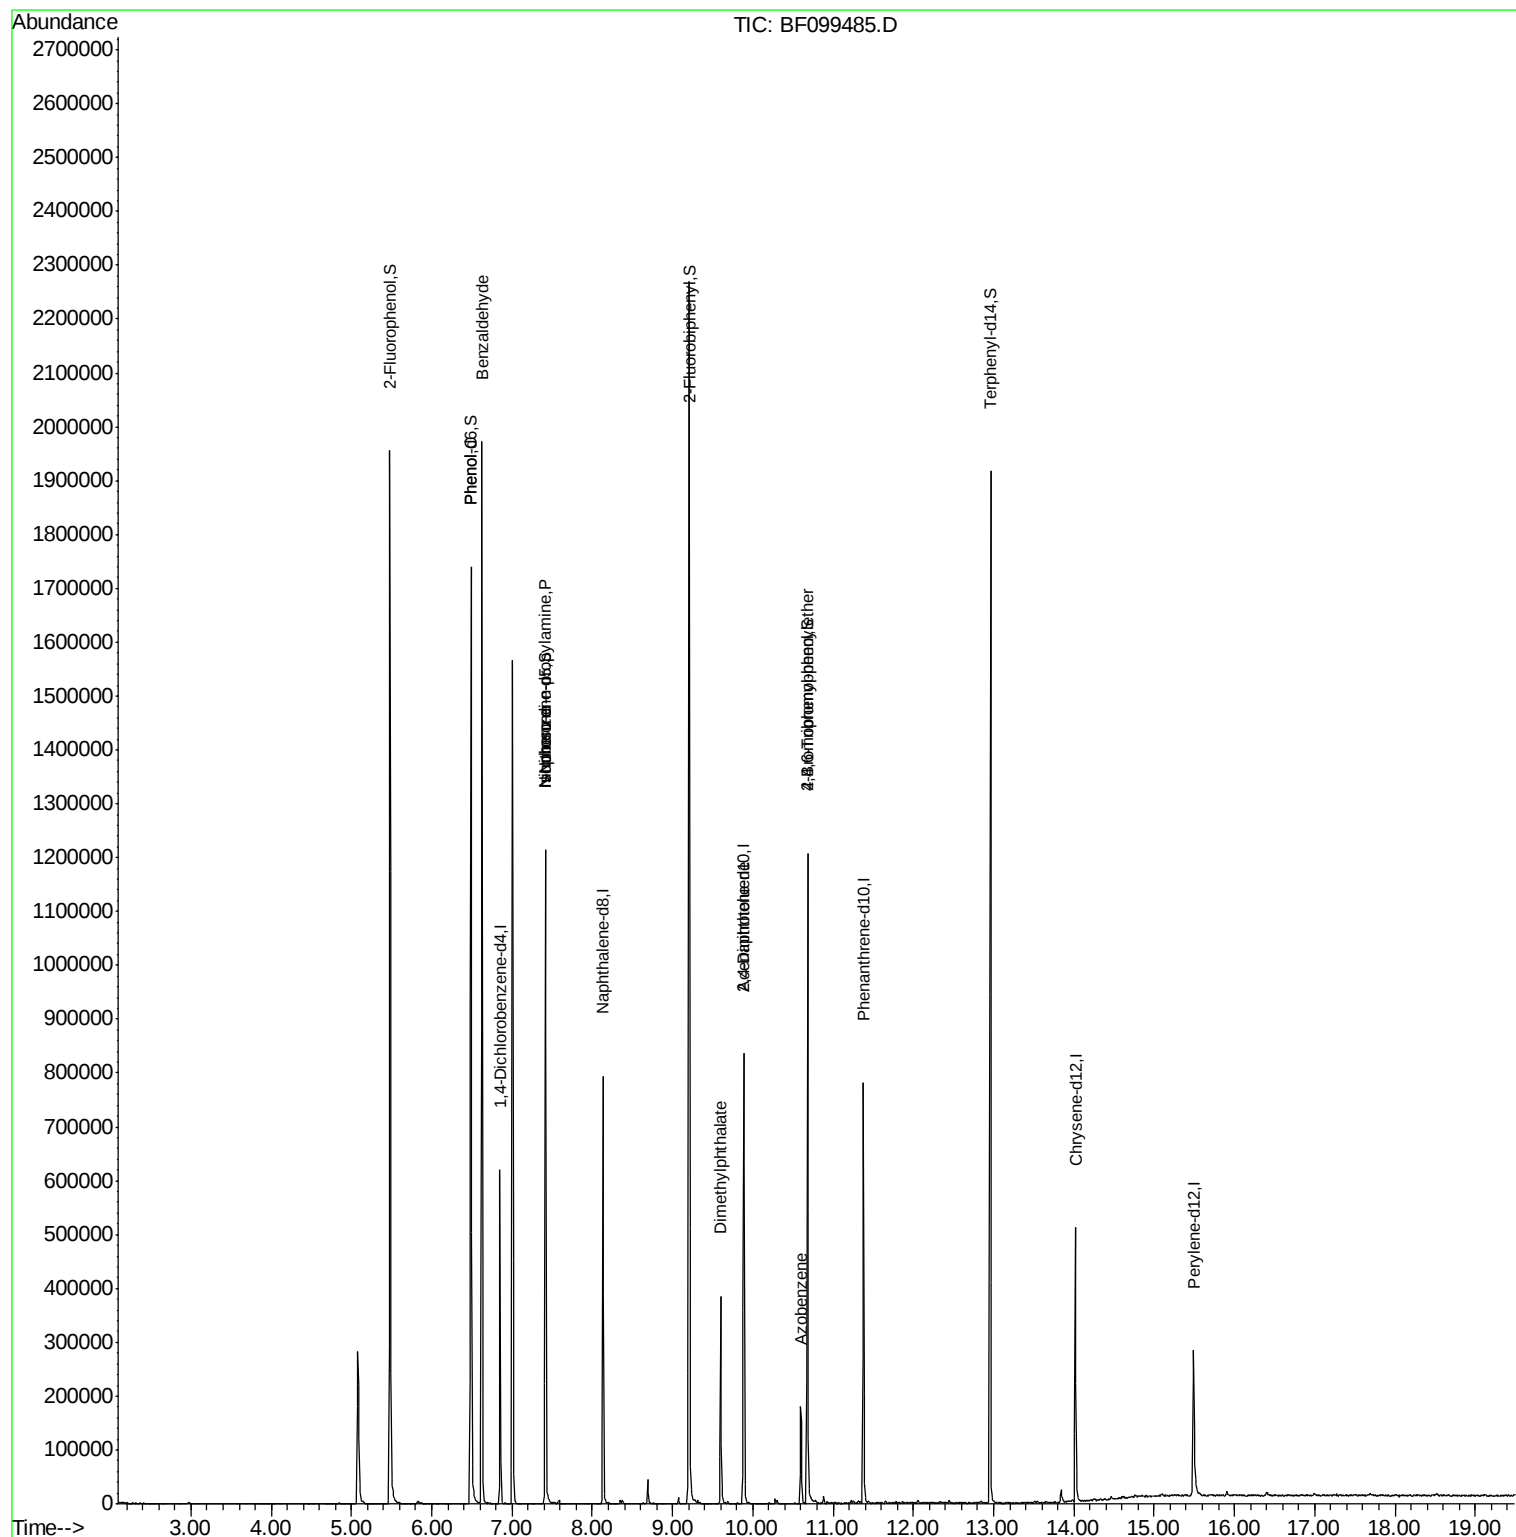

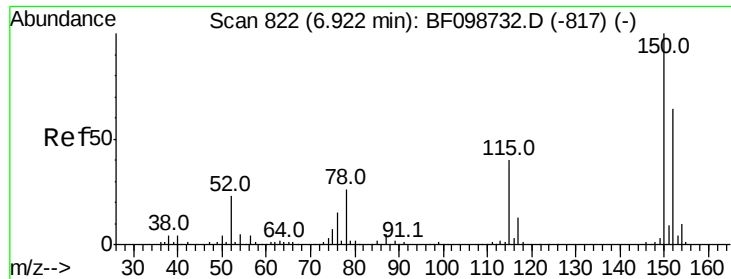


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.85 min Scan# 810
Delta R.T. -0.00 min
Lab File: BF099485.D
Acq: 14 Oct 2017 19:09

Instrument :
BNA_F
ClientSampled :

Tot Ion:152 Resp: 87198
Ion Ratio Lower Upper
152 100
150 159.0 124.6 186.8
115 59.3 50.1 75.1

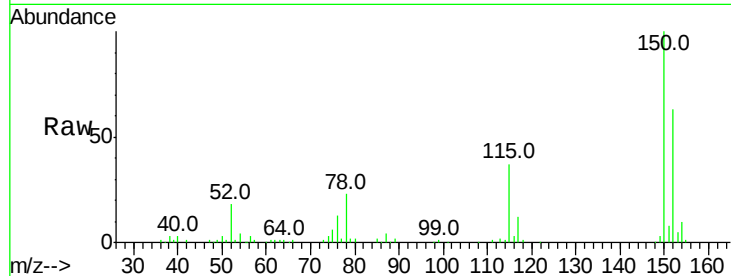


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

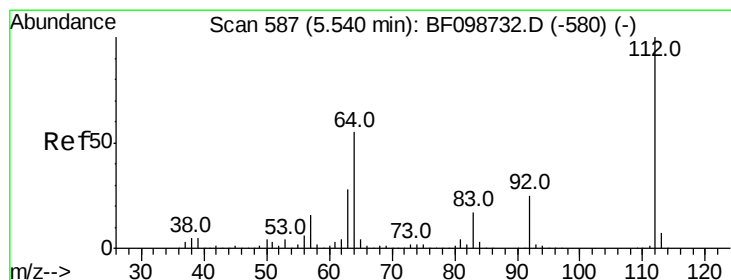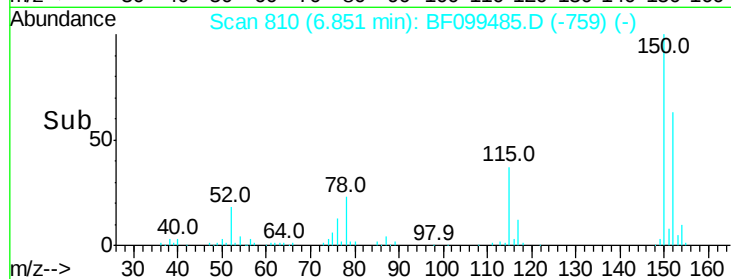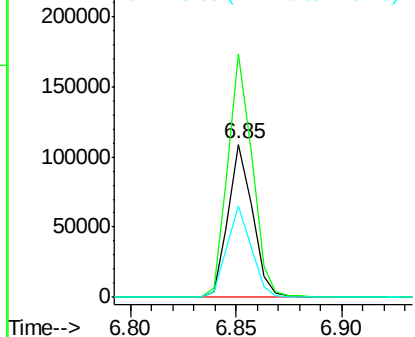



#5


2-Fluorophenol
Concen: 104.959 ng
RT: 5.48 min Scan# 577
Delta R.T. 0.01 min
Lab File: BF099485.D
Acq: 14 Oct 2017 19:09

Tgt Ion:112 Resp: 574926
Ion Ratio Lower Upper
112 100
64 55.2 47.9 71.9
63 26.9 23.7 35.5



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

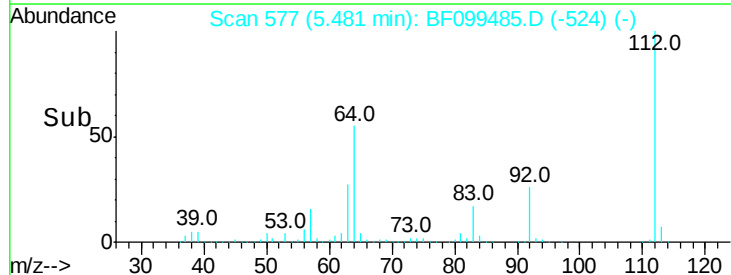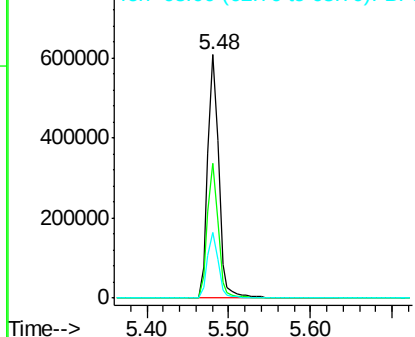

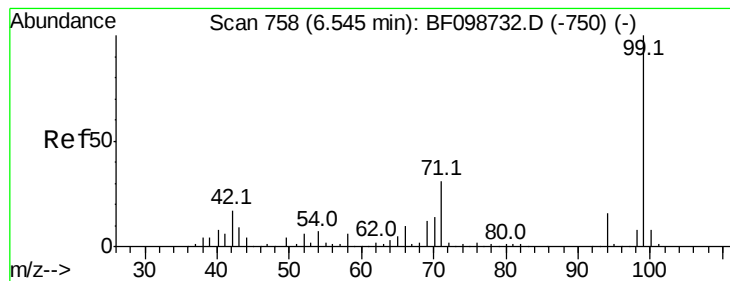

#7

Phenol-d6

Concen: 103.174 ng

RT: 6.49 min Scan# 749

Delta R.T. 0.01 min

Lab File: BF099485.D

Acq: 14 Oct 2017 19:09

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 99 Resp: 697172

Ion Ratio Lower Upper

99 100

42 14.7 14.5 21.7




71 29.5 25.4 38.0

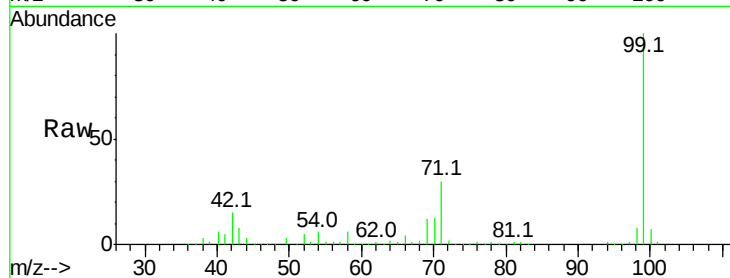

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

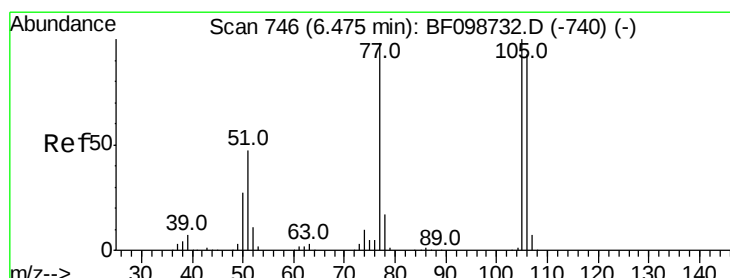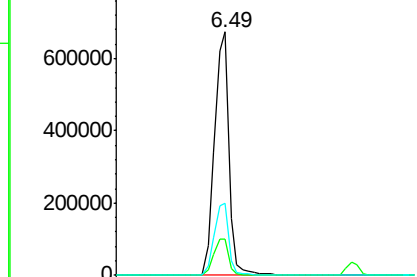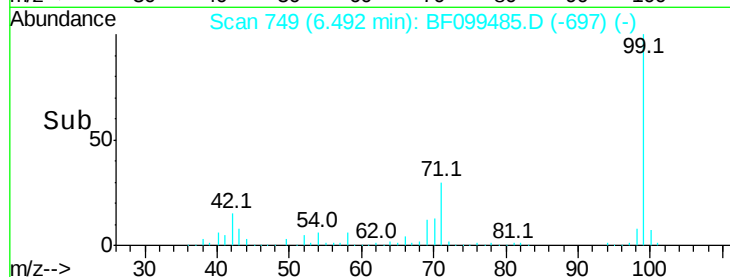

#9

Benzaldehyde

Concen: 2.955 ng

RT: 6.63 min Scan# 772

Delta R.T. 0.22 min

Lab File: BF099485.D

Acq: 14 Oct 2017 19:09


Tgt Ion: 77 Resp: 11584

Ion Ratio Lower Upper

77 100

105 81.7 81.1 121.1



106 84.6 74.5 114.5

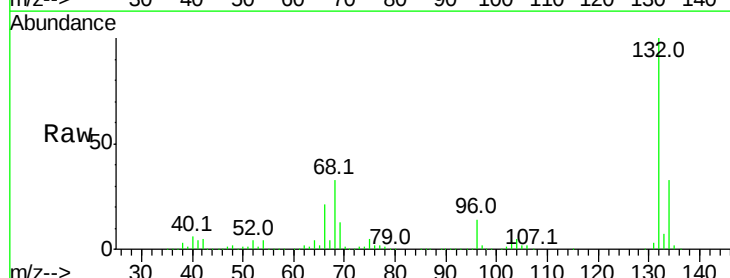


Abundance Ion 77.00 (76.70 to 77.70): BF0

Ion 105.00 (104.70 to 105.70): B

Ion 106.00 (105.70 to 106.70): B



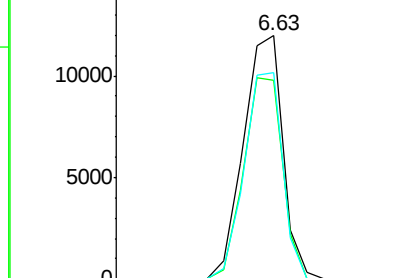
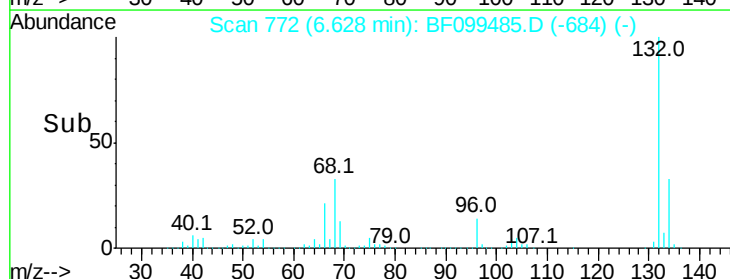


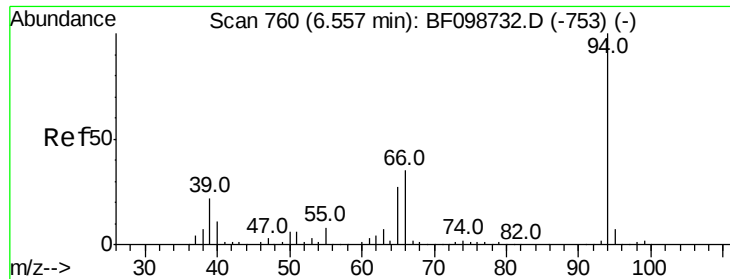

#10
Phenol
Concen: 4.905 ng
RT: 6.50 min Scan# 750
Delta R.T. -0.00 min
Lab File: BF099485.D
Acq: 14 Oct 2017 19:09




Instrument :
BNA_F
ClientSampled :


Tot Ion: 94 Resp: 37066
Ion Ratio Lower Upper
94 100
65 30.2 7.9 47.9
66 49.4 16.2 56.2

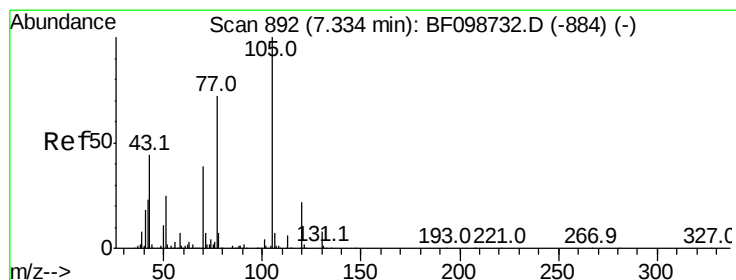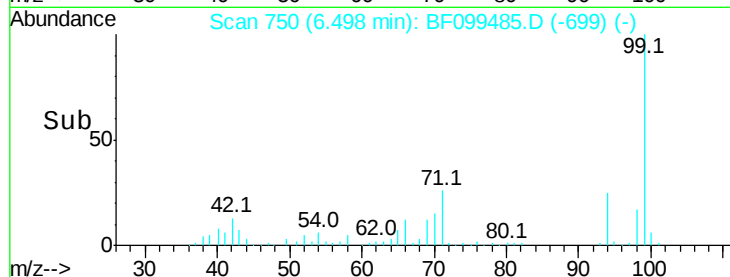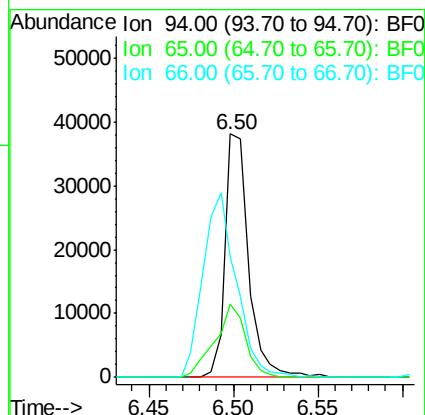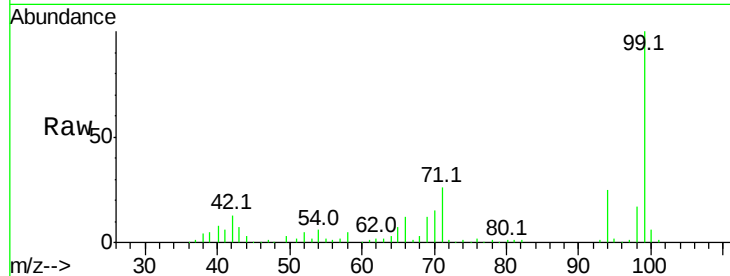

#19
n-Nitroso-di-n-propylamine
Concen: 12.182 ng
RT: 7.42 min Scan# 906
Delta R.T. 0.15 min
Lab File: BF099485.D
Acq: 14 Oct 2017 19:09

Tgt Ion: 70 Resp: 52557
Ion Ratio Lower Upper
70 100
42 43.8 47.5 71.3#
101 0.0 7.4 11.2#
130 2.4 16.6 25.0#

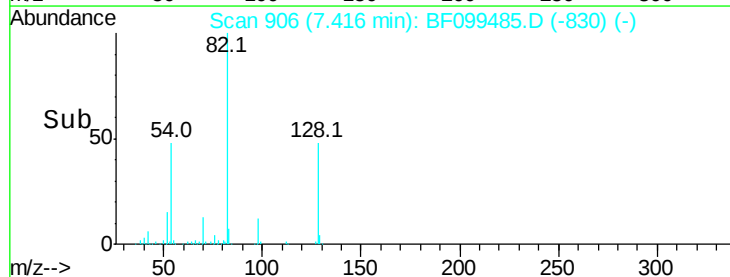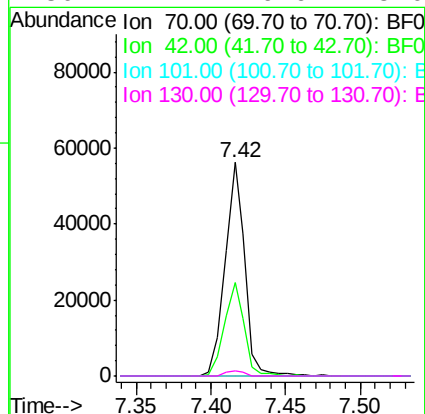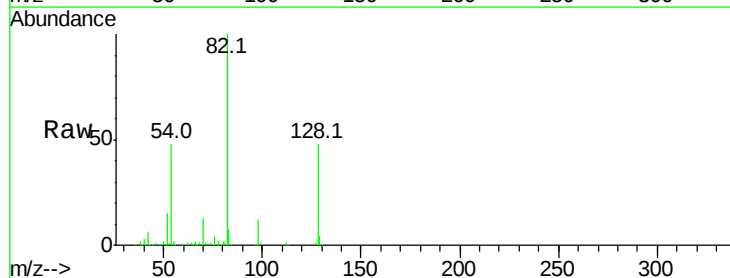


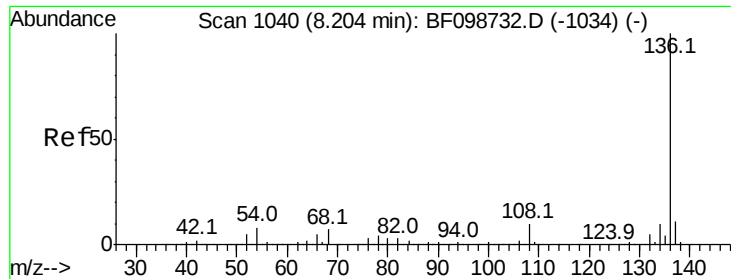




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.13 min Scan# 1028
Delta R.T. -0.00 min
Lab File: BF099485.D
Acq: 14 Oct 2017 19:09

Instrument :
BNA_F
ClientSampleId :

Tot Ion:	136	Resp:	362918
Ion	Ratio	Lower	Upper
136	100		
137	10.9	8.9	13.3
54	7.1	6.6	9.8
68	5.7	5.0	7.4




Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

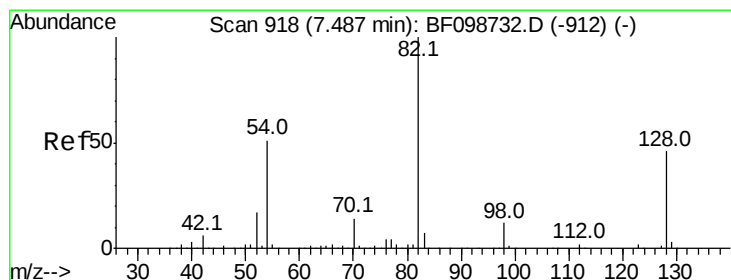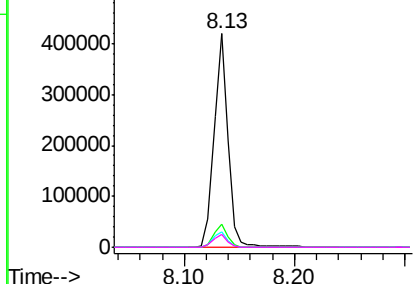
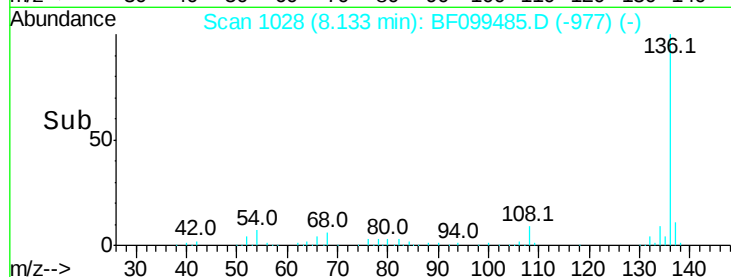



#23
Nitrobenzene-d5
Concen: 72.991 ng
RT: 7.42 min Scan# 906
Delta R.T. -0.01 min
Lab File: BF099485.D
Acq: 14 Oct 2017 19:09

Tgt Ion:	82	Resp:	413064
Ion	Ratio	Lower	Upper
82	100		
128	48.1	36.1	54.1
54	47.6	41.4	62.2

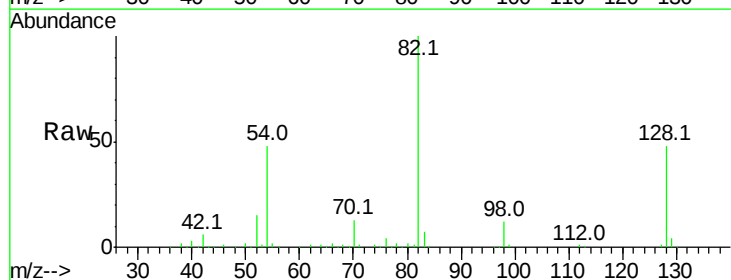

Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

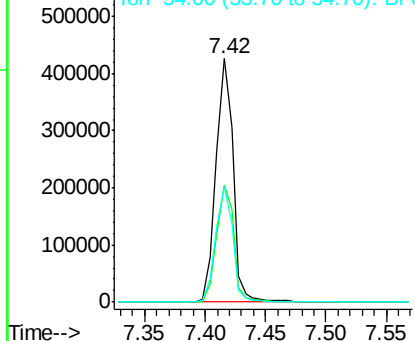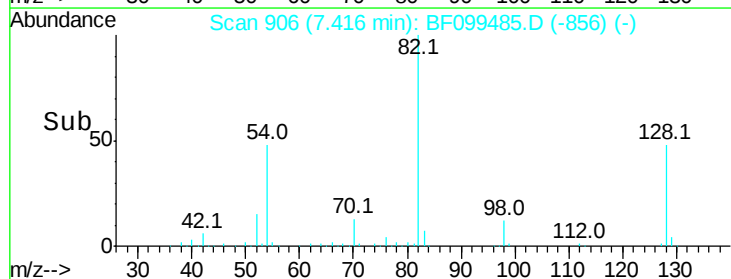

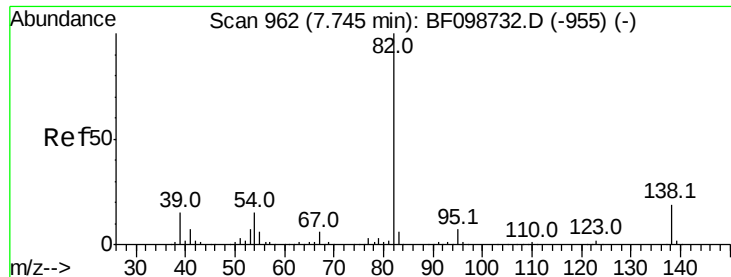

#25

Isophorone

Concen: 35.304 ng

RT: 7.42 min Scan# 906

Delta R.T. -0.26 min

Lab File: BF099485.D

Acq: 14 Oct 2017 19:09

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 82 Resp: 413059

Ion Ratio Lower Upper




82 100

95 0.0 5.2 7.8#

138 0.0 14.9 22.3#

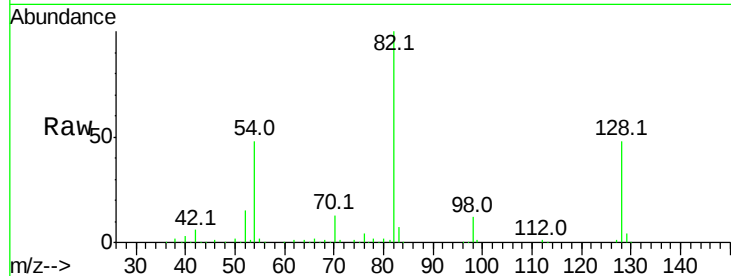

Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 95.00 (94.70 to 95.70): BF0
Ion 138.00 (137.70 to 138.70): BF0

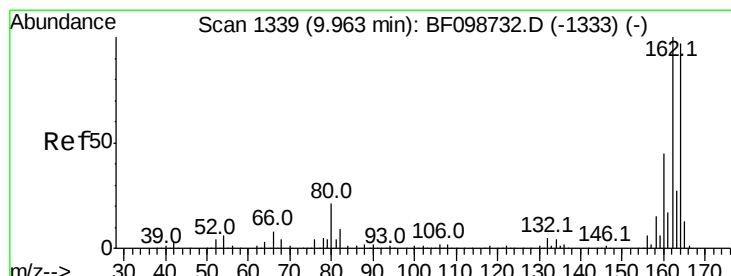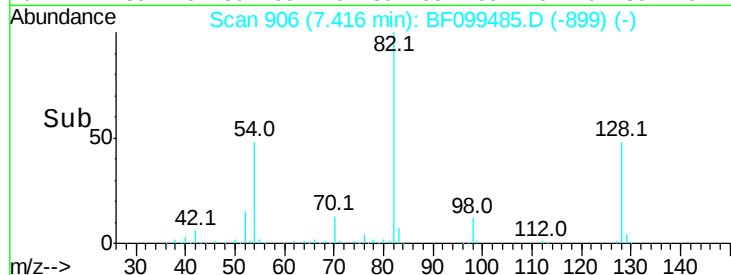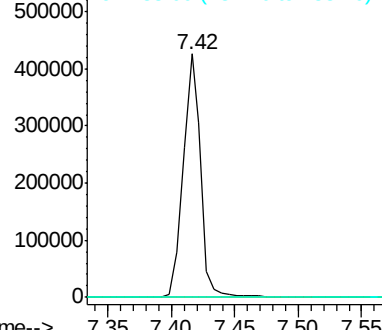

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.89 min Scan# 1326

Delta R.T. -0.01 min

Lab File: BF099485.D

Acq: 14 Oct 2017 19:09


Tgt Ion:164 Resp: 164570

Ion Ratio Lower Upper



164 100


162 103.8 86.1 129.1

160 45.7 38.3 57.5

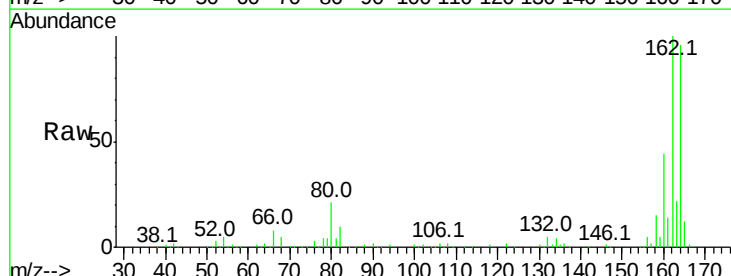

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E



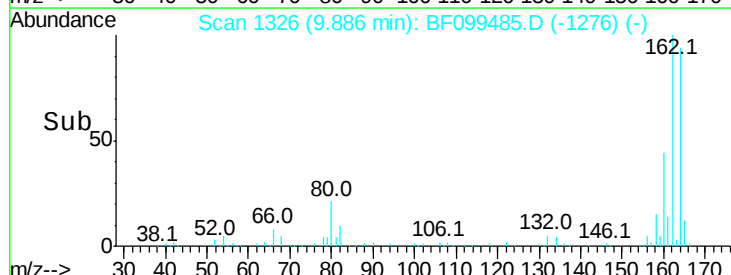
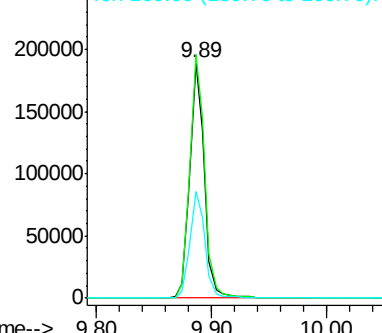


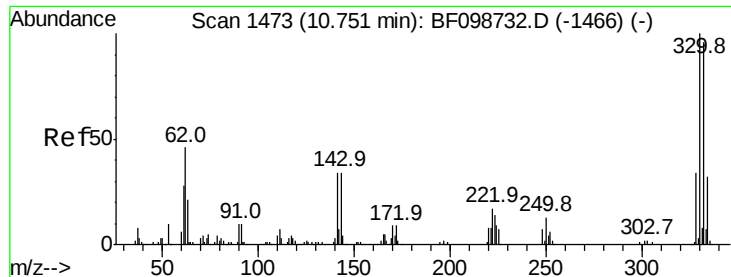

#41
 2,4,6-Tribromophenol
 Concen: 99.575 ng
 RT: 10.68 min Scan# 1461
 Delta R.T. -0.00 min
 Lab File: BF099485.D
 Acq: 14 Oct 2017 19:09




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
330	100		
332	97.4	77.0	115.6
141	39.9	29.9	44.9

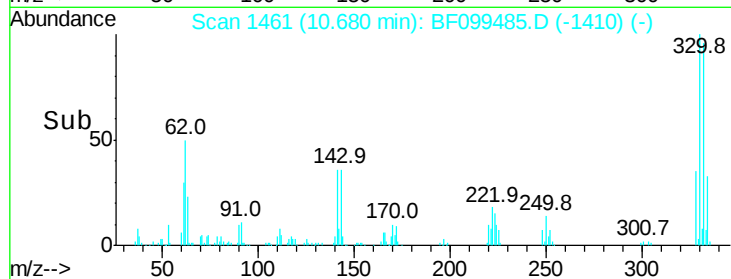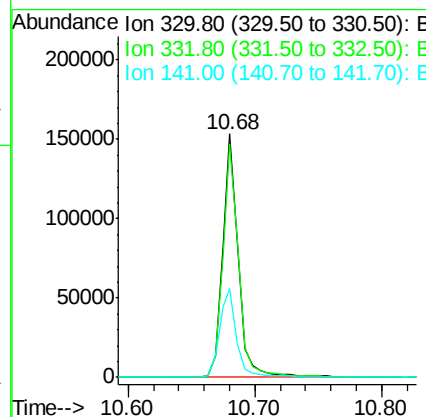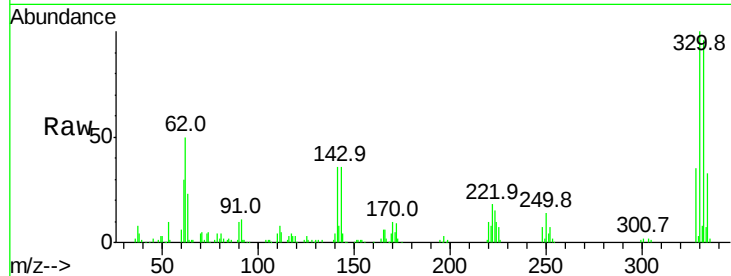

#44
 2-Fluorobiphenyl
 Concen: 80.774 ng
 RT: 9.21 min Scan# 1211
 Delta R.T. -0.00 min
 Lab File: BF099485.D
 Acq: 14 Oct 2017 19:09

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.0	29.7	44.5
170	23.4	19.6	29.4

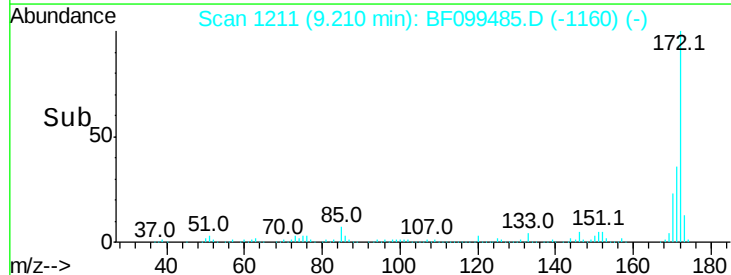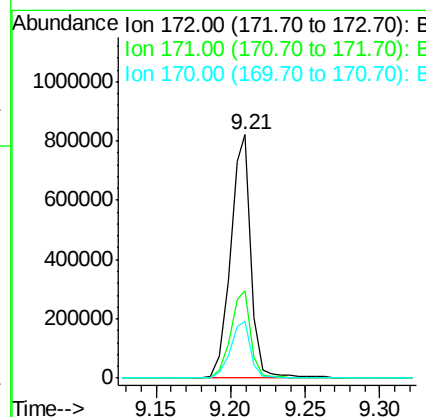

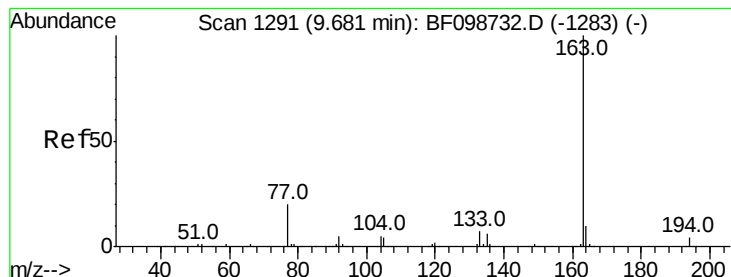

#49

Dimethylphthalate

Concen: 14.628 ng

RT: 9.60 min Scan# 1278

Delta R.T. -0.01 min

Lab File: BF099485.D

Acq: 14 Oct 2017 19:09

Instrument :

BNA_F

ClientSampleId :


Tot Ion:163 Resp: 181689

Ion Ratio Lower Upper

163 100

194 3.6 2.7 4.1




164 9.8 8.2 12.2



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

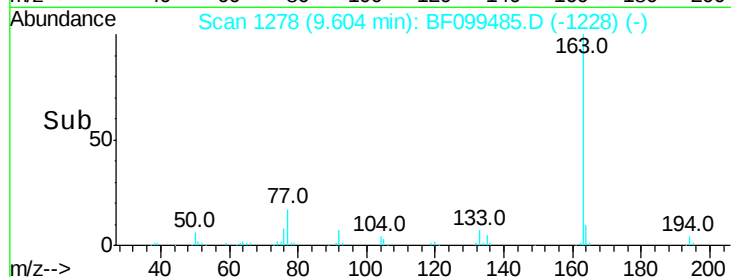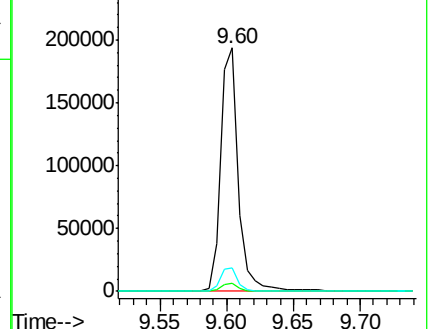

#56

2,4-Dinitrotoluene

Concen: 5.919 ng

RT: 9.89 min Scan# 1326

Delta R.T. -0.20 min

Lab File: BF099485.D

Acq: 14 Oct 2017 19:09

Tgt Ion:165 Resp: 20771


Ion Ratio Lower Upper

165 100

63 1.5 36.4 54.6#

89 0.0 57.8 86.6#

182 0.0 1.6 2.4#






Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0

Ion 182.00 (181.70 to 182.70): E

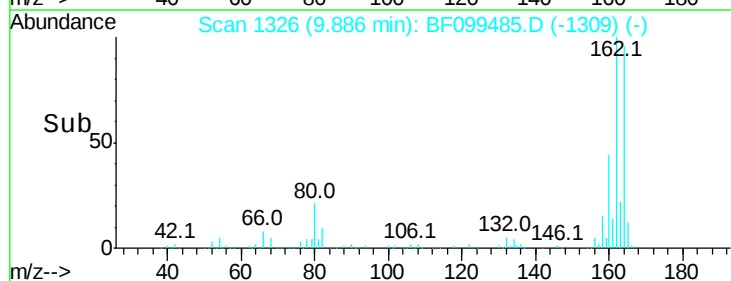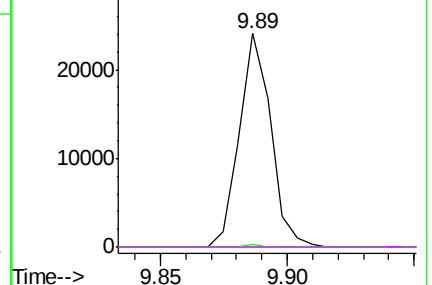


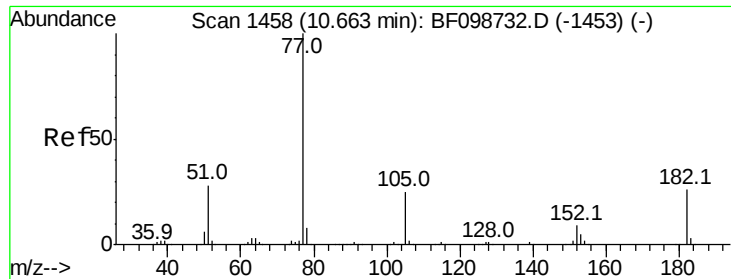




#62
Azobenzene
Concen: 3.018 ng
RT: 10.60 min Scan# 1447
Delta R.T. 0.01 min
Lab File: BF099485.D
Acq: 14 Oct 2017 19:09

Instrument :
BNA_F
ClientSampleId :

Tot Ion: 77 Resp: 33680
Ion Ratio Lower Upper
77 100
182 69.3 1.7 41.7#
105 166.4 3.0 43.0#
51 37.8 9.9 49.9




Abundance Ion 77.00 (76.70 to 77.70): BF0
Ion 182.00 (181.70 to 182.70): E
Ion 105.00 (104.70 to 105.70): E
Ion 51.00 (50.70 to 51.70): BF0

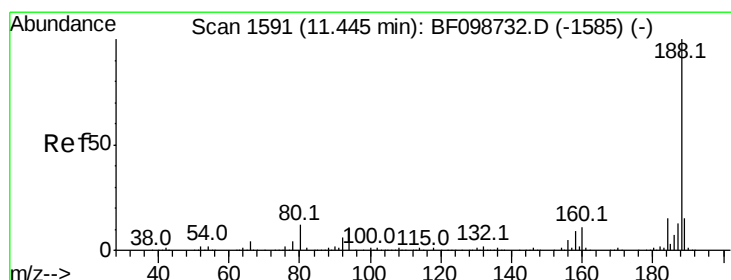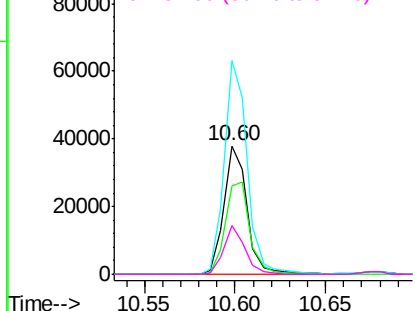
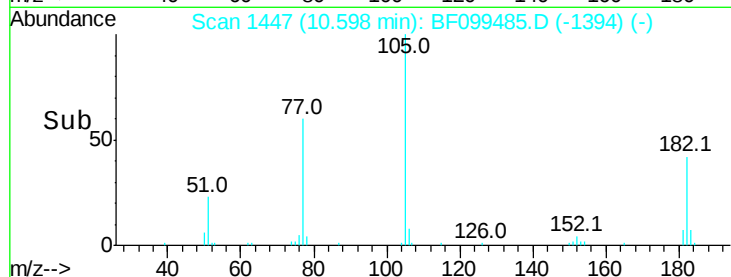



#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.37 min Scan# 1579
Delta R.T. -0.00 min
Lab File: BF099485.D
Acq: 14 Oct 2017 19:09

Tgt Ion: 188 Resp: 288784
Ion Ratio Lower Upper
188 100
94 11.8 8.5 12.7
80 12.4 9.2 13.8



Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

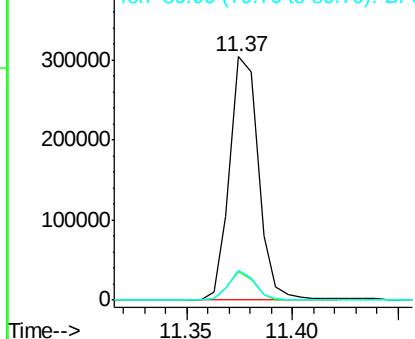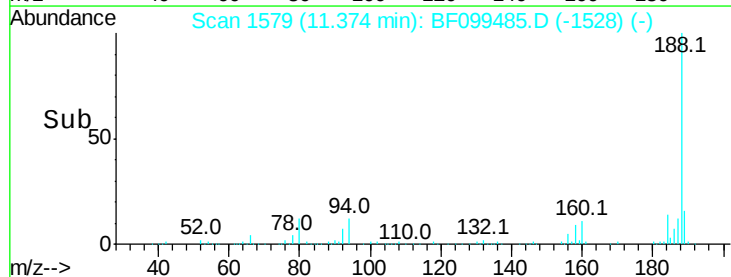


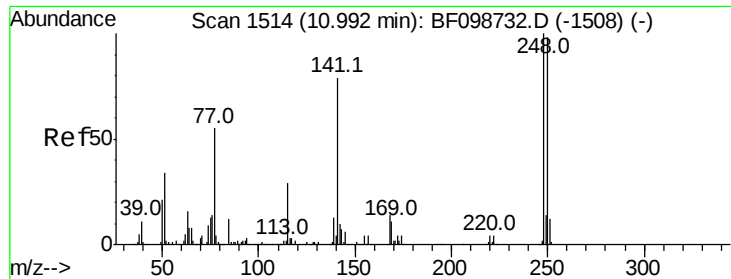




#66
 4-Bromophenyl-phenylether
 Concen: 3.086 ng
 RT: 10.68 min Scan# 1461
 Delta R.T. -0.24 min
 Lab File: BF099485.D
 Acq: 14 Oct 2017 19:09

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:248 Resp: 8724
 Ion Ratio Lower Upper
 248 100
 250 207.2 76.9 115.3#
 141 539.4 74.4 111.6#

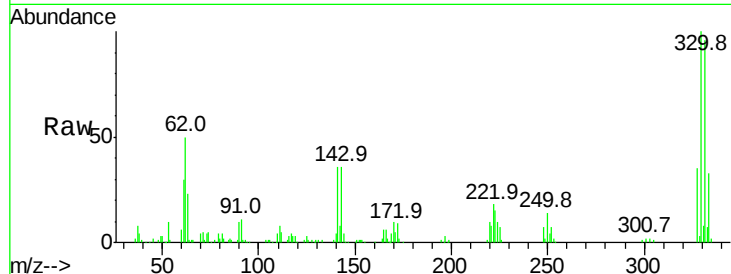


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

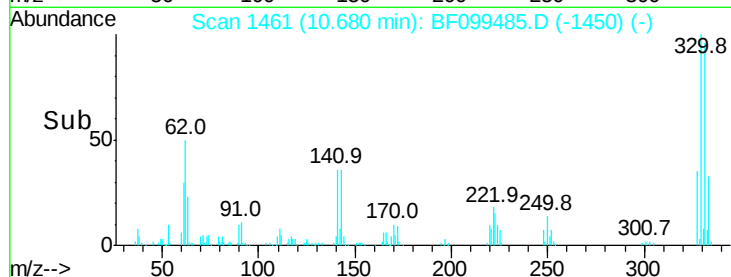
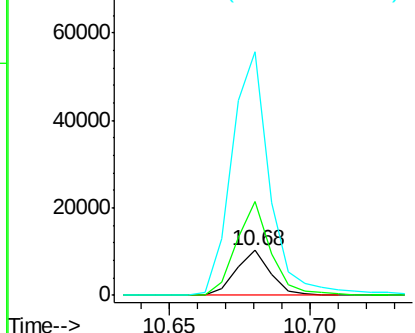



#75
 Chrysene-d12
 Concen: 20.000 ng
 RT: 14.02 min Scan# 2029
 Delta R.T. 0.01 min
 Lab File: BF099485.D
 Acq: 14 Oct 2017 19:09

Tgt Ion:240 Resp: 176505
 Ion Ratio Lower Upper
 240 100
 120 12.7 9.5 14.3
 236 26.2 20.7 31.1



Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E



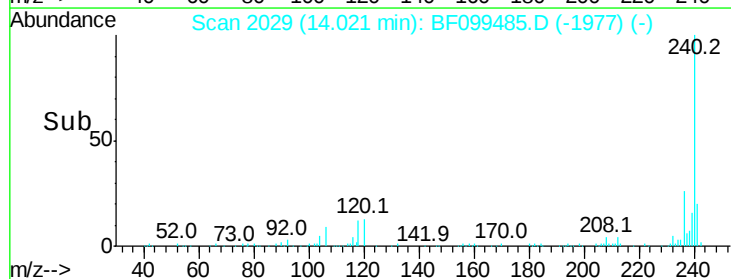
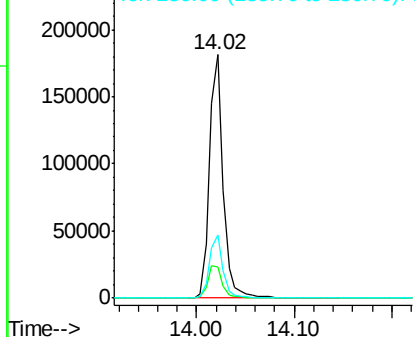


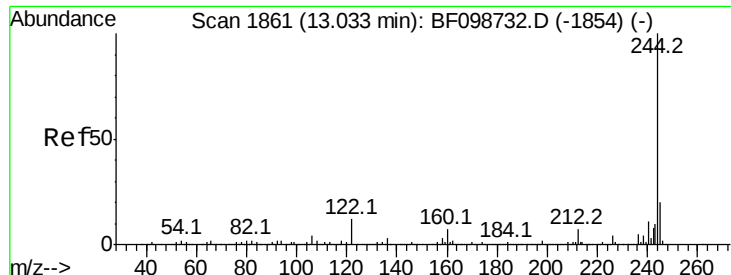

#78
 Terphenyl-d14
 Concen: 84.428 ng
 RT: 12.96 min Scan# 1849
 Delta R.T. 0.01 min
 Lab File: BF099485.D
 Acq: 14 Oct 2017 19:09

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:244 Resp: 655263
 Ion Ratio Lower Upper
 244 100
 212 6.9 5.4 8.0
 122 12.0 11.0 16.4

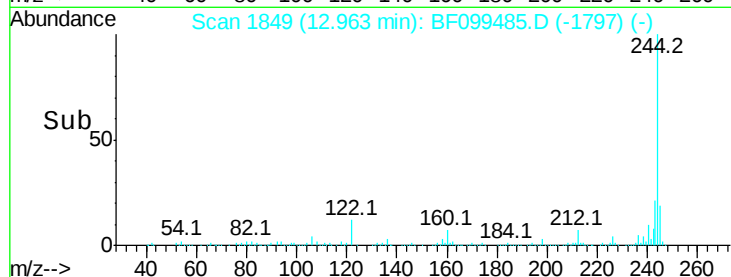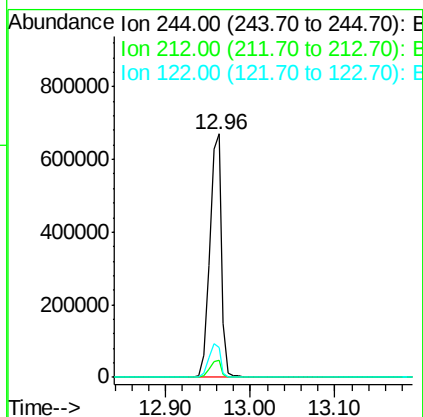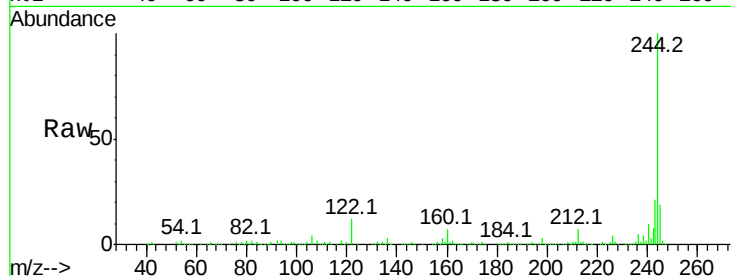

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.49 min Scan# 2279
 Delta R.T. 0.01 min
 Lab File: BF099485.D
 Acq: 14 Oct 2017 19:09

Tgt Ion:264 Resp: 138875
 Ion Ratio Lower Upper
 264 100
 260 23.7 19.2 28.8
 265 20.5 17.5 26.3

