

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF101417\
 Data File : BF099488.D
 Acq On : 14 Oct 2017 20:33
 Operator : SJ/JU
 Sample : I5865-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Oct 14 22:09:53 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 11 16:25:21 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.85	152	93768	20.00	ng	0.00
21) Naphthalene-d8	8.13	136	393644	20.00	ng	0.00
38) Acenaphthene-d10	9.89	164	178875	20.00	ng	0.00
63) Phenanthrene-d10	11.37	188	312556	20.00	ng	0.00
75) Chrysene-d12	14.02	240	190567	20.00	ng	0.00
86) Perylene-d12	15.49	264	159594	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.48	112	614072	104.25	ng	0.01
7) Phenol-d6	6.49	99	745876	102.65	ng	0.00
23) Nitrobenzene-d5	7.42	82	448910	73.13	ng	0.00
41) 2,4,6-Tribromophenol	10.68	330	182401	124.62	ng	0.00
44) 2-Fluorobiphenyl	9.21	172	909131	84.85	ng	0.00
78) Terphenyl-d14	12.96	244	943071	112.54	ng	0.00
Target Compounds						Qvalue
9) Benzaldehyde	6.62	77	12050	2.859	ng	89
10) Phenol	6.50	94	34363	4.228	ng	84
19) n-Nitroso-di-n-propylamine	7.42	70	56743	12.231	ng	# 73
25) Isophorone	7.42	82	448905	35.373	ng	# 64
49) Dimethylphthalate	9.60	163	105812	7.838	ng	98
56) 2,4-Dinitrotoluene	9.89	165	22830	5.985	ng	# 22
62) Azobenzene	10.60	77	46427	3.828	ng	# 1
66) 4-Bromophenyl-phenylether	10.68	248	12307	4.023	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF101417\
Data File : BF099488.D
Acq On : 14 Oct 2017 20:33
Operator : SJ/JU
Sample : I5865-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Oct 14 22:09:53 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 11 16:25:21 2017
Response via : Initial Calibration

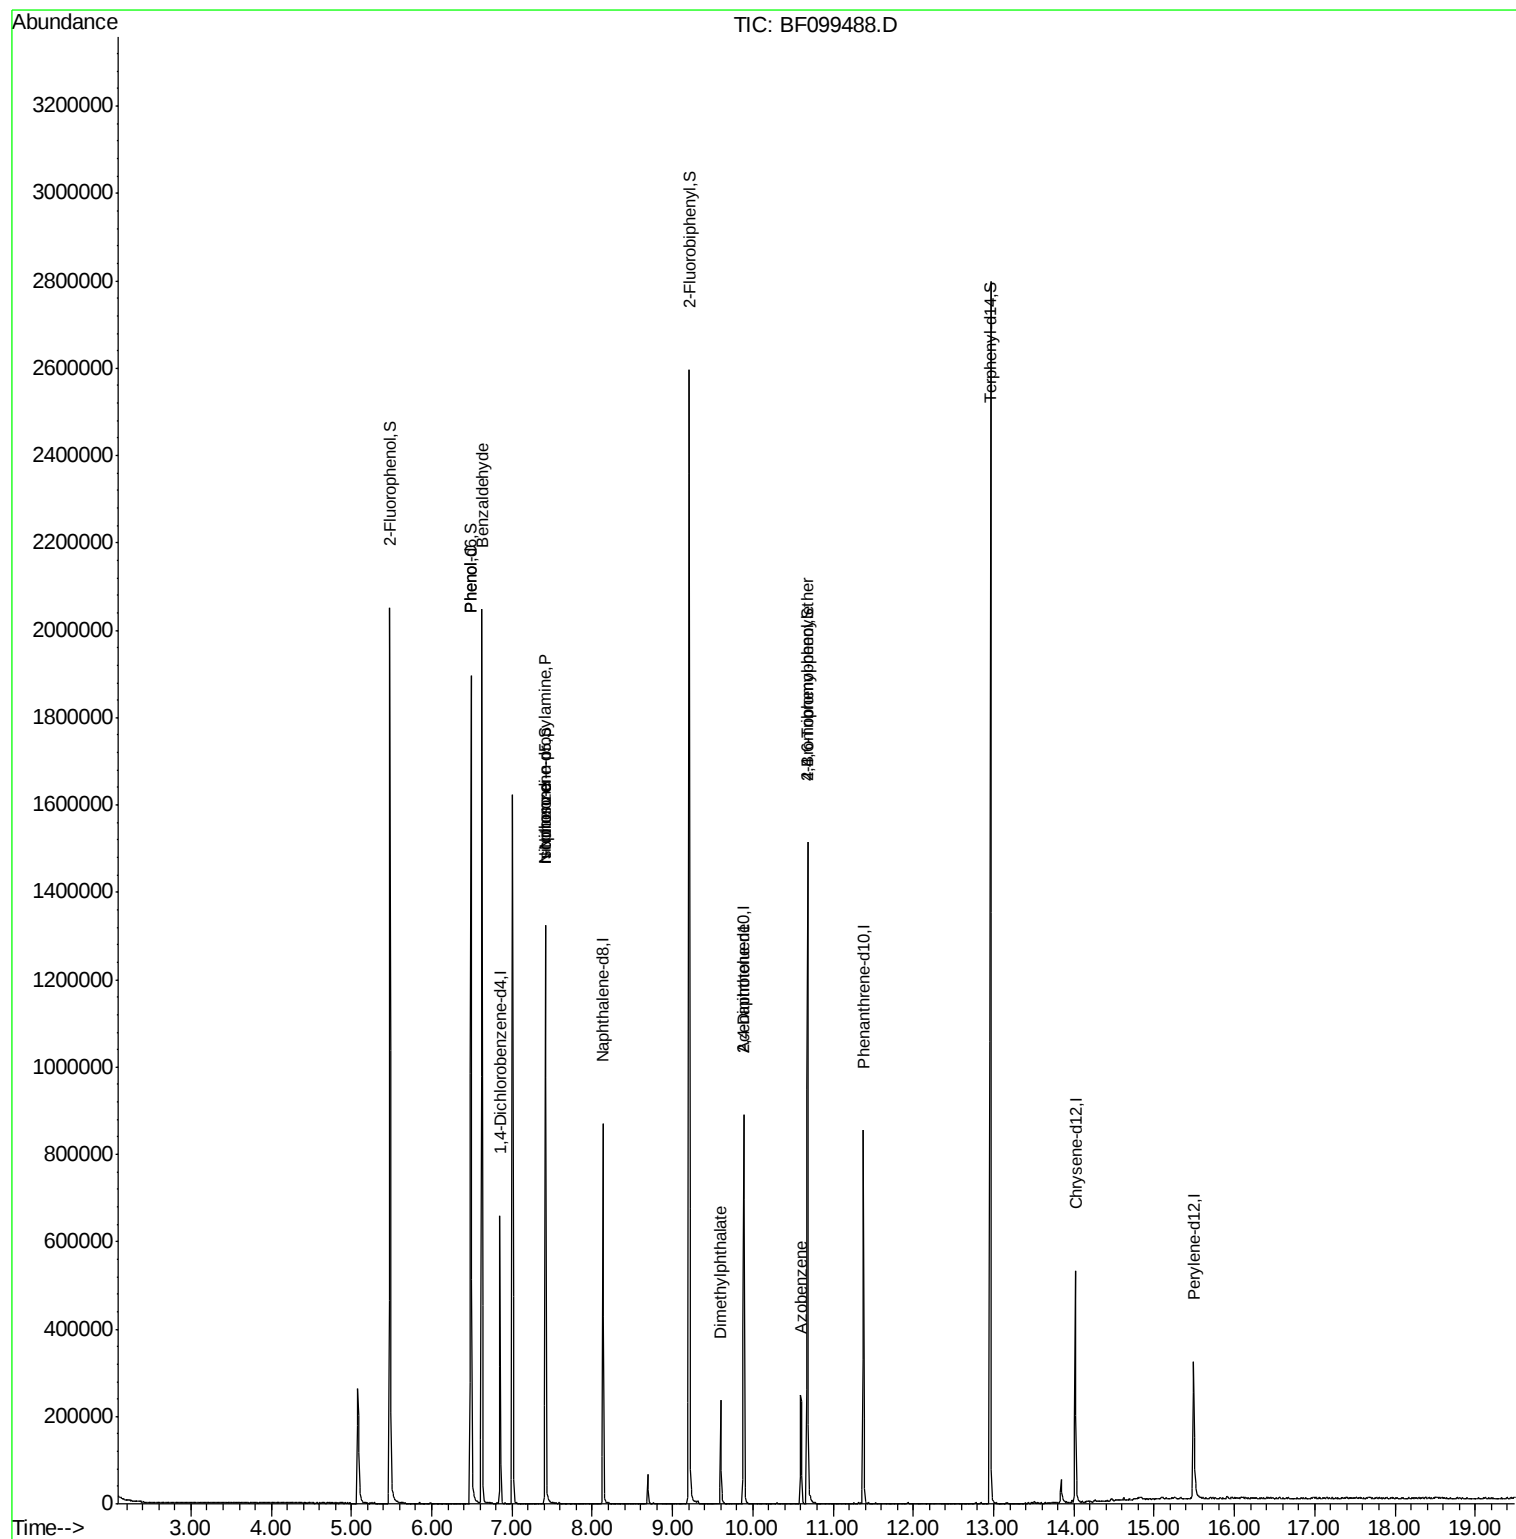

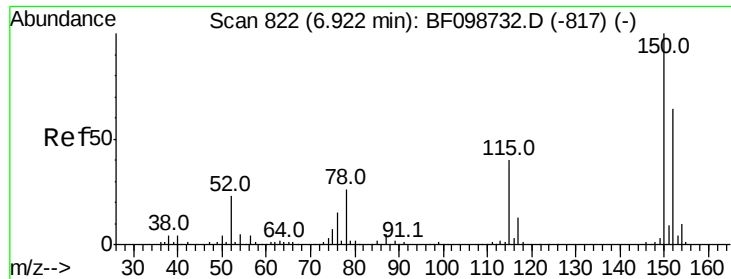


#1




1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.85 min Scan# 810
 Delta R.T. 0.00 min
 Lab File: BF099488.D
 Acq: 14 Oct 2017 20:33

Instrument :
 BNA_F
 ClientSampled :

Tot Ion:152 Resp: 93768
 Ion Ratio Lower Upper
 152 100
 150 156.7 124.6 186.8
 115 60.7 50.1 75.1

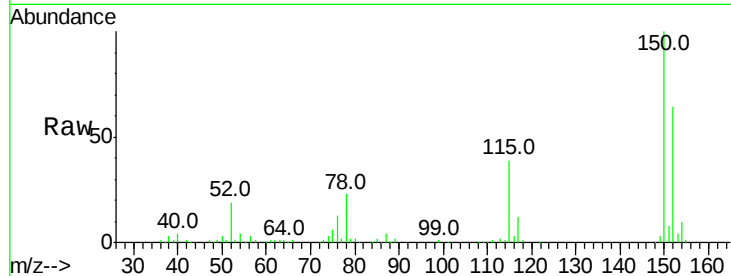


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

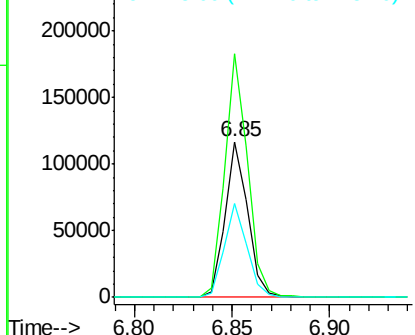



#5


2-Fluorophenol
 Concen: 104.251 ng
 RT: 5.48 min Scan# 577
 Delta R.T. 0.01 min
 Lab File: BF099488.D
 Acq: 14 Oct 2017 20:33

Tgt Ion:112 Resp: 614072
 Ion Ratio Lower Upper
 112 100
 64 54.1 47.9 71.9
 63 26.9 23.7 35.5



Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

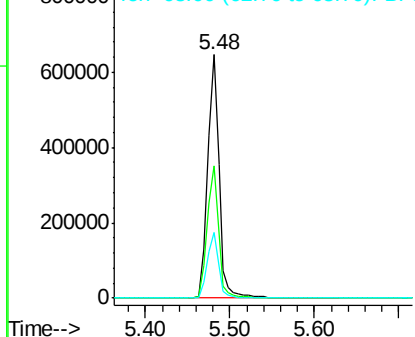



#7

Phenol-d6

Concen: 102.648 ng

RT: 6.49 min Scan# 749

Delta R.T. 0.01 min

Lab File: BF099488.D

Acq: 14 Oct 2017 20:33

Instrument :

BNA_F

ClientSampled :


Tot Ion: 99 Resp: 745876

Ion Ratio Lower Upper




99 100

42 15.0 14.5 21.7

71 30.1 25.4 38.0

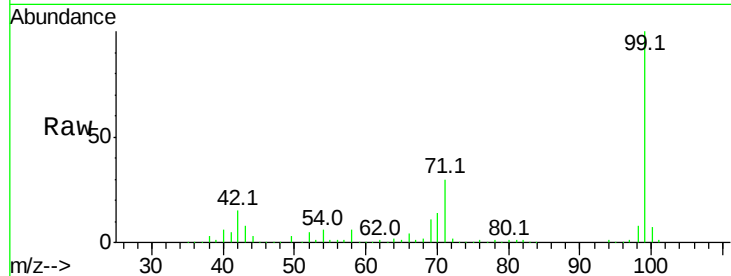

Abundance Ion 99.00 (98.70 to 99.70): BF0
Ion 42.00 (41.70 to 42.70): BF0
Ion 71.00 (70.70 to 71.70): BF0

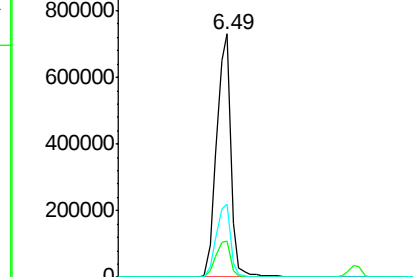

#9

Benzaldehyde

Concen: 2.859 ng

RT: 6.62 min Scan# 771

Delta R.T. 0.21 min

Lab File: BF099488.D

Acq: 14 Oct 2017 20:33


Tgt Ion: 77 Resp: 12050

Ion Ratio Lower Upper



77 100


105 90.9 81.1 121.1

106 82.4 74.5 114.5



Abundance Ion 77.00 (76.70 to 77.70): BF0
Ion 105.00 (104.70 to 105.70): BF0
Ion 106.00 (105.70 to 106.70): BF0



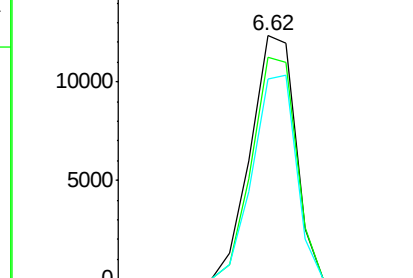





#10
Phenol
Concen: 4.228 ng
RT: 6.50 min Scan# 750
Delta R.T. 0.00 min
Lab File: BF099488.D
Acq: 14 Oct 2017 20:33




Instrument :
BNA_F
ClientSampleId :


Tot Ion: 94 Resp: 34363
Ion Ratio Lower Upper
94 100
65 30.5 7.9 47.9
66 50.7 16.2 56.2

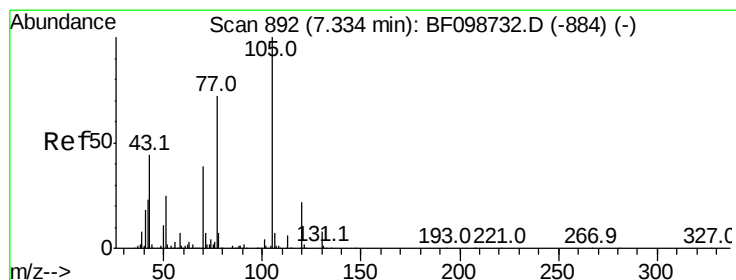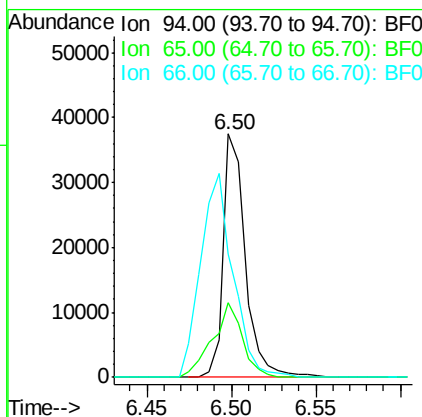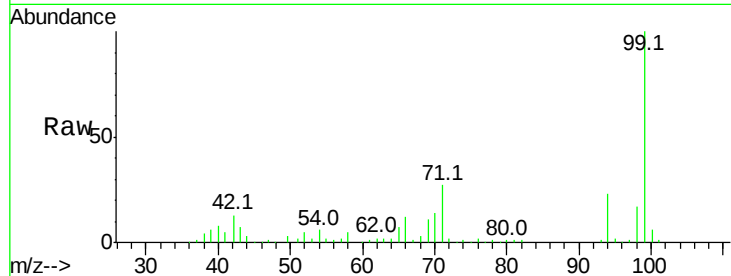

#19
n-Nitroso-di-n-propylamine
Concen: 12.231 ng
RT: 7.42 min Scan# 906
Delta R.T. 0.15 min
Lab File: BF099488.D
Acq: 14 Oct 2017 20:33

Tgt Ion: 70 Resp: 56743
Ion Ratio Lower Upper
70 100
42 42.2 47.5 71.3#
101 0.0 7.4 11.2#
130 2.7 16.6 25.0#

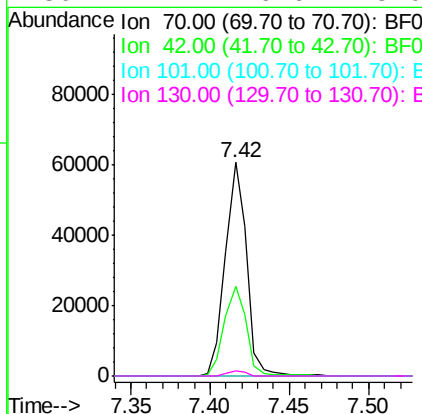


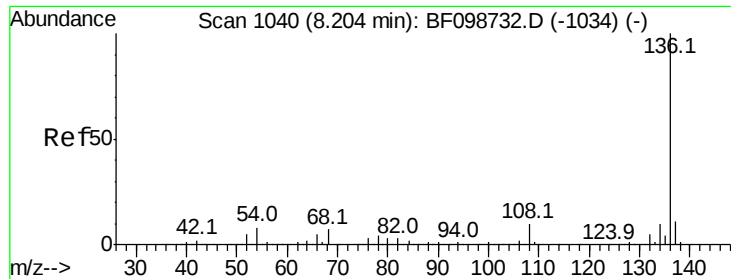




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.13 min Scan# 1028
Delta R.T. 0.00 min
Lab File: BF099488.D
Acq: 14 Oct 2017 20:33

Instrument :
BNA_F
ClientSampleId :

Tot Ion:	136	Resp:	393644
Ion	Ratio	Lower	Upper
136	100		
137	11.2	8.9	13.3
54	6.7	6.6	9.8
68	5.9	5.0	7.4




Abundance Ion 136.00 (135.70 to 136.70): B
Ion 137.00 (136.70 to 137.70): B
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

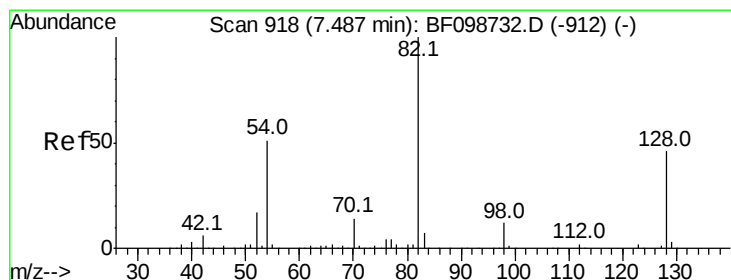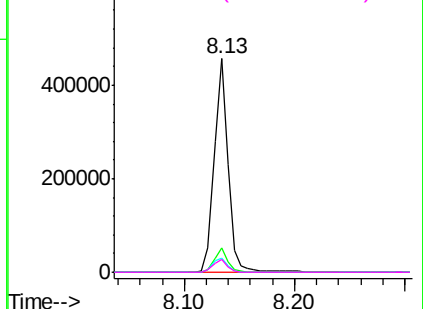




#23
Nitrobenzene-d5
Concen: 73.134 ng
RT: 7.42 min Scan# 906
Delta R.T. -0.01 min
Lab File: BF099488.D
Acq: 14 Oct 2017 20:33

Tgt Ion:	82	Resp:	448910
Ion	Ratio	Lower	Upper
82	100		
128	46.1	36.1	54.1
54	47.9	41.4	62.2



Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): B
Ion 54.00 (53.70 to 54.70): BF0

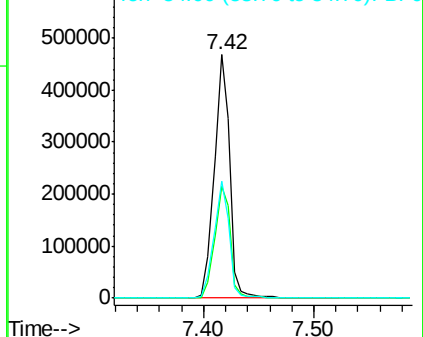

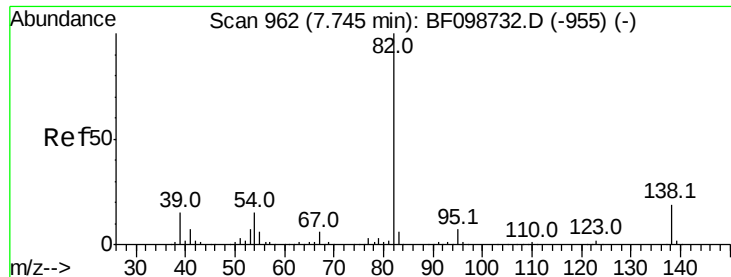

#25

Isophorone

Concen: 35.373 ng

RT: 7.42 min Scan# 906

Delta R.T. -0.26 min

Lab File: BF099488.D

Acq: 14 Oct 2017 20:33

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 82 Resp: 448905

Ion Ratio Lower Upper




82 100

95 0.0 5.2 7.8#

138 0.0 14.9 22.3#

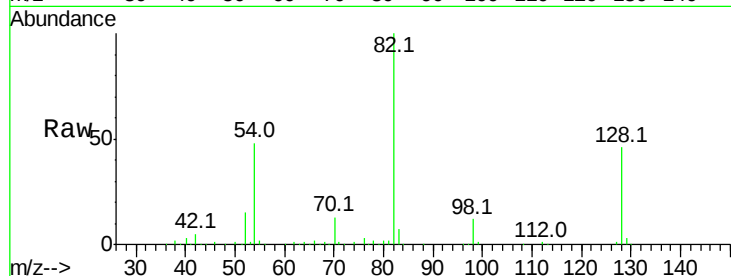

Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 95.00 (94.70 to 95.70): BF0
Ion 138.00 (137.70 to 138.70): E

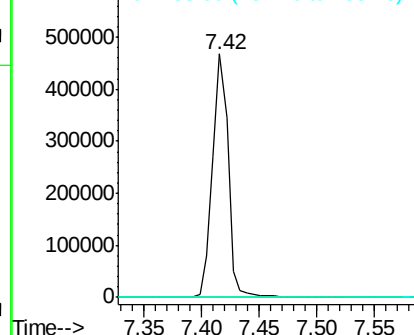

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.89 min Scan# 1326

Delta R.T. -0.01 min

Lab File: BF099488.D

Acq: 14 Oct 2017 20:33


Tgt Ion:164 Resp: 178875

Ion Ratio Lower Upper



164 100


162 106.5 86.1 129.1

160 46.5 38.3 57.5



Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

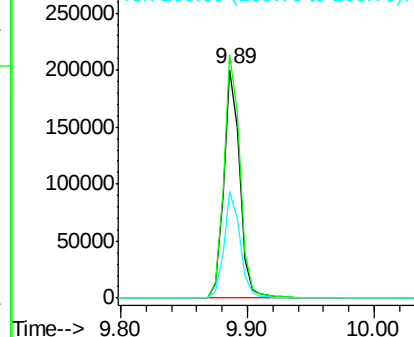







#41
 2,4,6-Tribromophenol
 Concen: 124.618 ng
 RT: 10.68 min Scan# 1461
 Delta R.T. 0.00 min
 Lab File: BF099488.D
 Acq: 14 Oct 2017 20:33

Instrument :
 BNA_F
 ClientSampled :

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.4	77.0	115.6
141	38.7	29.9	44.9




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

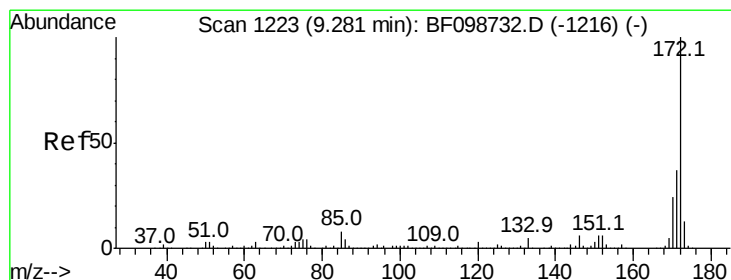
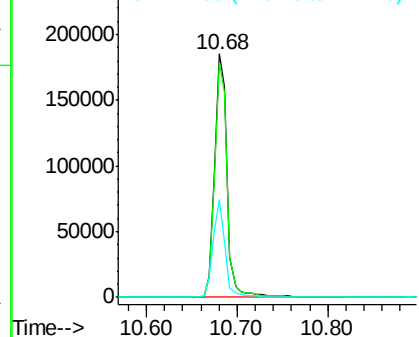



#44
 2-Fluorobiphenyl
 Concen: 84.848 ng
 RT: 9.21 min Scan# 1211
 Delta R.T. 0.00 min
 Lab File: BF099488.D
 Acq: 14 Oct 2017 20:33

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.3	29.7	44.5
170	23.8	19.6	29.4

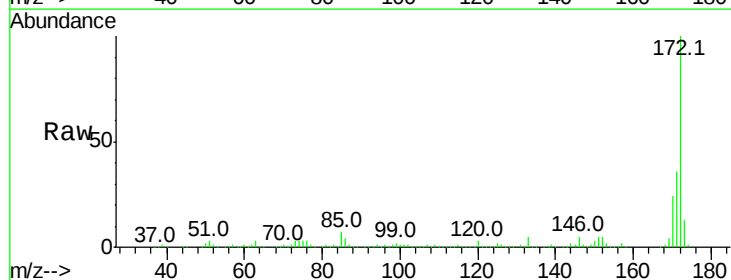

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

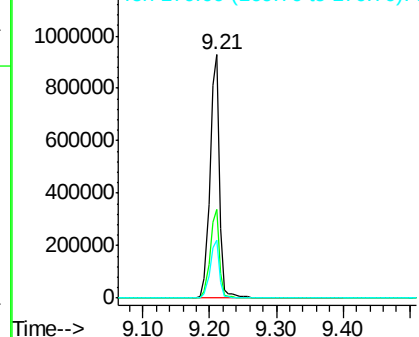

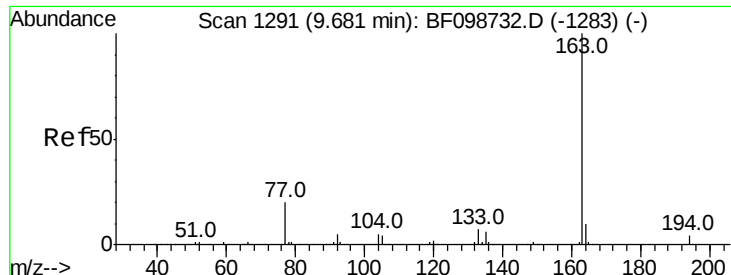

#49

Dimethylphthalate

Concen: 7.838 ng

RT: 9.60 min Scan# 1278

Delta R.T. -0.01 min

Lab File: BF099488.D

Acq: 14 Oct 2017 20:33

Instrument :

BNA_F

ClientSampleId :


Tot Ion:163 Resp: 105812

Ion Ratio Lower Upper

163 100

194 3.3 2.7 4.1




164 9.3 8.2 12.2

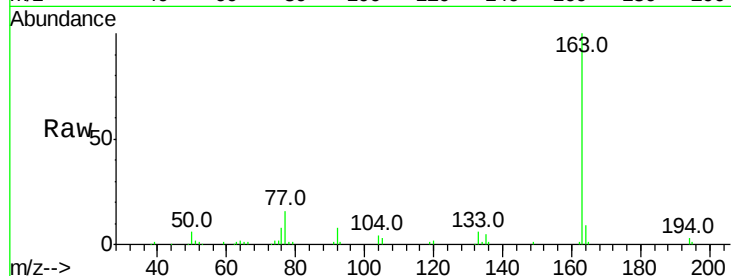

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

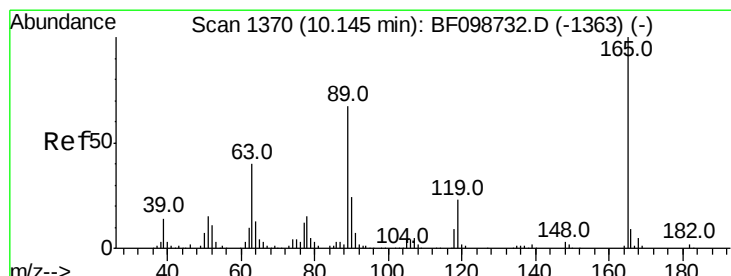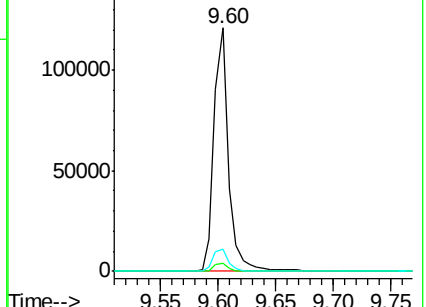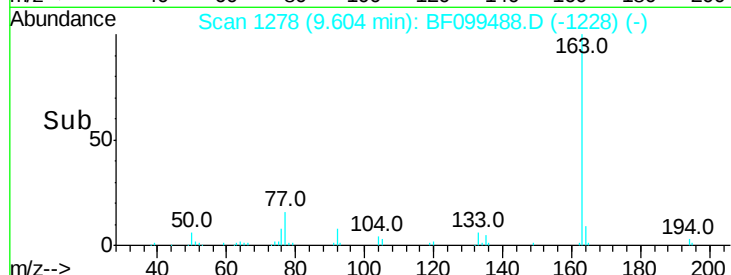

#56

2,4-Dinitrotoluene

Concen: 5.985 ng

RT: 9.89 min Scan# 1326

Delta R.T. -0.20 min

Lab File: BF099488.D

Acq: 14 Oct 2017 20:33

Tgt Ion:165 Resp: 22830


Ion Ratio Lower Upper

165 100

63 0.0 36.4 54.6#

89 1.2 57.8 86.6#

182 0.0 1.6 2.4#


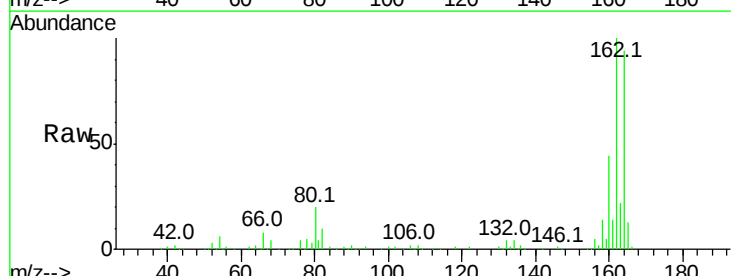



Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0

Ion 182.00 (181.70 to 182.70): E

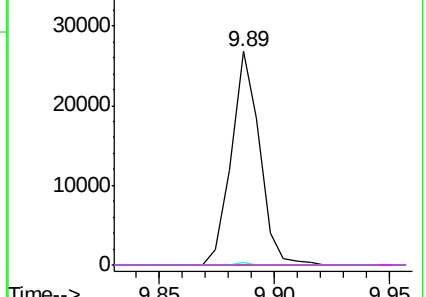

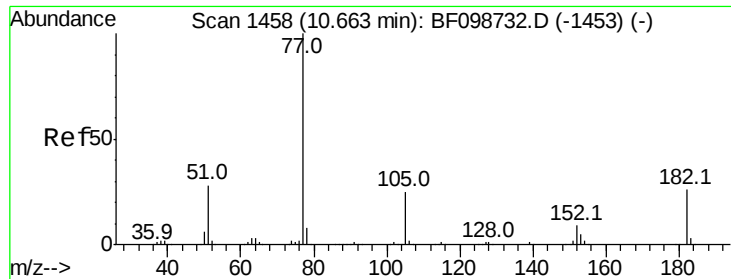

#62

Azobenzene

Concen: 3.828 ng

RT: 10.60 min Scan# 1447

Delta R.T. 0.01 min

Lab File: BF099488.D

Acq: 14 Oct 2017 20:33

Instrument :

BNA_F

ClientSampleId :

Tot Ion: 77 Resp: 46427


Ion Ratio Lower Upper

77 100

182 70.3 1.7 41.7#

105 157.5 3.0 43.0#

51 35.7 9.9 49.9



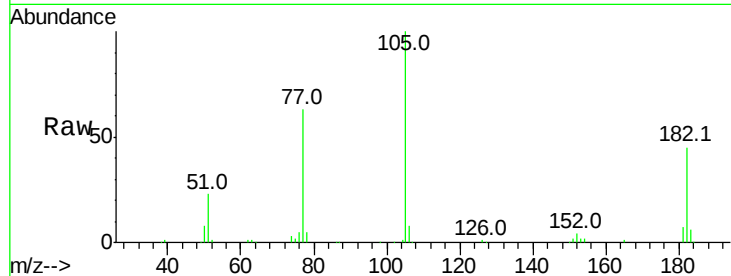


Abundance Ion 77.00 (76.70 to 77.70): BF0

Ion 182.00 (181.70 to 182.70): E

Ion 105.00 (104.70 to 105.70): E

Ion 51.00 (50.70 to 51.70): BF0

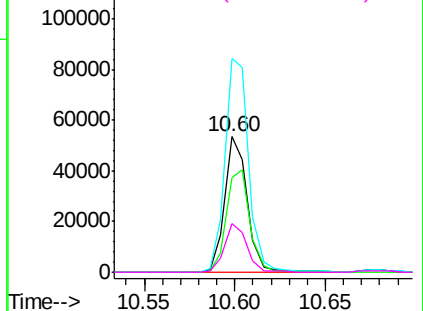

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.37 min Scan# 1579

Delta R.T. 0.00 min

Lab File: BF099488.D

Acq: 14 Oct 2017 20:33


Tgt Ion: 188 Resp: 312556

Ion Ratio Lower Upper

188 100

94 10.7 8.5 12.7



80 12.2 9.2 13.8




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

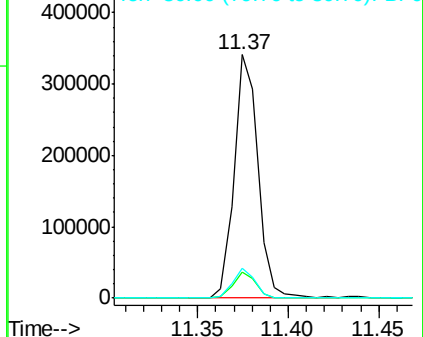


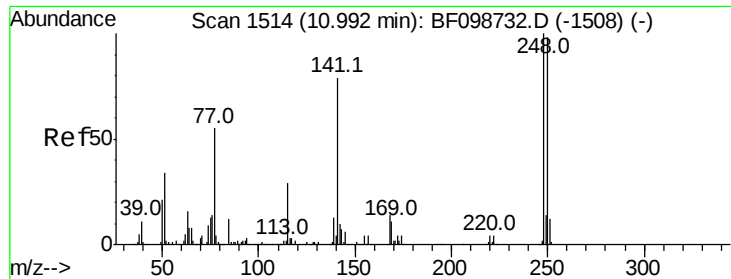




#66
4-Bromophenyl-phenylether
Concen: 4.023 ng
RT: 10.68 min Scan# 1461
Delta R.T. -0.24 min
Lab File: BF099488.D
Acq: 14 Oct 2017 20:33

Instrument :
BNA_F
ClientSampled :

Tot Ion:248 Resp: 12307
Ion Ratio Lower Upper
248 100
250 199.8 76.9 115.3#
141 577.9 74.4 111.6#

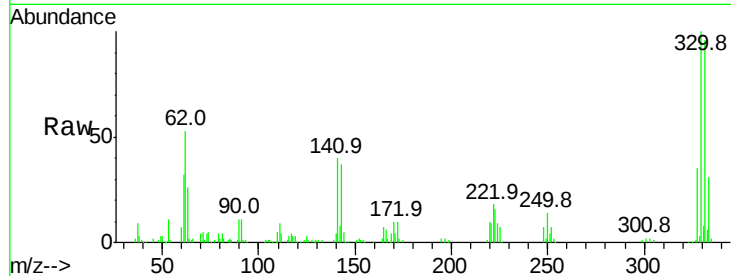


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

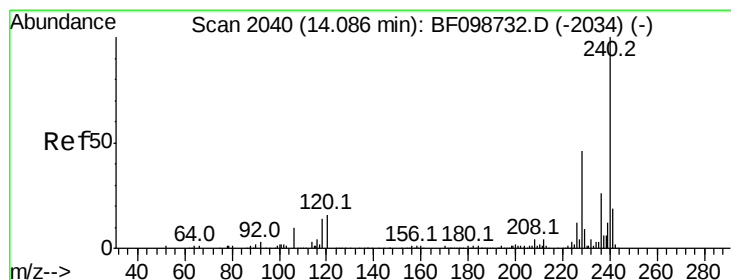
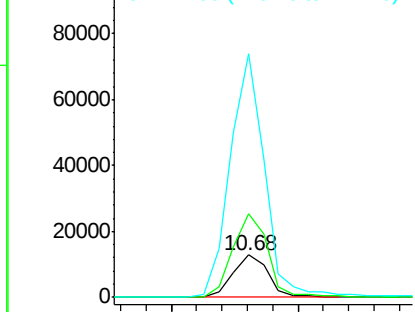



#75
Chrysene-d12
Concen: 20.000 ng
RT: 14.02 min Scan# 2029
Delta R.T. 0.01 min
Lab File: BF099488.D
Acq: 14 Oct 2017 20:33

Tgt Ion:240 Resp: 190567
Ion Ratio Lower Upper
240 100
120 12.7 9.5 14.3
236 25.9 20.7 31.1



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

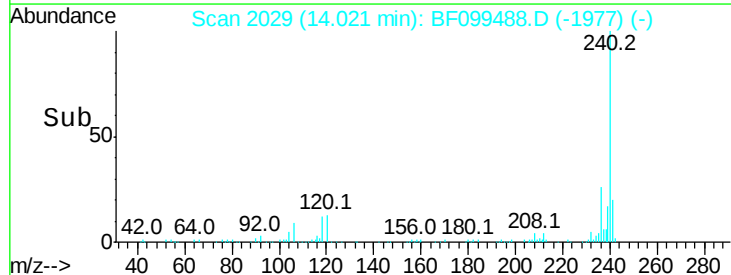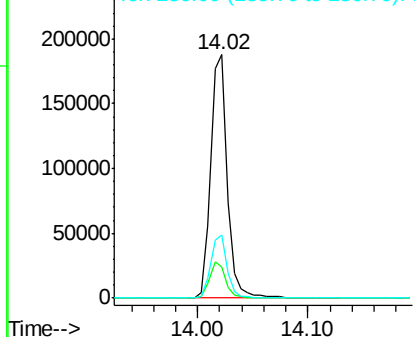

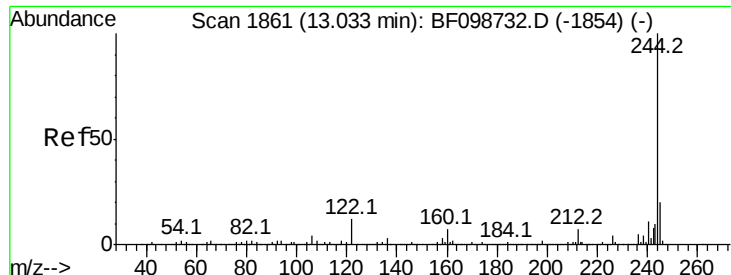

#78

Terphenyl-d14

Concen: 112.545 ng

RT: 12.96 min Scan# 1849

Delta R.T. 0.01 min

Lab File: BF099488.D

Acq: 14 Oct 2017 20:33

Instrument :

BNA_F

ClientSampleId :


Tot Ion:244 Resp: 943071

Ion Ratio Lower Upper

244 100

212 7.2 5.4 8.0




122 13.5 11.0 16.4



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

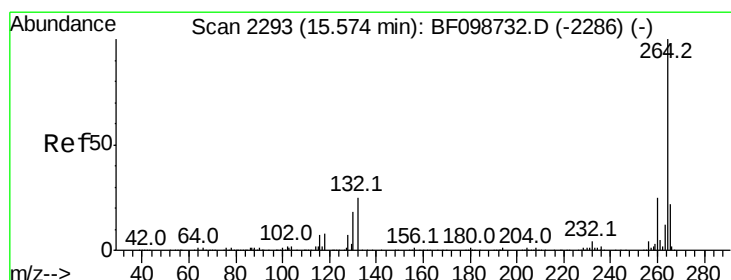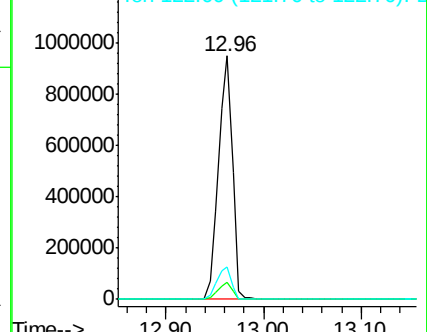

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.49 min Scan# 2279

Delta R.T. 0.01 min

Lab File: BF099488.D

Acq: 14 Oct 2017 20:33


Tgt Ion:264 Resp: 159594

Ion Ratio Lower Upper

264 100

260 25.1 19.2 28.8

265 21.9 17.5 26.3



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

