


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101417\
 Data File : BF099471.D
 Acq On : 14 Oct 2017 12:30
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 11 16:25:21 2017

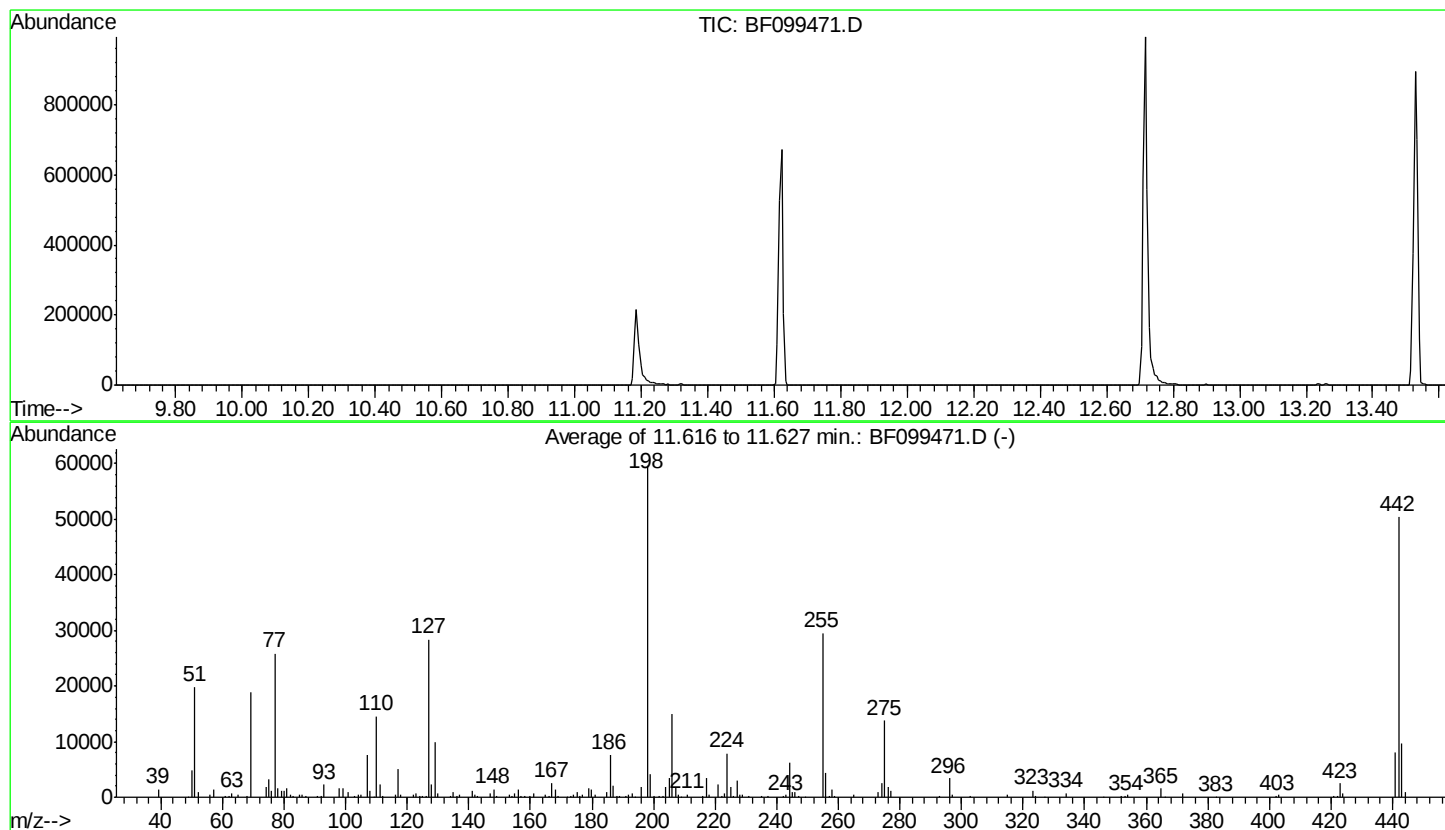

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.3	19867	PASS
68	69	0.00	2	1.5	291	PASS
69	198	0.00	100	31.6	18820	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.6	28394	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	59650	PASS
199	198	5	9	6.9	4126	PASS
275	198	10	60	23.1	13799	PASS
365	198	1	100	2.6	1539	PASS
441	442	0.01	24	15.8	7962	PASS
442	198	50	100	84.6	50477	PASS
443	442	15	24	19.3	9735	PASS