


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101417\
 Data File : BF099497.D
 Acq On : 15 Oct 2017 1:15
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 11 16:25:21 2017

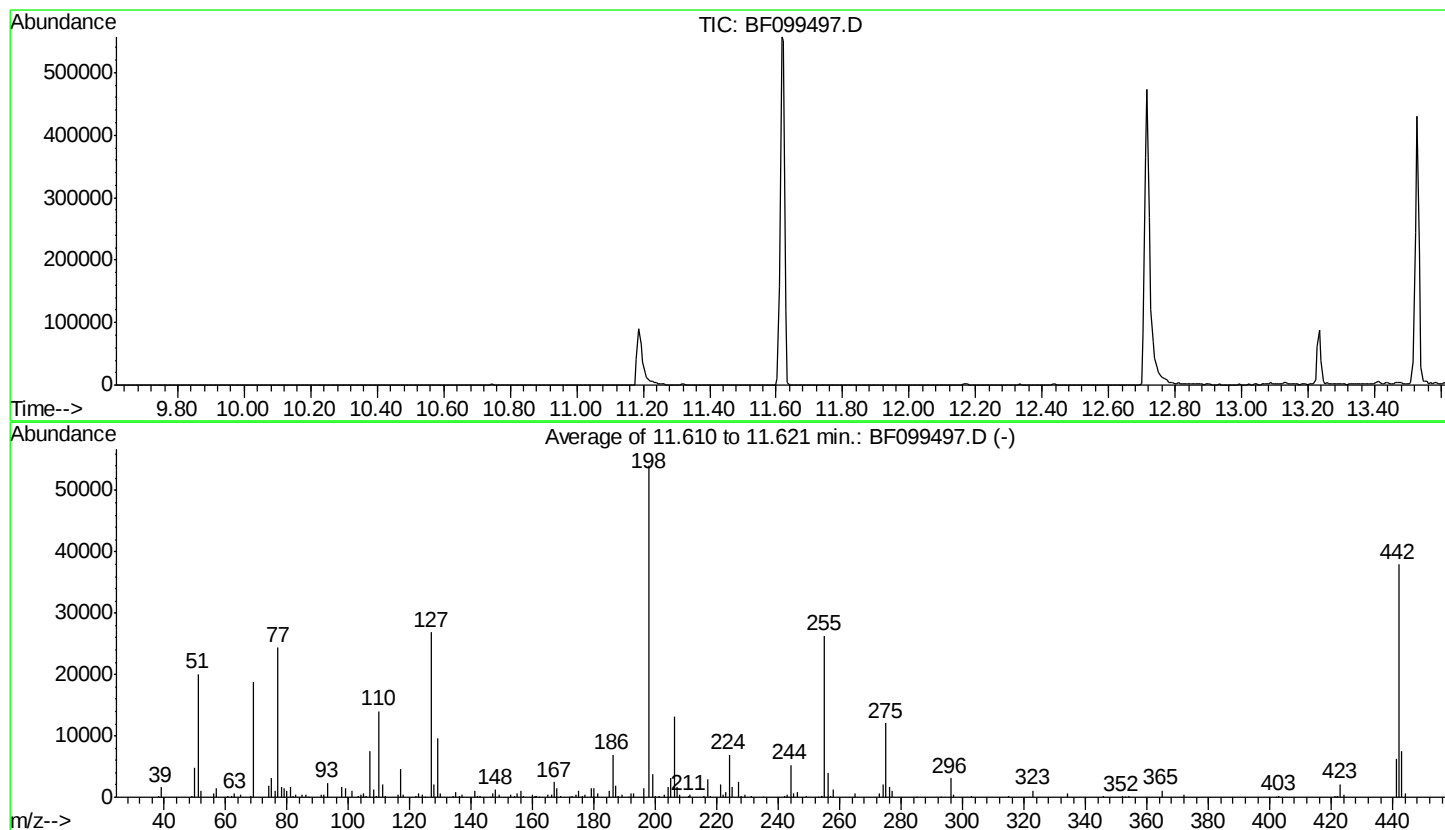

AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	20067	PASS
68	69	0.00	2	0.9	169	PASS
69	198	0.00	100	34.9	18852	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.7	26859	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	54061	PASS
199	198	5	9	7.0	3809	PASS
275	198	10	60	22.2	12018	PASS
365	198	1	100	2.1	1112	PASS
441	442	0.01	24	16.7	6331	PASS
442	198	50	100	70.2	37955	PASS
443	442	15	24	19.8	7528	PASS