
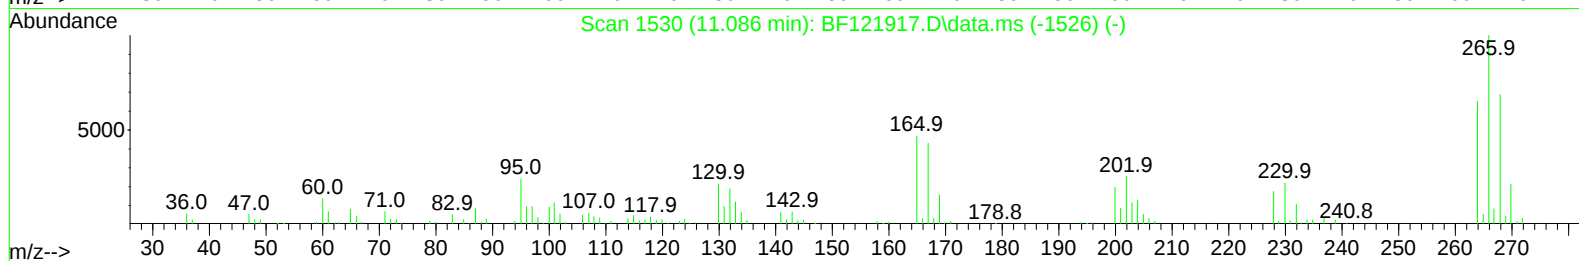
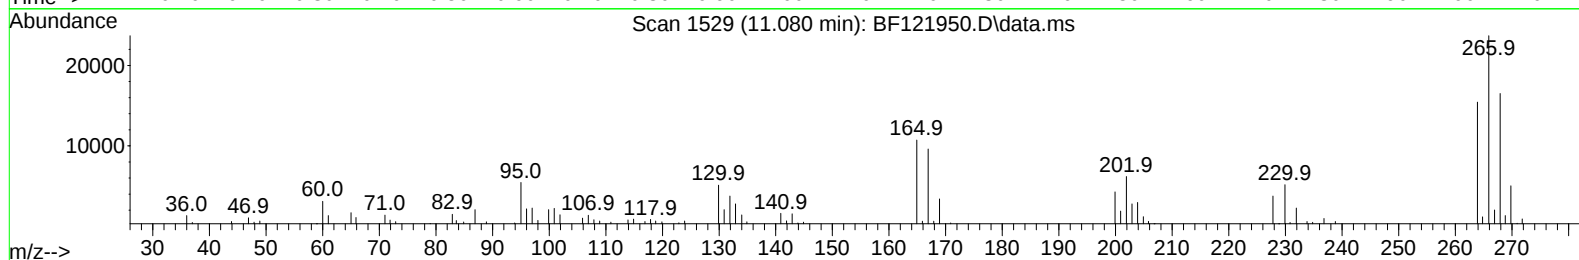


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101420\
Data File : BF121950.D
Acq On : 14 Oct 2020 10:02
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 15 03:16:02 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 12 16:22:33 2020
Response via : Initial Calibration

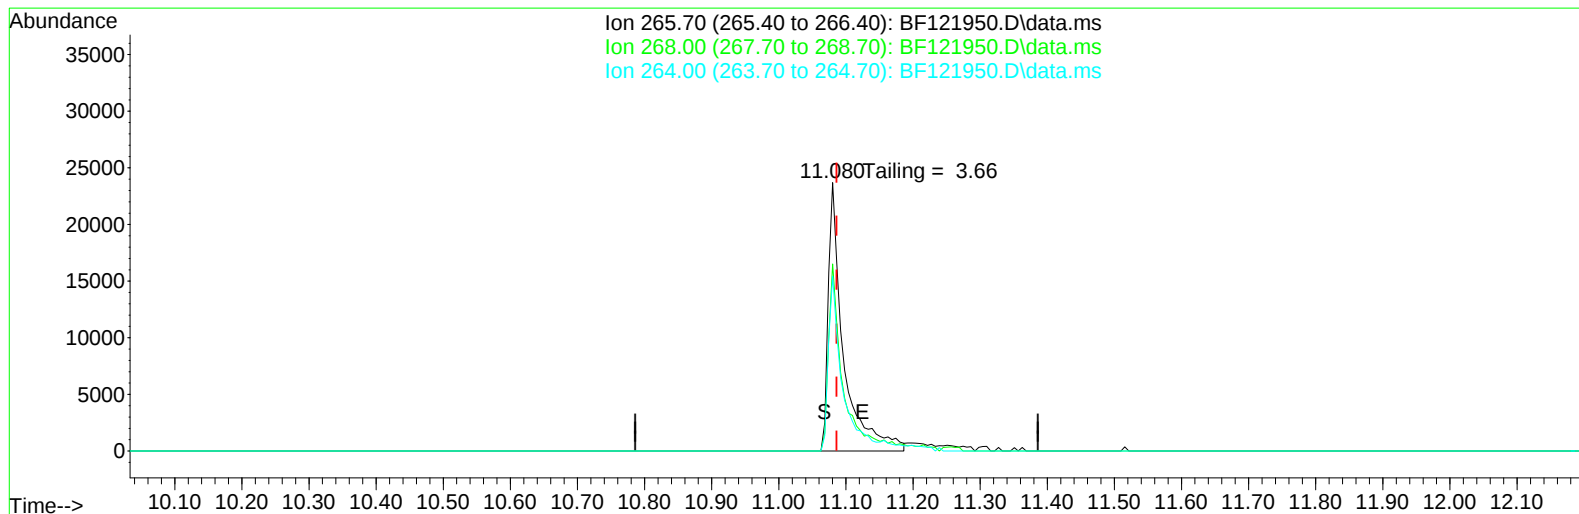

TIC: BF121950.D\data.ms

(70) Pentachlorophenol (C)




11.080min (-0.006) 51791.23 ng

response 37837

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.50	69.68
264.00	62.40	65.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101420\
Data File : BF121950.D
Acq On : 14 Oct 2020 10:02
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 15 03:16:02 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 12 16:22:33 2020
Response via : Initial Calibration

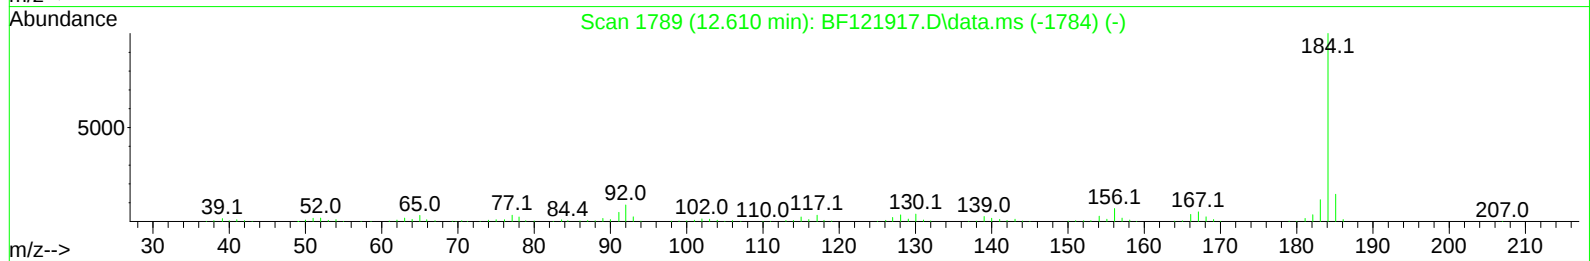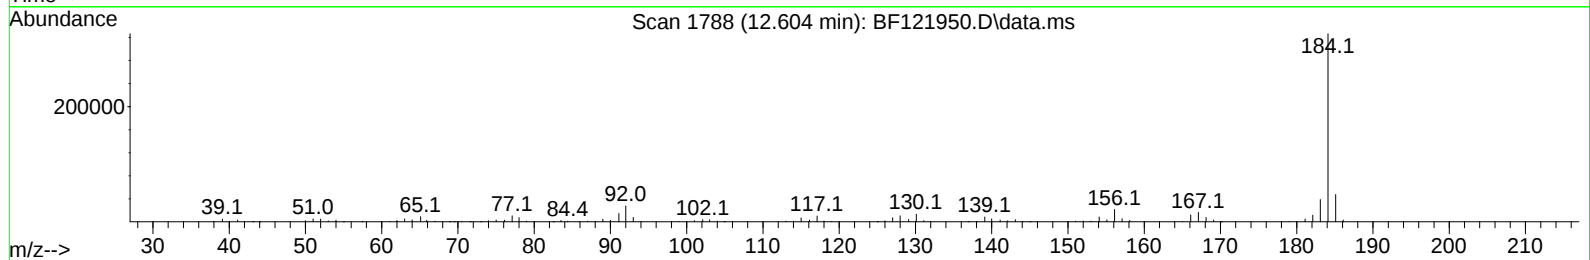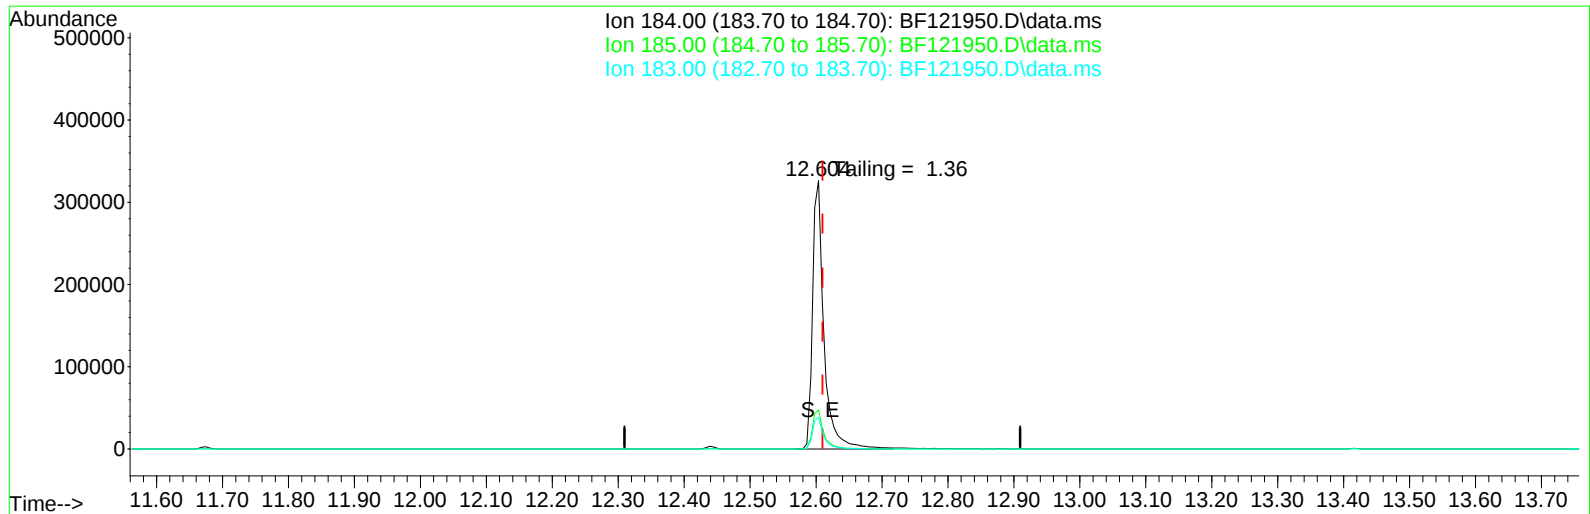

TIC: BF121950.D\data.ms

(77) Benzidine

12.604min (-0.006) 0.00 ng

response 396404

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.58
183.00	11.70	11.88
0.00	0.00	0.00