

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101420\
 Data File : BF121959.D
 Acq On : 14 Oct 2020 15:56
 Operator : JU/CG
 Sample : L4353-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 EFF-WW

Quant Time: Oct 14 17:16:25 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 12 16:22:33 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.745	152	107297	20.00	ng	0.00
21) Naphthalene-d8	8.028	136	196329	20.00	ng	# 0.00
39) Acenaphthene-d10	9.786	164	202080	20.00	ng	0.00
64) Phenanthrene-d10	11.269	188	333352	20.00	ng	0.00
76) Chrysene-d12	13.910	240	228731	20.00	ng	0.00
86) Perylene-d12	15.339	264	236265	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.369	112	187397	25.78	ng	0.00
7) Phenol-d6	6.398	99	156506	16.72	ng	0.00
23) Nitrobenzene-d5	7.310	82	560444	146.40	ng	-0.01
42) 2,4,6-Tribromophenol	10.581	330	172306	68.93	ng	0.00
45) 2-Fluorobiphenyl	9.110	172	873970	63.63	ng	0.00
79) Terphenyl-d14	12.857	244	897619	74.79	ng	0.00
Target Compounds						
50) Dimethylphthalate	9.516	163	112937	7.64	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101420\
Data File : BF121959.D
Acq On : 14 Oct 2020 15:56
Operator : JU/CG
Sample : L4353-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EFF-WW

Quant Time: Oct 14 17:16:25 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 12 16:22:33 2020
Response via : Initial Calibration




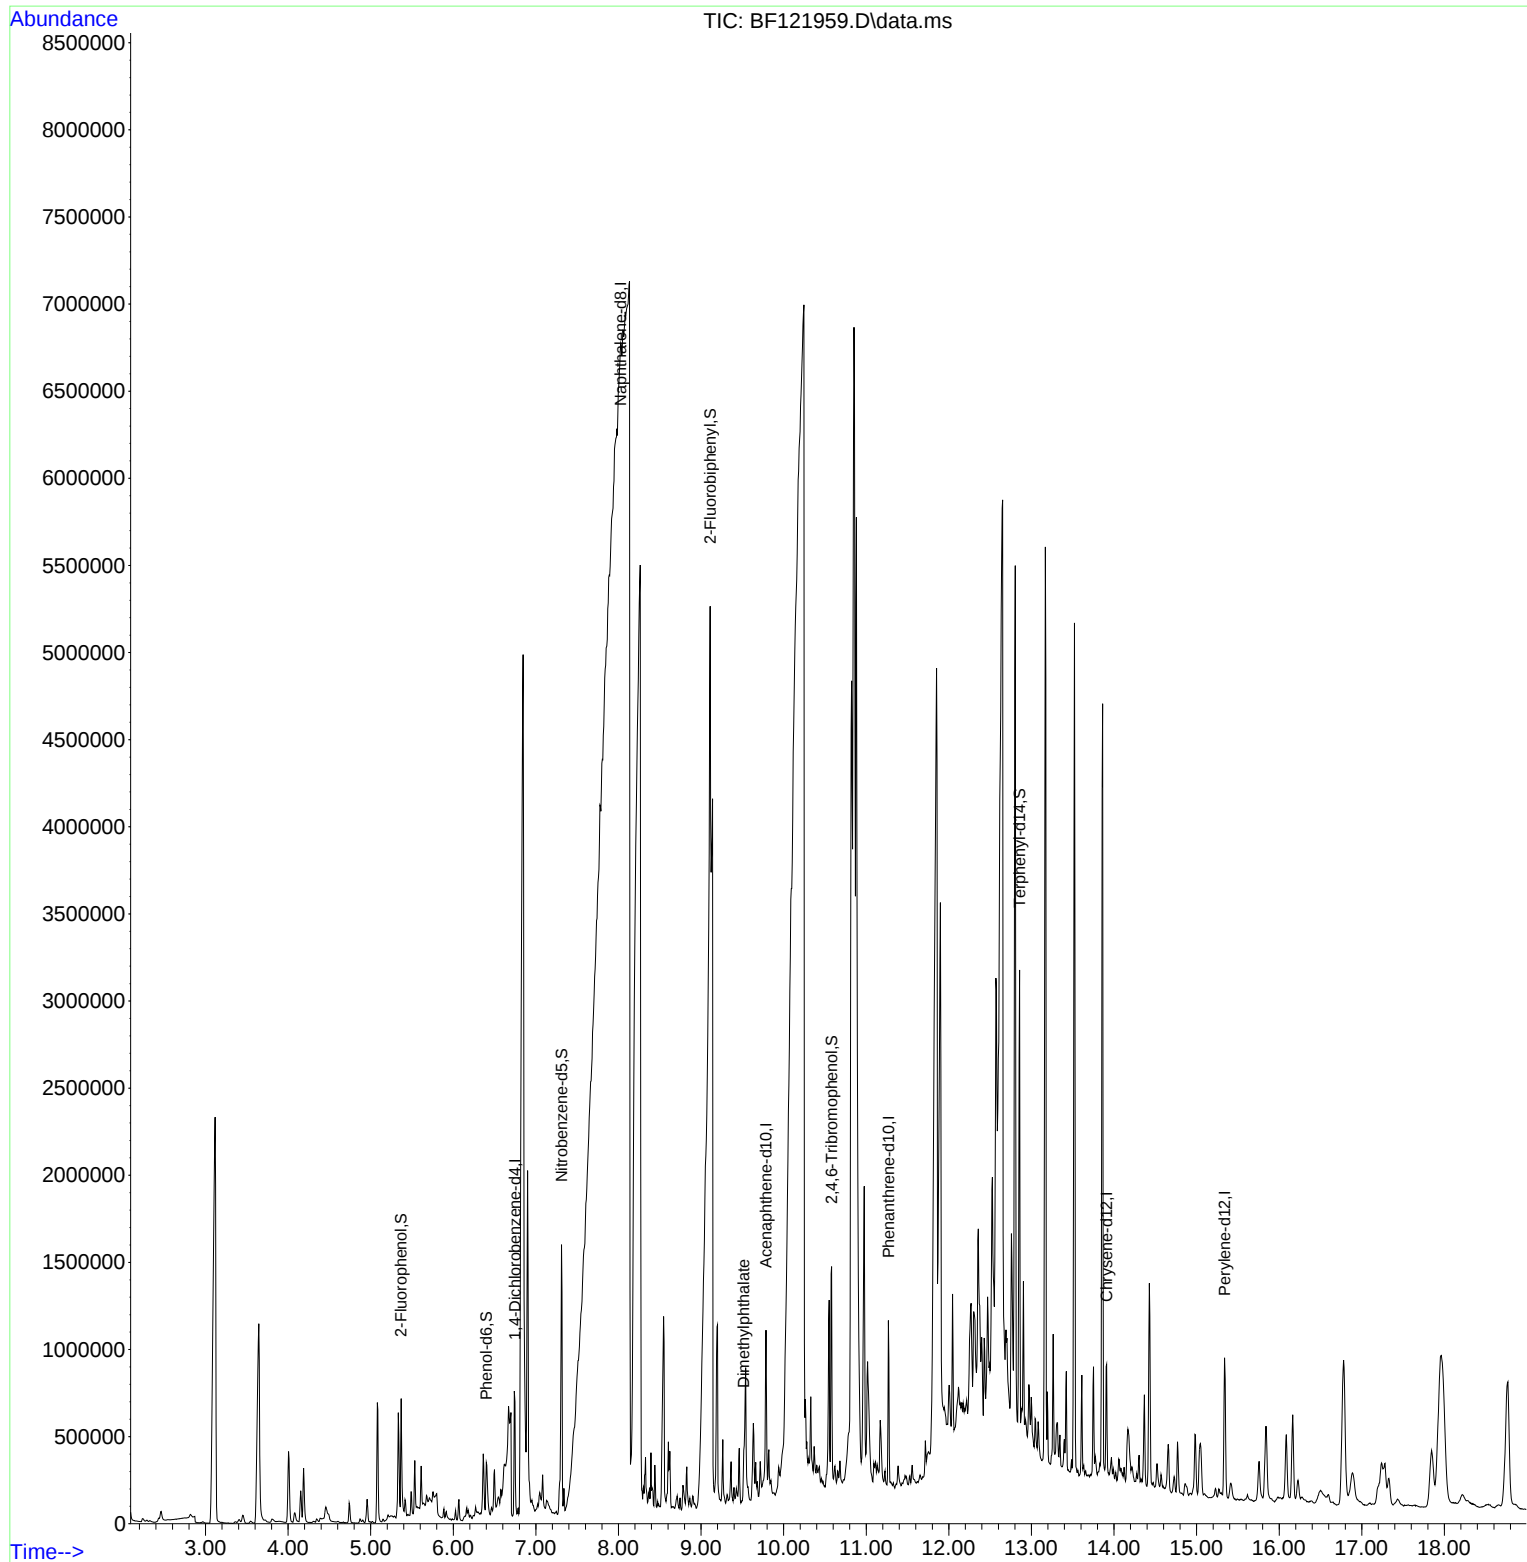


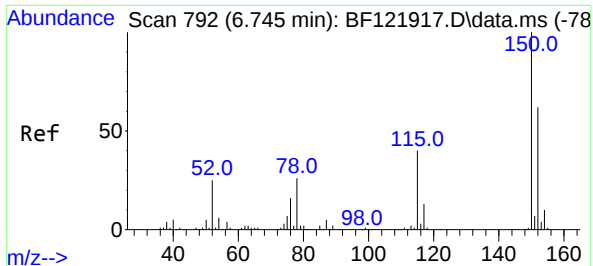

#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.745 min Scan# 792
Delta R.T. 0.000 min
Lab File: BF121959.D
Acq: 14 Oct 2020 15:56




Instrument :
BNA_F
ClientSampleId :
EFF-WW


Tgt Ion:152 Resp: 107297
Ion Ratio Lower Upper
152 100
150 158.2 125.3 187.9
115 60.4 51.9 77.9

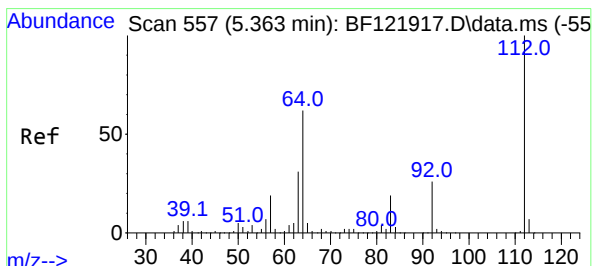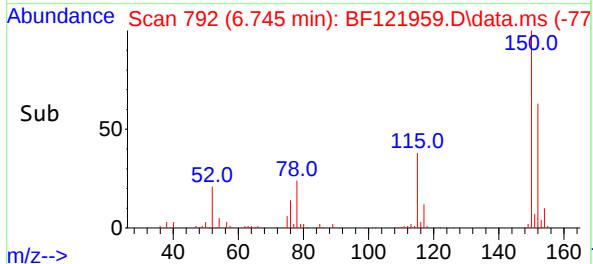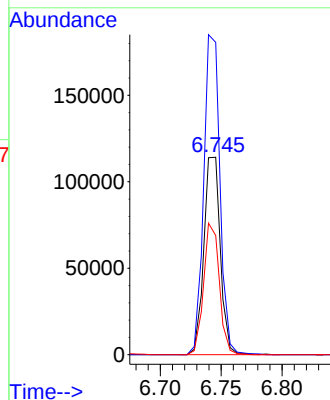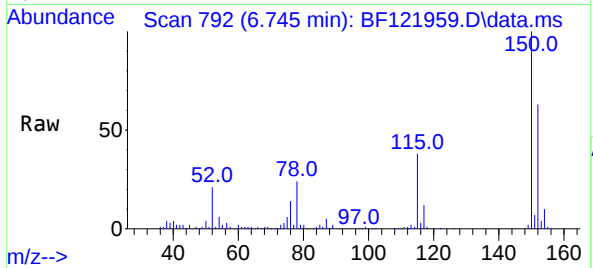

#5
2-Fluorophenol
Concen: 25.78 ng
RT: 5.369 min Scan# 558
Delta R.T. 0.006 min
Lab File: BF121959.D
Acq: 14 Oct 2020 15:56

Tgt Ion:112 Resp: 187397
Ion Ratio Lower Upper
112 100
64 63.0 50.4 75.6
63 31.5 25.8 38.6


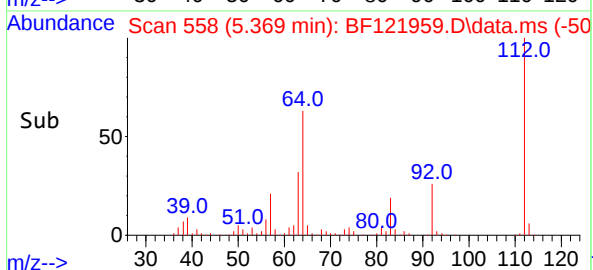
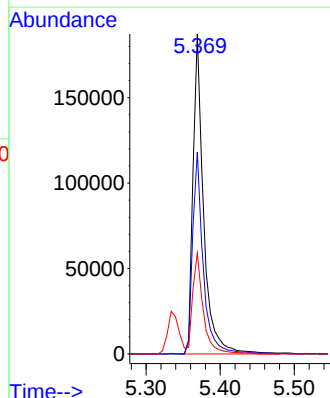
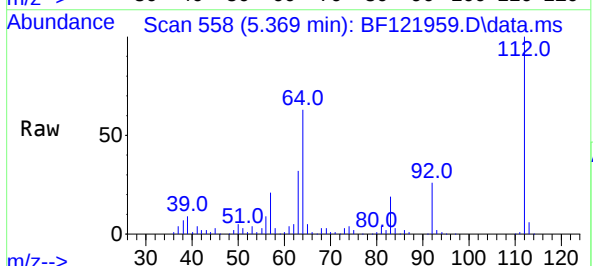


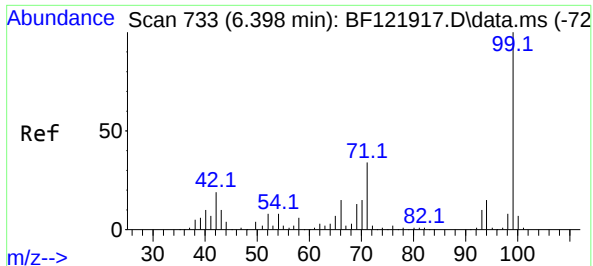

#7
Phenol-d6
Concen: 16.72 ng
RT: 6.398 min Scan# 733
Delta R.T. 0.000 min
Lab File: BF121959.D
Acq: 14 Oct 2020 15:56




Instrument :
BNA_F
ClientSampleId :
EFF-WW


Tgt Ion: 99 Resp: 156506
Ion Ratio Lower Upper
99 100
42 21.0 15.9 23.9
71 33.2 27.1 40.7

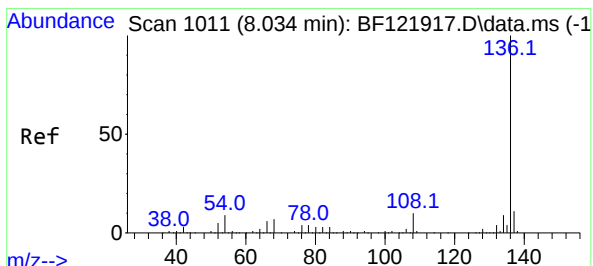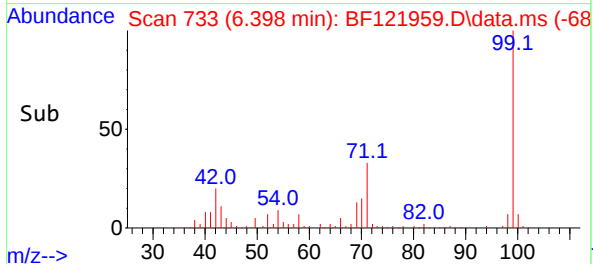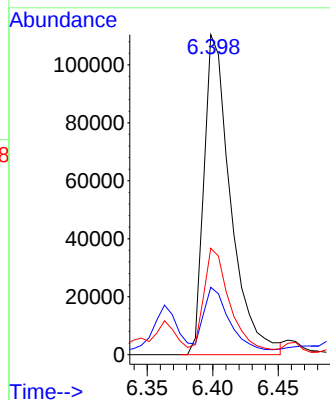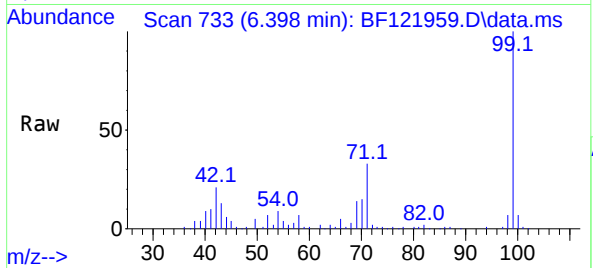

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.028 min Scan# 1010
Delta R.T. -0.006 min
Lab File: BF121959.D
Acq: 14 Oct 2020 15:56

Tgt Ion:136 Resp: 196329
Ion Ratio Lower Upper
136 100
137 10.7 8.6 13.0
54 15.9 7.1 10.7#
68 15.8 5.0 7.4#


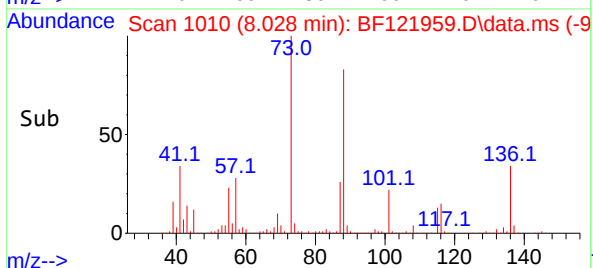
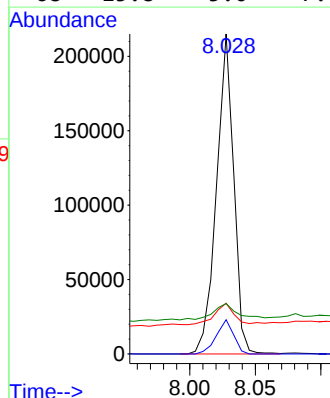
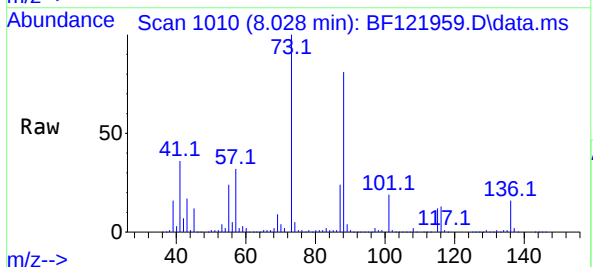


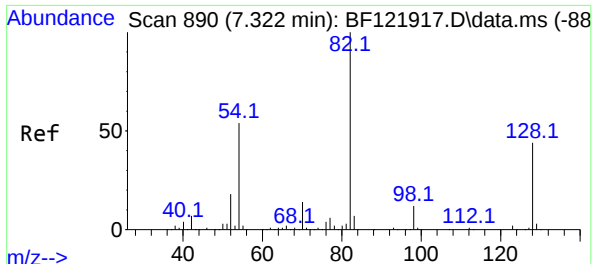

#23
Nitrobenzene-d5
Concen: 146.40 ng
RT: 7.310 min Scan# 888
Delta R.T. -0.012 min
Lab File: BF121959.D
Acq: 14 Oct 2020 15:56




Instrument :
BNA_F
ClientSampleId :
EFF-WW


Tgt Ion: 82 Resp: 560444
Ion Ratio Lower Upper
82 100
128 41.8 35.0 52.4
54 54.2 43.9 65.9

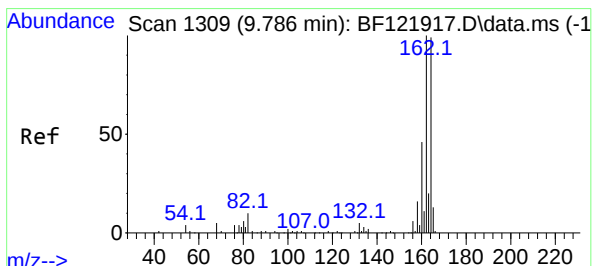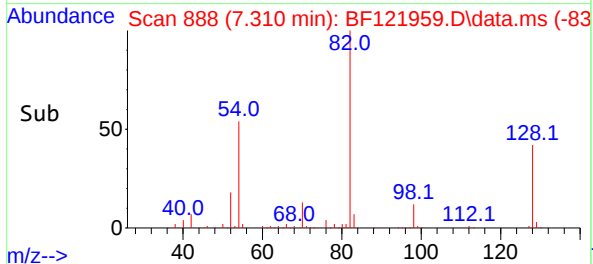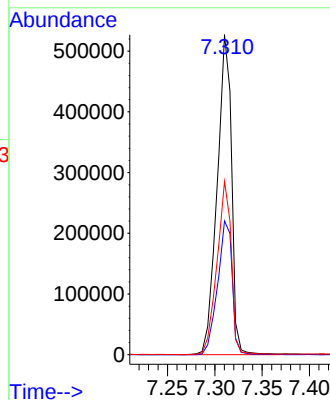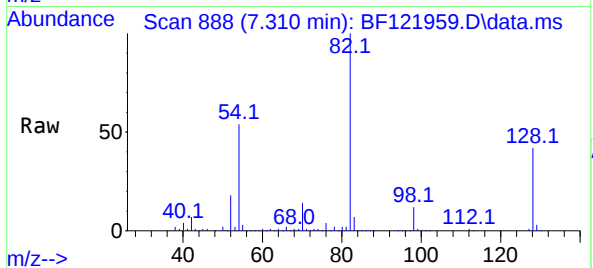

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.786 min Scan# 1309
Delta R.T. 0.000 min
Lab File: BF121959.D
Acq: 14 Oct 2020 15:56

Tgt Ion: 164 Resp: 202080
Ion Ratio Lower Upper
164 100
162 102.7 83.2 124.8
160 46.7 37.5 56.3


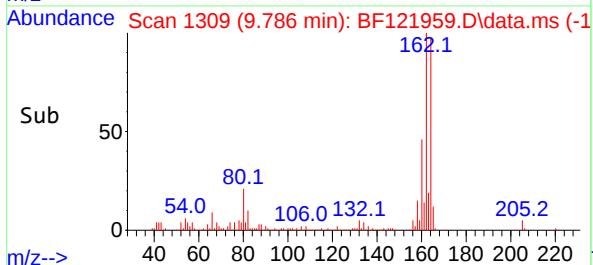
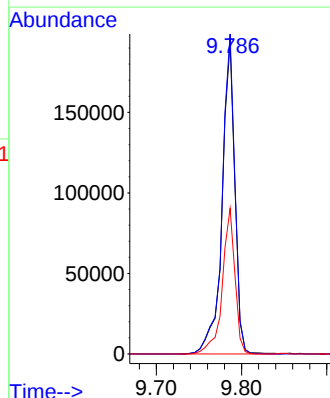
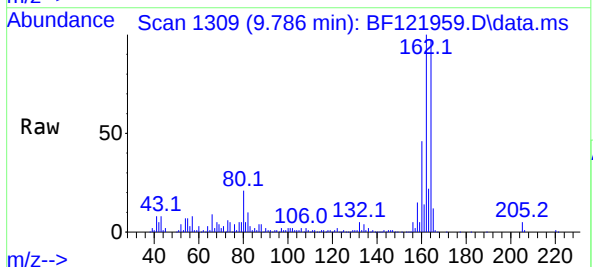


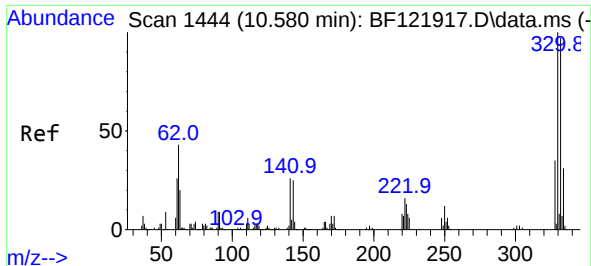

#42
2,4,6-Tribromophenol
Concen: 68.93 ng
RT: 10.581 min Scan# 1444
Delta R.T. 0.000 min
Lab File: BF121959.D
Acq: 14 Oct 2020 15:56




Instrument :
BNA_F
ClientSampleId :
EFF-WW


Tgt Ion:330 Resp: 172306
Ion Ratio Lower Upper
330 100
332 96.0 77.3 115.9
141 28.8 22.3 33.5

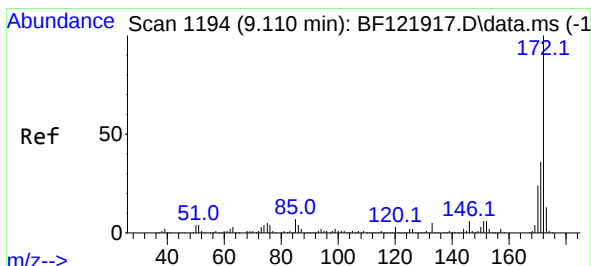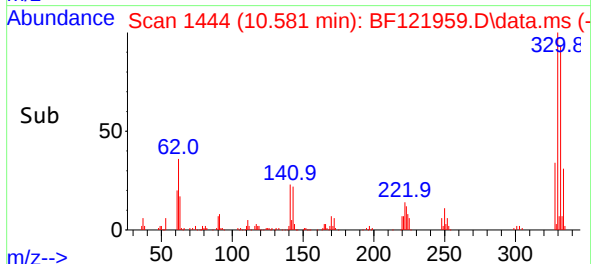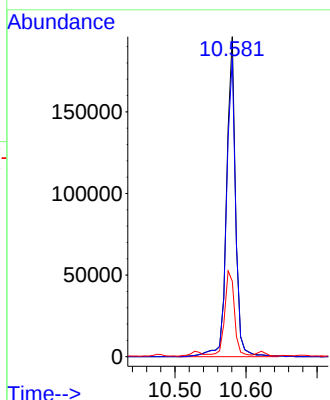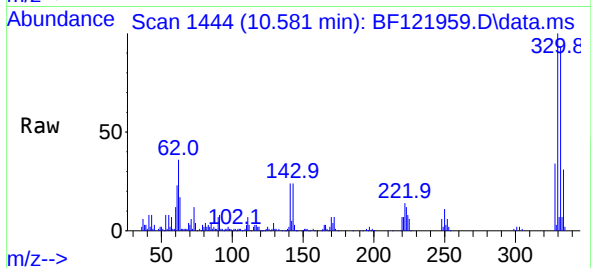

#45
2-Fluorobiphenyl
Concen: 63.63 ng
RT: 9.110 min Scan# 1194
Delta R.T. 0.000 min
Lab File: BF121959.D
Acq: 14 Oct 2020 15:56

Tgt Ion:172 Resp: 873970
Ion Ratio Lower Upper
172 100
171 35.4 29.1 43.7
170 23.5 19.8 29.6


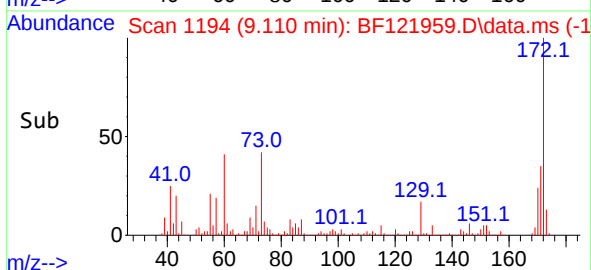
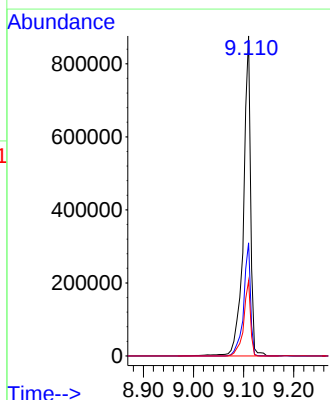
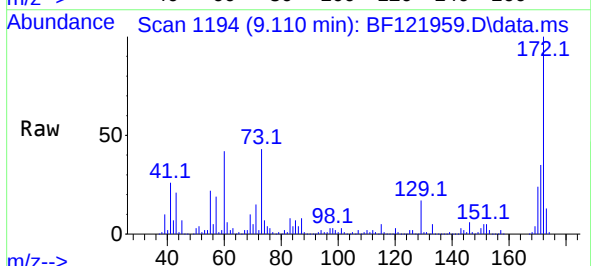


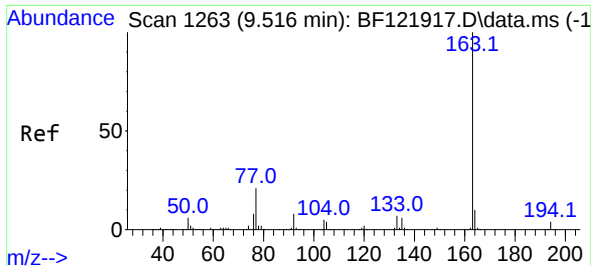

#50
Dimethylphthalate
Concen: 7.64 ng
RT: 9.516 min Scan# 1263
Delta R.T. 0.000 min
Lab File: BF121959.D
Acq: 14 Oct 2020 15:56




Instrument :
BNA_F
ClientSampleId :
EFF-WW


Tgt Ion:163 Resp: 112937
Ion Ratio Lower Upper
163 100
194 4.0 3.3 4.9
164 10.7 8.2 12.4

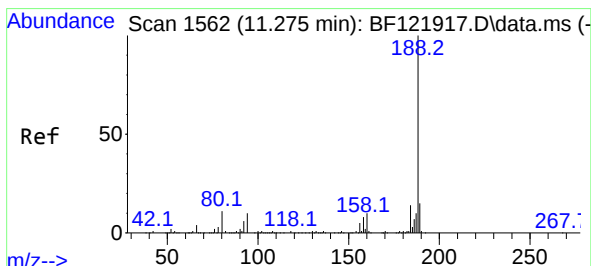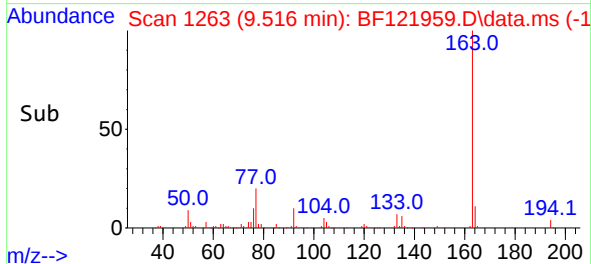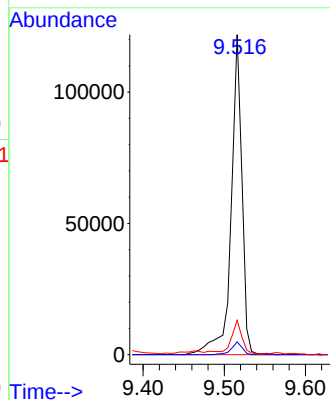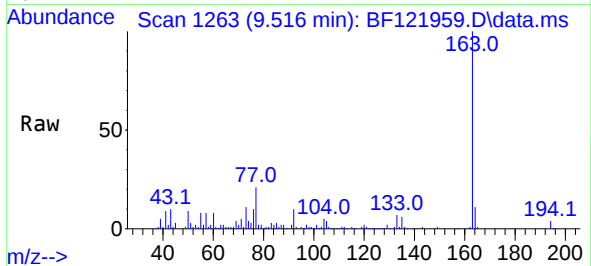

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.269 min Scan# 1561
Delta R.T. -0.006 min
Lab File: BF121959.D
Acq: 14 Oct 2020 15:56

Tgt Ion:188 Resp: 333352
Ion Ratio Lower Upper
188 100
94 11.0 8.3 12.5
80 11.6 9.1 13.7


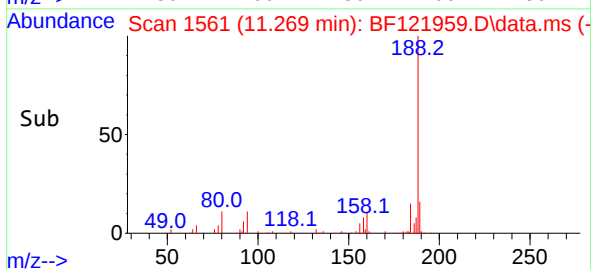
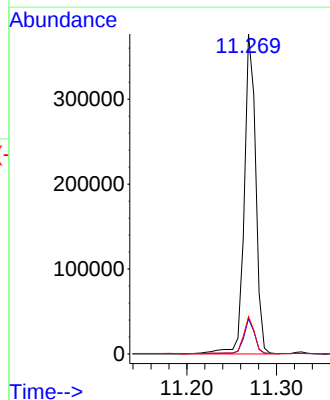
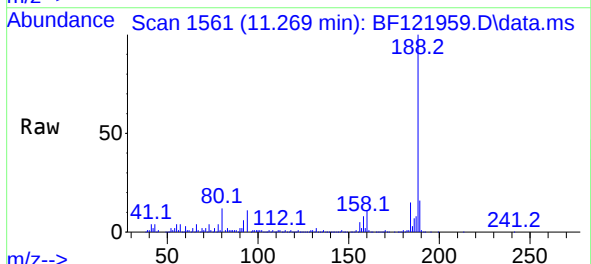


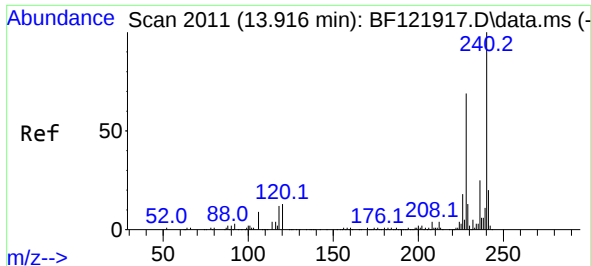

#76
Chrysene-d12
Concen: 20.00 ng
RT: 13.910 min Scan# 2010
Delta R.T. -0.006 min
Lab File: BF121959.D
Acq: 14 Oct 2020 15:56




Instrument :
BNA_F
ClientSampleId :
EFF-WW


Tgt Ion:240 Resp: 228731
Ion Ratio Lower Upper
240 100
120 10.2 9.2 13.8
236 25.4 20.9 31.3

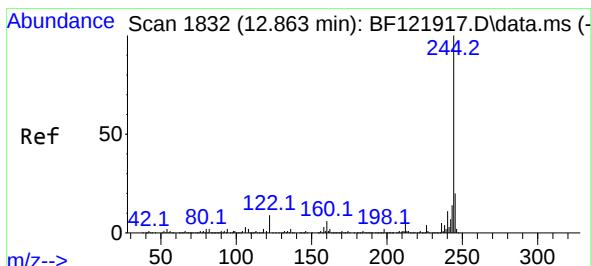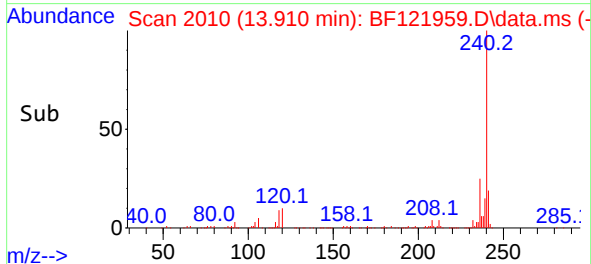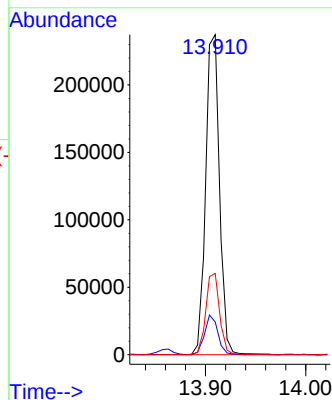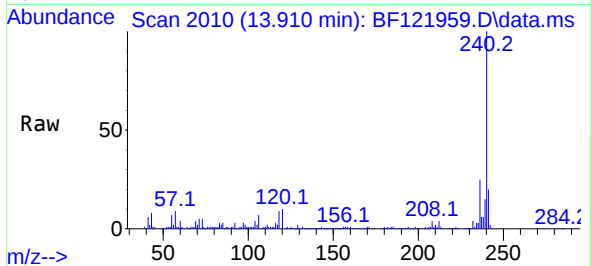

#79
Terphenyl-d14
Concen: 74.79 ng
RT: 12.857 min Scan# 1831
Delta R.T. -0.006 min
Lab File: BF121959.D
Acq: 14 Oct 2020 15:56

Tgt Ion:244 Resp: 897619
Ion Ratio Lower Upper
244 100
212 6.8 5.4 8.2
122 9.8 8.1 12.1

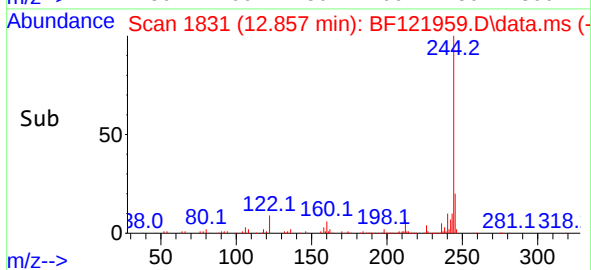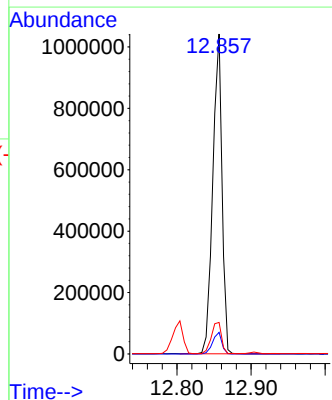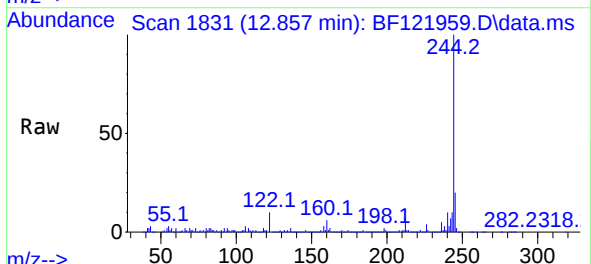

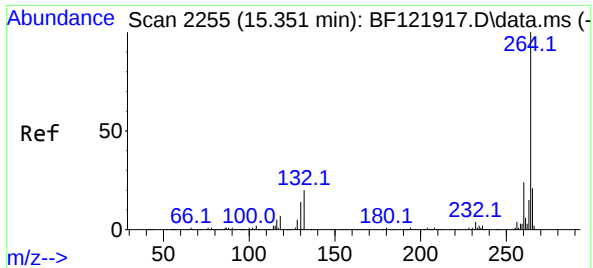

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.339 min Scan# 2253
 Delta R.T. -0.012 min
 Lab File: BF121959.D
 Acq: 14 Oct 2020 15:56

Instrument :
 BNA_F
 ClientSampleId :
 EFF-WW

Tgt Ion:264 Resp: 236265

Ion	Ratio	Lower	Upper
264	100		
260	24.2	18.7	28.1
265	21.5	17.3	25.9

