


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101420\
 Data File : BF121950.D
 Acq On : 14 Oct 2020 10:02
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 12 16:22:33 2020

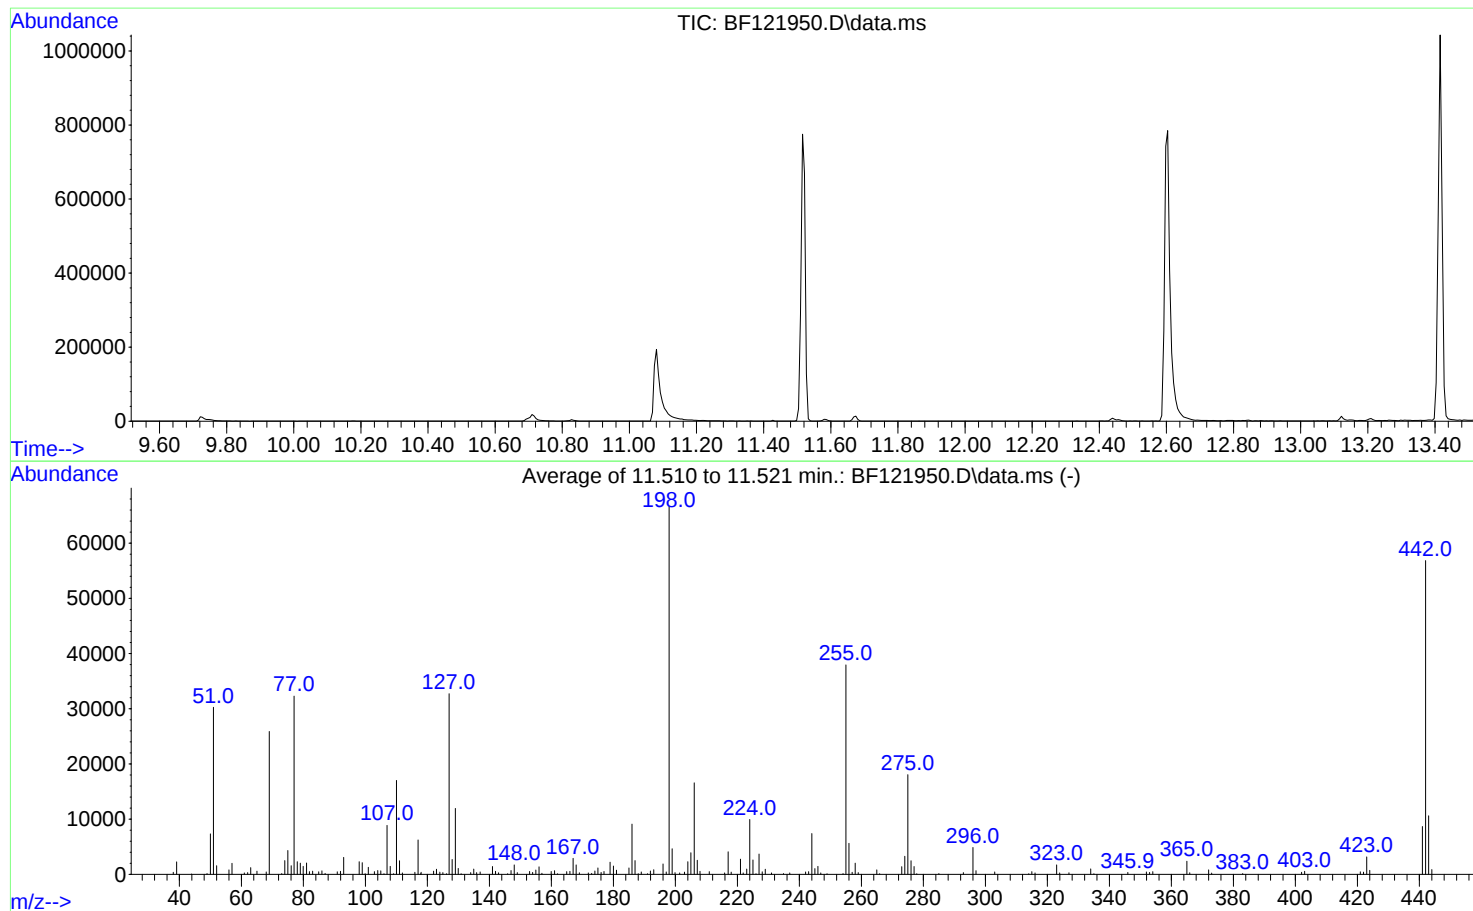

AutoFind: Scans 1602, 1603, 1604; Background Corrected with Scan 1597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.4	30251	PASS
68	69	0.00	2	1.7	428	PASS
69	198	0.00	100	38.8	25872	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.1	32712	PASS
197	198	0.00	2	0.6	429	PASS
198	198	100	100	100.0	66637	PASS
199	198	5	9	7.0	4650	PASS
275	198	10	60	27.1	18068	PASS
365	198	1	100	3.6	2378	PASS
441	198	0.01	100	13.0	8659	PASS
442	198	50	100	85.3	56845	PASS
443	442	15	24	18.7	10602	PASS