


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101420\
Data File : BF121970.D
Acq On : 14 Oct 2020 23:16
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 12 16:22:33 2020

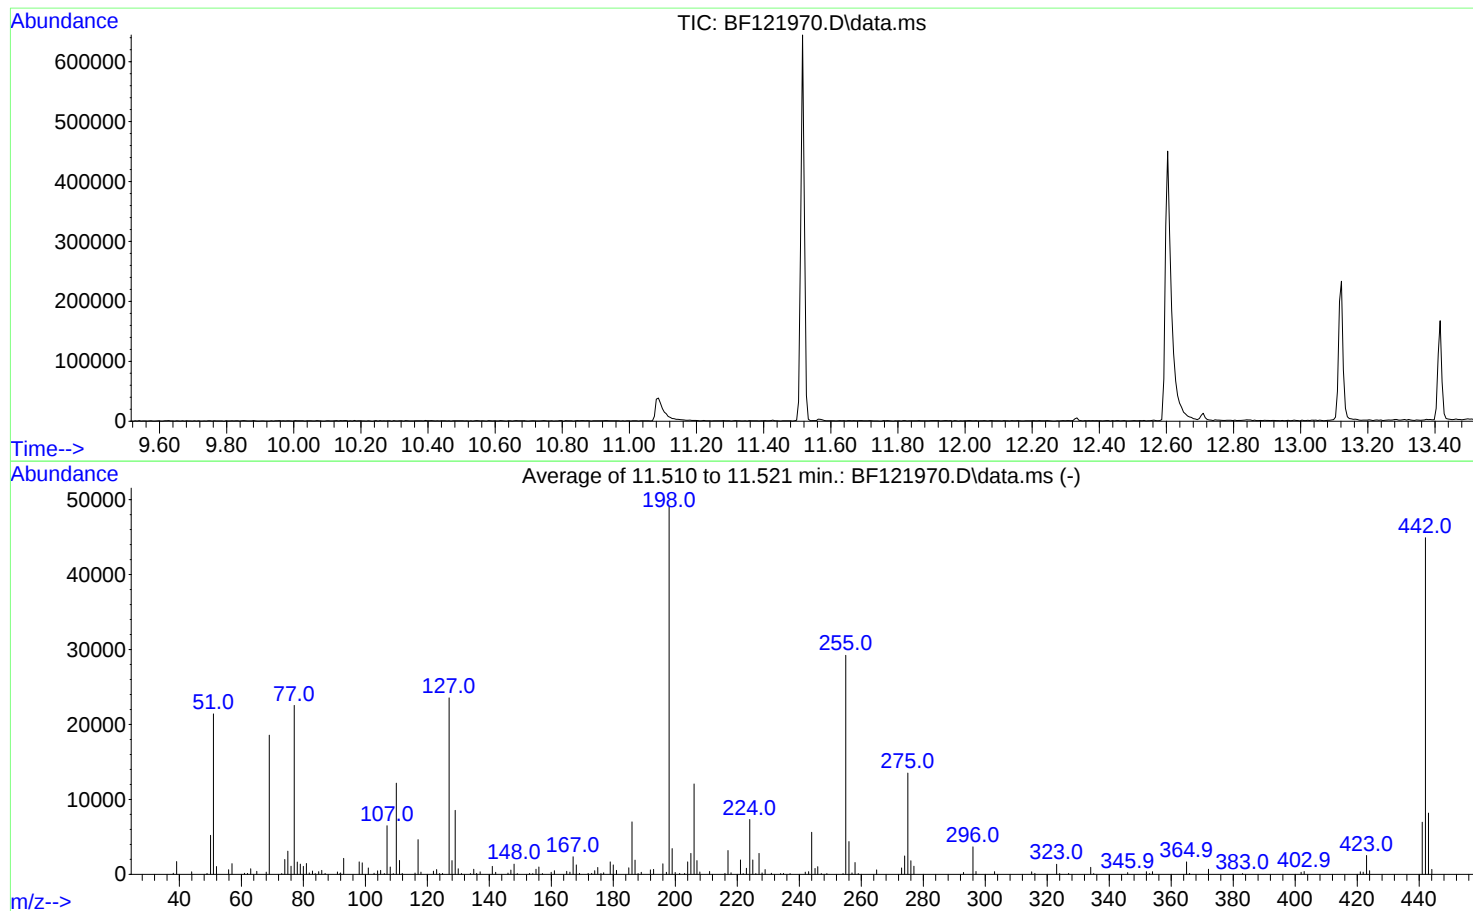

AutoFind: Scans 1602, 1603, 1604; Background Corrected with Scan 1598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.6	21415	PASS
68	69	0.00	2	1.6	293	PASS
69	198	0.00	100	37.8	18570	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.0	23553	PASS
197	198	0.00	2	0.6	279	PASS
198	198	100	100	100.0	49083	PASS
199	198	5	9	7.0	3449	PASS
275	198	10	60	27.5	13510	PASS
365	198	1	100	3.4	1658	PASS
441	198	0.01	100	14.2	6968	PASS
442	198	50	100	91.5	44921	PASS
443	442	15	24	18.2	8186	PASS