


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101422\
 Data File : BF130661.D
 Acq On : 14 Oct 2022 11:01
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 12 06:52:52 2022

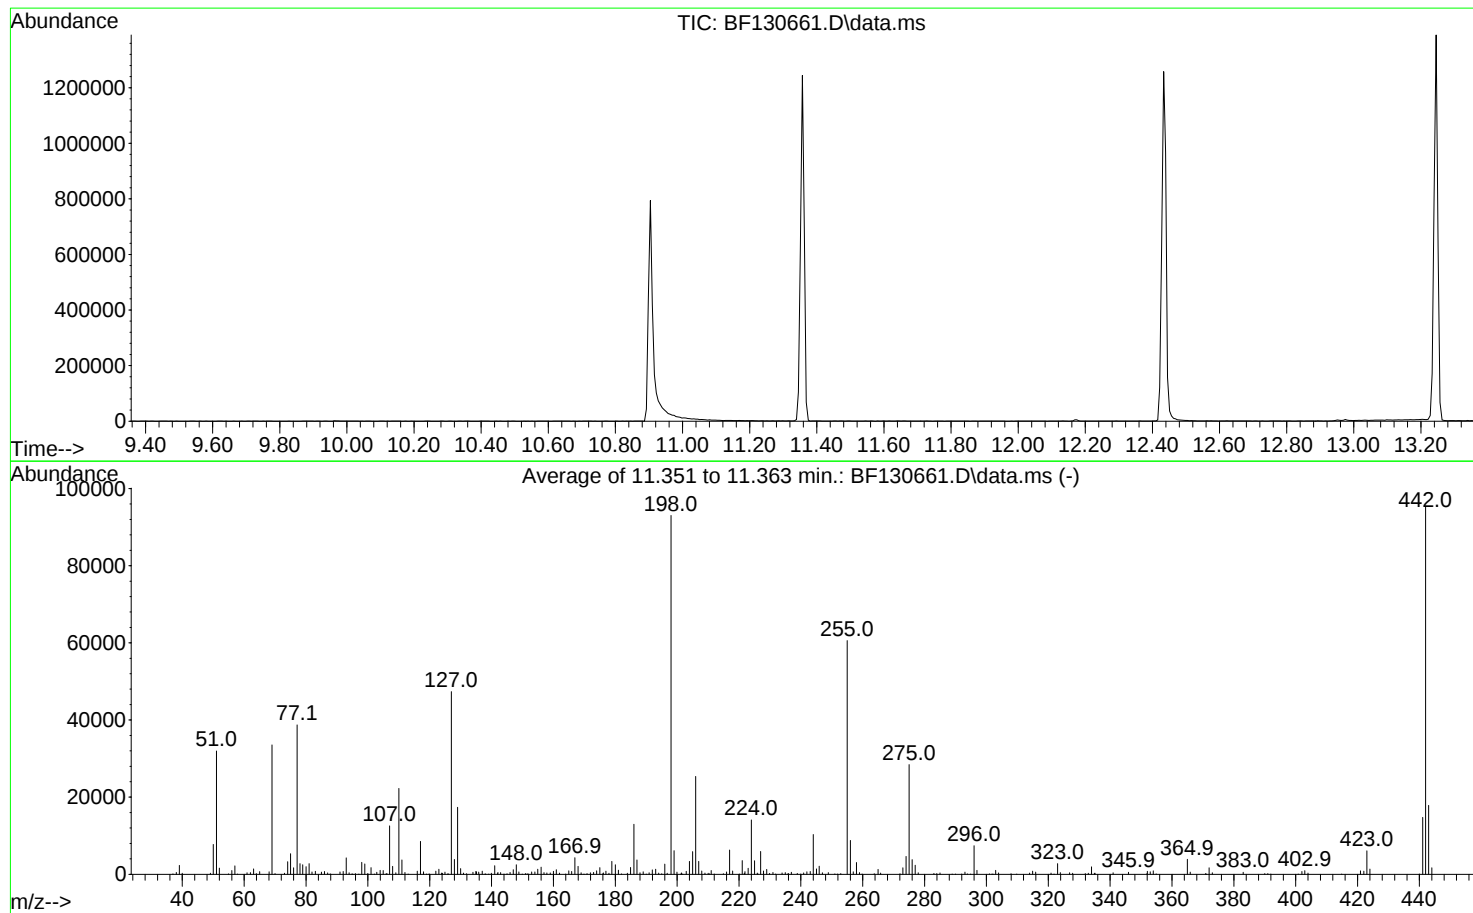




AutoFind: Scans 1575, 1576, 1577; Background Corrected with Scan 1570

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.4	31976	PASS
68	69	0.00	2	1.9	629	PASS
69	198	0.00	100	36.1	33549	PASS
70	69	0.00	2	0.5	182	PASS
127	198	10	80	50.9	47371	PASS
197	198	0.00	2	0.3	282	PASS
198	198	100	100	100.0	93035	PASS
199	198	5	9	6.6	6135	PASS
275	198	10	60	30.6	28456	PASS
365	198	1	100	4.2	3869	PASS
441	198	0.01	100	15.9	14750	PASS
442	442	50	100	100.0	95376	PASS
443	442	15	24	18.7	17851	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101422\
Data File : BF130661.D
Acq On : 14 Oct 2022 11:01
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 17 05:52:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 12 06:52:52 2022
Response via : Initial Calibration

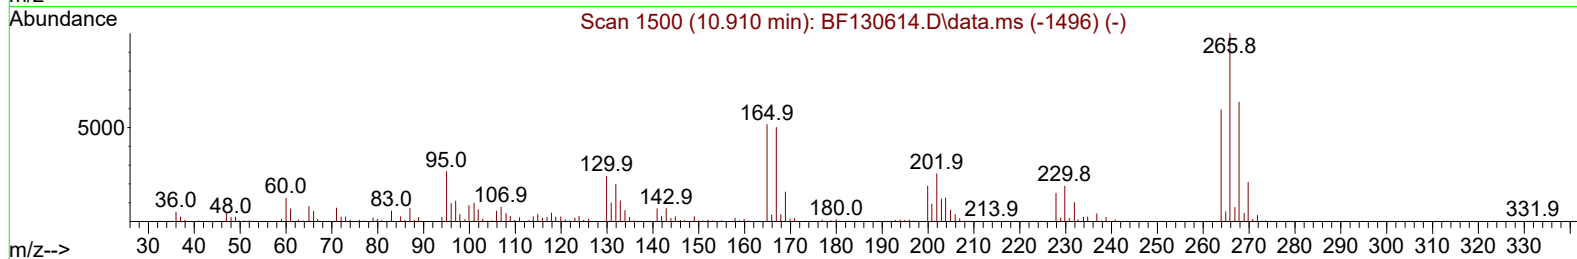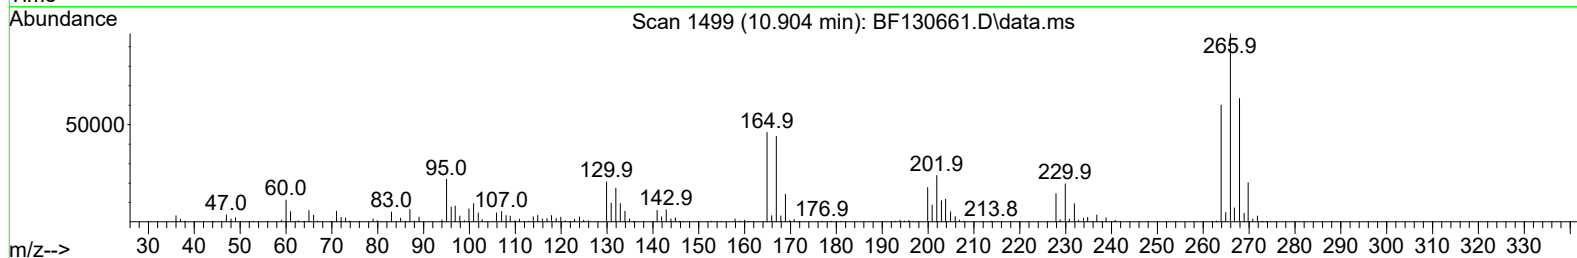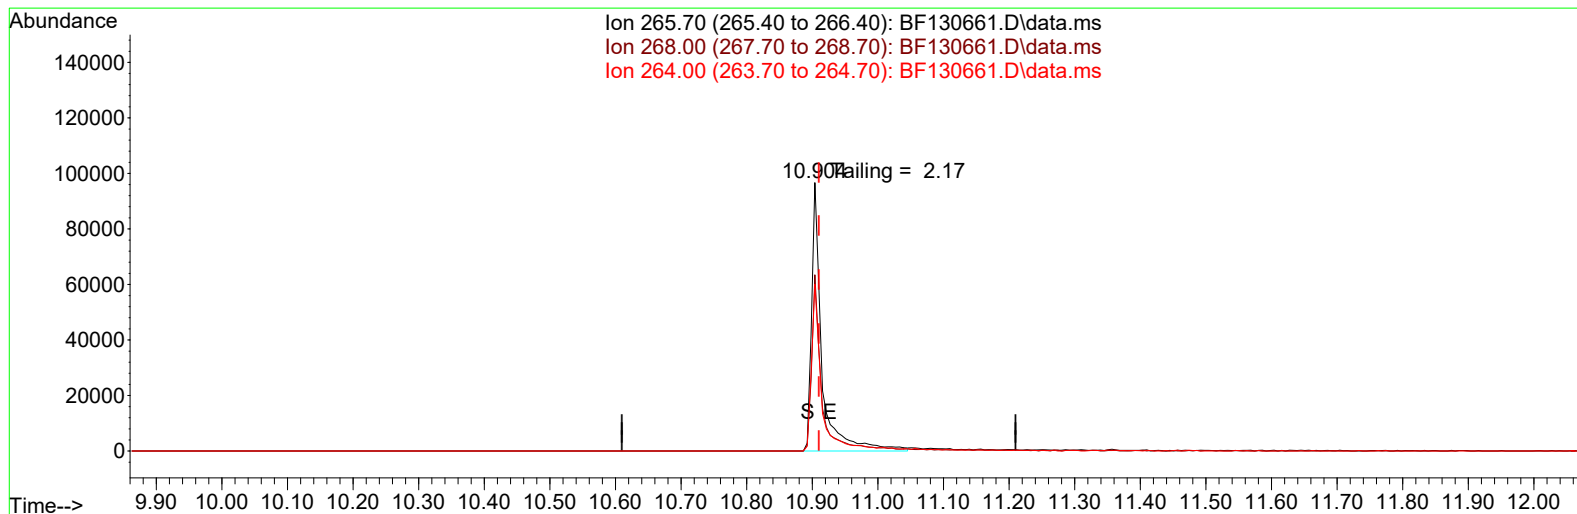

TIC: BF130661.D\data.ms

(70) Pentachlorophenol (C)

10.904min (-0.006) 54946.98 ng




response 108866

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	65.63
264.00	59.40	62.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101422\
Data File : BF130661.D
Acq On : 14 Oct 2022 11:01
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 17 05:52:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 12 06:52:52 2022
Response via : Initial Calibration

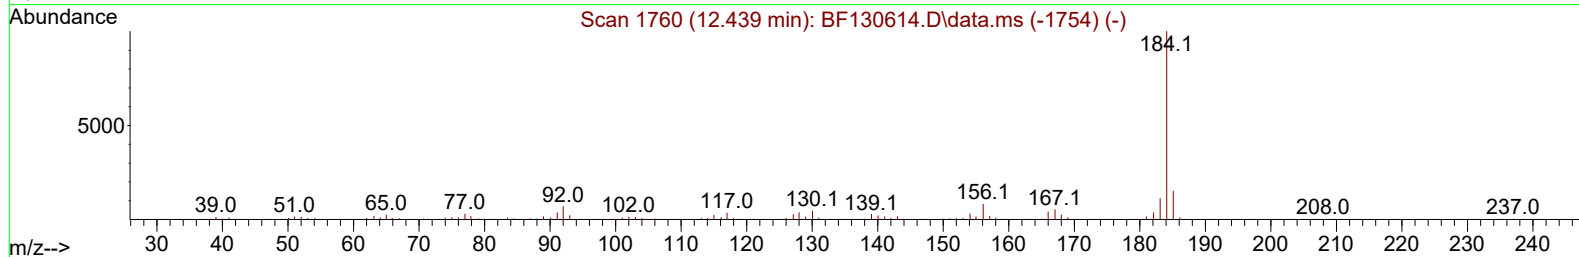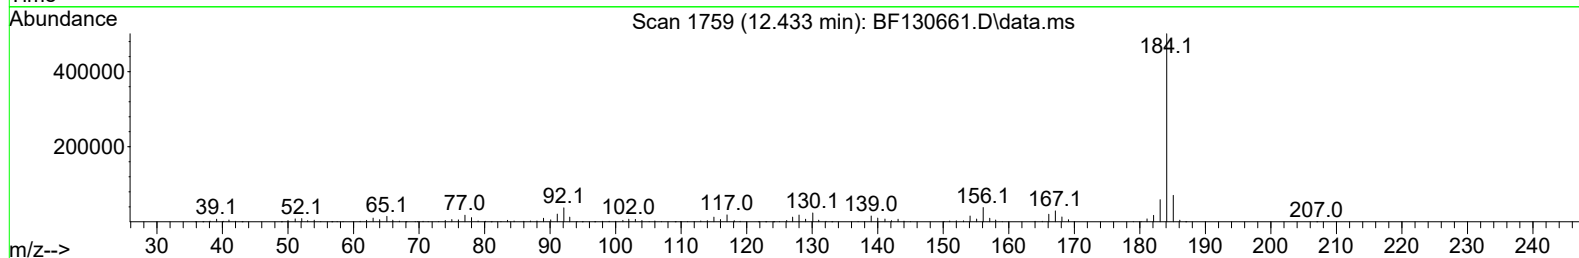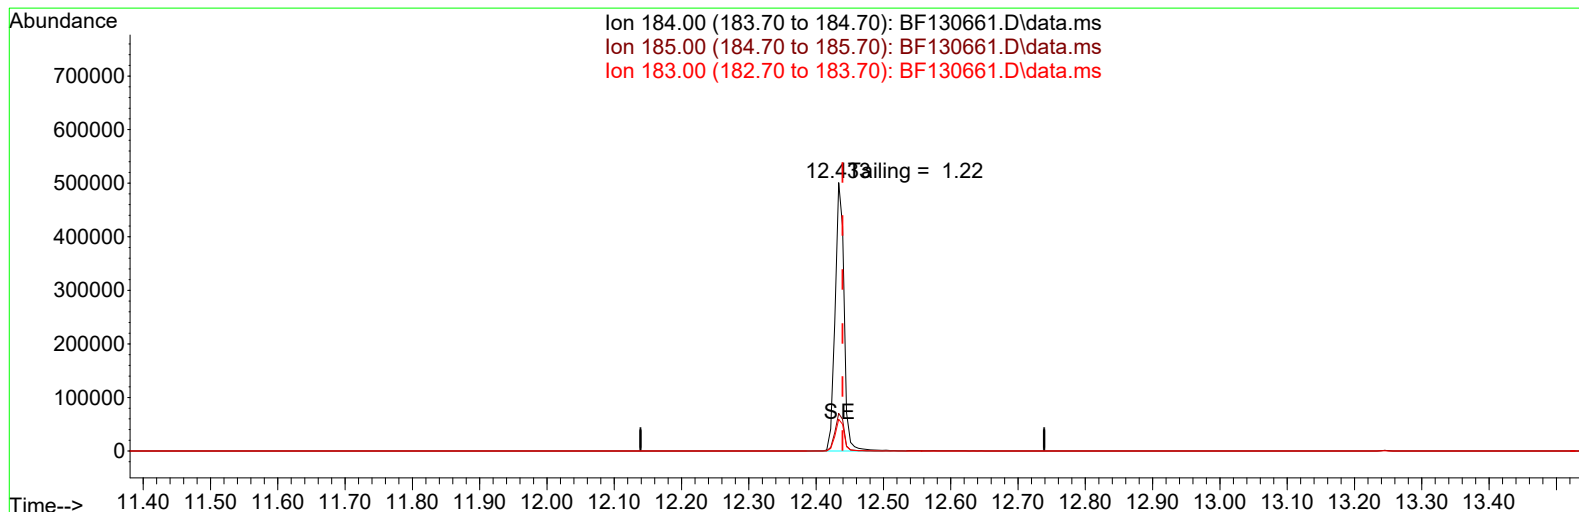

TIC: BF130661.D\data.ms

(77) Benzidine

12.433min (-0.006) 0.00 ng

response 466866

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.06
183.00	11.20	11.81
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/14/2022	BNA_F	<u>BF130661.D</u>
Compound Name	Response	Retention Time
DDT	214077	13.245
DDD	2405	12.975
DDE	144	12.616
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2549	216626	1.18

Instrument :
BNA_F
ClientSampleId :
DFTPP