
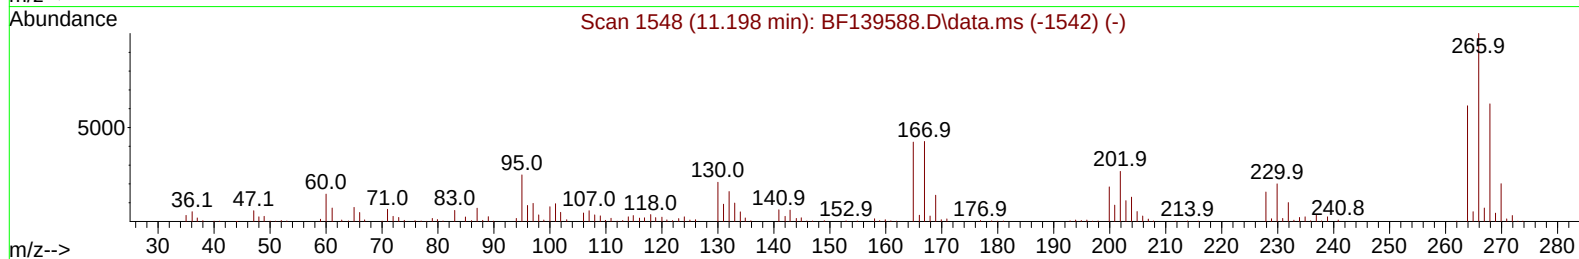
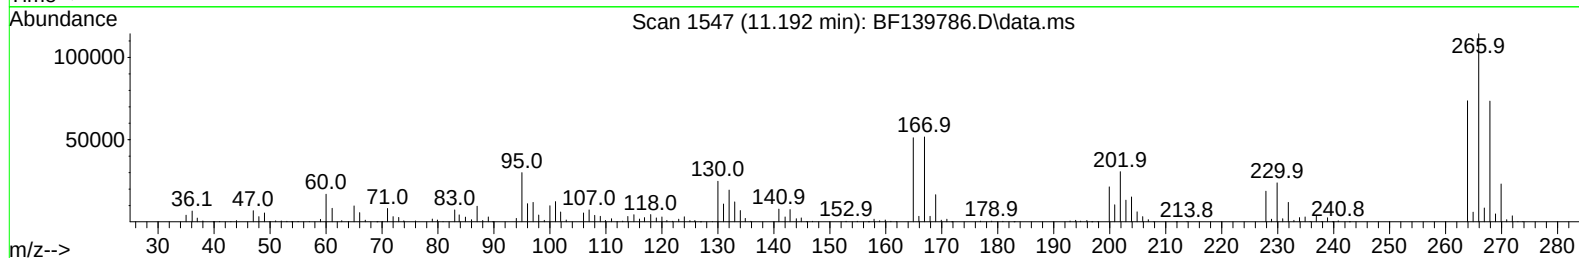


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101424\
Data File : BF139786.D
Acq On : 14 Oct 2024 12:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 14 13:41:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 02 04:58:47 2024
Response via : Initial Calibration

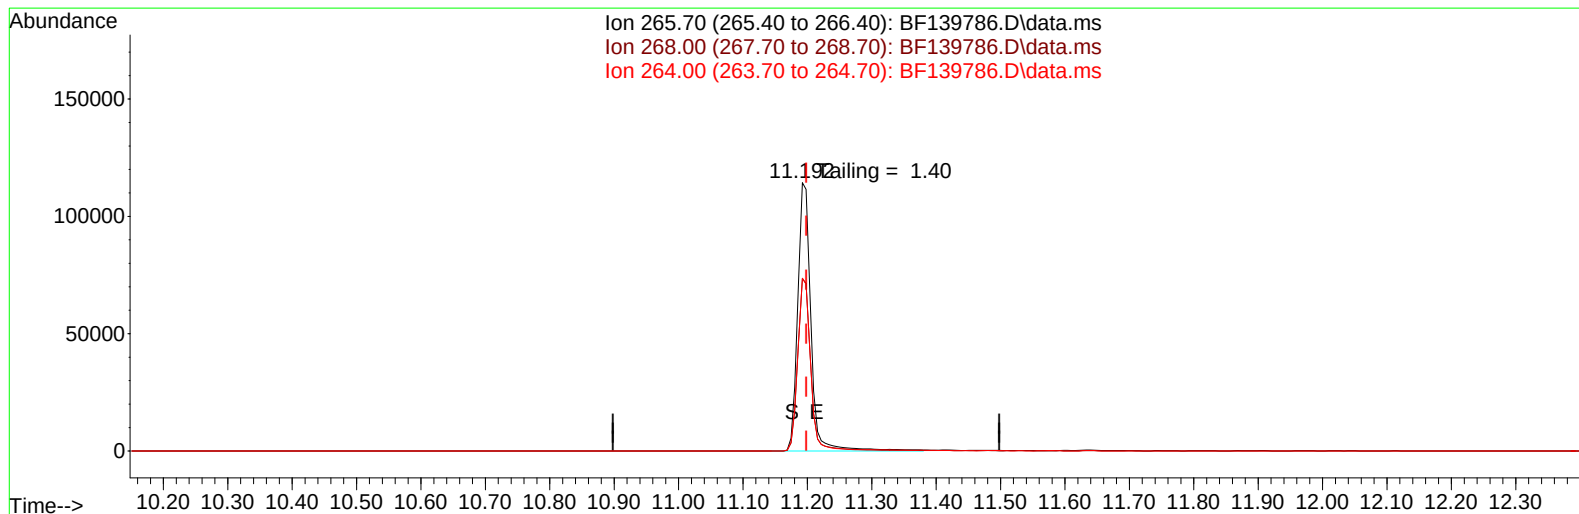

TIC: BF139786.D\data.ms




(70) Pentachlorophenol (C)

11.192min (-0.006) 59036.40 ng

response 164778

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.50	64.26
264.00	61.60	64.37
0.00	0.00	0.00

Quant Time: Oct 14 13:41:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 02 04:58:47 2024
Response via : Initial Calibration

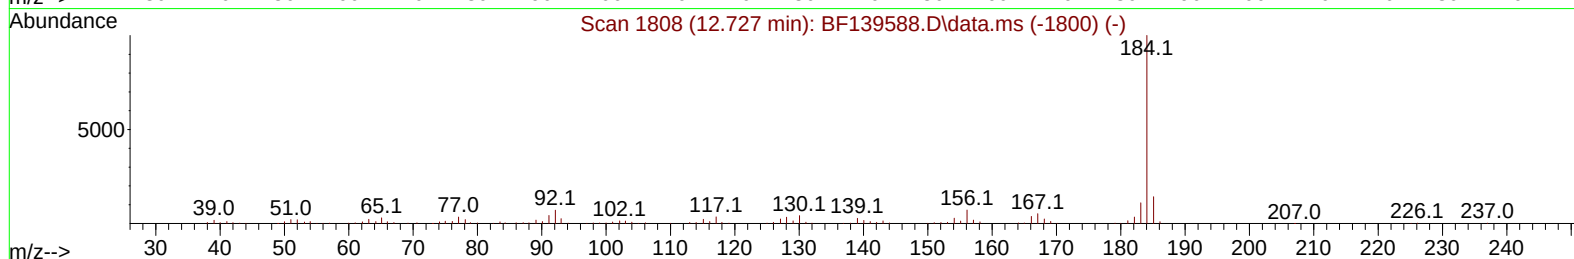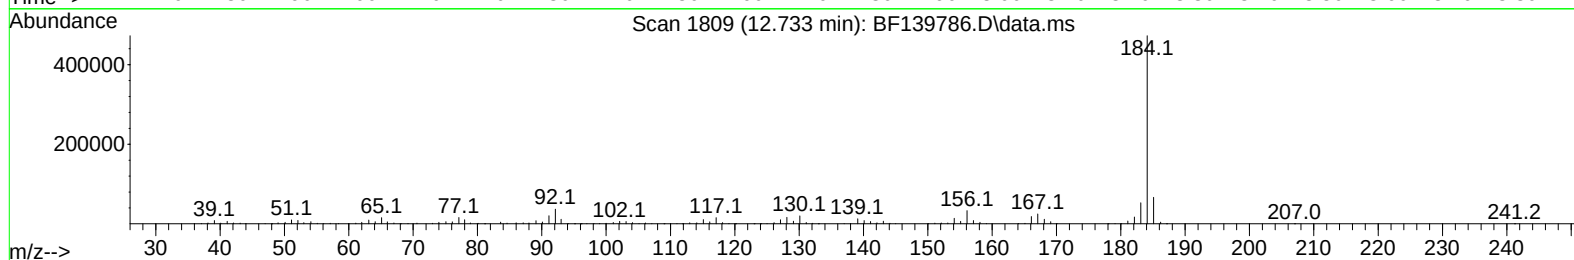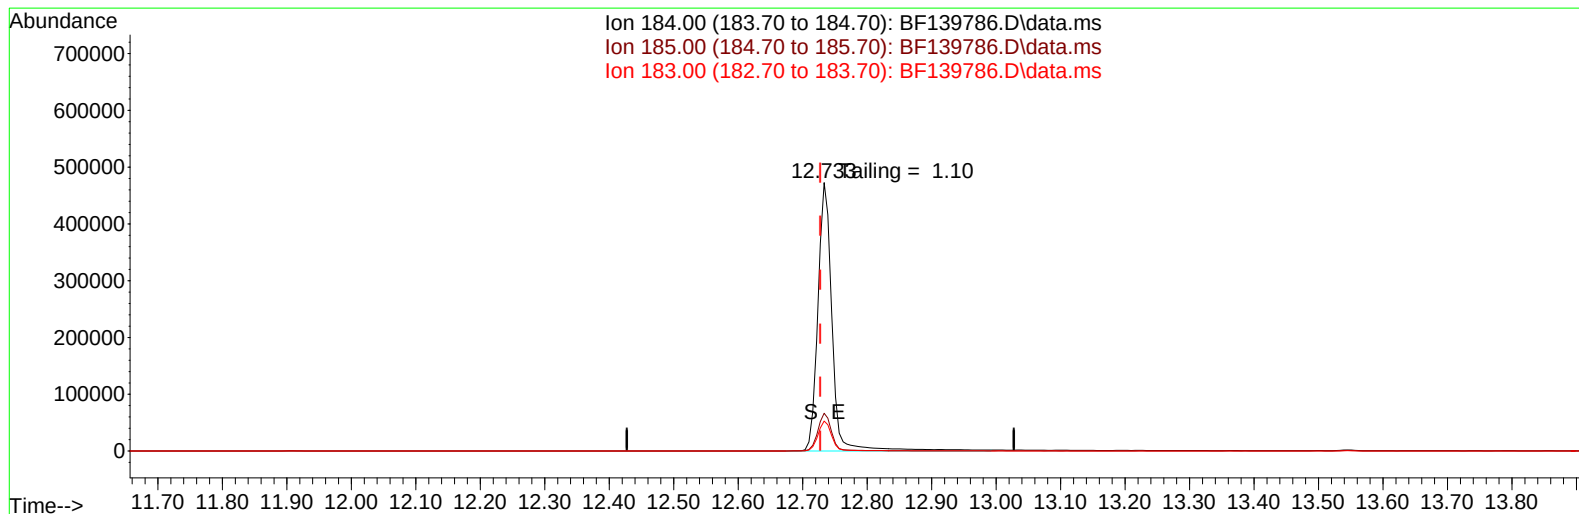

TIC: BF139786.D\data.ms

(77) Benzidine

12.733min (+ 0.006) 81640.97 ng

response **721465**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.09
183.00	11.00	11.15
0.00	0.00	0.00