


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101424\
Data File : BF139786.D
Acq On : 14 Oct 2024 12:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 02 04:58:47 2024

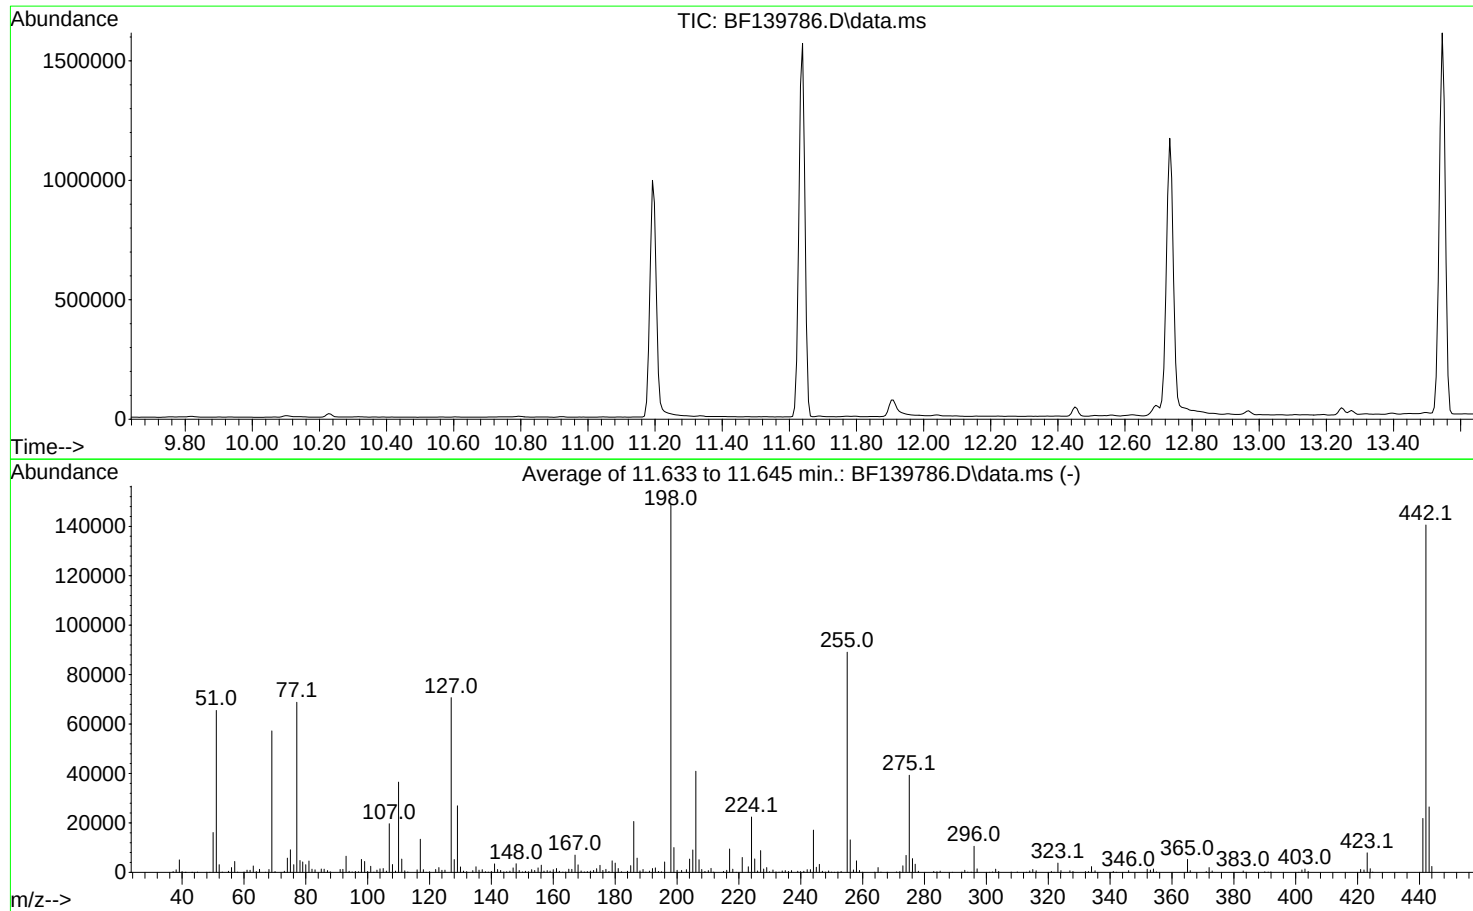

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.0	65522	PASS
68	69	0.00	2	2.0	1137	PASS
69	198	0.00	100	38.5	57235	PASS
70	69	0.00	2	0.6	348	PASS
127	198	10	80	47.5	70691	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	148840	PASS
199	198	5	9	6.8	10061	PASS
275	198	10	60	26.4	39296	PASS
365	198	1	100	3.5	5242	PASS
441	198	0.01	100	14.7	21840	PASS
442	442	50	100	100.0	140523	PASS
443	442	15	24	18.8	26461	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/14/2024	BNA_F	<u>BF139786.D</u>
Compound Name	Response	Retention Time
DDT	391467	13.545
DDD	13352	13.245
DDE	449	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13801	405268	3.41

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101424\
Data File : BF139786.D
Acq On : 14 Oct 2024 12:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 14 13:41:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 02 04:58:47 2024
Response via : Initial Calibration

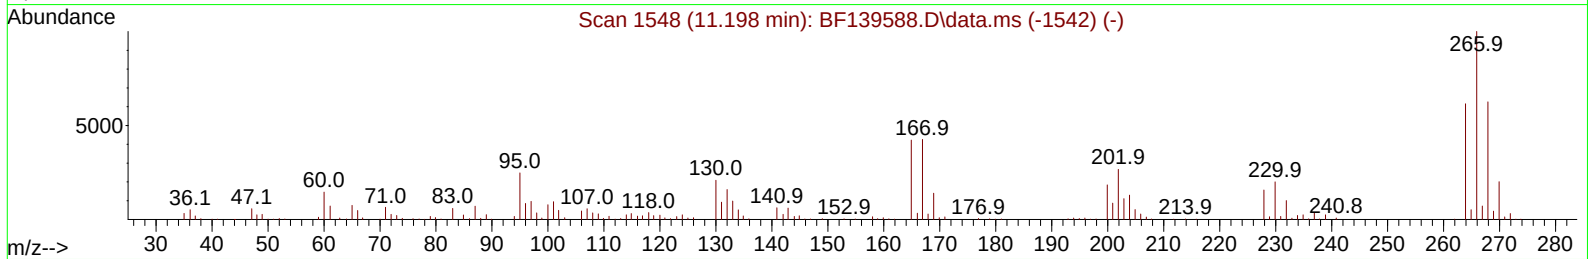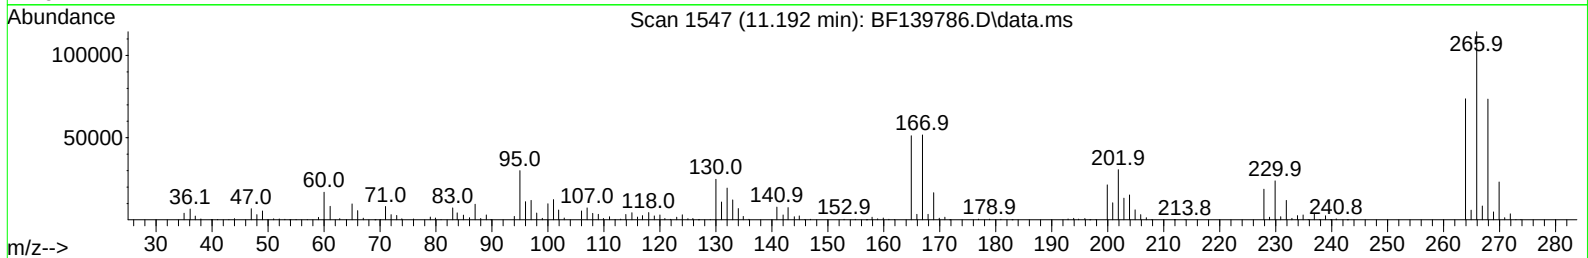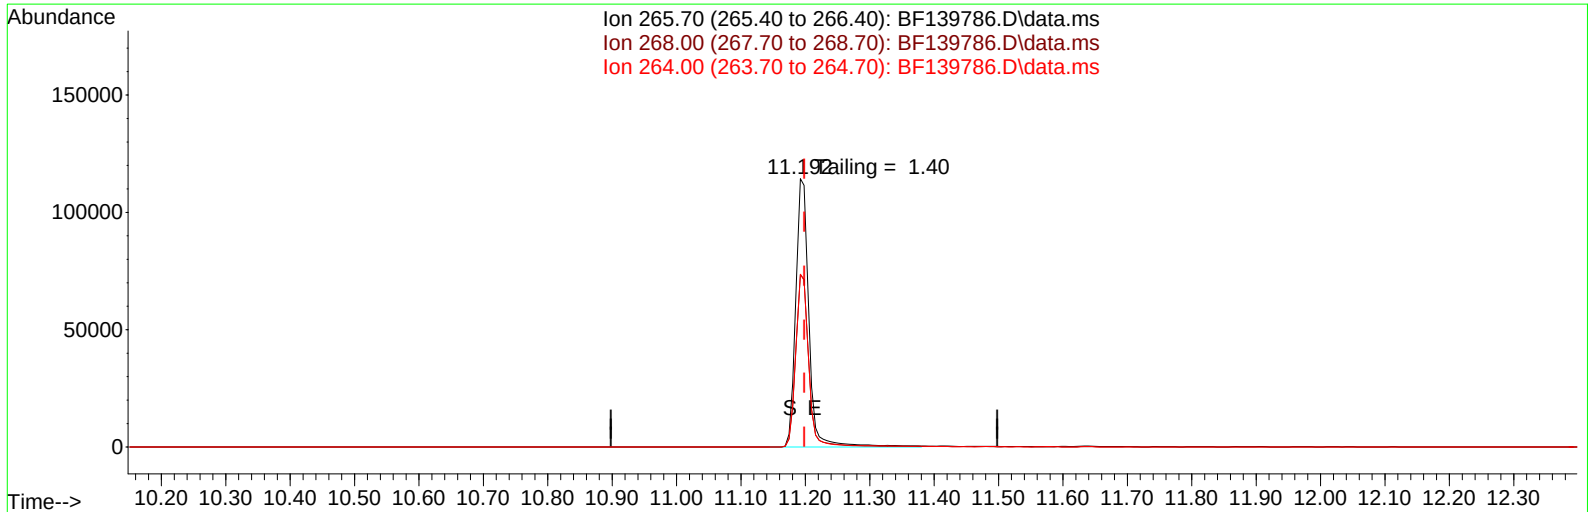

TIC: BF139786.D\data.ms

(70) Pentachlorophenol (C)

11.192min (-0.006) 59036.40 ng




response 164778

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.50	64.26
264.00	61.60	64.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101424\
Data File : BF139786.D
Acq On : 14 Oct 2024 12:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 14 13:41:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 02 04:58:47 2024
Response via : Initial Calibration

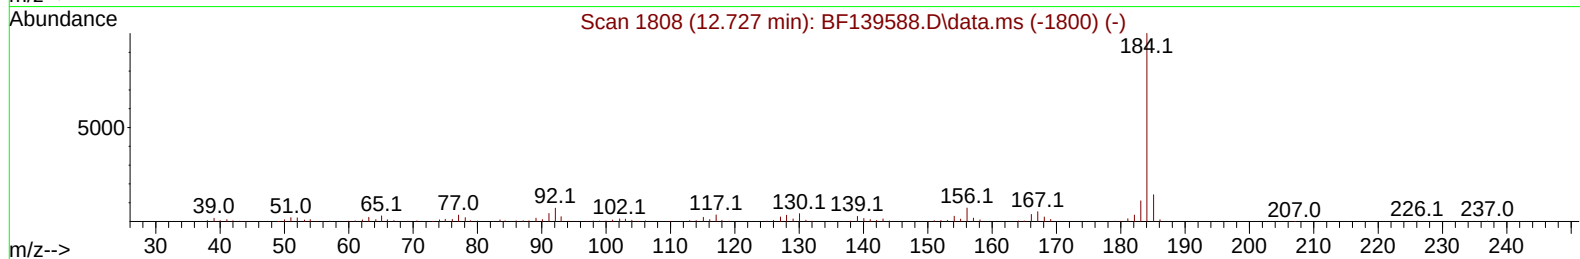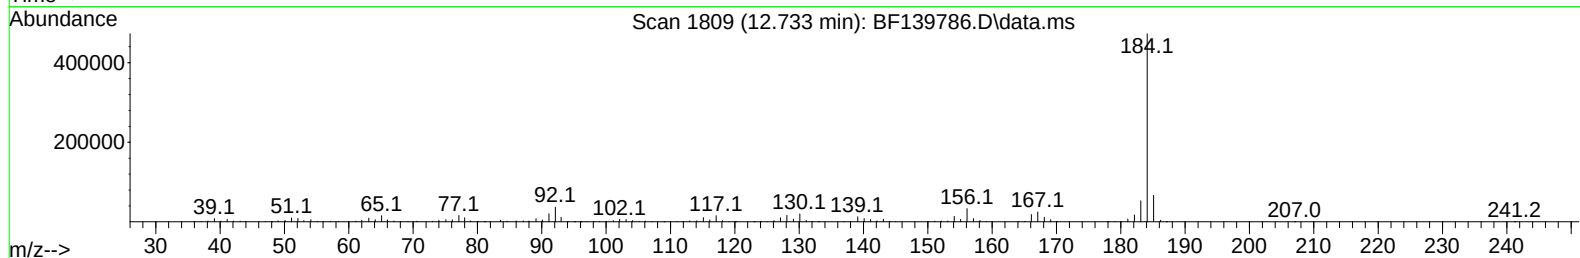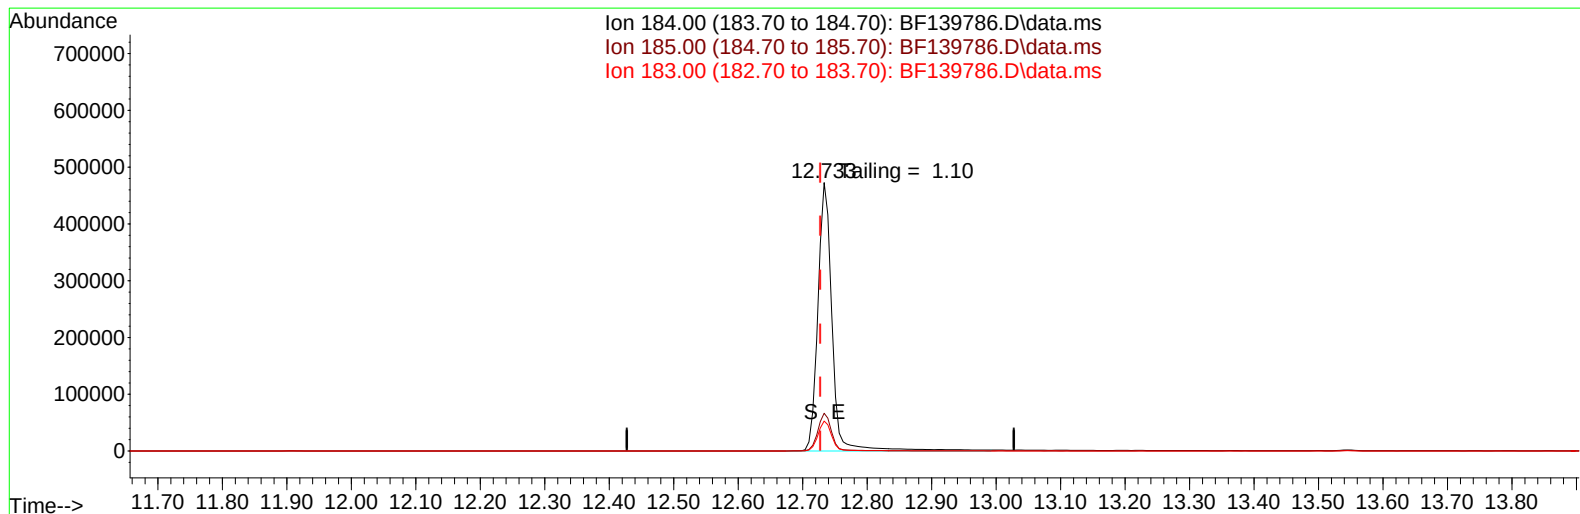

TIC: BF139786.D\data.ms

(77) Benzidine

12.733min (+ 0.006) 81640.97 ng

response 721465

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.09
183.00	11.00	11.15
0.00	0.00	0.00