

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101515\
 Data File : BF082299.D
 Acq On : 15 Oct 2015 4:48
 Operator : UM/IZ
 Sample : G4016-11
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CS-12

Quant Time: Oct 15 06:07:34 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF101015.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 15 04:19:20 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.82	152	78412	20.00	ng	0.00
21) Naphthalene-d8	8.11	136	317010	20.00	ng	0.00
38) Acenaphthene-d10	9.87	164	156048	20.00	ng	0.00
63) Phenanthrene-d10	11.36	188	311929	20.00	ng	0.00
75) Chrysene-d12	14.04	240	241093	20.00	ng	0.00
86) Perylene-d12	15.54	264	187518	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.42	112	5196	1.34	ng	0.01
7) Phenol-d6	6.46	99	153411	30.34	ng	-0.01
23) Nitrobenzene-d5	7.39	82	397924	84.30	ng	-0.01
41) 2,4,6-Tribromophenol	0.00	330	0	0.00	ng	
44) 2-Fluorobiphenyl	9.19	172	754935	80.23	ng	-0.01
78) Terphenyl-d14	12.96	244	817823	89.89	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.39	70	51062	14.38	ng	# 79
25) Isophorone	7.39	82	298862	31.37	ng	# 66
49) Dimethylphthalate	9.59	163	159913	14.55	ng	99
50) 2,6-Dinitrotoluene	9.62	165	5775	2.49	ng	# 30
56) 2,4-Dinitrotoluene	9.87	165	20252	6.99	ng	# 21


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101515\
Data File : BF082299.D
Acq On : 15 Oct 2015 4:48
Operator : UM/IZ
Sample : G4016-11
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CS-12

Quant Time: Oct 15 06:07:34 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 15 04:19:20 2015
Response via : Initial Calibration

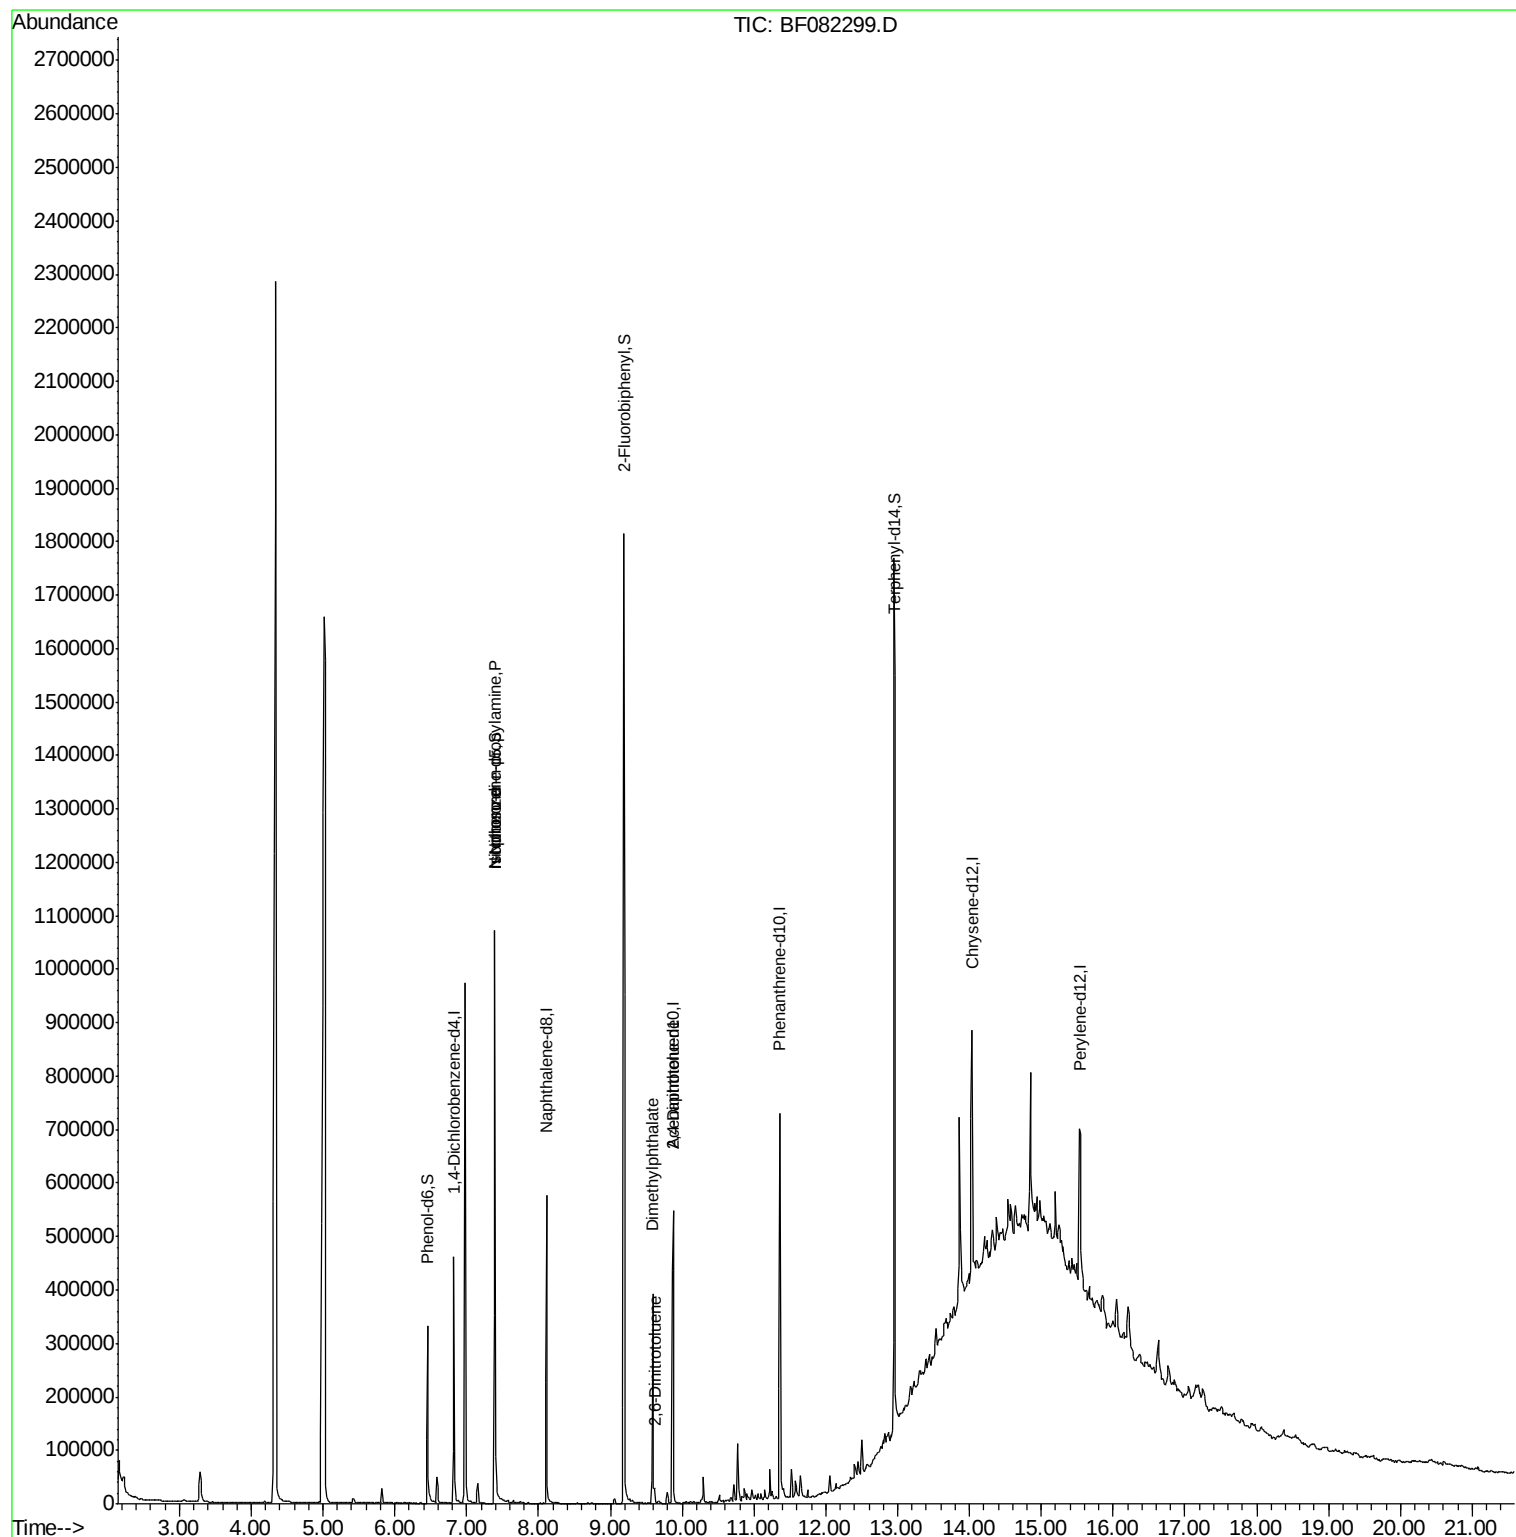



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.82 min Scan# 410

Delta R.T. 0.00 min

Lab File: BF082299.D

Acq: 15 Oct 2015 4:48

Instrument :

BNA_F

ClientSampleId :

CS-12


Tot Ion:152 Resp: 78412

Ion Ratio Lower Upper

152 100

150 158.1 129.0 193.4




115 54.2 52.1 78.1



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

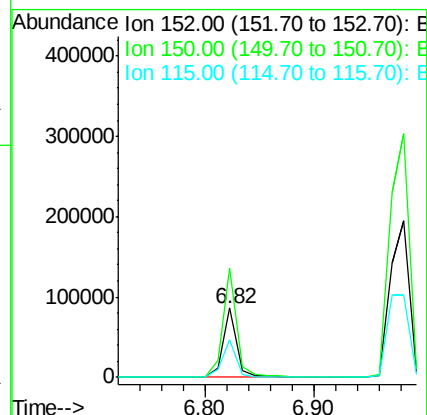

#5

2-Fluorophenol

Concen: 1.34 ng

RT: 5.42 min Scan# 287

Delta R.T. 0.01 min

Lab File: BF082299.D

Acq: 15 Oct 2015 4:48


Tgt Ion:112 Resp: 5196

Ion Ratio Lower Upper

112 100

64 69.9 48.6 73.0



63 34.2 25.1 37.7






Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

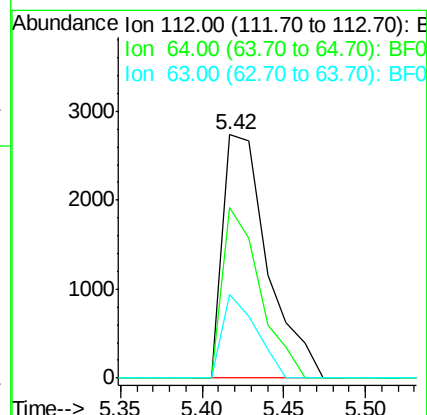

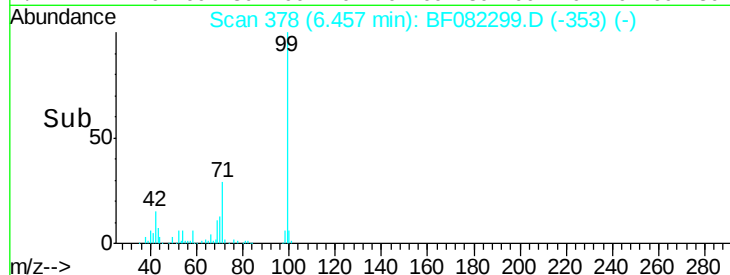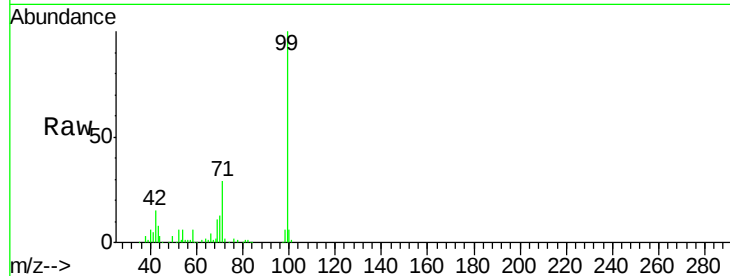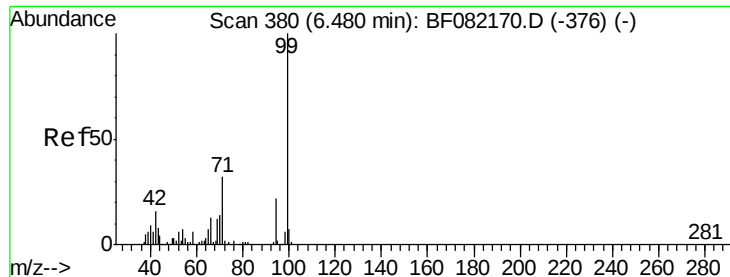

#7

Phenol-d6

Concen: 30.34 ng

RT: 6.46 min Scan# 378

Delta R.T. -0.01 min

Lab File: BF082299.D

Acq: 15 Oct 2015 4:48

Instrument :

BNA_F

ClientSampleId :

CS-12





Tot Ion: 99 Resp: 153411

Ion Ratio Lower Upper

99 100

42 14.8 13.2 19.8

71 29.3 25.6 38.4

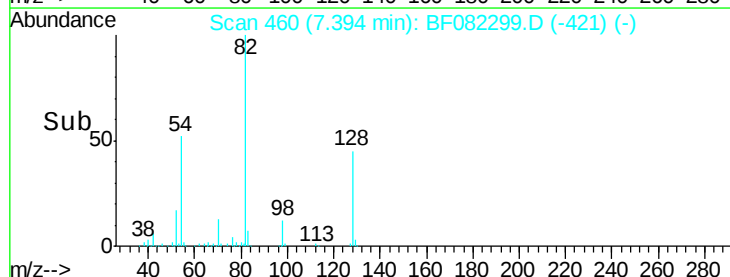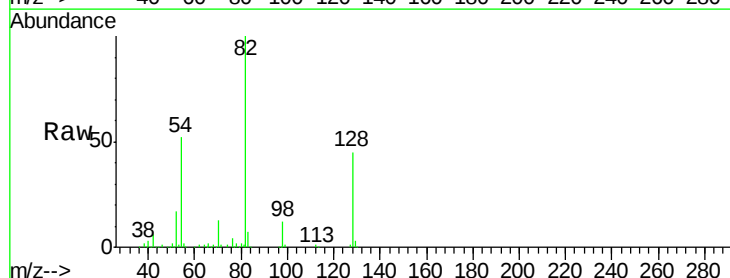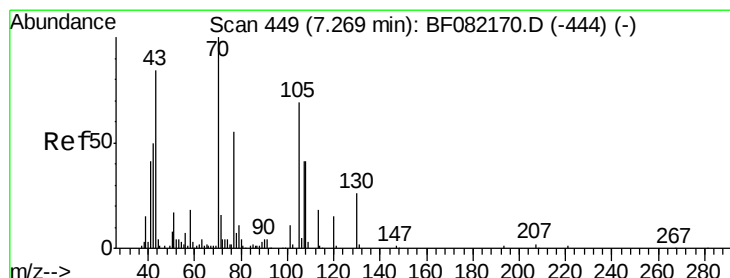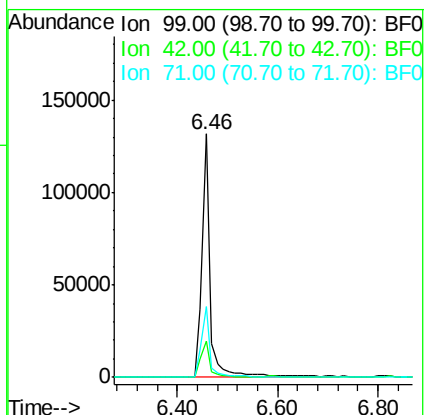

#19

n-Nitroso-di-n-propylamine

Concen: 14.38 ng

RT: 7.39 min Scan# 460

Delta R.T. 0.15 min

Lab File: BF082299.D

Acq: 15 Oct 2015 4:48

Tgt Ion: 70 Resp: 51062


Ion Ratio Lower Upper


70 100

42 45.1 39.8 59.8

101 0.0 8.6 13.0#

130 2.2 20.5 30.7#

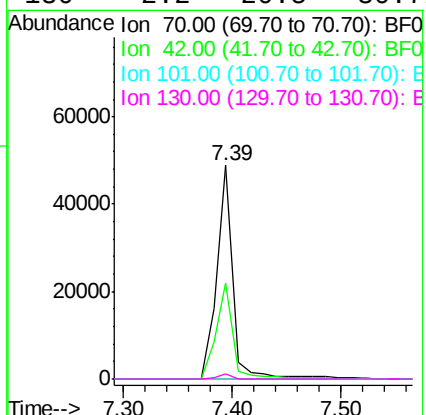



#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.11 min Scan# 523

Delta R.T. 0.00 min

Lab File: BF082299.D

Acq: 15 Oct 2015 4:48

Instrument :

BNA_F

ClientSampleId :

CS-12

Tot Ion:136 Resp: 317010


Ion Ratio Lower Upper

136 100

137 10.7 9.0 13.6

54 6.0 7.5 11.3#

68 4.4 4.6 7.0#



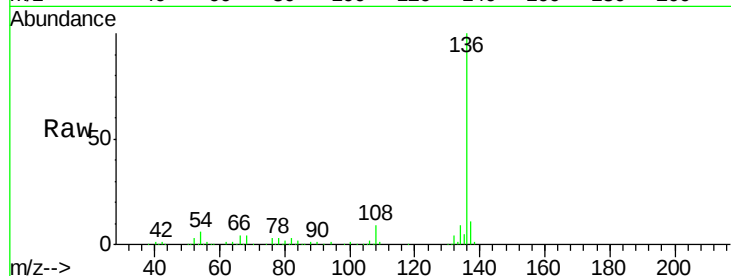


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

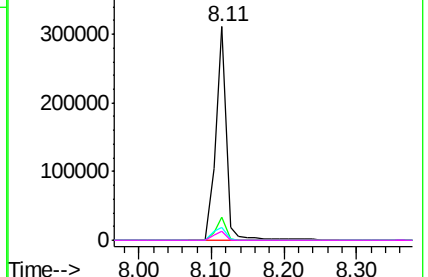

#23

Nitrobenzene-d5

Concen: 84.30 ng

RT: 7.39 min Scan# 460

Delta R.T. -0.01 min

Lab File: BF082299.D

Acq: 15 Oct 2015 4:48


Tgt Ion: 82 Resp: 397924

Ion Ratio Lower Upper

82 100

128 45.4 38.7 58.1



54 51.8 40.1 60.1




Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

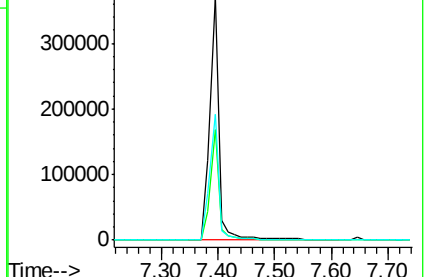



#25

Isophorone

Concen: 31.37 ng

RT: 7.39 min Scan# 460

Delta R.T. -0.26 min

Lab File: BF082299.D

Acq: 15 Oct 2015 4:48

Instrument :

BNA_F

ClientSampled :

CS-12


Tot Ion: 82 Resp: 298862

Ion Ratio Lower Upper




82 100

95 0.0 5.6 8.4#

138 0.0 13.6 20.4#



Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 95.00 (94.70 to 95.70): BF0
Ion 138.00 (137.70 to 138.70): BF0

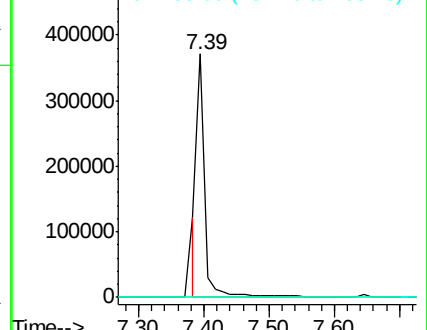

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.87 min Scan# 677

Delta R.T. 0.00 min

Lab File: BF082299.D

Acq: 15 Oct 2015 4:48


Tgt Ion: 164 Resp: 156048

Ion Ratio Lower Upper



164 100


162 107.0 81.6 122.4

160 46.6 36.4 54.6



Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

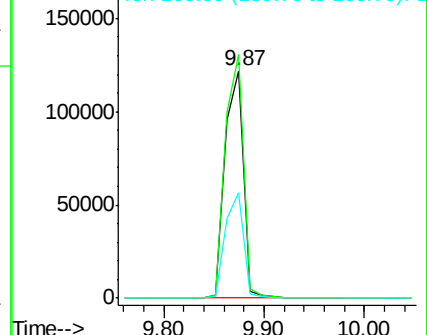

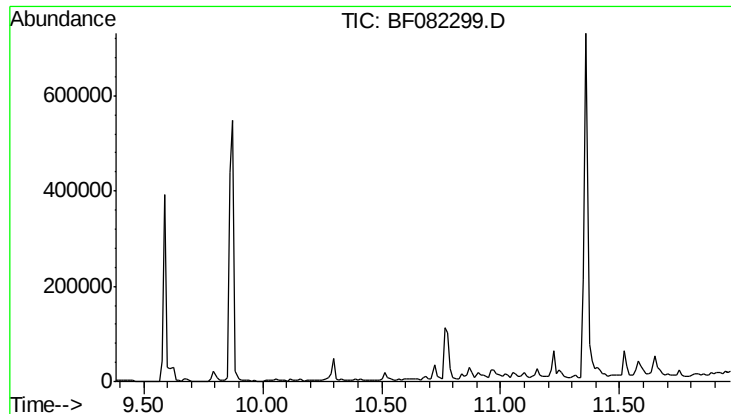

#41

2,4,6-Tribromophenol

Concen: 0.00 ng

Expected RT: 10.67 min

Lab File: BF082299.D

Acq: 15 Oct 2015 4:48

Instrument :

BNA_F

ClientSampleId :

CS-12



Tot Ion: 330

Sig Exp Ratio

330 100

332 96.4

141 37.3

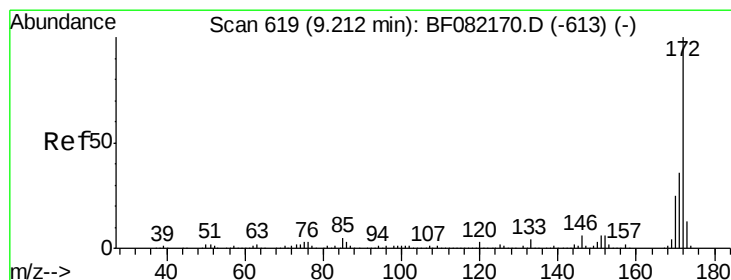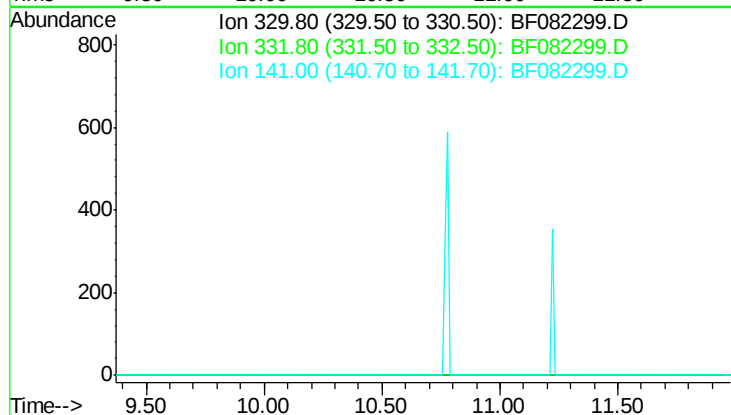

#44

2-Fluorobiphenyl

Concen: 80.23 ng

RT: 9.19 min Scan# 617

Delta R.T. -0.01 min

Lab File: BF082299.D

Acq: 15 Oct 2015 4:48




Tgt Ion:172 Resp: 754935


Ion Ratio Lower Upper

172 100

171 35.8 28.6 42.8

170 24.2 19.7 29.5

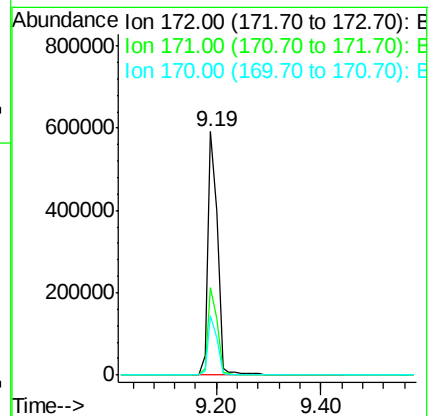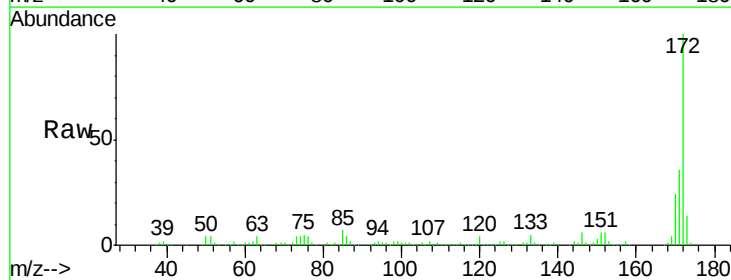

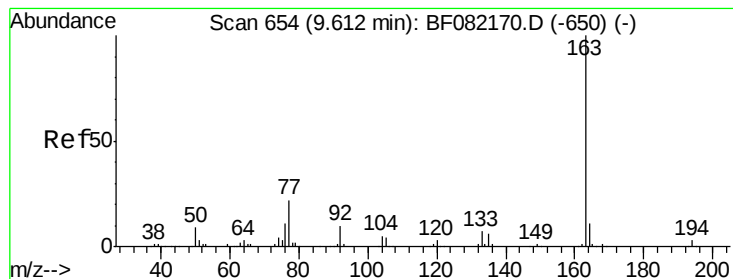

#49

Dimethylphthalate

Concen: 14.55 ng

RT: 9.59 min Scan# 652

Delta R.T. -0.01 min

Lab File: BF082299.D

Acq: 15 Oct 2015 4:48

Instrument :

BNA_F

ClientSampled :

CS-12


Tot Ion:163 Resp: 159913

Ion Ratio Lower Upper

163 100

194 3.4 2.6 4.0




164 10.1 8.5 12.7

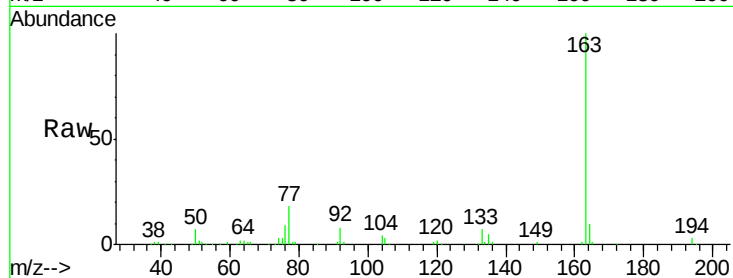

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

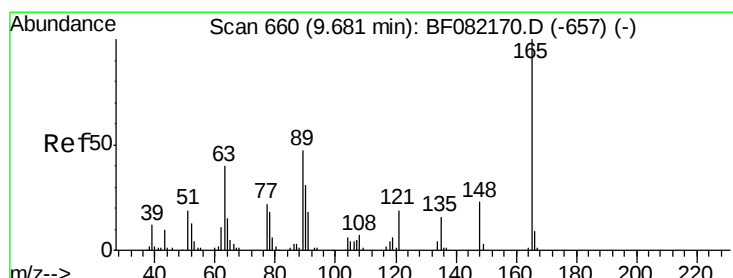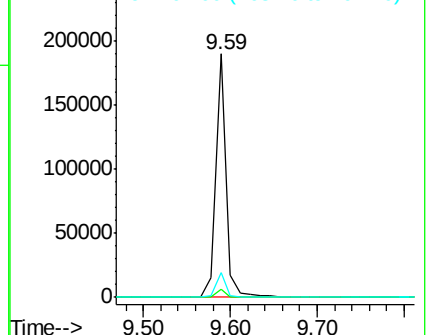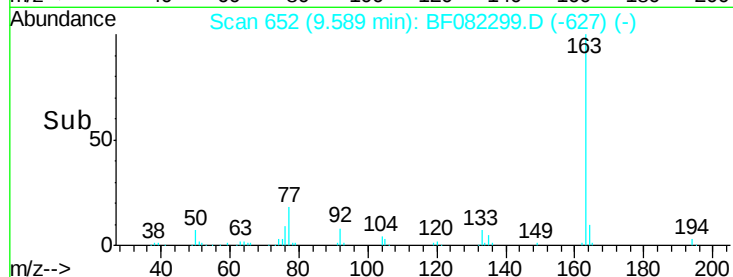

#50

2,6-Dinitrotoluene

Concen: 2.49 ng

RT: 9.62 min Scan# 655

Delta R.T. -0.05 min

Lab File: BF082299.D

Acq: 15 Oct 2015 4:48


Tgt Ion:165 Resp: 5775

Ion Ratio Lower Upper

165 100

63 0.0 36.7 55.1#



89 0.0 37.8 56.6#

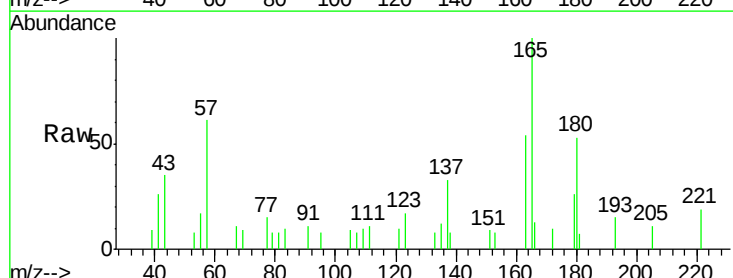


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0

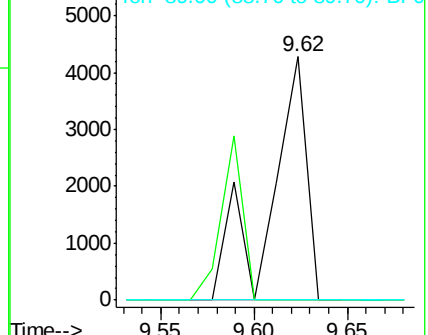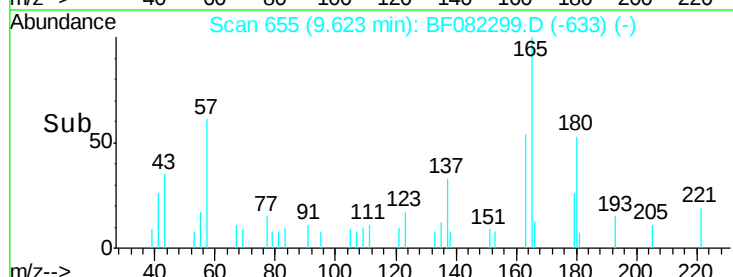

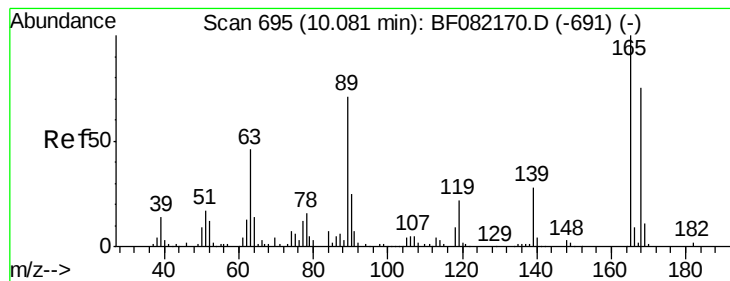

#56

2,4-Dinitrotoluene

Concen: 6.99 ng

RT: 9.87 min Scan# 677

Delta R.T. -0.19 min

Lab File: BF082299.D

Acq: 15 Oct 2015 4:48

Instrument :

BNA_F

ClientSampleId :

CS-12

Tot Ion:165 Resp: 20252


Ion Ratio Lower Upper

165 100

63 0.0 38.6 58.0#

89 0.0 57.0 85.6#

182 0.0 1.8 2.6#



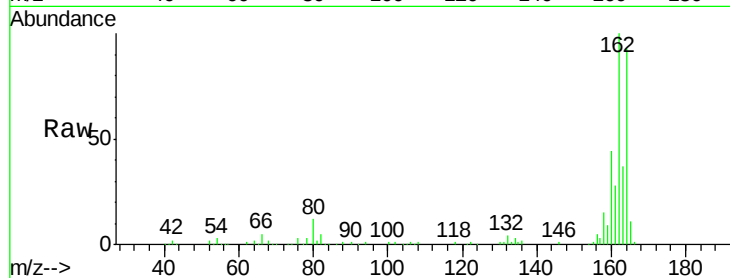


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0

Ion 182.00 (181.70 to 182.70): E

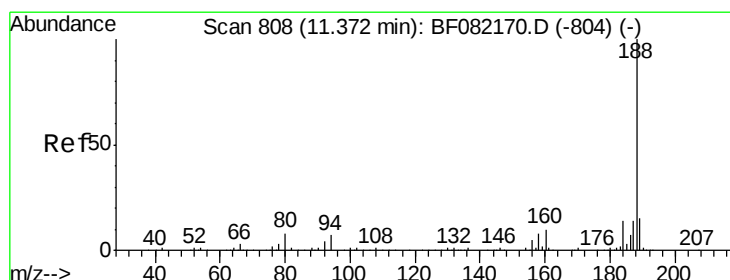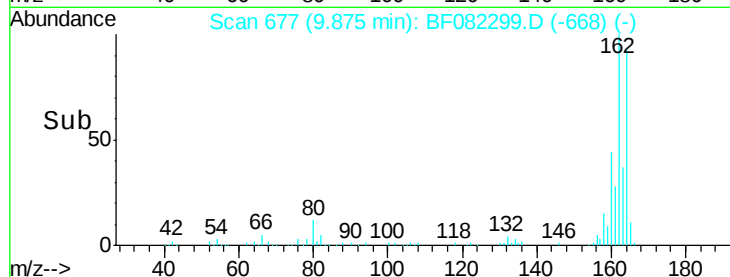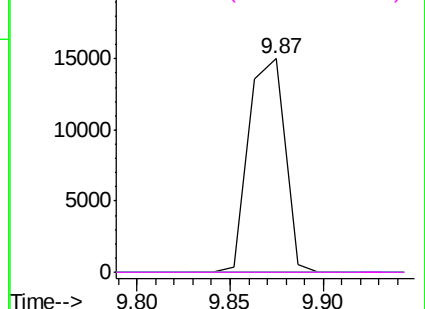

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.36 min Scan# 807

Delta R.T. 0.00 min

Lab File: BF082299.D

Acq: 15 Oct 2015 4:48


Tgt Ion:188 Resp: 311929

Ion Ratio Lower Upper

188 100

94 6.8 5.8 8.6



80 7.1 6.4 9.6

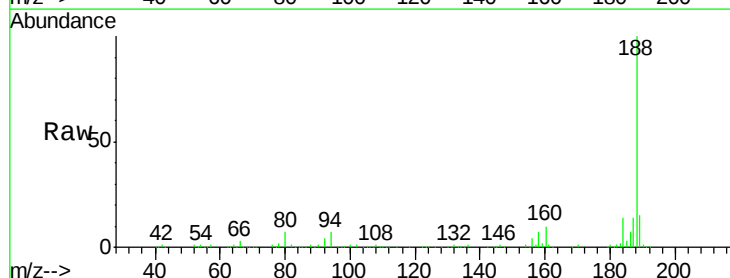


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

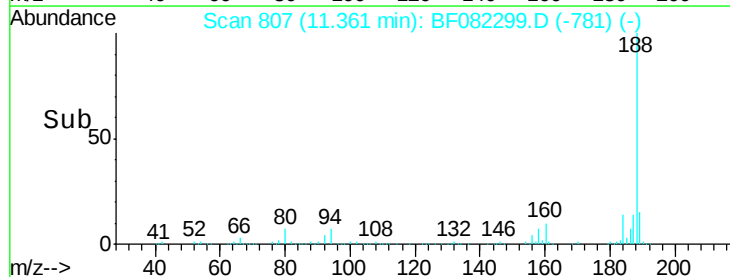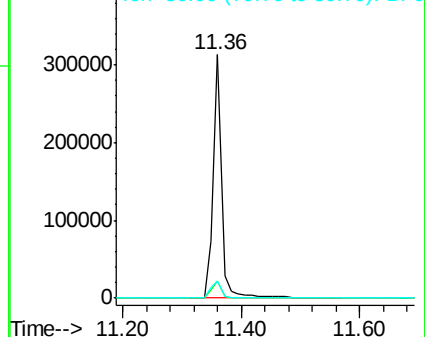



#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.04 min Scan# 1041

Delta R.T. 0.00 min

Lab File: BF082299.D

Acq: 15 Oct 2015 4:48

Instrument :

BNA_F

ClientSampleId :

CS-12


Tot Ion:240 Resp: 241093

Ion Ratio Lower Upper

240 100

120 7.6 8.1 12.1#

236 26.0 21.3 31.9




Abundance Ion 240.00 (239.70 to 240.70): E


Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

14.04



Time-->



#78

Terphenyl-d14

Concen: 89.89 ng

RT: 12.96 min Scan# 947

Delta R.T. 0.00 min

Lab File: BF082299.D

Acq: 15 Oct 2015 4:48


Tgt Ion:244 Resp: 817823

Ion Ratio Lower Upper

244 100

212 6.2 5.8 8.6

122 4.9 5.9 8.9#




Abundance Ion 244.00 (243.70 to 244.70): E




Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

12.96



Time-->

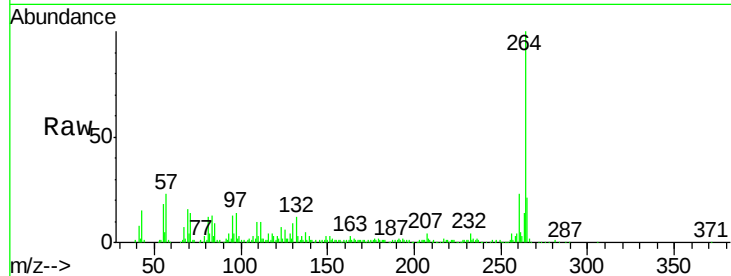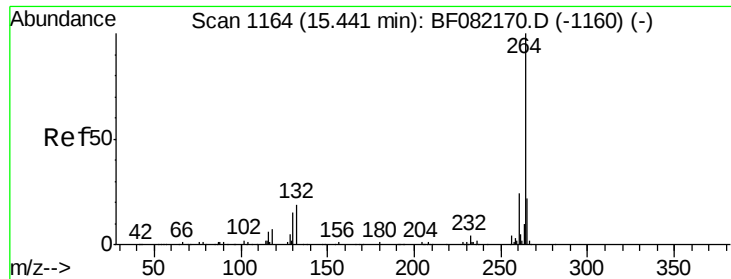

#86
Pervlene-d12
Concen: 20.00 ng
RT: 15.54 min Scan# 1173
Delta R.T. 0.01 min
Lab File: BF082299.D
Acq: 15 Oct 2015 4:48

Instrument :
BNA_F
ClientSampleId :
CS-12

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.2	19.0	28.6
265	20.8	17.3	25.9

