
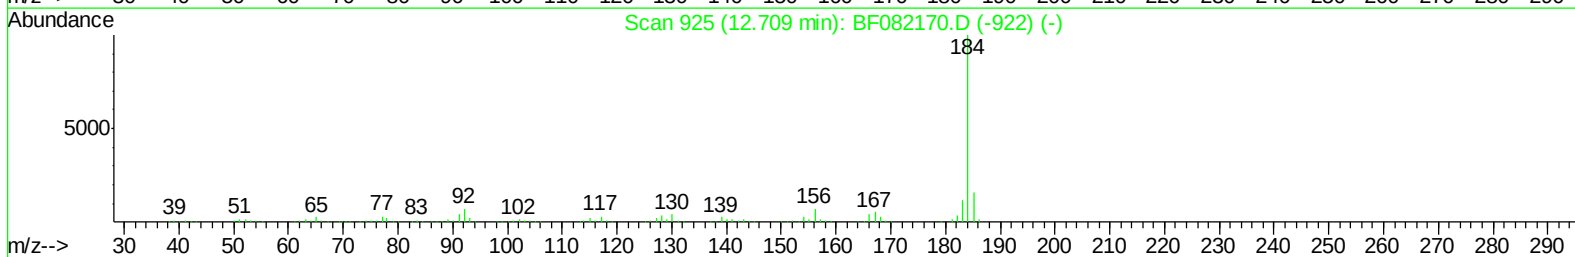
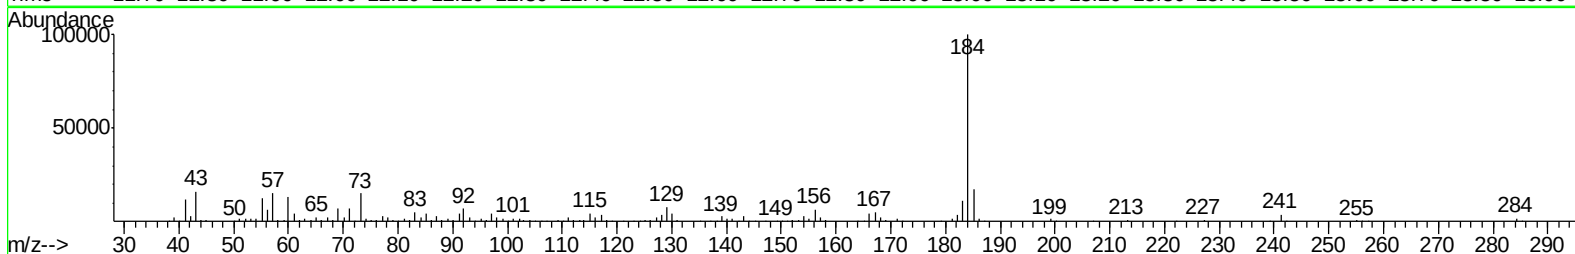


Data Path : Z:\HPCHEM1\BNA F\DATA\BF101515\
Data File : BF082274.D
Acq On : 14 Oct 2015 11:38
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 15 04:28:22 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 15 04:19:20 2015
Response via : Initial Calibration

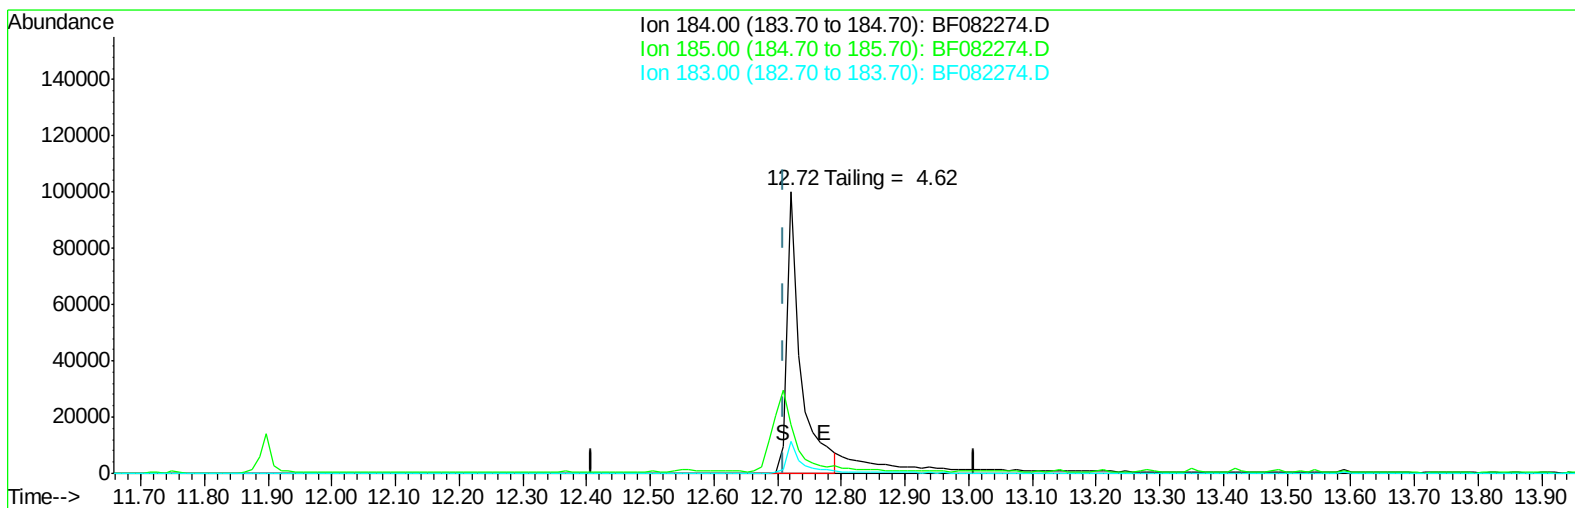

TIC: BF082274.D

(76) Benzidine




12.721min (+0.012) 0.00ng m

response 147906

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	17.50
183.00	11.40	11.27
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101515\
Data File : BF082274.D
Acq On : 14 Oct 2015 11:38
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 15 04:28:22 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 15 04:19:20 2015
Response via : Initial Calibration

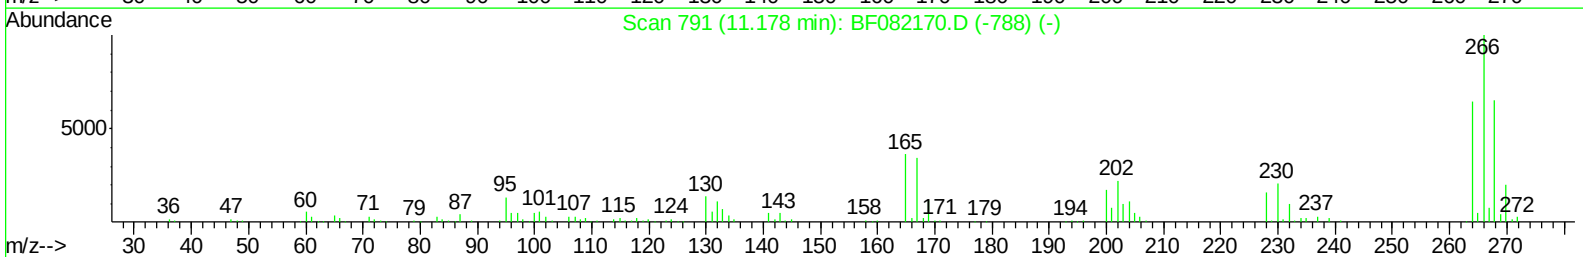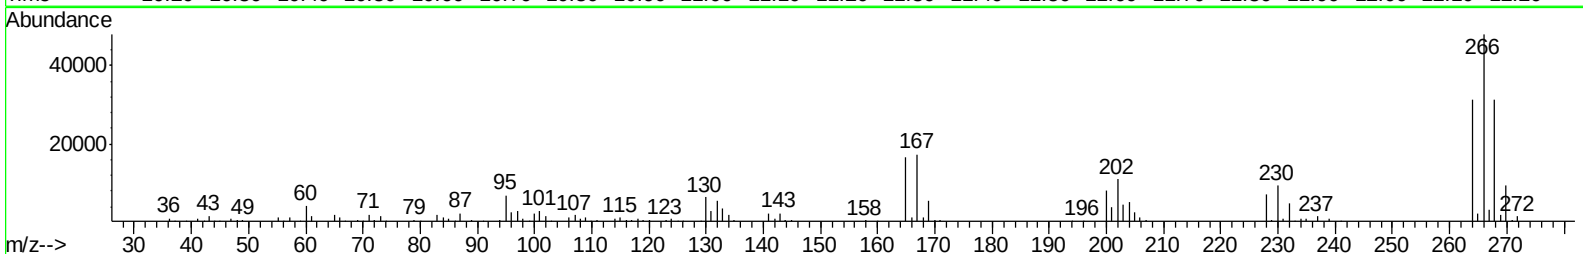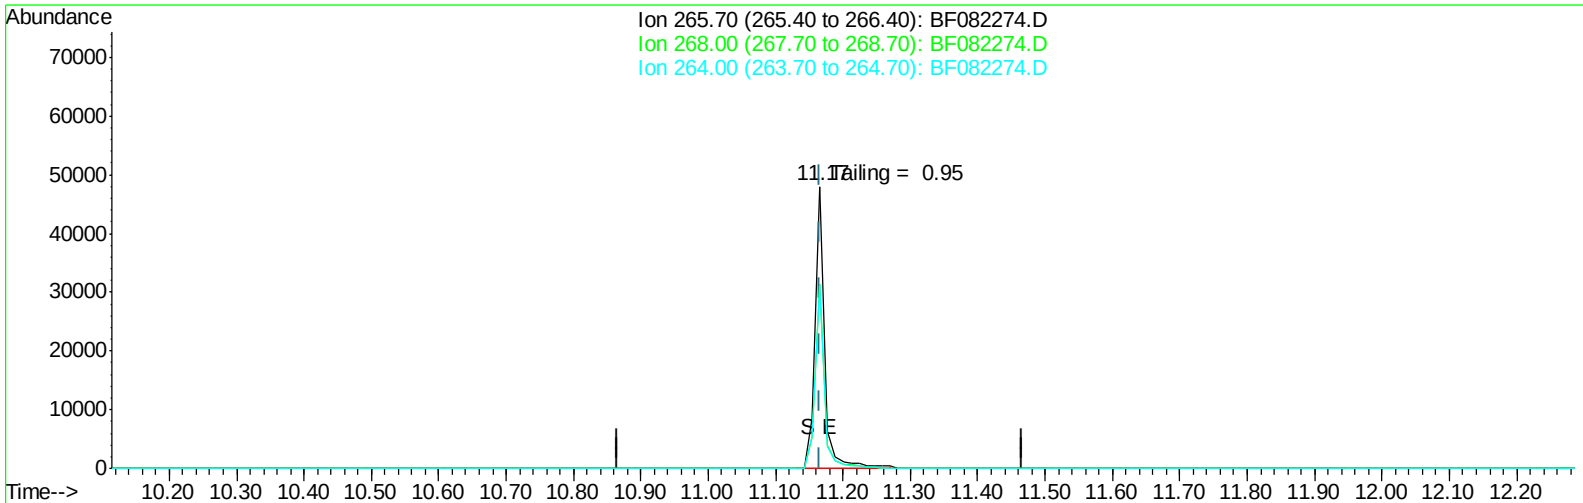

TIC: BF082274.D

(69) Pentachlorophenol (C)

11.166min (+0.000) 0.00ng

response 47515

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	65.42
264.00	64.20	65.19
0.00	0.00	0.00