


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101515\
 Data File : BF082274.D
 Acq On : 14 Oct 2015 11:38
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 12 01:46:21 2015

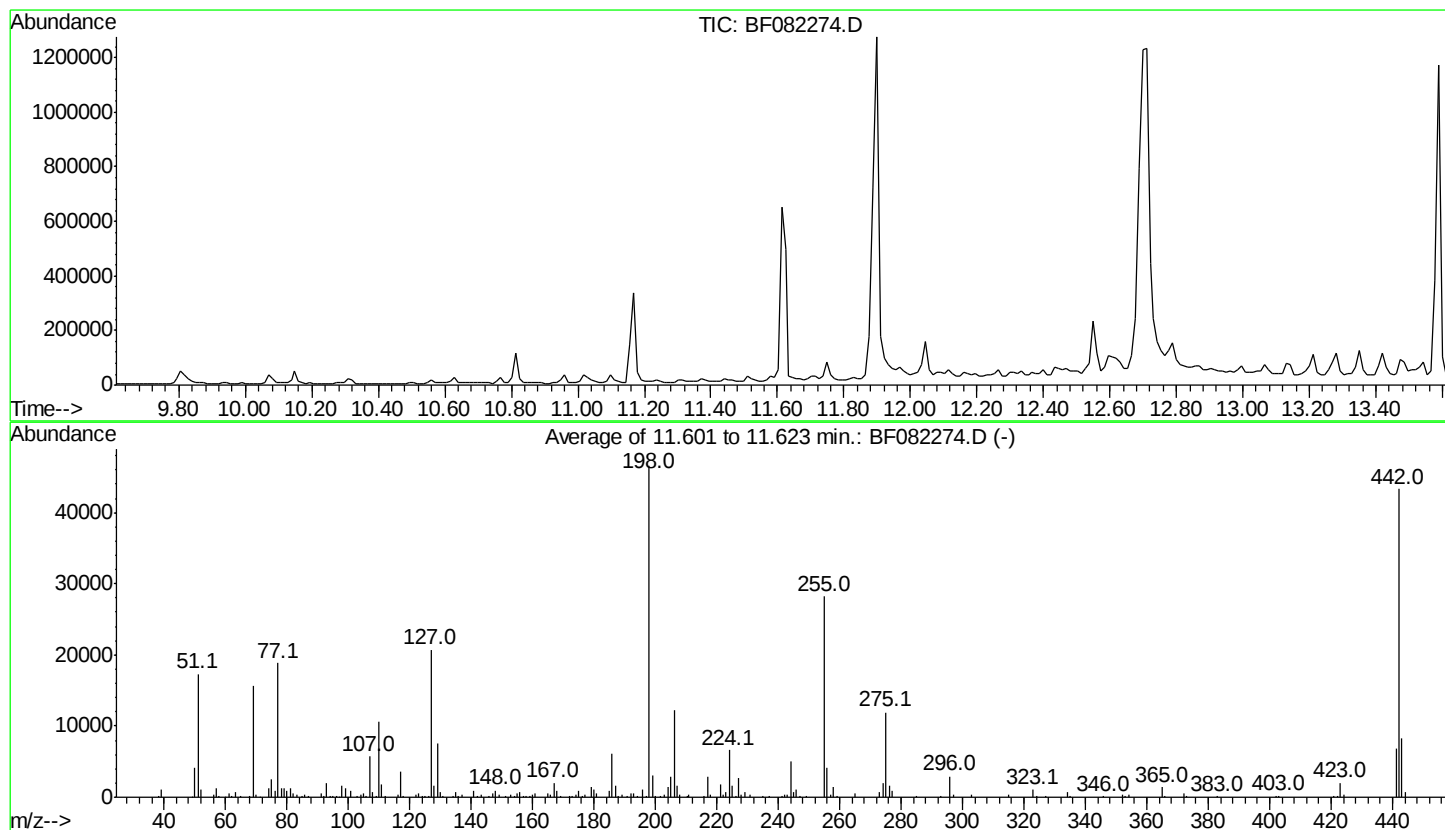

AutoFind: Scans 828, 829, 830; Background Corrected with Scan 825

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	17285	PASS
68	69	0.00	2	1.5	240	PASS
69	198	0.00	100	33.6	15669	PASS
70	69	0.00	2	1.8	286	PASS
127	198	10	80	44.6	20763	PASS
197	198	0.00	2	0.3	161	PASS
198	198	100	100	100.0	46593	PASS
199	198	5	9	6.6	3074	PASS
275	198	10	60	25.6	11938	PASS
365	198	1	100	3.0	1377	PASS
441	442	0.01	24	15.9	6868	PASS
442	198	50	100	92.9	43269	PASS
443	442	15	24	18.9	8192	PASS