
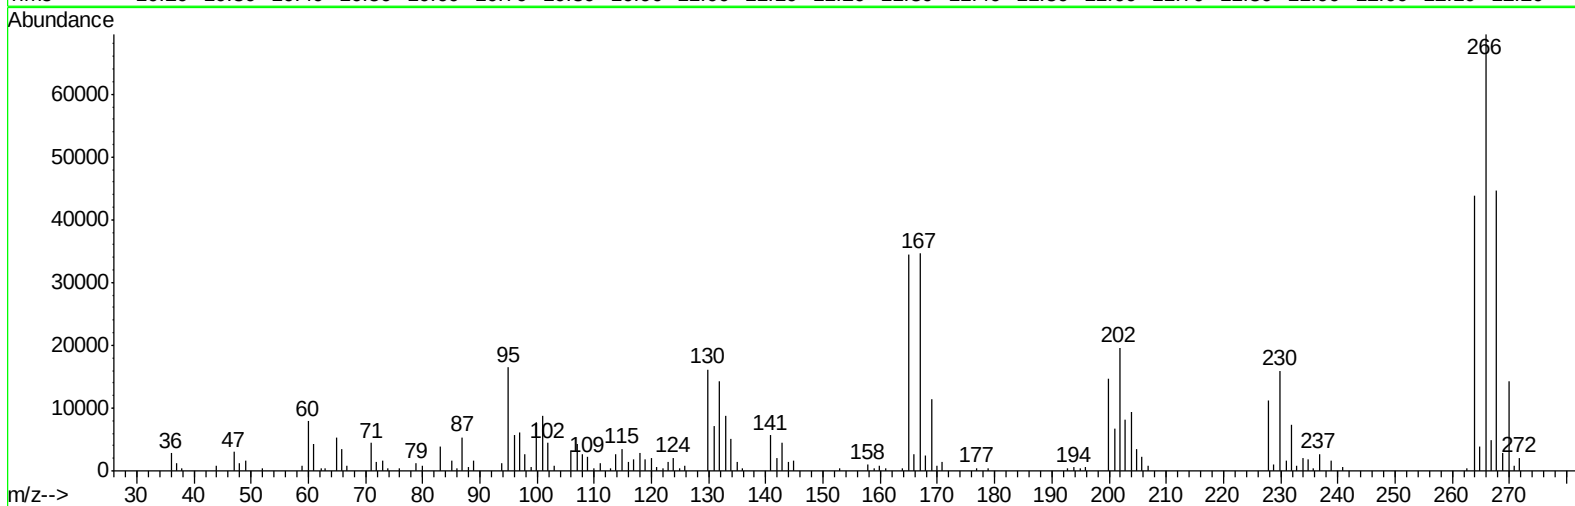


Data Path : Z:\HPCHEM1\BNA F\DATA\BF101517\
Data File : BF099505.D
Acq On : 15 Oct 2017 11:06
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 16 04:11:29 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 11 16:25:21 2017
Response via : Initial Calibration

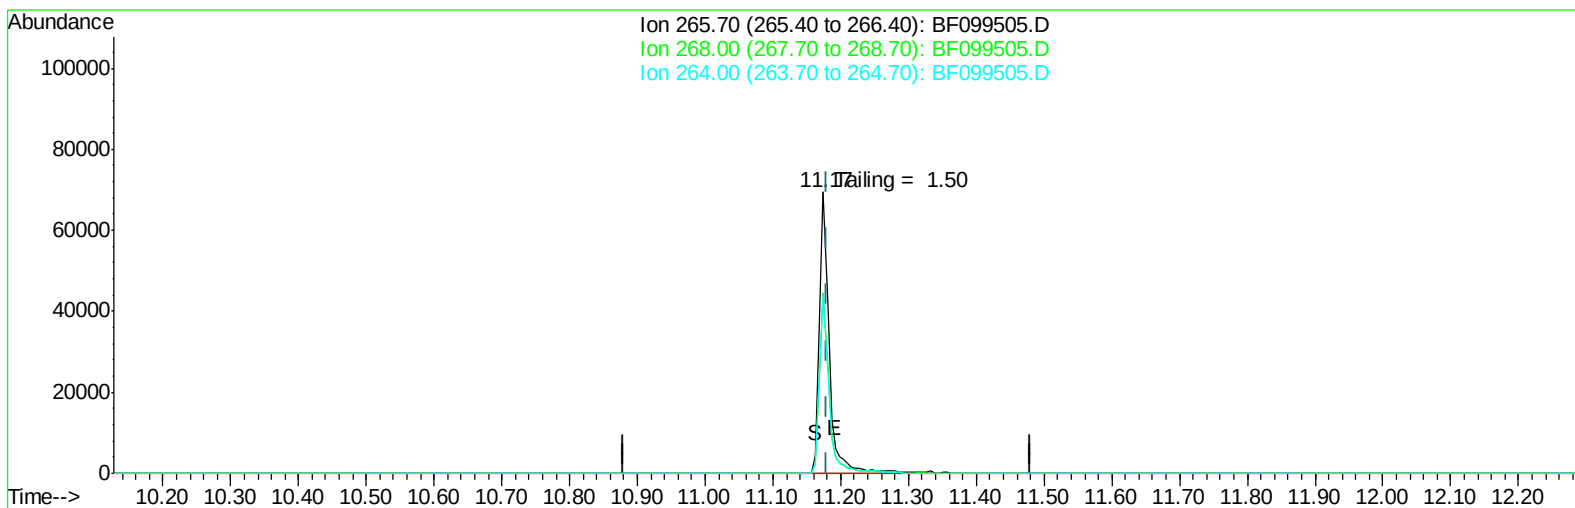

TIC: BF099505.D

(69) Pentachlorophenol (C)



11.175min (-0.006) 31154.33ng m

response 68716

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.18
264.00	61.90	63.18
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101517\
Data File : BF099505.D
Acq On : 15 Oct 2017 11:06
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 16 04:11:29 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 11 16:25:21 2017
Response via : Initial Calibration

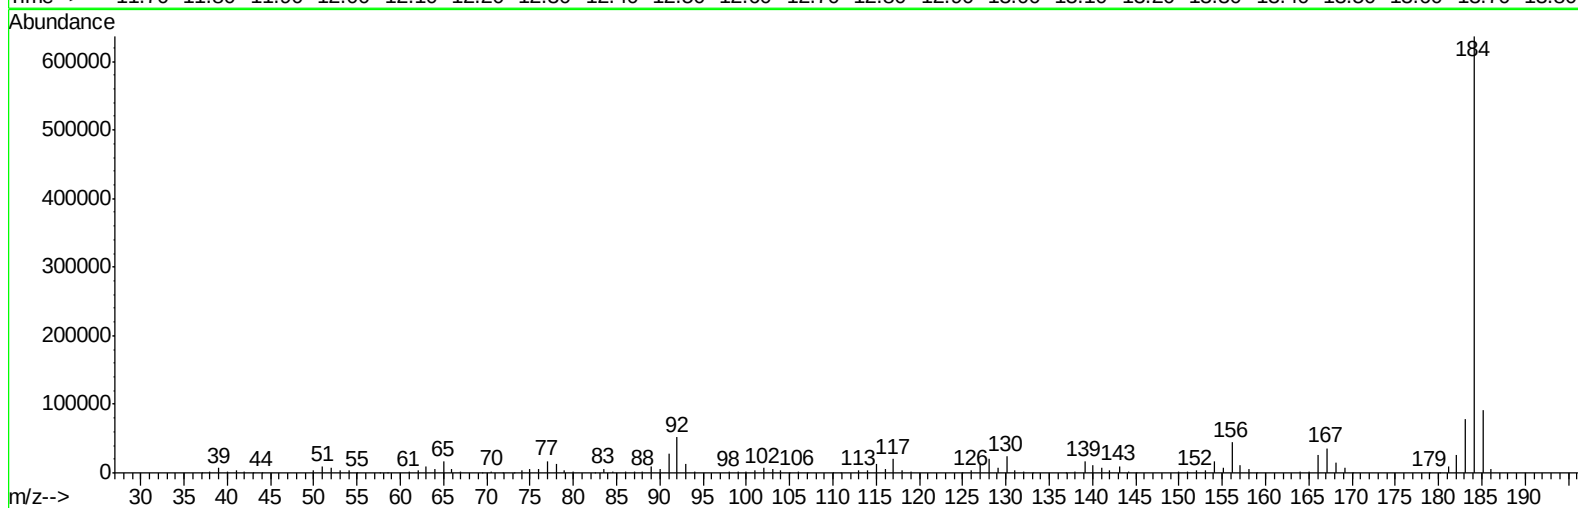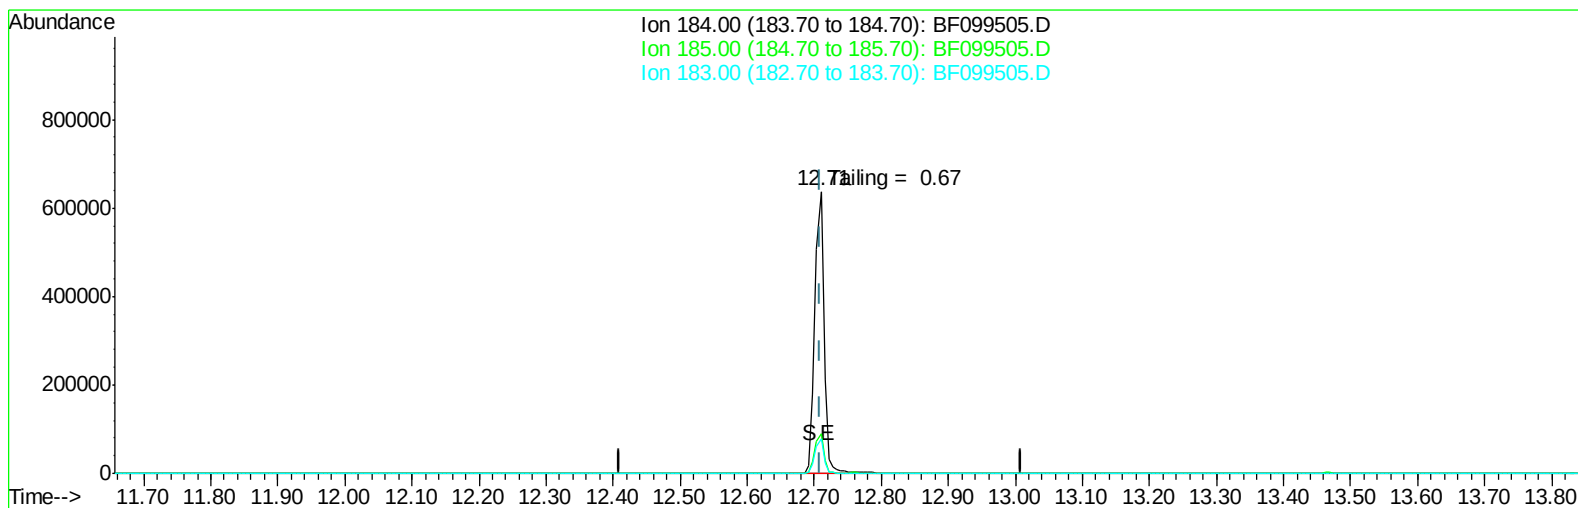

TIC: BF099505.D

(76) Benzidine

12.710min (+0.000) 0.00ng

response 579138

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.31
183.00	11.60	12.18
0.00	0.00	0.00