

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF101517\
 Data File : BF099508.D
 Acq On : 15 Oct 2017 12:36
 Operator : SJ/JU
 Sample : PB103252BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB103252BL

Quant Time: Oct 16 01:31:43 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 11 16:25:21 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.85	152	87471	20.00	ng	0.00
21) Naphthalene-d8	8.12	136	366865	20.00	ng	-0.01
38) Acenaphthene-d10	9.88	164	166345	20.00	ng	-0.01
63) Phenanthrene-d10	11.37	188	308059	20.00	ng	0.00
75) Chrysene-d12	14.01	240	226817	20.00	ng	0.00
86) Perylene-d12	15.48	264	158594	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.47	112	635957	115.74	ng	0.00
7) Phenol-d6	6.48	99	751828	110.92	ng	0.00
23) Nitrobenzene-d5	7.41	82	450534	78.76	ng	-0.01
41) 2,4,6-Tribromophenol	10.67	330	159691	117.32	ng	0.00
44) 2-Fluorobiphenyl	9.20	172	871087	87.42	ng	-0.01
78) Terphenyl-d14	12.95	244	799020	80.11	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF101517\
Data File : BF099508.D
Acq On : 15 Oct 2017 12:36
Operator : SJ/JU
Sample : PB103252BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB103252BL

Quant Time: Oct 16 01:31:43 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 11 16:25:21 2017
Response via : Initial Calibration

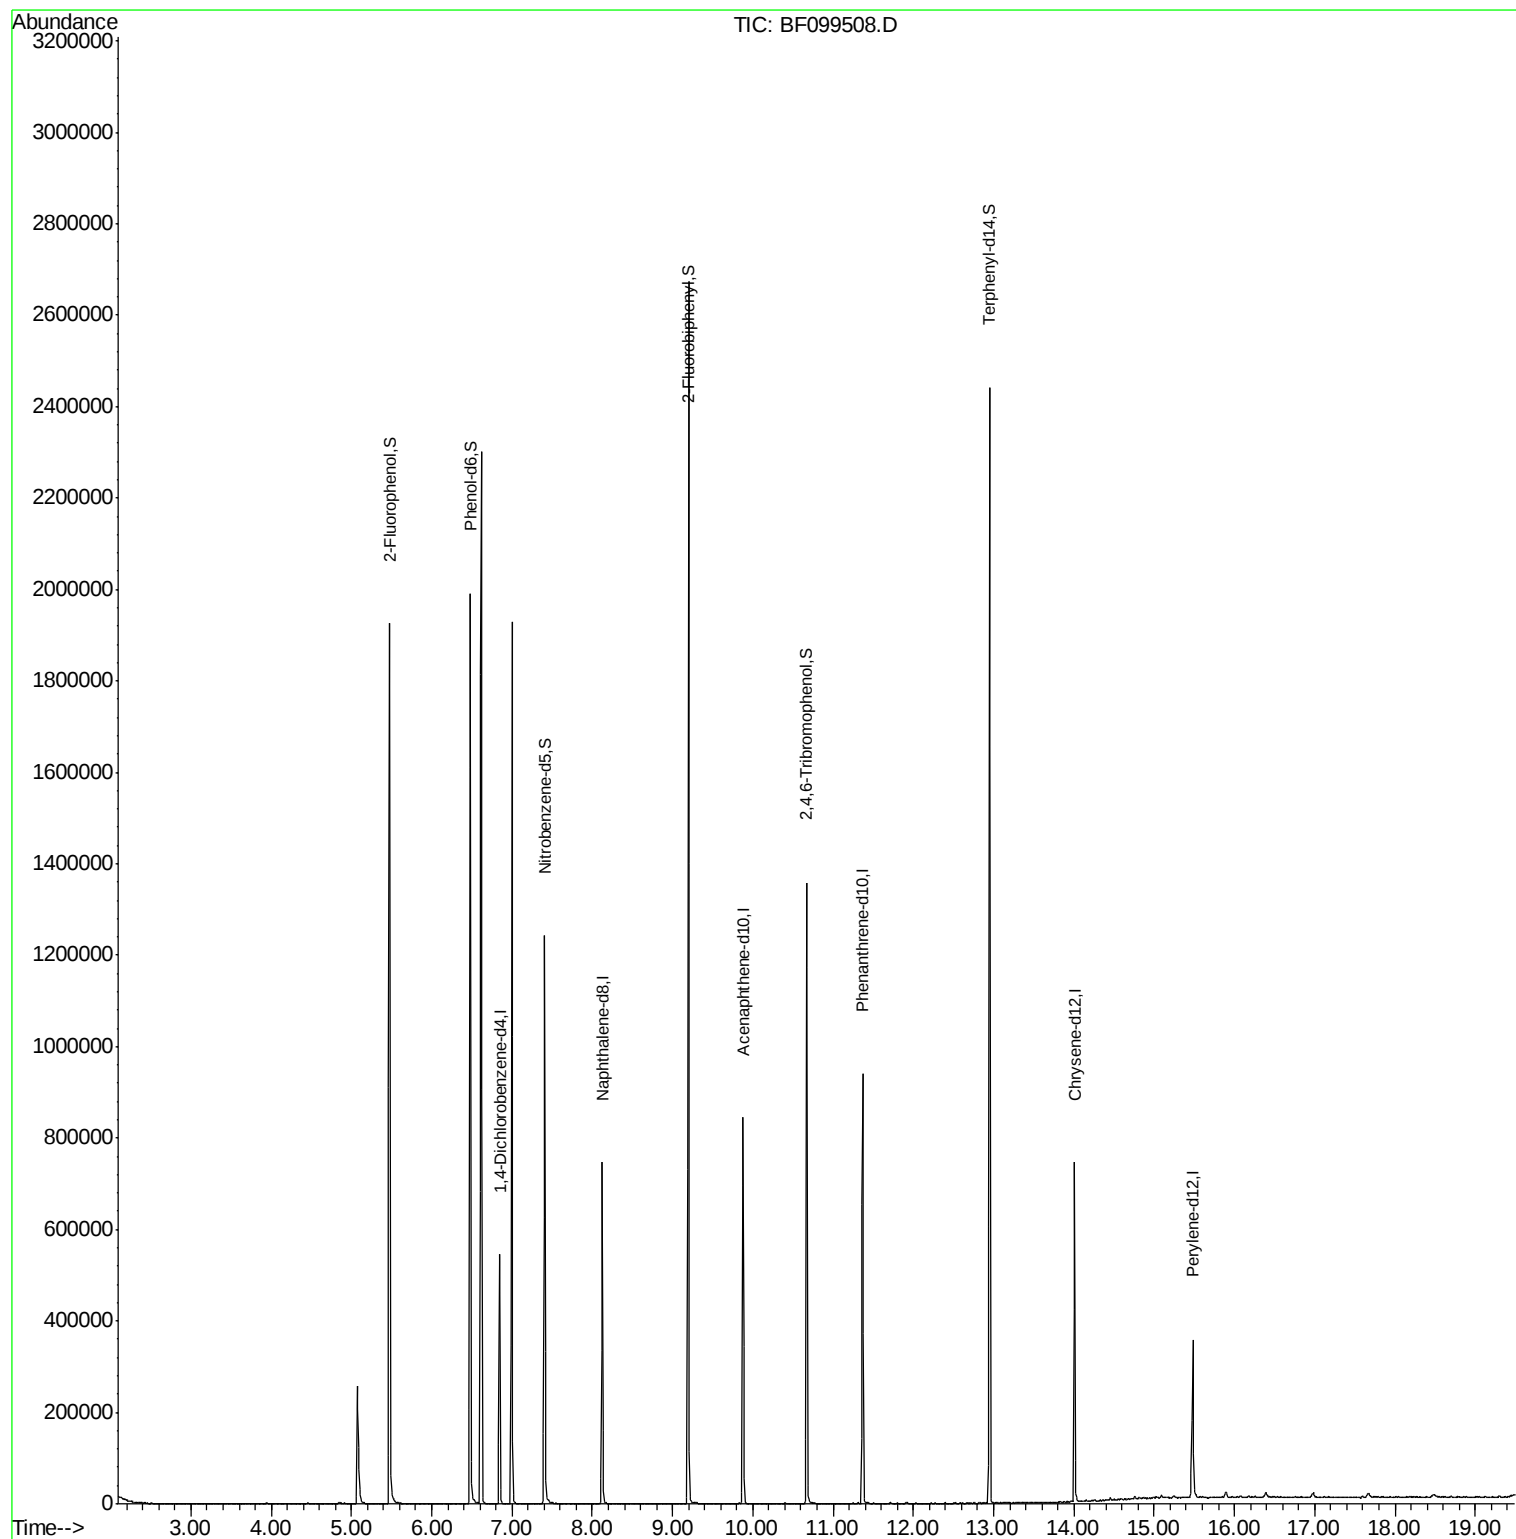

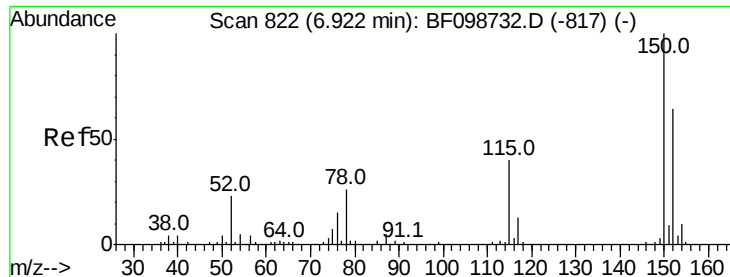


#1



1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.85 min Scan# 809
 Delta R.T. -0.01 min
 Lab File: BF099508.D
 Acq: 15 Oct 2017 12:36

Instrument :
 BNA_F
 ClientSampleId :
 PB103252BL

Tot Ion:152 Resp: 87471
 Ion Ratio Lower Upper
 152 100
 150 159.5 124.6 186.8
 115 58.7 50.1 75.1

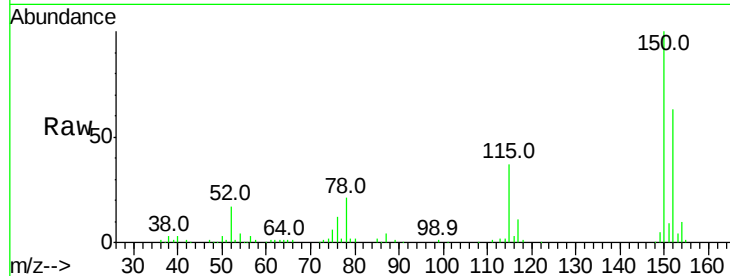


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

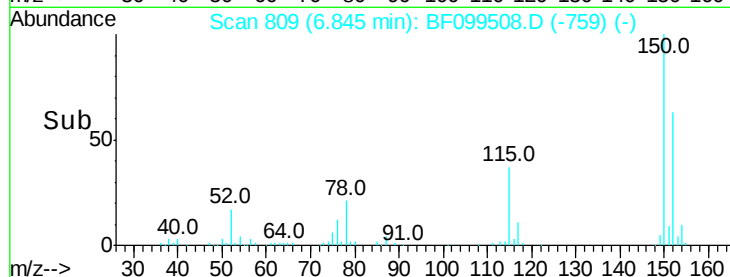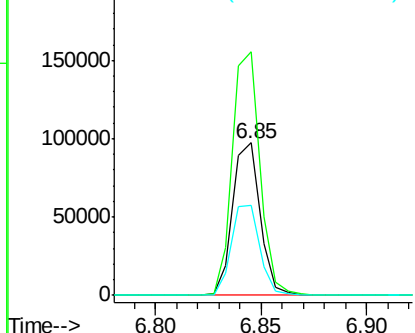



#5

2-Fluorophenol
 Concen: 115.739 ng
 RT: 5.47 min Scan# 576
 Delta R.T. 0.01 min
 Lab File: BF099508.D
 Acq: 15 Oct 2017 12:36

Tgt Ion:112 Resp: 635957
 Ion Ratio Lower Upper
 112 100
 64 52.0 47.9 71.9
 63 25.5 23.7 35.5

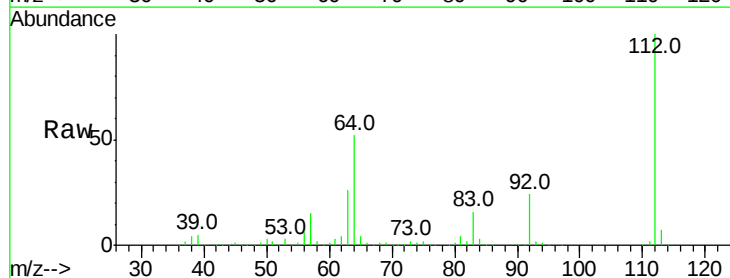

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

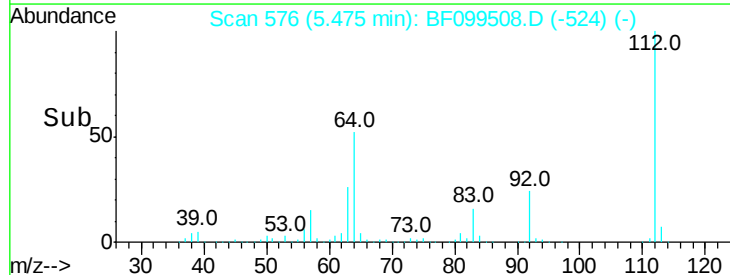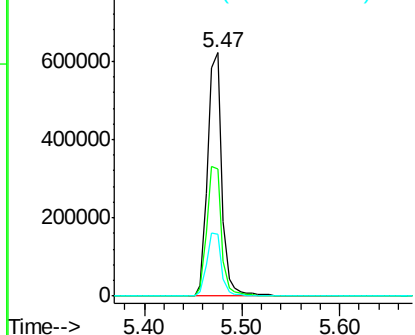



#7

Phenol-d6

Concen: 110.915 ng

RT: 6.48 min Scan# 747

Delta R.T. -0.01 min

Lab File: BF099508.D

Acq: 15 Oct 2017 12:36

Instrument :

BNA_F

ClientSampleId :

PB103252BL


Tot Ion: 99 Resp: 751828

Ion Ratio Lower Upper




99 100

42 15.2 14.5 21.7

71 30.3 25.4 38.0

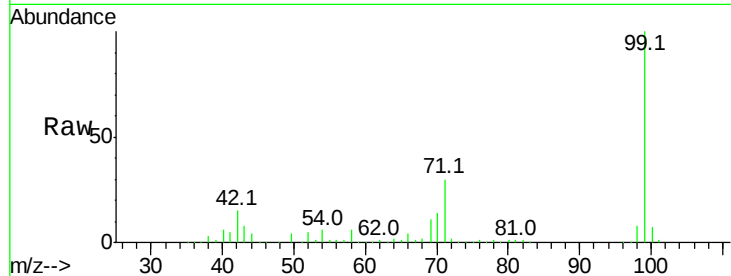

Abundance Ion 99.00 (98.70 to 99.70): BF0
Ion 42.00 (41.70 to 42.70): BF0
Ion 71.00 (70.70 to 71.70): BF0

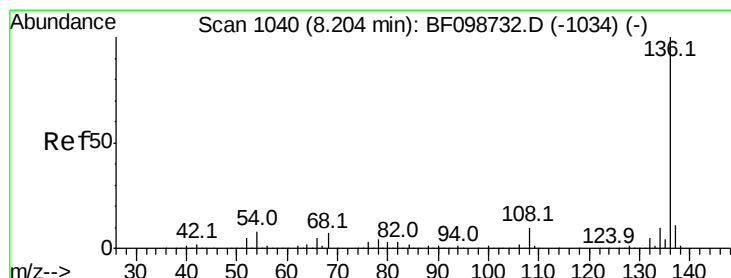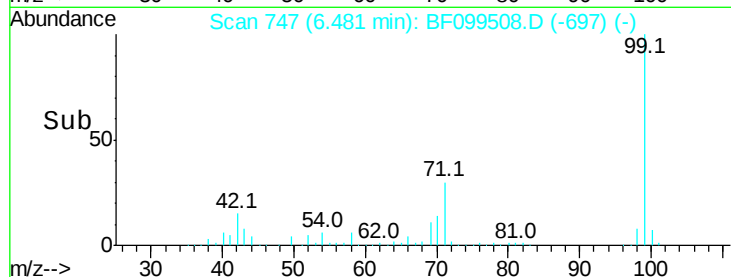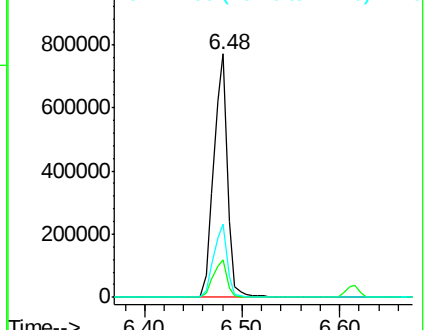

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.12 min Scan# 1026

Delta R.T. -0.01 min

Lab File: BF099508.D

Acq: 15 Oct 2017 12:36

Tgt Ion: 136 Resp: 366865


Ion Ratio Lower Upper

136 100



137 11.1 8.9 13.3

54 7.3 6.6 9.8

68 5.9 5.0 7.4

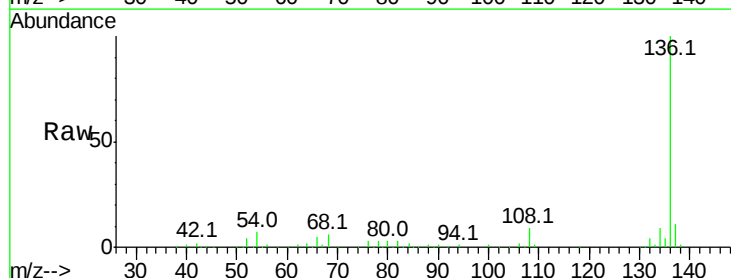

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0



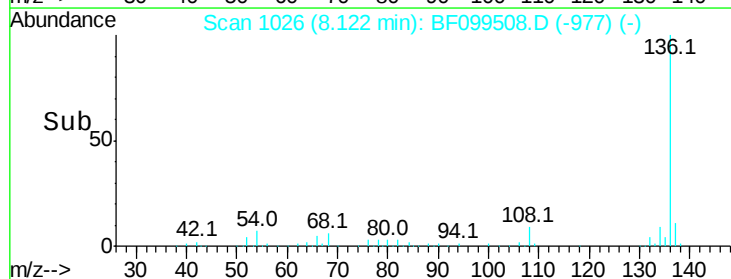
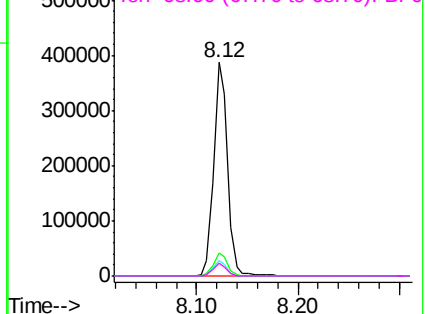




#23
 Nitrobenzene-d5
 Concen: 78.756 ng
 RT: 7.41 min Scan# 905
 Delta R.T. -0.01 min
 Lab File: BF099508.D
 Acq: 15 Oct 2017 12:36




Instrument :
 BNA_F
 ClientSampleId :
 PB103252BL

Tot Ion: 82 Resp: 450534
 Ion Ratio Lower Upper
 82 100
 128 50.1 36.1 54.1
 54 46.4 41.4 62.2

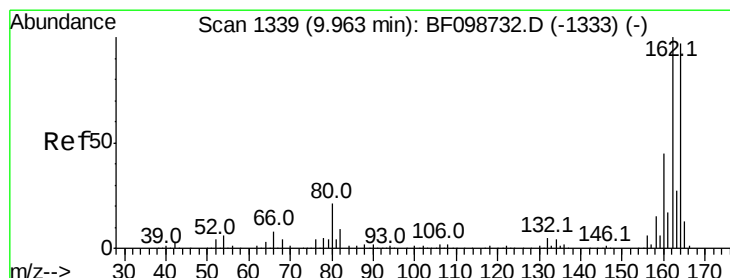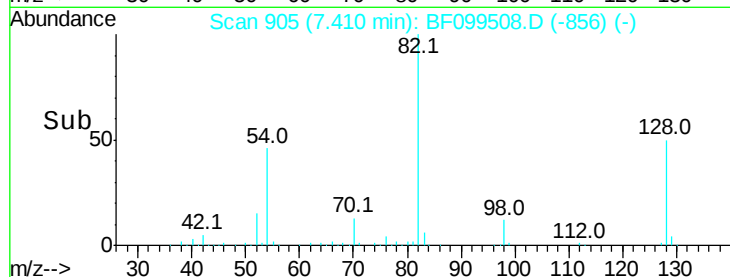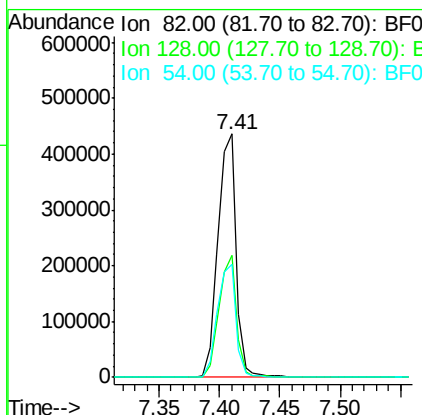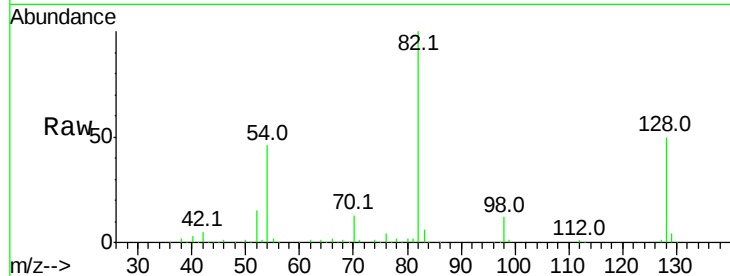

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.88 min Scan# 1325
 Delta R.T. -0.01 min
 Lab File: BF099508.D
 Acq: 15 Oct 2017 12:36

Tgt Ion:164 Resp: 166345
 Ion Ratio Lower Upper
 164 100
 162 107.8 86.1 129.1
 160 47.7 38.3 57.5

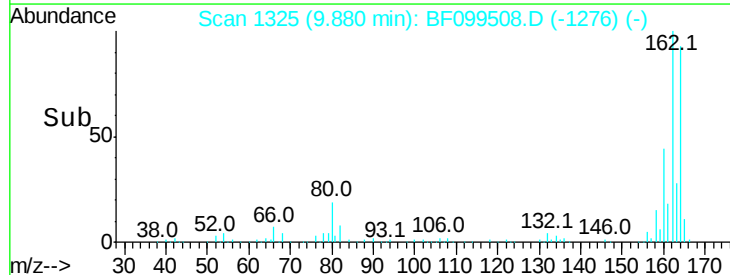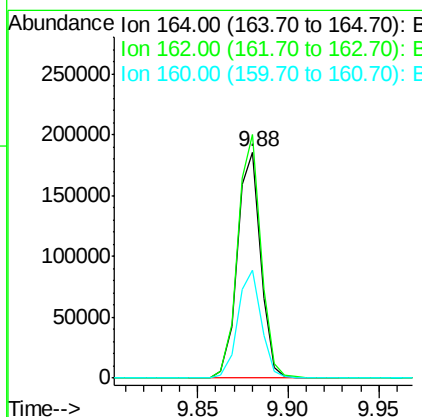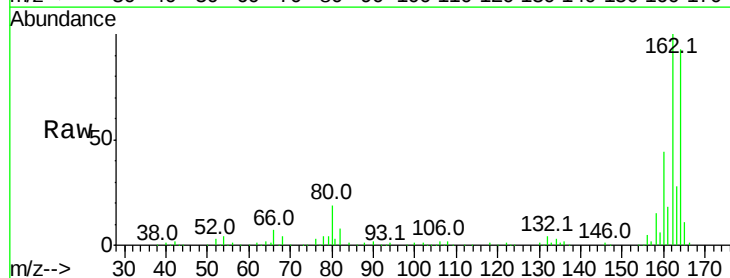






#41
 2,4,6-Tribromophenol
 Concen: 117.320 ng
 RT: 10.67 min Scan# 1460
 Delta R.T. -0.01 min
 Lab File: BF099508.D
 Acq: 15 Oct 2017 12:36

Instrument :
 BNA_F
 ClientSampleId :
 PB103252BL

Tot Ion:330 Resp: 159691
 Ion Ratio Lower Upper
 330 100
 332 95.9 77.0 115.6
 141 39.4 29.9 44.9

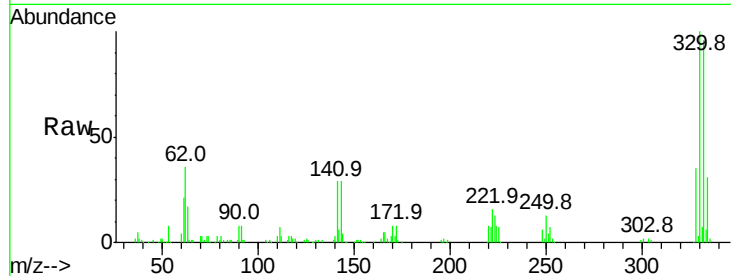


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

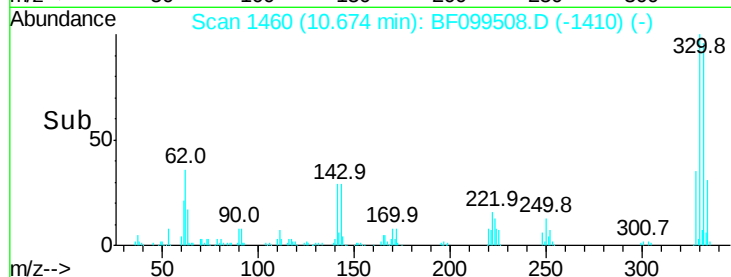
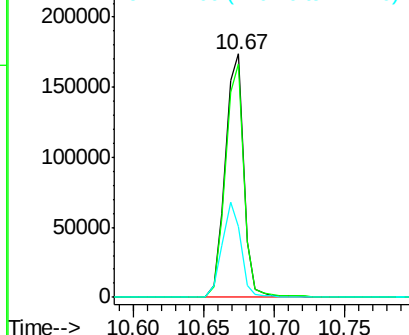



#44
 2-Fluorobiphenyl
 Concen: 87.421 ng
 RT: 9.20 min Scan# 1209
 Delta R.T. -0.01 min
 Lab File: BF099508.D
 Acq: 15 Oct 2017 12:36

Tgt Ion:172 Resp: 871087
 Ion Ratio Lower Upper
 172 100
 171 36.5 29.7 44.5
 170 24.2 19.6 29.4

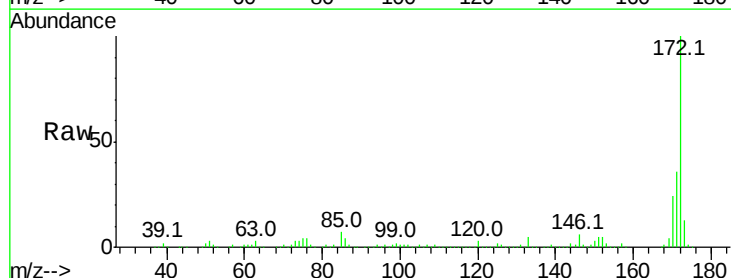

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

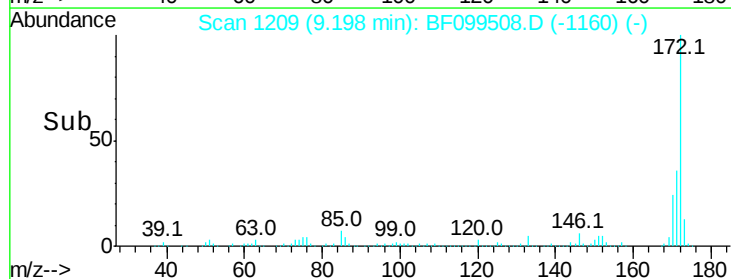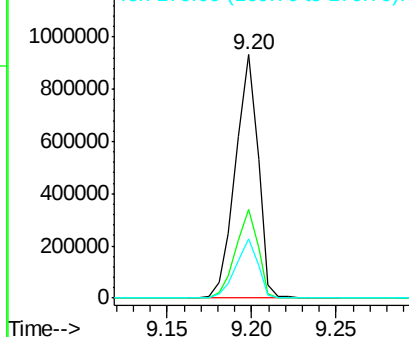


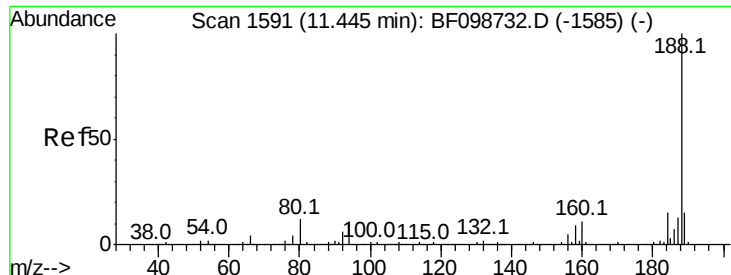




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.37 min Scan# 1578
Delta R.T. -0.01 min
Lab File: BF099508.D
Acq: 15 Oct 2017 12:36

Instrument :
BNA_F
ClientSampleId :
PB103252BL

Tot Ion:188 Resp: 308059
Ion Ratio Lower Upper
188 100
94 10.4 8.5 12.7
80 10.9 9.2 13.8

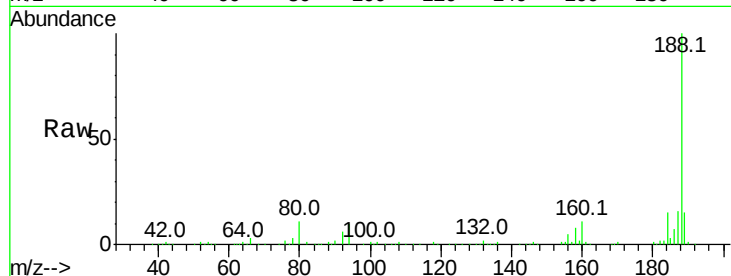


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

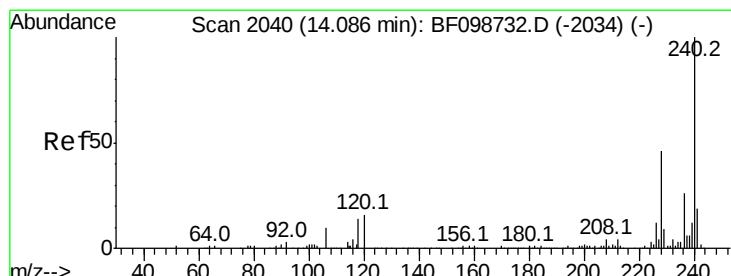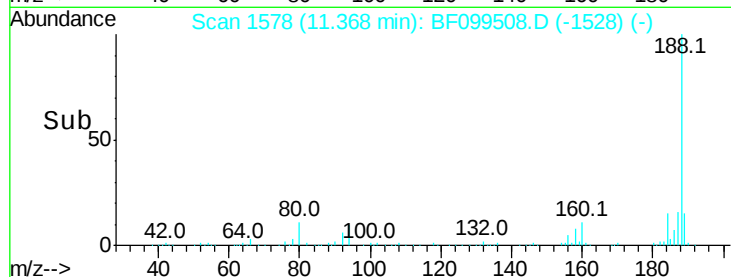
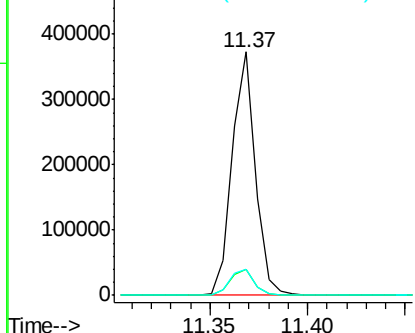



#75
Chrysene-d12
Concen: 20.000 ng
RT: 14.01 min Scan# 2027
Delta R.T. -0.01 min
Lab File: BF099508.D
Acq: 15 Oct 2017 12:36

Tgt Ion:240 Resp: 226817
Ion Ratio Lower Upper
240 100
120 14.4 9.5 14.3#
236 26.3 20.7 31.1

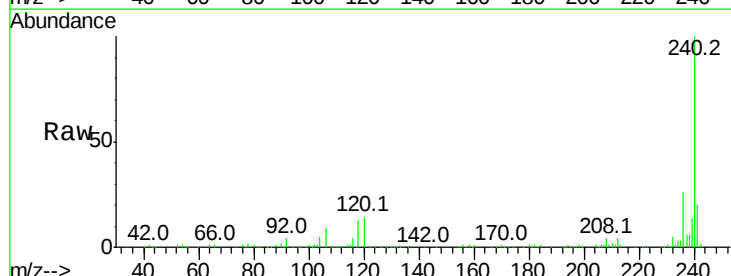

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

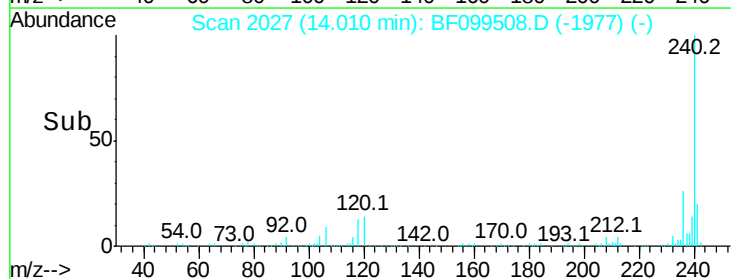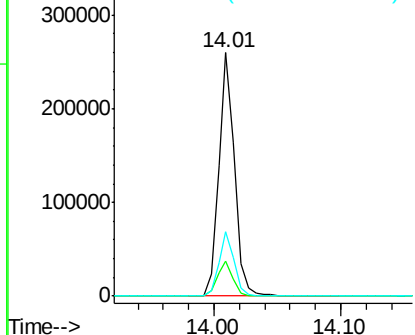

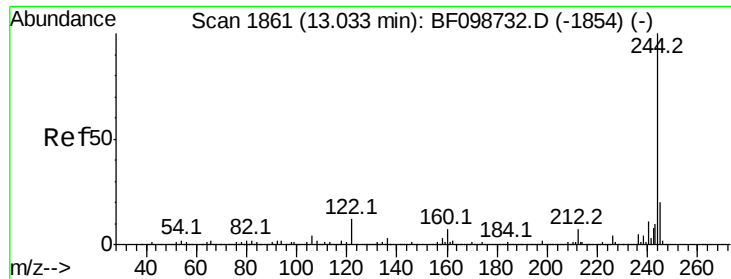

#78

Terphenyl-d14

Concen: 80.114 ng

RT: 12.95 min Scan# 1847

Delta R.T. -0.01 min

Lab File: BF099508.D

Acq: 15 Oct 2017 12:36

Instrument :

BNA_F

ClientSampleId :

PB103252BL


Tot Ion:244 Resp: 799020

Ion Ratio Lower Upper

244 100

212 7.0 5.4 8.0




122 13.6 11.0 16.4

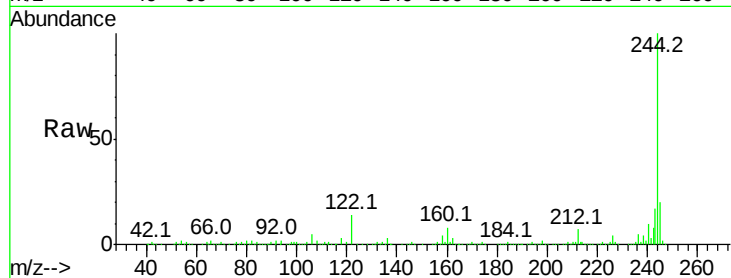

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

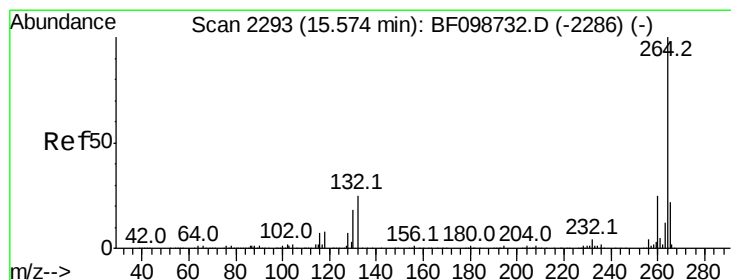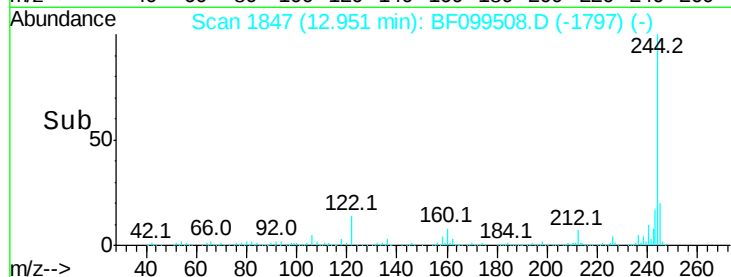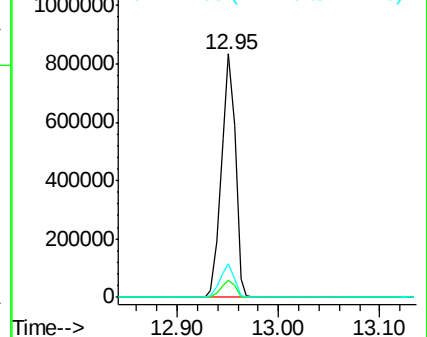

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.48 min Scan# 2277

Delta R.T. -0.00 min

Lab File: BF099508.D

Acq: 15 Oct 2017 12:36


Tgt Ion:264 Resp: 158594

Ion Ratio Lower Upper

264 100

260 23.3 19.2 28.8

265 21.0 17.5 26.3

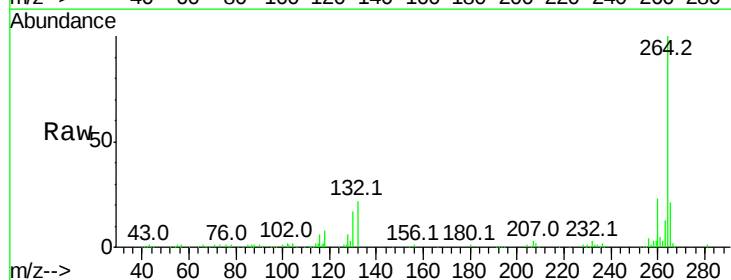

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

