
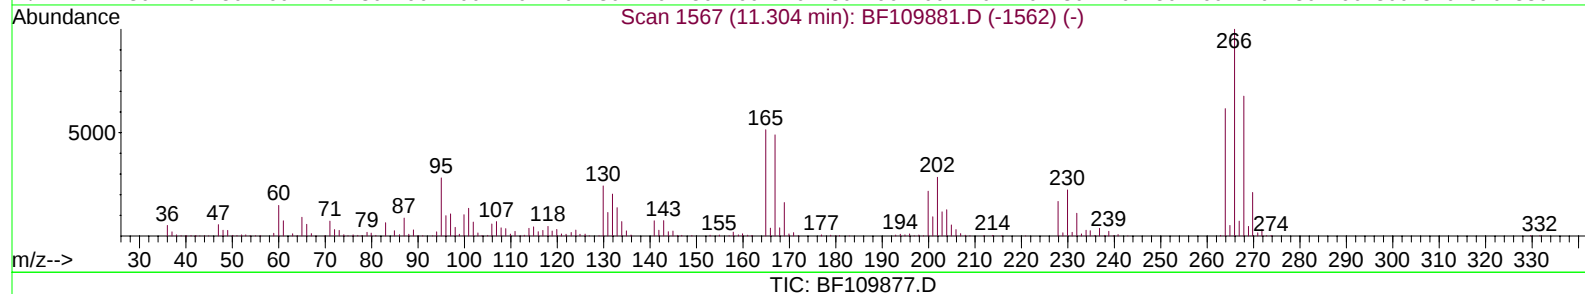
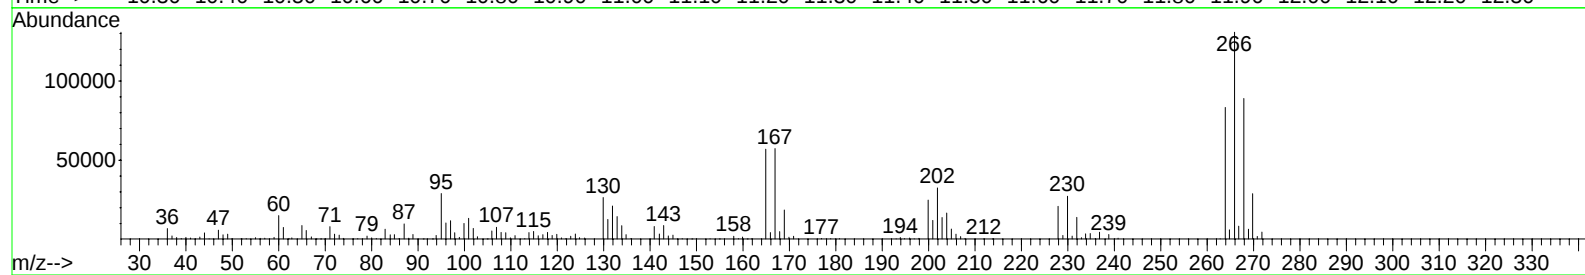


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF101518\
Data File : BF109877.D
Acq On : 15 Oct 2018 14:25
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 16 03:57:29 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 15 18:09:48 2018
Response via : Initial Calibration

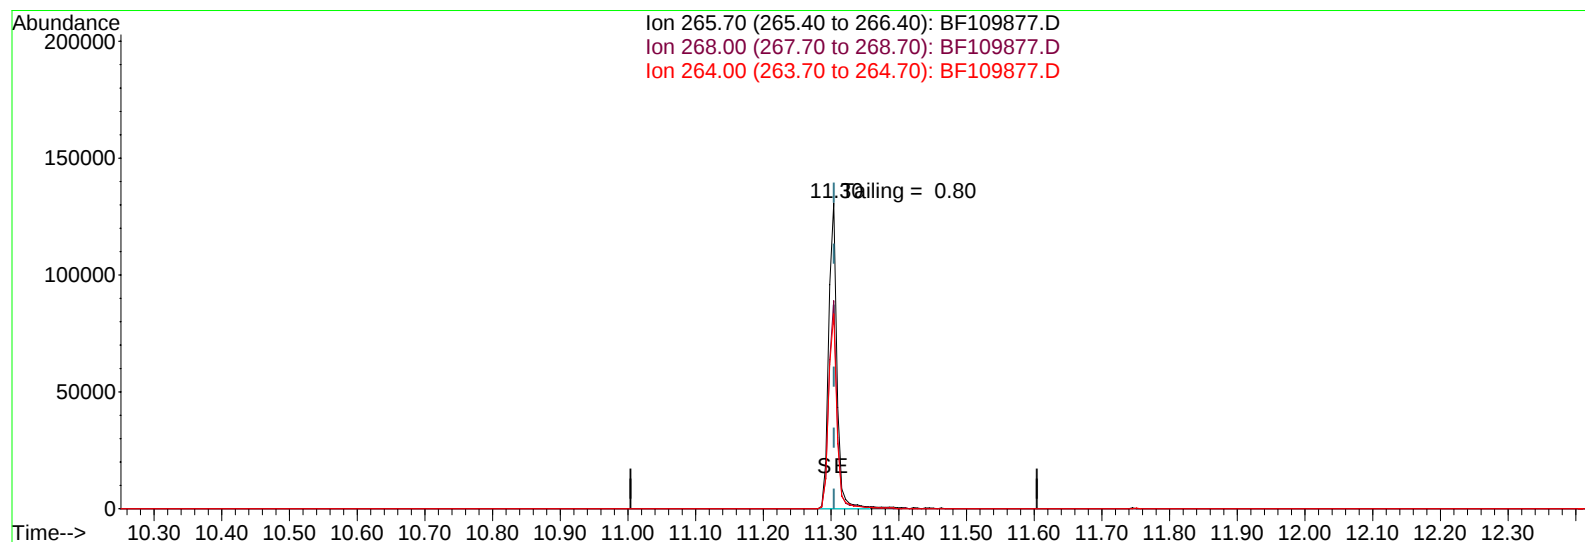

(70) Pentachlorophenol (C)




11.304min (0.000) 36340.00ng

response 111855

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	68.01
264.00	63.20	63.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF101518\
 Data File : BF109877.D
 Acq On : 15 Oct 2018 14:25
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 16 03:57:29 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101518.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 15 18:09:48 2018
 Response via : Initial Calibration

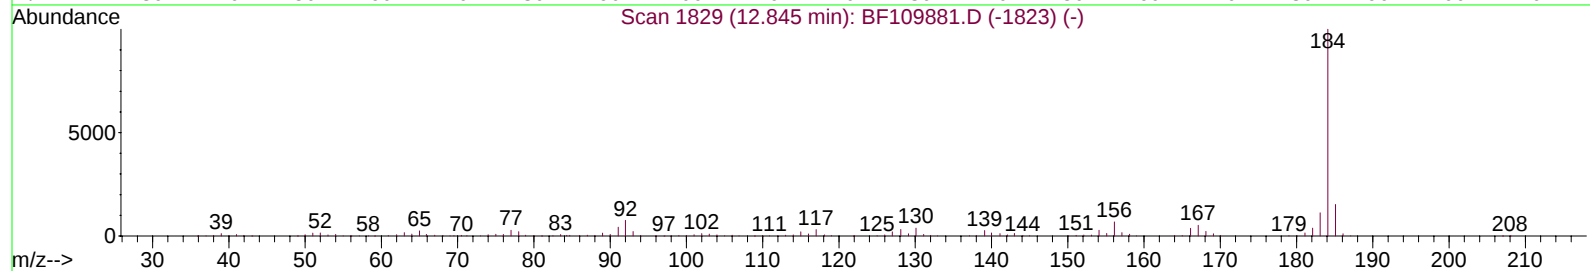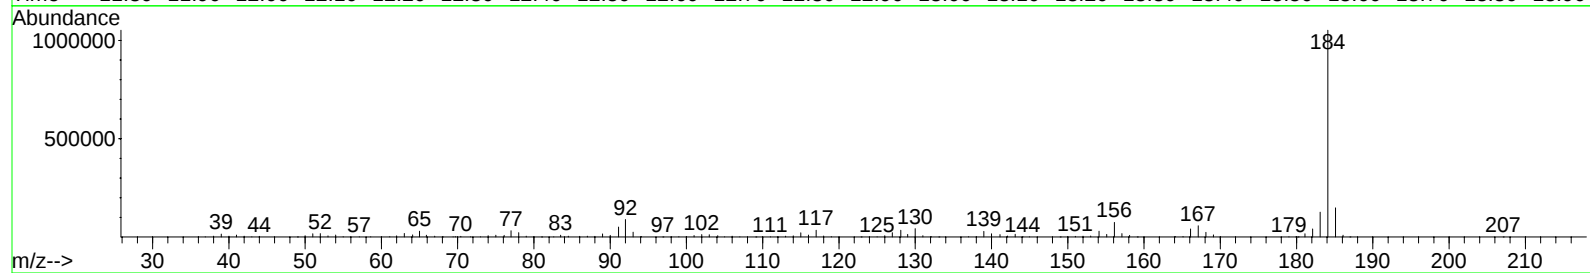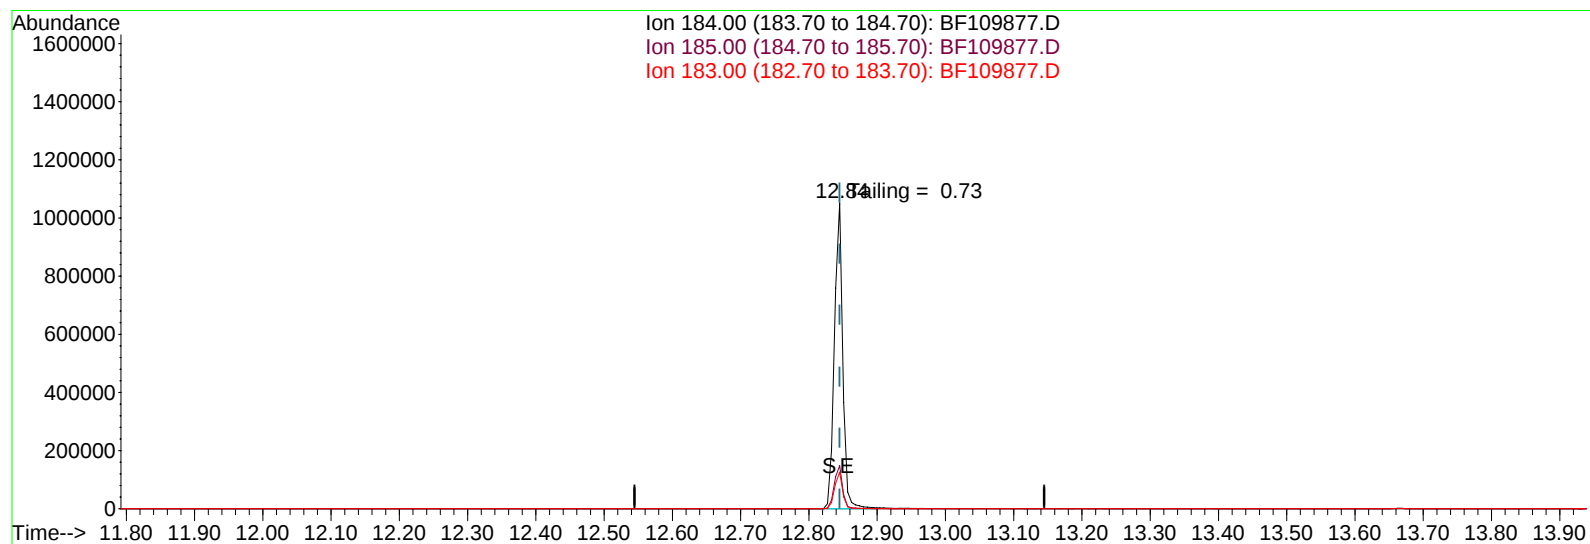

TIC: BF109877.D

(77) Benzidine

12.845min (-0.000) 0.00ng

response 893196

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	14.09
183.00	11.80	11.99
0.00	0.00	0.00