


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101518\
 Data File : BF109877.D
 Acq On : 15 Oct 2018 14:25
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 15 18:09:48 2018

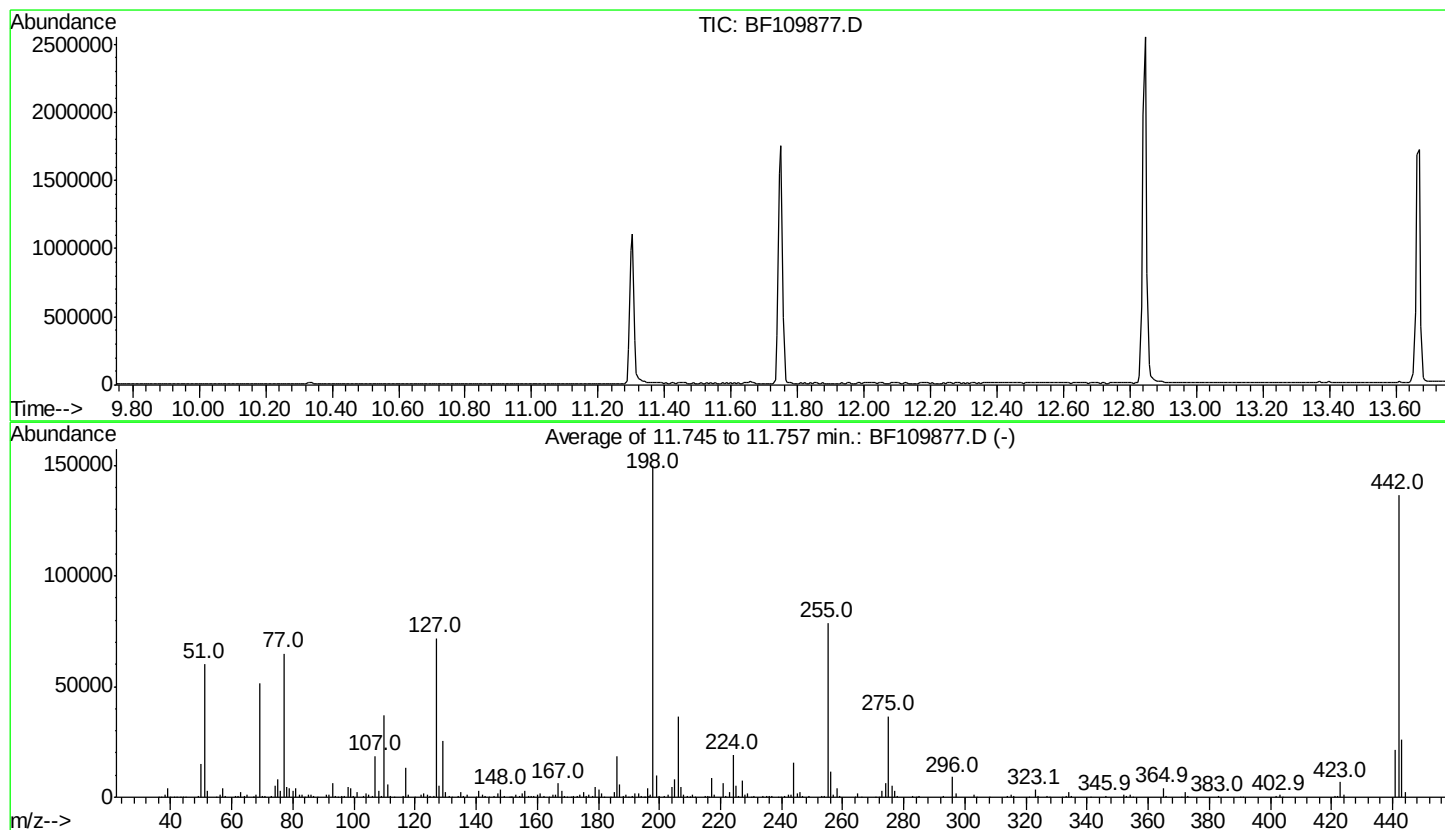

AutoFind: Scans 1642, 1643, 1644; Background Corrected with Scan 1637

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.3	60351	PASS
68	69	0.00	2	1.9	999	PASS
69	198	0.00	100	34.4	51444	PASS
70	69	0.00	2	0.7	378	PASS
127	198	10	80	48.0	71802	PASS
197	198	0.00	2	0.6	966	PASS
198	198	100	100	100.0	149722	PASS
199	198	5	9	6.6	9810	PASS
275	198	10	60	24.5	36677	PASS
365	198	1	100	2.7	4081	PASS
441	198	0.01	100	14.5	21676	PASS
442	198	50	100	91.3	136656	PASS
443	442	15	24	19.2	26170	PASS